

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121819\
 Data File : VW014434.D
 Acq On : 18 Dec 2019 15:52
 Operator : SY/VA
 Sample : K6257-14
 Misc : 5.08G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFF01

Manual Integrations
 APPROVED

MMDadoda
 12/19/2019 2:01:48 PM

Quant Time: Dec 19 02:43:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 19 01:06:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1008147	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	916485	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	373198	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	286115	18.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.96%
7) Chloroethane-d5	2.89	69	246822	21.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.96%
10) 1,1-Dichloroethene-d2	4.02	63	430435	15.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.84%
20) 2-Butanone-d5	7.07	46	160122	40.25	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.50%
24) Chloroform-d	7.65	84	613182	23.89	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.56%
26) 1,2-Dichloroethane-d4	8.31	65	312727m	23.24	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.96%
29) Benzene-d6	8.27	84	1225796	22.82	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.28%
33) 1,2-Dichloropropane-d6	9.27	67	397065	24.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.12%
37) Toluene-d8	10.32	98	1078171	22.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.80%
38) trans-1,3-Dichloropropene-	10.57	79	141142	20.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.44%
39) 2-Hexanone-d5	10.92	63	122240	37.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	278121	20.65	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.60%
61) 1,2-Dichlorobenzene-d4	13.85	152	341436	23.94	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.76%

Target Compounds					Ovalue
13) Acetone	4.13	43	10344	2.697 ug/L	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW121819\
Data File : VW014434.D
Acq On : 18 Dec 2019 15:52
Operator : SY/VA
Sample : K6257-14
Misc : 5.08G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BFF01

Manual Integrations
APPROVED

MMDadoda
12/19/2019 2:01:48 PM

Quant Time: Dec 19 02:43:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 19 01:06:45 2019
Response via : Initial Calibration

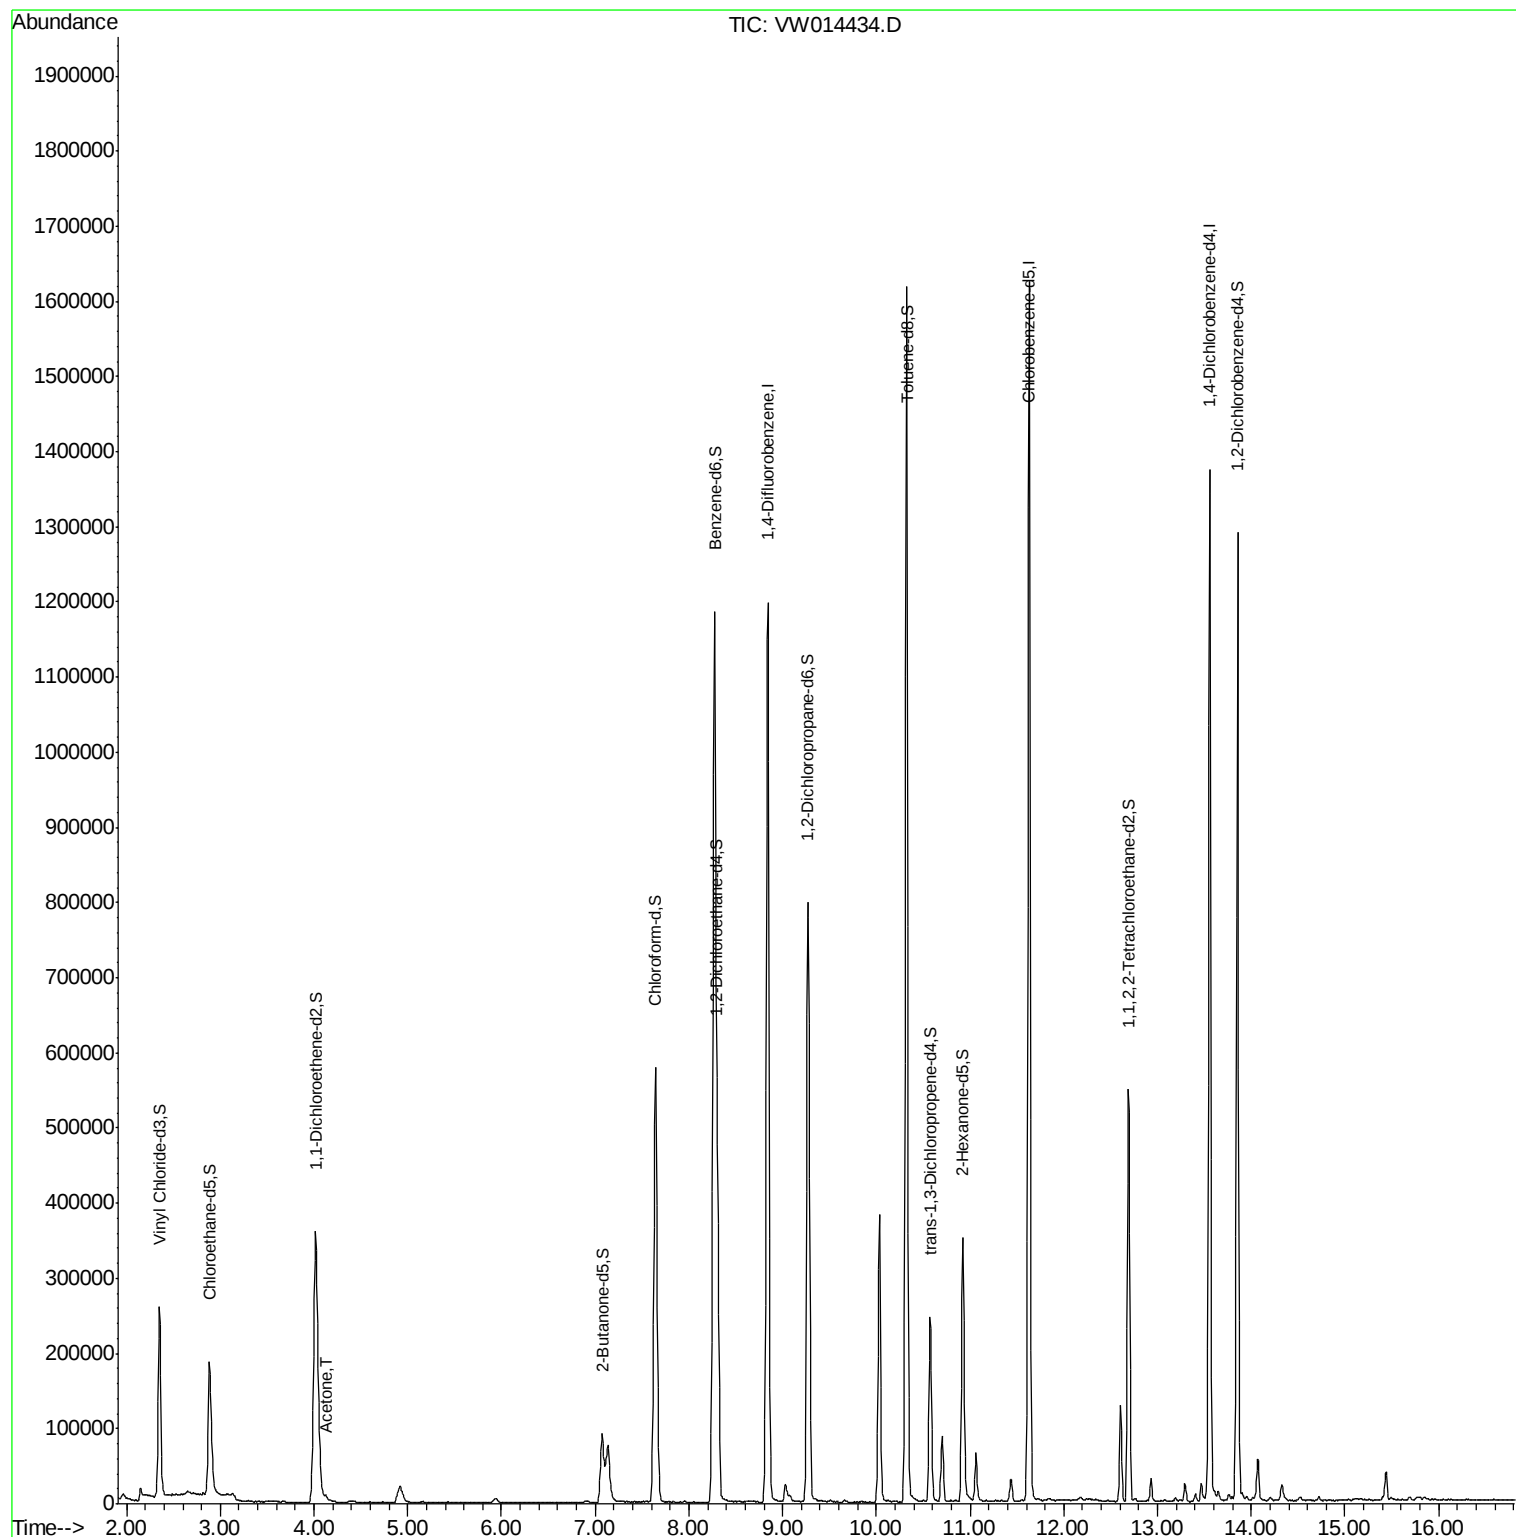

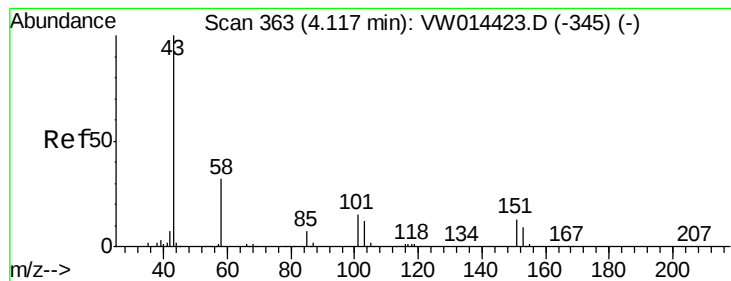

#13

Acetone

Concen: 2.697 ug/L

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW014434.D

Acq: 18 Dec 2019 15:52

Instrument :
MSVOA_W
ClientSampleId :
BFF01

Tot Ion	Ion	Ratio	Lower	Upper
43	100			
58	19.5	0.0	65.4	

Manual Integrations
APPROVED

MMDadoda
12/19/2019 2:01:48 PM

