


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121820\
Data File : VW017665.D
Acq On : 18 Dec 2020 09:11
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W121420S.M
Title : SW846 8260
Last Update : Mon Dec 14 12:39:23 2020

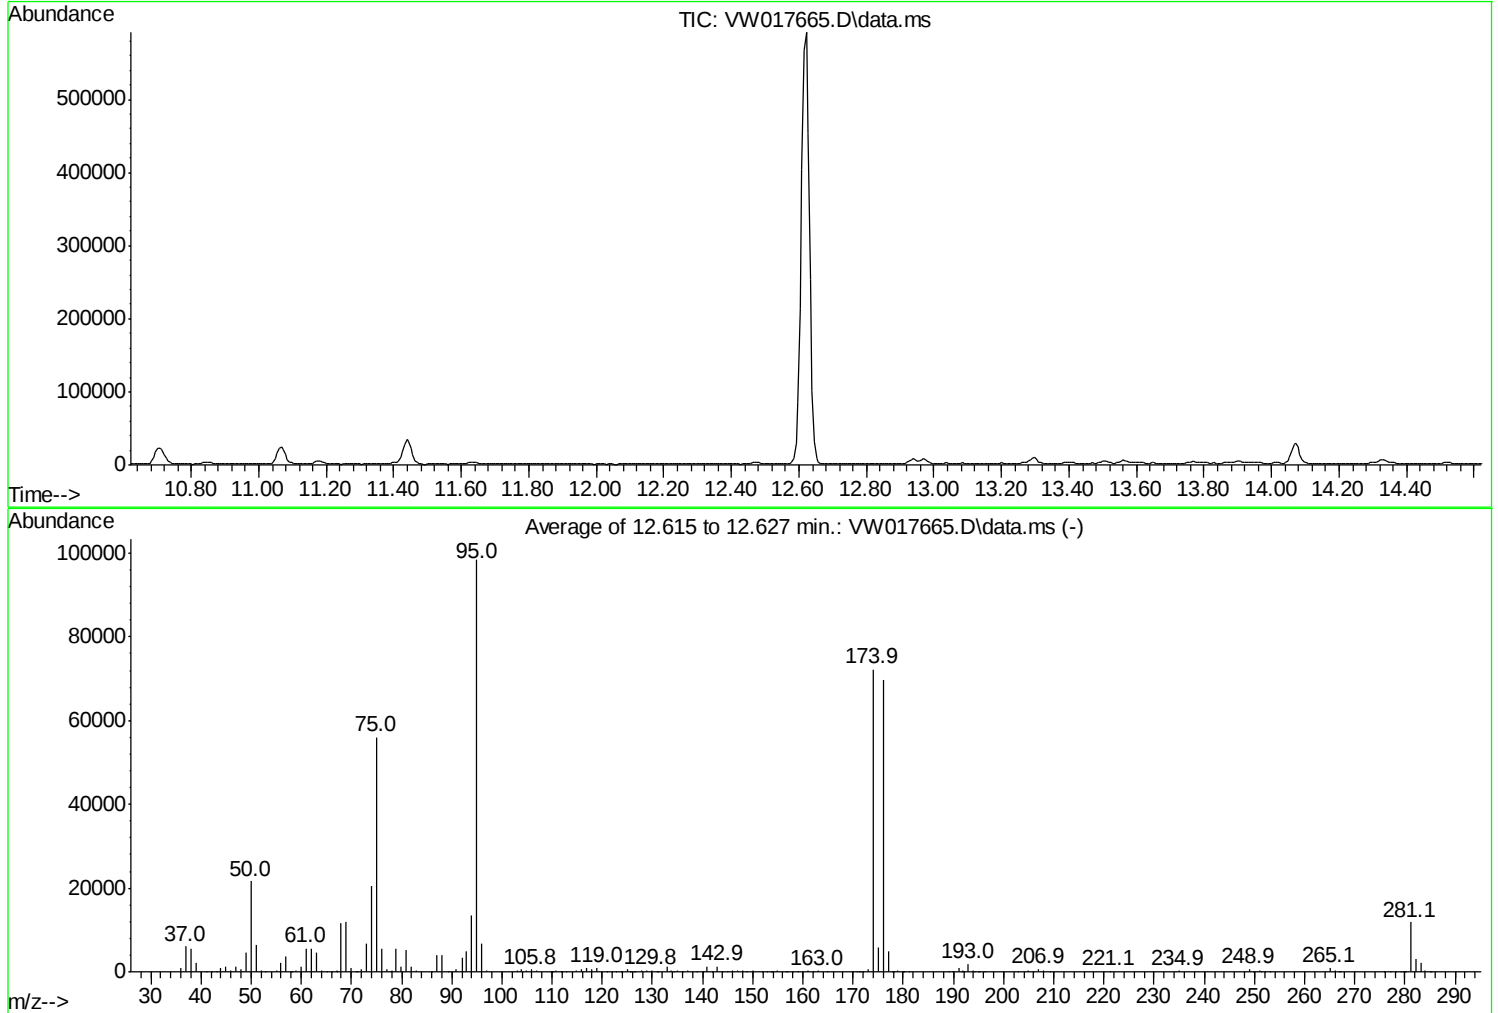

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	21640	PASS
75	95	30	60	57.0	56107	PASS
95	95	100	100	100.0	98429	PASS
96	95	5	9	6.8	6740	PASS
173	174	0.00	2	0.7	479	PASS
174	95	50	100	73.4	72211	PASS
175	174	5	9	8.3	5966	PASS
176	174	95	101	96.4	69624	PASS
177	176	5	9	7.1	4916	PASS