

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121821\
 Data File : VW021456.D
 Acq On : 18 Dec 2021 05:40
 Operator : SY/VA
 Sample : VIBLK545
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK545

Quant Time: Dec 18 23:09:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 18 00:55:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	135074	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	134302	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	76505	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	33276	13.527	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.120%
7) Chloroethane-d5	2.879	69	23436	14.411	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.640%
11) 1,1-Dichloroethene-d2	4.013	63	48340	14.739	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.960%
21) 2-Butanone-d5	7.080	46	18172	52.404	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.800%
24) Chloroform-d	7.653	84	77028	20.463	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.840%
26) 1,2-Dichloroethane-d4	8.305	65	43299	21.625	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.480%
32) Benzene-d6	8.275	84	155836	21.169	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.680%
36) 1,2-Dichloropropane-d6	9.274	67	42959	21.759	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.040%
41) Toluene-d8	10.323	98	153923	20.464	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.840%
43) trans-1,3-Dichloroprop...	10.579	79	17187	18.907	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.640%
47) 2-Hexanone-d5	10.927	63	14833	50.808	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.620%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	35165	20.720	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	60604	20.440	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.760%
Target Compounds					Qvalue	
13) Acetone	4.135	43	1386	4.458	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121821\
Data File : VW021456.D
Acq On : 18 Dec 2021 05:40
Operator : SY/VA
Sample : VIBLK545
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK545

Quant Time: Dec 18 23:09:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

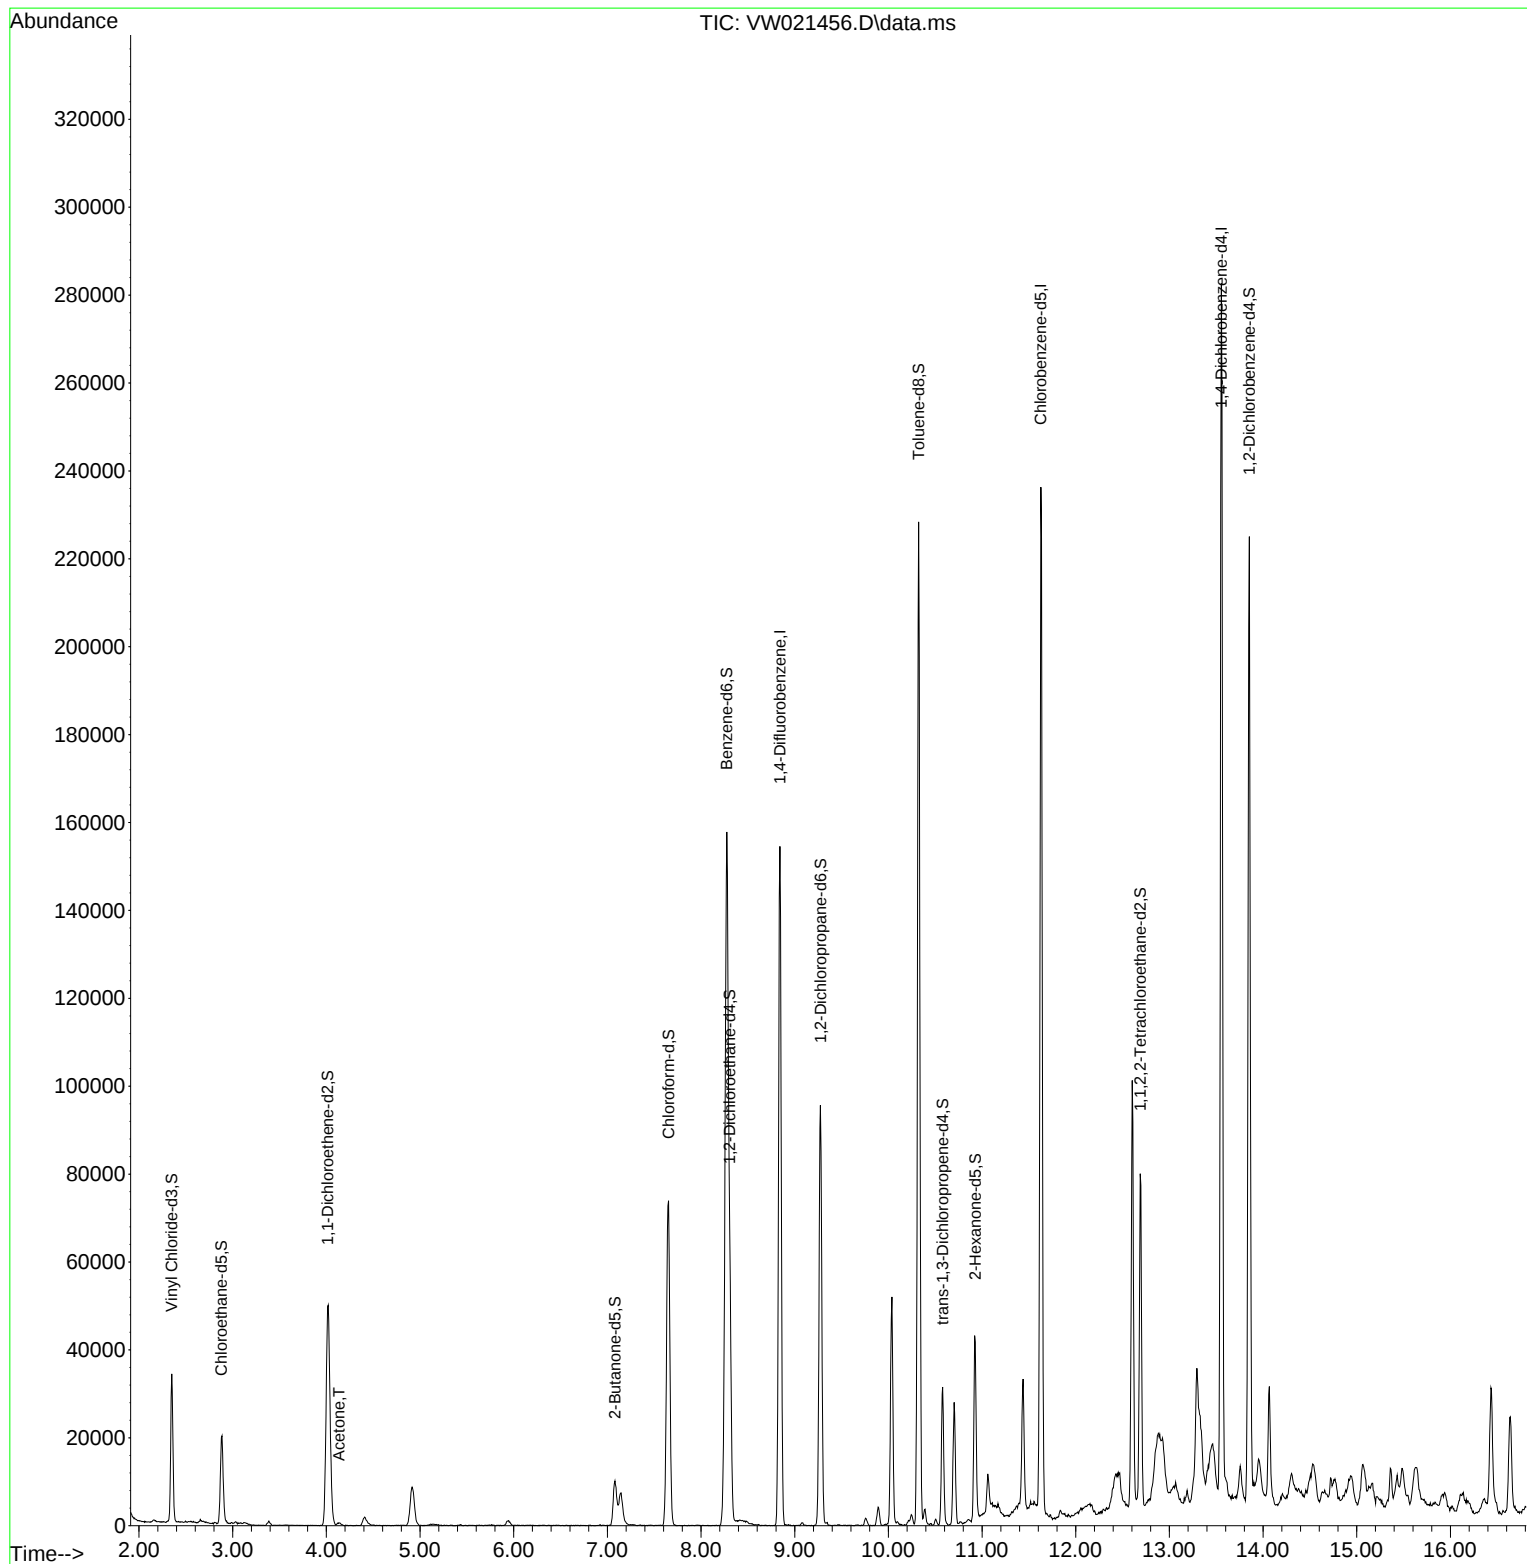

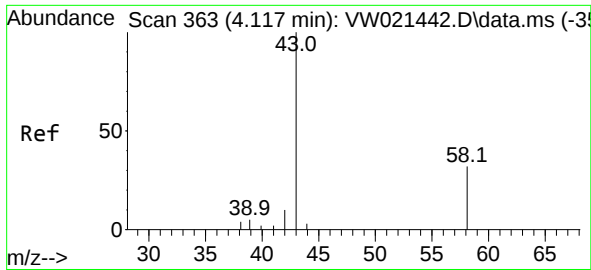

#13
 Acetone
 Concen: 4.458 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.018 min
 Lab File: VW021456.D
 Acq: 18 Dec 2021 05:40

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK545

Tgt Ion: 43 Resp: 1386

Ion	Ratio	Lower	Upper
43	100		
58	21.0	0.0	52.8

