

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121821\
 Data File : VW021460.D
 Acq On : 18 Dec 2021 07:17
 Operator : SY/VA
 Sample : M5121-01
 Misc : 5.84g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGL50

Quant Time: Dec 18 23:10:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 18 00:55:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	114206	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.627	117	85780	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	29169	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	38722	18.616	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.480%
7) Chloroethane-d5	2.879	69	26085	18.970	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.880%
11) 1,1-Dichloroethene-d2	4.013	63	43952	15.850	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.400%
21) 2-Butanone-d5	7.085	46	15301	52.187	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.380%
24) Chloroform-d	7.646	84	66754	20.974	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.880%
26) 1,2-Dichloroethane-d4	8.305	65	36589	21.613	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.440%
32) Benzene-d6	8.274	84	123128	26.187	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.760%
36) 1,2-Dichloropropane-d6	9.274	67	35182	27.900	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.600%
41) Toluene-d8	10.323	98	106848	22.241	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.960%
43) trans-1,3-Dichloroprop...	10.579	79	10557	18.182	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.720%
47) 2-Hexanone-d5	10.926	63	10640	57.061	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.120%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	22498	20.755	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.000%
66) 1,2-Dichlorobenzene-d4	13.853	152	21432	18.959	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.840%
Target Compounds						
					Qvalue	
13) Acetone	4.141	43	4211	16.021	ug/L	81
14) Carbon disulfide	4.385	76	8206	2.245	ug/L	98
20) cis-1,2-Dichloroethene	7.171	96	1041	0.644	ug/L	# 59
27) 1,2-Dichloroethane	8.402	62	1661	0.939	ug/L	98
33) Benzene	8.323	78	54283	11.617	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121821\
Data File : VW021460.D
Acq On : 18 Dec 2021 07:17
Operator : SY/VA
Sample : M5121-01
Misc : 5.84g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGL50

Quant Time: Dec 18 23:10:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

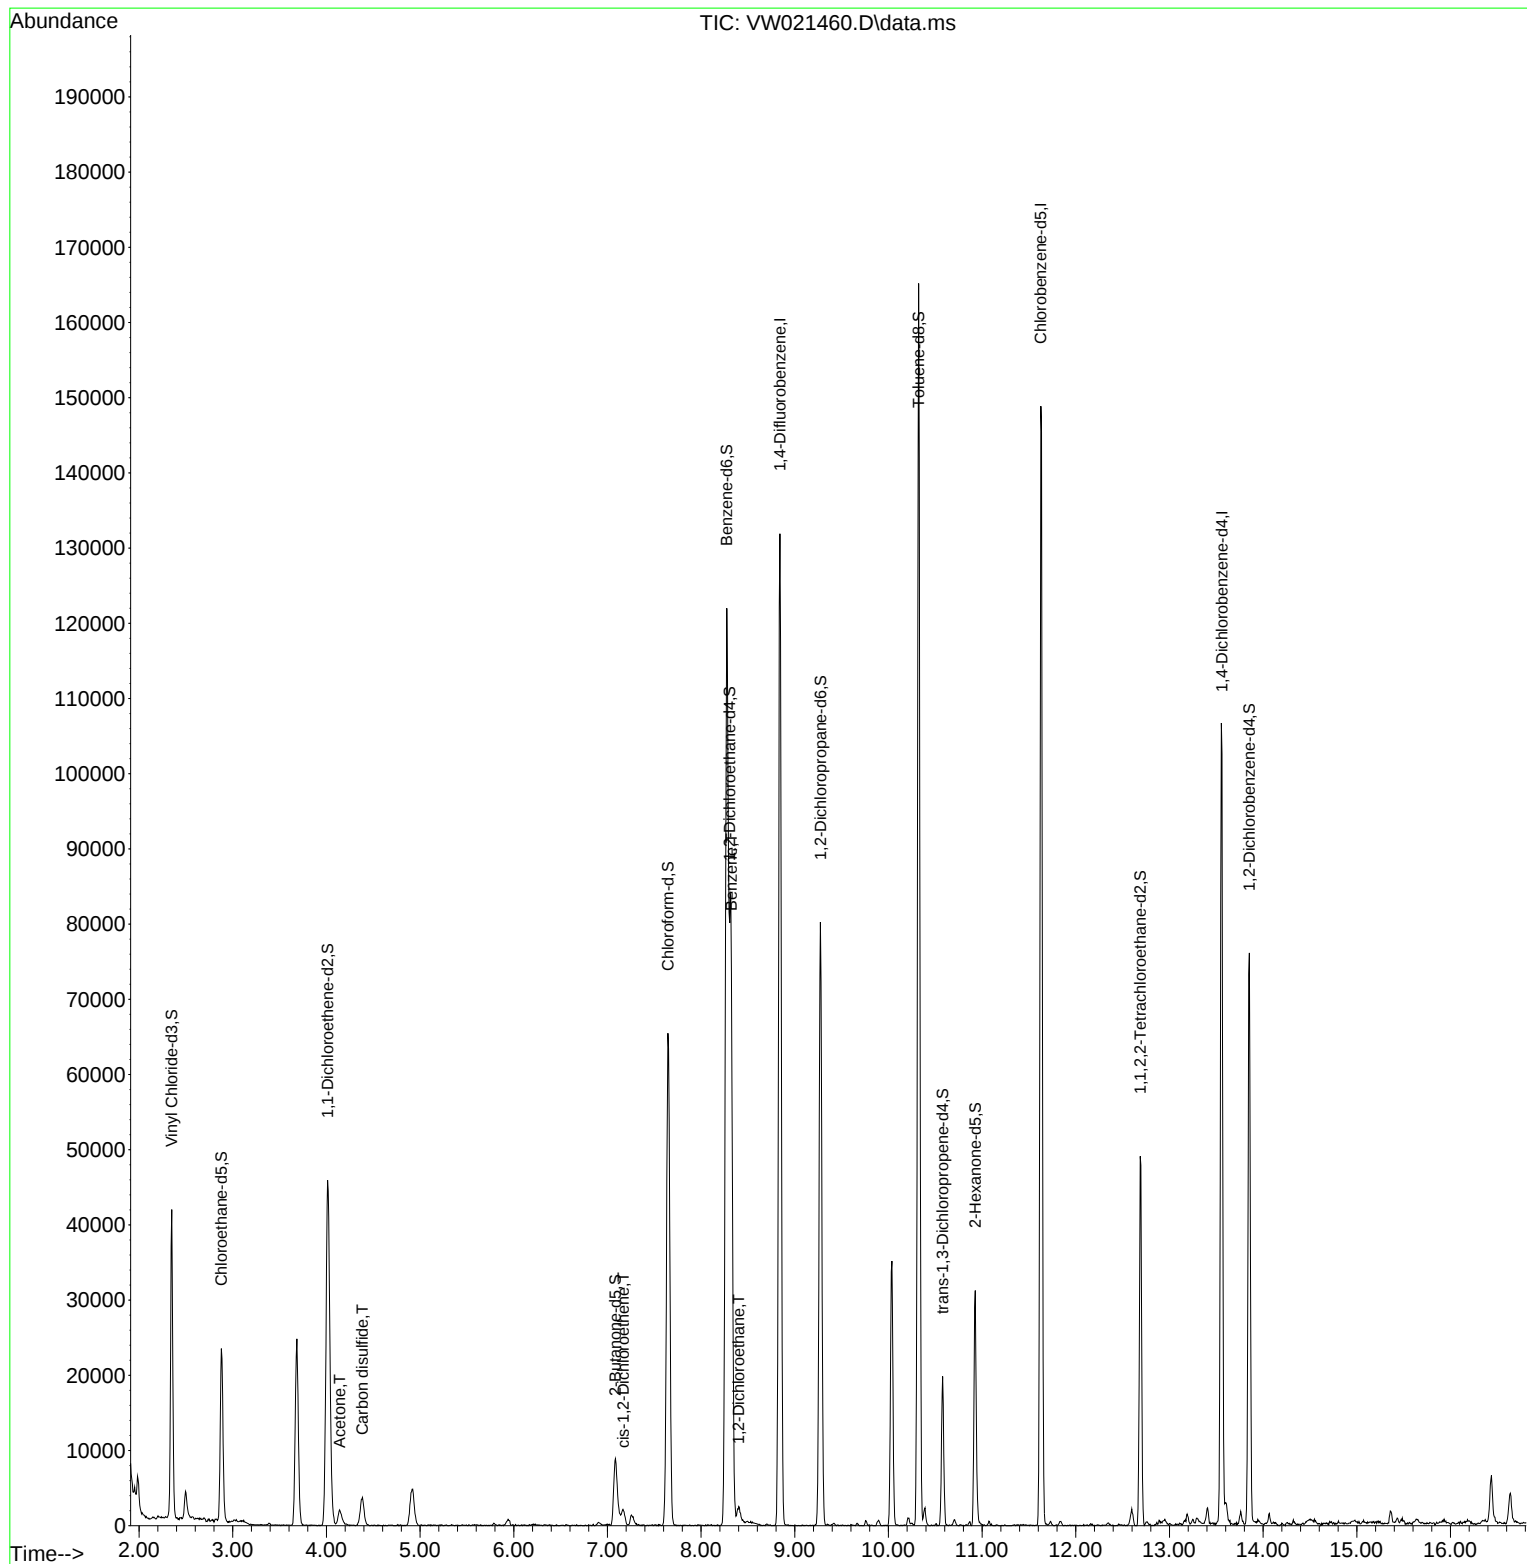

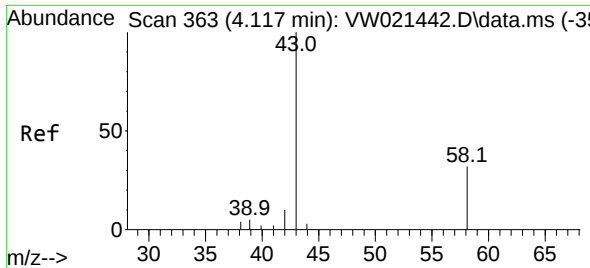

#13

Acetone

Concen: 16.021 ug/L

RT: 4.141 min Scan# 3

Delta R.T. 0.024 min

Lab File: VW021460.D

Acq: 18 Dec 2021 07:17

Instrument :

MSVOA_W

ClientSampleId :





BGL50

Tgt Ion: 43 Resp: 4211

Ion Ratio Lower Upper

43 100

58 16.6 0.0 52.8

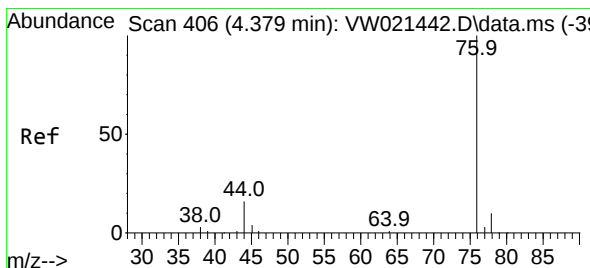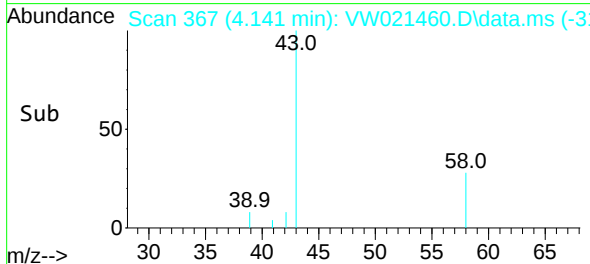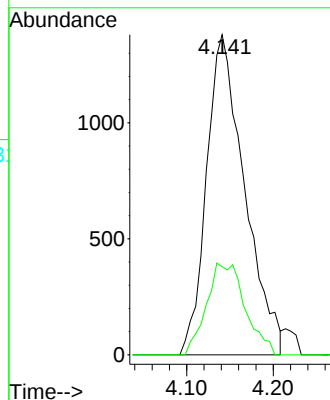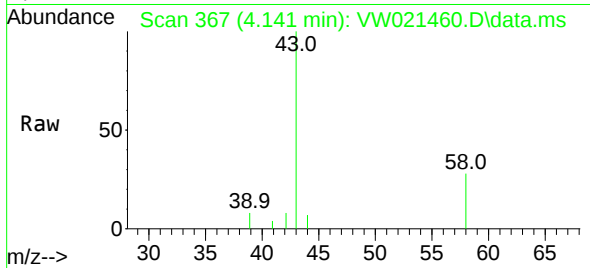

#14

Carbon disulfide

Concen: 2.245 ug/L

RT: 4.385 min Scan# 407

Delta R.T. 0.006 min

Lab File: VW021460.D




Acq: 18 Dec 2021 07:17


Tgt Ion: 76 Resp: 8206

Ion Ratio Lower Upper

76 100

78 9.5 7.1 10.7


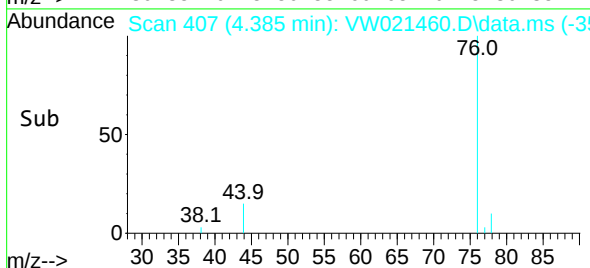
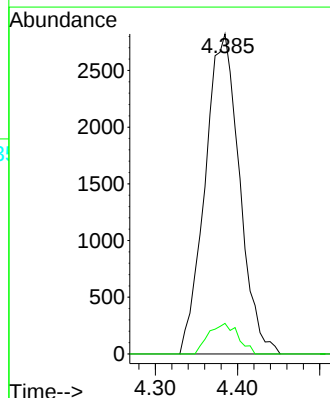
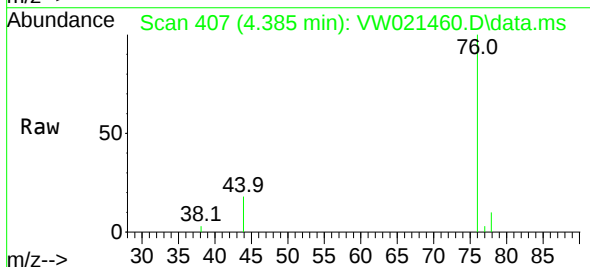


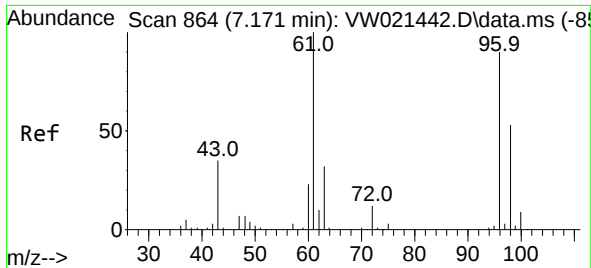

#20
 cis-1,2-Dichloroethene
 Concen: 0.644 ug/L
 RT: 7.171 min Scan# 864
 Delta R.T. -0.000 min
 Lab File: VW021460.D
 Acq: 18 Dec 2021 07:17




Instrument :
 MSVOA_W
 ClientSampleId :
 BGL50


Tgt Ion: 96 Resp: 1041
 Ion Ratio Lower Upper
 96 100
 61 96.1 103.7 192.7#
 68 0.0 0.0 0.0

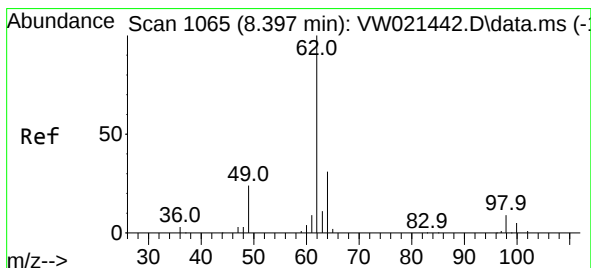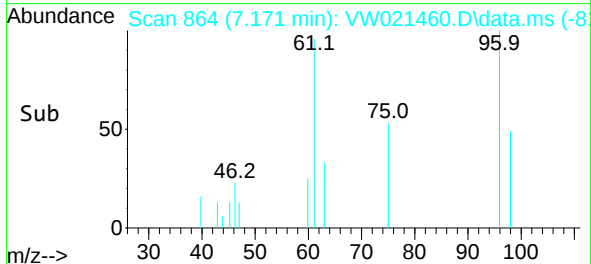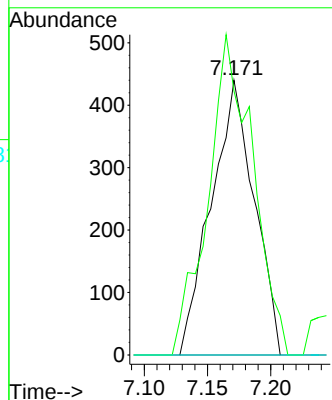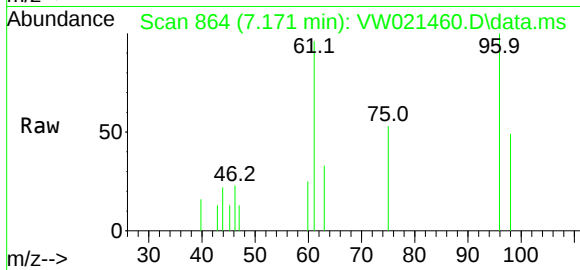

#27
 1,2-Dichloroethane
 Concen: 0.939 ug/L
 RT: 8.402 min Scan# 1066
 Delta R.T. 0.006 min
 Lab File: VW021460.D
 Acq: 18 Dec 2021 07:17

Tgt Ion: 62 Resp: 1661
 Ion Ratio Lower Upper
 62 100
 98 8.9 6.5 9.7

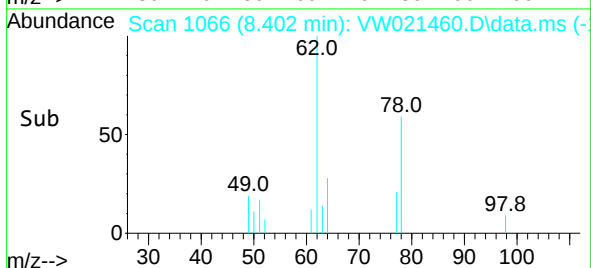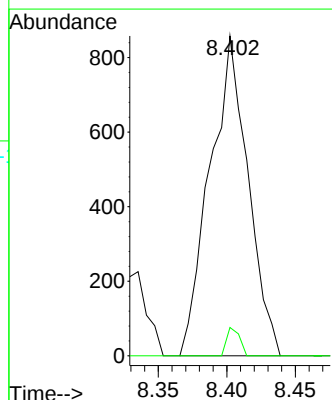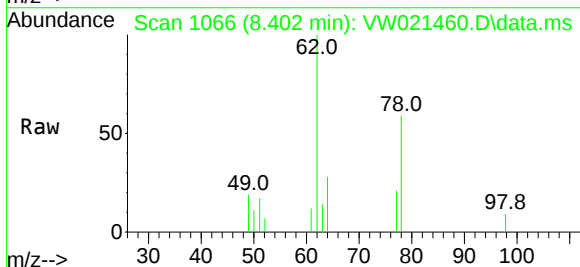

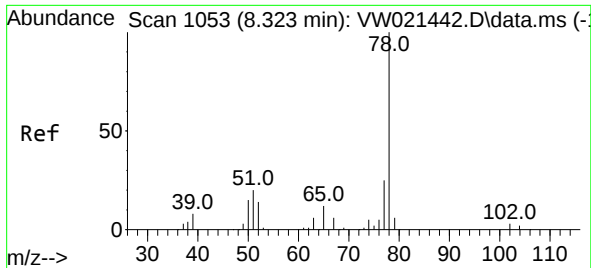

#33

Benzene

Concen: 11.617 ug/L

RT: 8.323 min Scan# 10

Delta R.T. -0.000 min

Lab File: VW021460.D

Acq: 18 Dec 2021 07:17

Instrument :

MSVOA_W

ClientSampleId :

BGL50

Tgt Ion: 78 Resp: 54283

