

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121821\
 Data File : VW021473.D
 Acq On : 18 Dec 2021 13:54
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK549

Quant Time: Dec 18 23:11:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 18 00:55:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	136769	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	132058	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77361	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	41853	16.802	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.200%
7) Chloroethane-d5	2.885	69	25537	15.508	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.040%
11) 1,1-Dichloroethene-d2	4.019	63	58223	17.532	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.120%
21) 2-Butanone-d5	7.080	46	20596	58.658	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.320%
24) Chloroform-d	7.647	84	82738	21.708	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.840%
26) 1,2-Dichloroethane-d4	8.305	65	46905	23.135	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.560%
32) Benzene-d6	8.275	84	170511	23.556	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.240%
36) 1,2-Dichloropropane-d6	9.268	67	46308	23.854	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.400%
41) Toluene-d8	10.323	98	172662	23.346	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.400%
43) trans-1,3-Dichloroprop...	10.579	79	20011	22.387	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.560%
47) 2-Hexanone-d5	10.921	63	17794	61.986	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.980%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	38980	23.358	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	68089	22.710	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.840%
Target Compounds						
13) Acetone	4.135	43	1934	6.144	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121821\
Data File : VW021473.D
Acq On : 18 Dec 2021 13:54
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK549

Quant Time: Dec 18 23:11:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

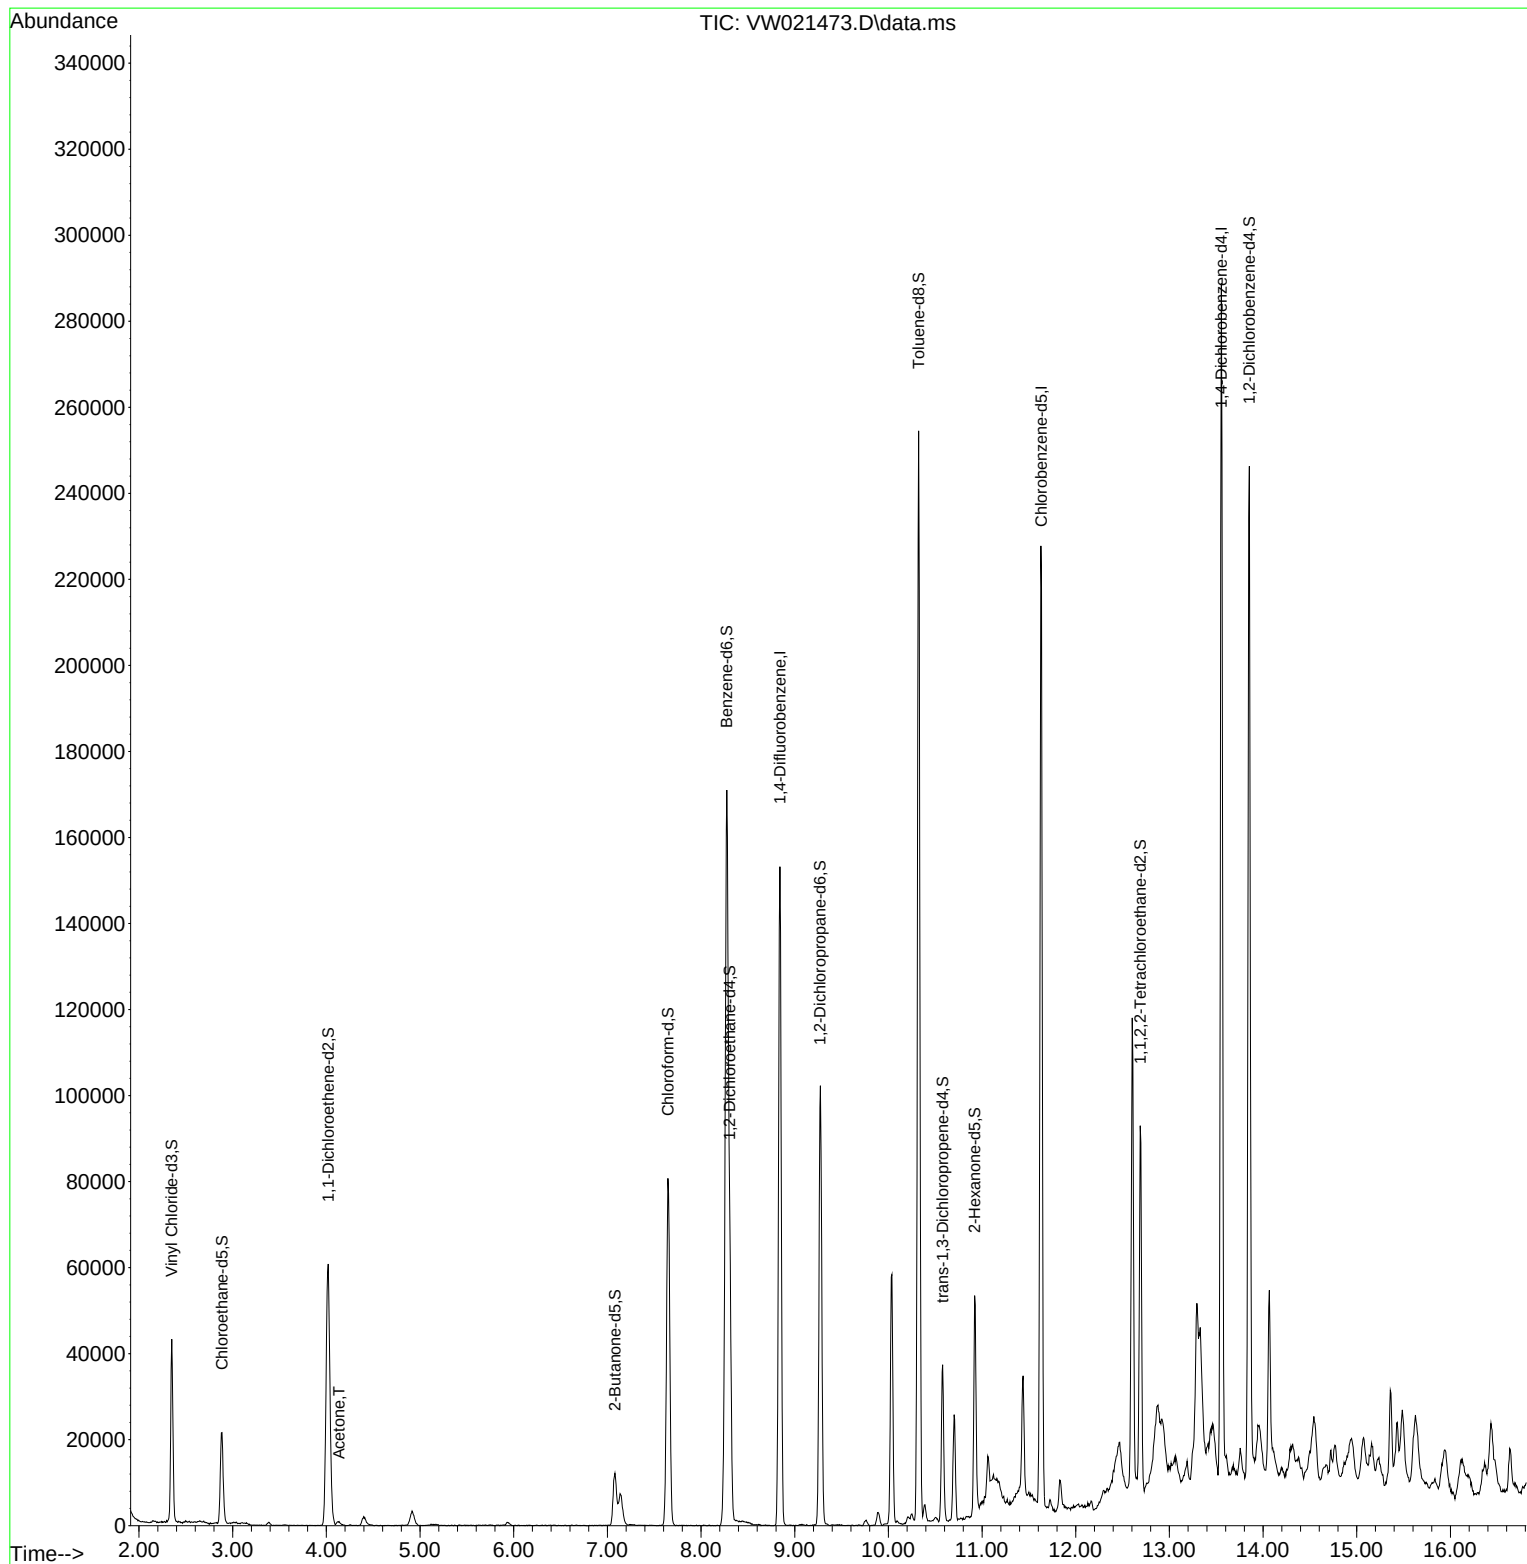

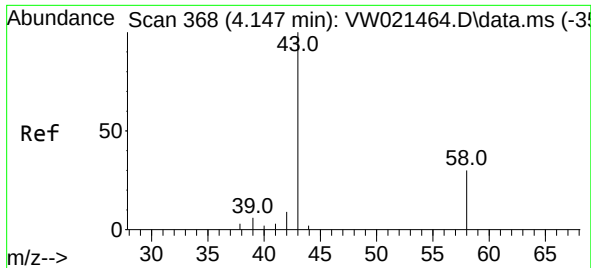

#13
 Acetone
 Concen: 6.144 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.018 min
 Lab File: VW021473.D
 Acq: 18 Dec 2021 13:54

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK549

Tgt Ion: 43 Resp: 1934
 Ion Ratio Lower Upper
 43 100
 58 28.9 0.0 52.8

