

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121821\
 Data File : VW021475.D
 Acq On : 18 Dec 2021 14:42
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK550

Quant Time: Dec 18 23:12:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 18 00:55:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	141933	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	137102	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	79769	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	41592	16.090	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.360%
7) Chloroethane-d5	2.885	69	25095	14.685	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.760%
11) 1,1-Dichloroethene-d2	4.013	63	56807	16.484	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.920%
21) 2-Butanone-d5	7.074	46	24737	67.888	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	135.780%#
24) Chloroform-d	7.647	84	84500	21.363	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.440%
26) 1,2-Dichloroethane-d4	8.305	65	48599	23.099	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.400%
32) Benzene-d6	8.275	84	170445	22.680	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.720%
36) 1,2-Dichloropropane-d6	9.274	67	46659	23.151	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.600%
41) Toluene-d8	10.323	98	171686	22.360	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.440%
43) trans-1,3-Dichloroprop...	10.579	79	21030	22.662	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.640%
47) 2-Hexanone-d5	10.921	63	21100	70.798	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	141.600%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	44056	25.428	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.720%
66) 1,2-Dichlorobenzene-d4	13.853	152	69453	22.466	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.880%
Target Compounds						
13) Acetone	4.129	43	2092	6.404	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121821\
Data File : VW021475.D
Acq On : 18 Dec 2021 14:42
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK550

Quant Time: Dec 18 23:12:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

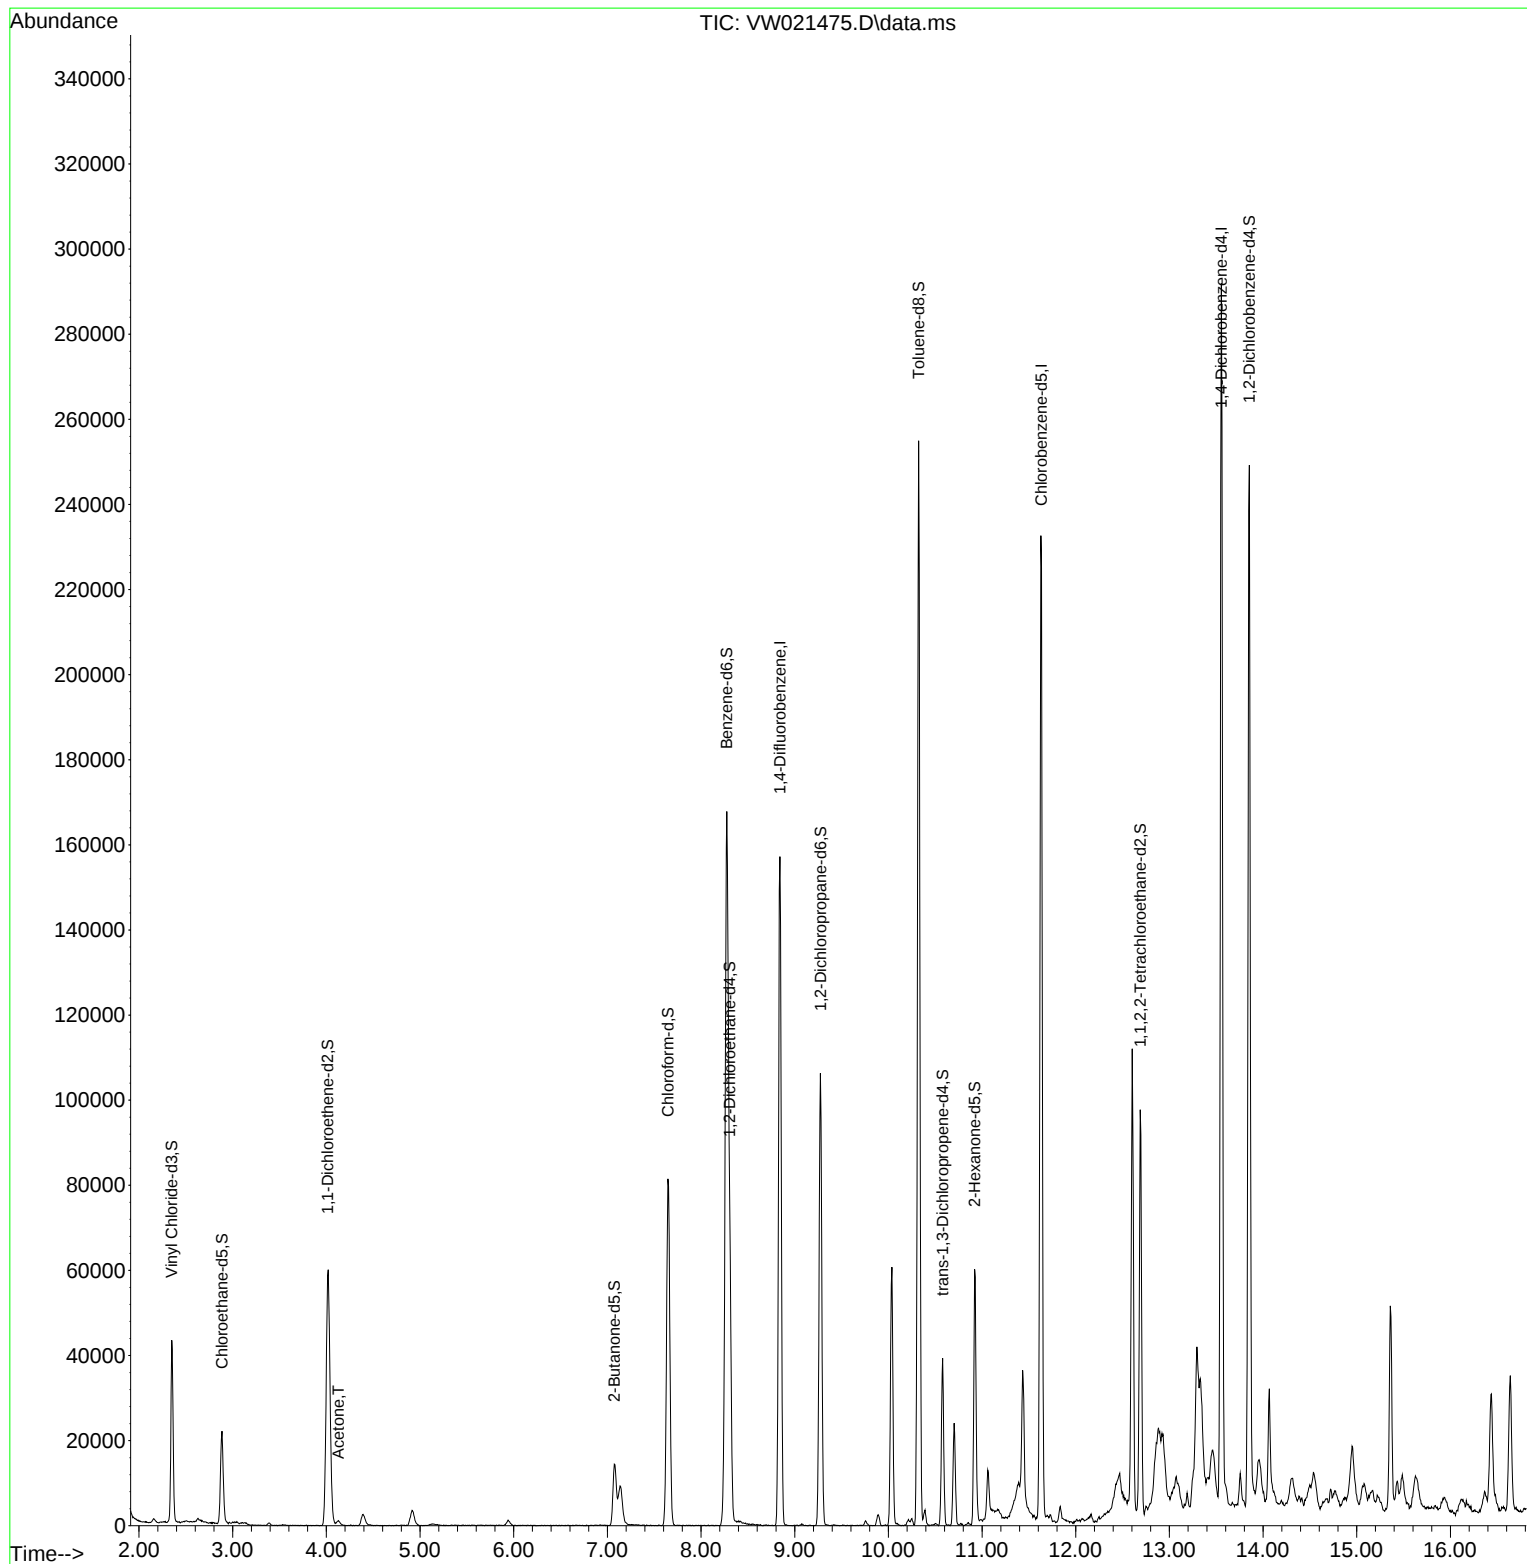

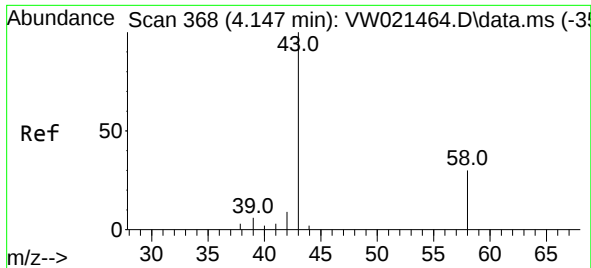

#13
 Acetone
 Concen: 6.404 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW021475.D
 Acq: 18 Dec 2021 14:42

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK550

Tgt Ion: 43 Resp: 2092
 Ion Ratio Lower Upper
 43 100
 58 33.4 0.0 52.8

