

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121823\
 Data File : VW027755.D
 Acq On : 19 Dec 2023 02:07
 Operator : SY/MD
 Sample : 05891-07
 Misc : 5.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 19 04:56:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sun Dec 17 01:25:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	662749	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	586047	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	266737	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	171220	18.242	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.960%
7) Chloroethane-d5	2.899	69	137449	18.808	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.240%
11) 1,1-Dichloroethene-d2	4.021	65	69415	18.466	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.880%
21) 2-Butanone-d5	7.099	46	61143	38.255	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.520%
24) Chloroform-d	7.648	84	311046	19.723	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.880%
26) 1,2-Dichloroethane-d4	8.307	65	150949	20.386	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.560%
32) Benzene-d6	8.276	84	678855	19.820	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.280%
36) 1,2-Dichloropropane-d6	9.276	67	193436	19.935	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.720%
41) Toluene-d8	10.325	98	618704	19.470	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.880%
43) trans-1,3-Dichloroprop...	10.574	79	71941	19.149	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.600%
47) 2-Hexanone-d5	10.922	63	59109	41.801	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.600%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	144988	19.758	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.040%
66) 1,2-Dichlorobenzene-d4	13.848	152	201722	21.127	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.520%
Target Compounds						Qvalue
34) Trichloroethene	8.843	95	18377	1.984	ug/L #	3
39) cis-1,3-Dichloropropene	10.032	75	4913	0.393	ug/L #	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121823\
Data File : VW027755.D
Acq On : 19 Dec 2023 02:07
Operator : SY/MD
Sample : 05891-07
Misc : 5.44g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 19 04:56:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121523SMA.M
Quant Title : SFAM01.0
QLast Update : Sun Dec 17 01:25:09 2023
Response via : Initial Calibration

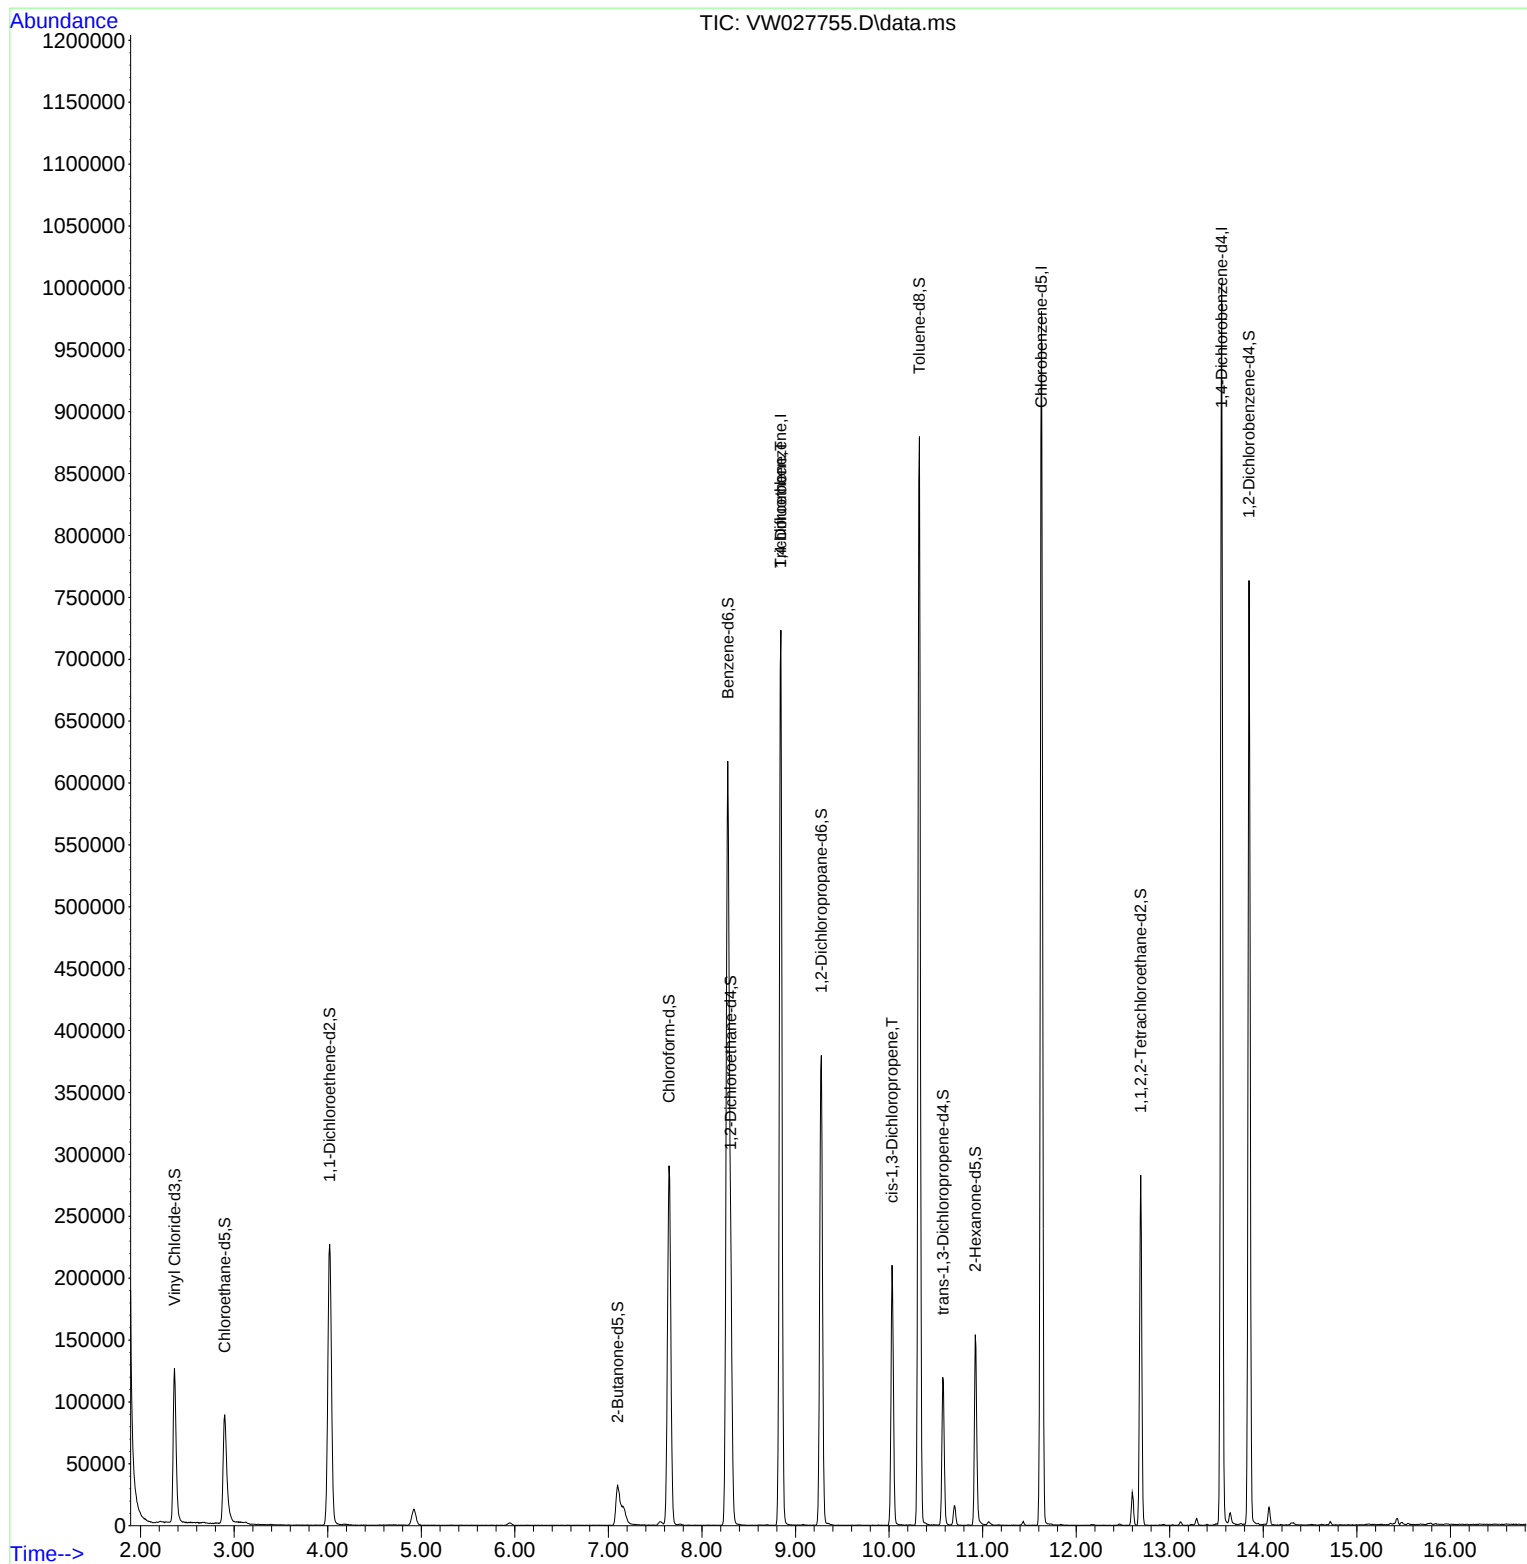

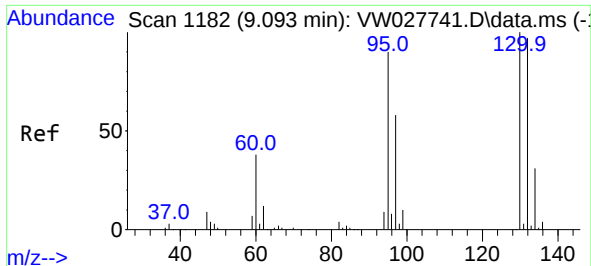




#34
Trichloroethene
Concen: 1.984 ug/L
RT: 8.843 min Scan# 1182
Delta R.T. -0.244 min
Lab File: VW027755.D
Acq: 19 Dec 2023 02:07

Instrument :
MSVOA_W
ClientSampleId :

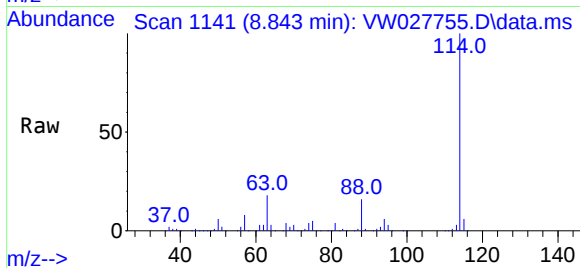

Tgt Ion: 95 Resp: 18377

Ion	Ratio	Lower	Upper
95	100		
97	0.0	45.9	85.3#
132	0.0	70.4	130.8#
130	0.0	74.8	139.0#

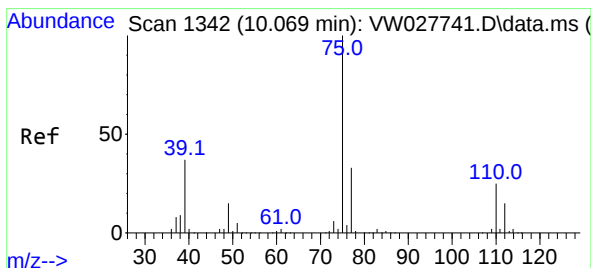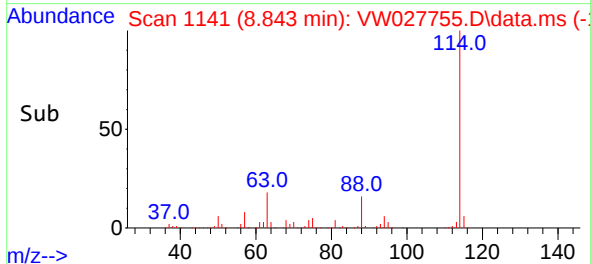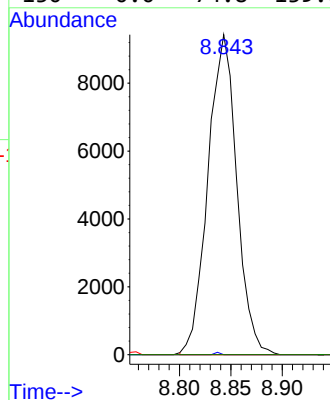

#39
cis-1,3-Dichloropropene
Concen: 0.393 ug/L
RT: 10.032 min Scan# 1336
Delta R.T. -0.037 min
Lab File: VW027755.D
Acq: 19 Dec 2023 02:07

Tgt Ion: 75 Resp: 4913

Ion	Ratio	Lower	Upper
75	100		
77	53.4	21.8	40.6#

