




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121824\
Data File : VW031342.D
Acq On : 18 Dec 2024 16:03
Operator : SY/MD
Sample : P5265-10
Misc : 4.97g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 19 00:24:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 19 00:20:44 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/19/2024
Supervised By :Mahesh Dadoda 12/20/2024

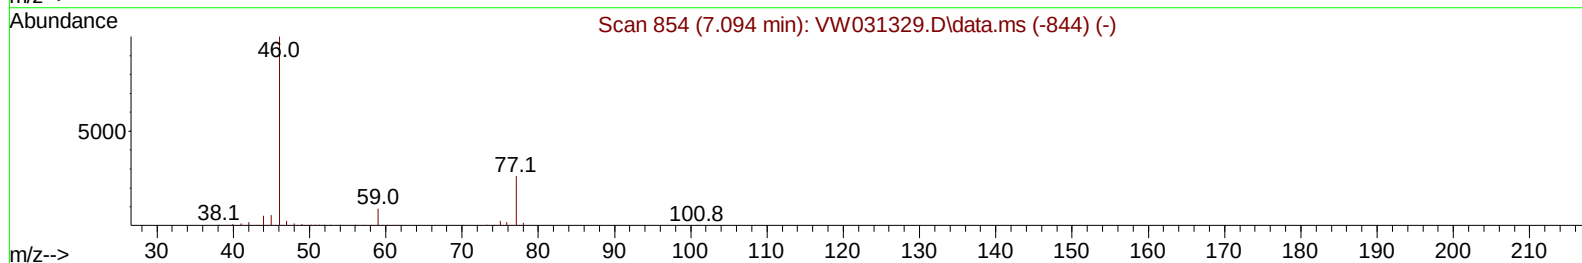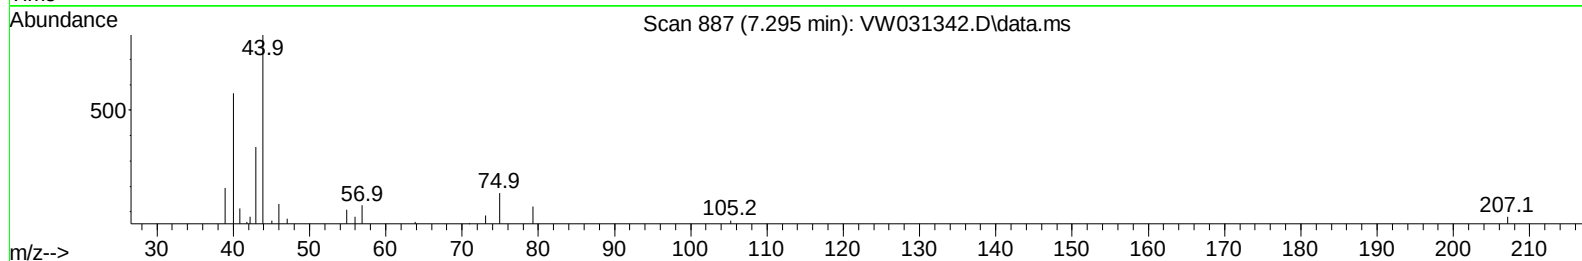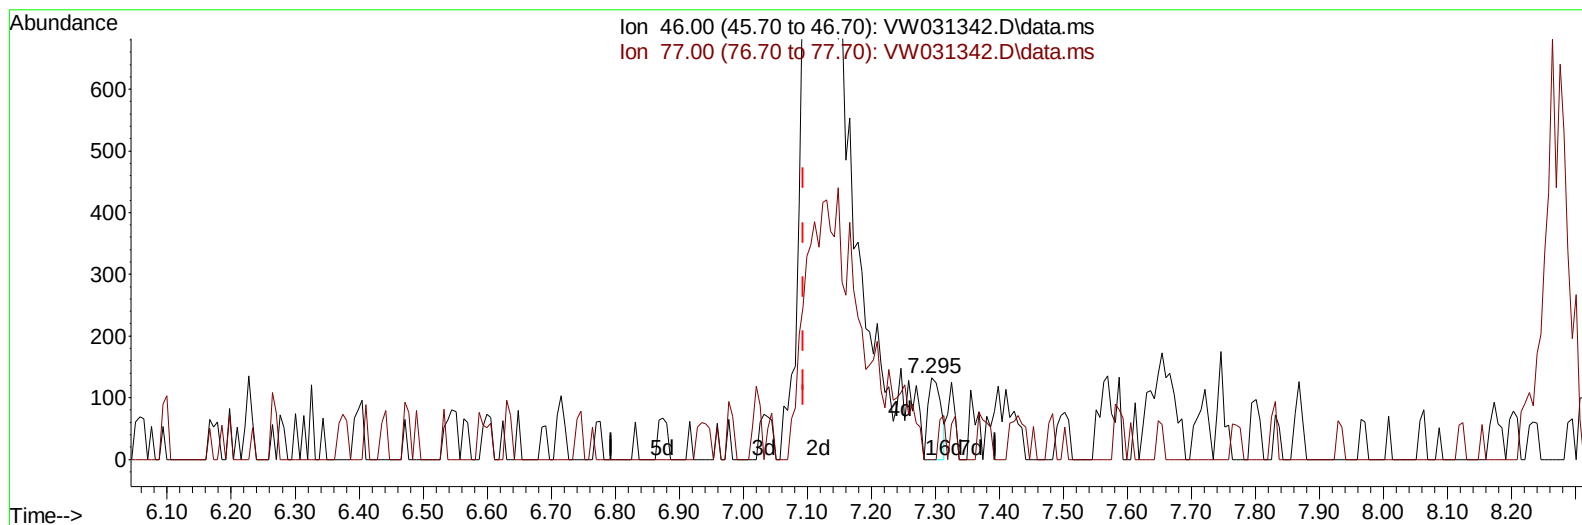

TIC: VW031342.D\data.ms

(21) 2-Butanone-d5 (S)

7.295min (+ 0.201) 0.06 ug/L

response 182

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	29.60	27.47
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121824\
 Data File : VW031342.D
 Acq On : 18 Dec 2024 16:03
 Operator : SY/MD
 Sample : P5265-10
 Misc : 4.97g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 19 00:24:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 19 00:20:44 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/19/2024
 Supervised By :Mahesh Dadoda 12/20/2024

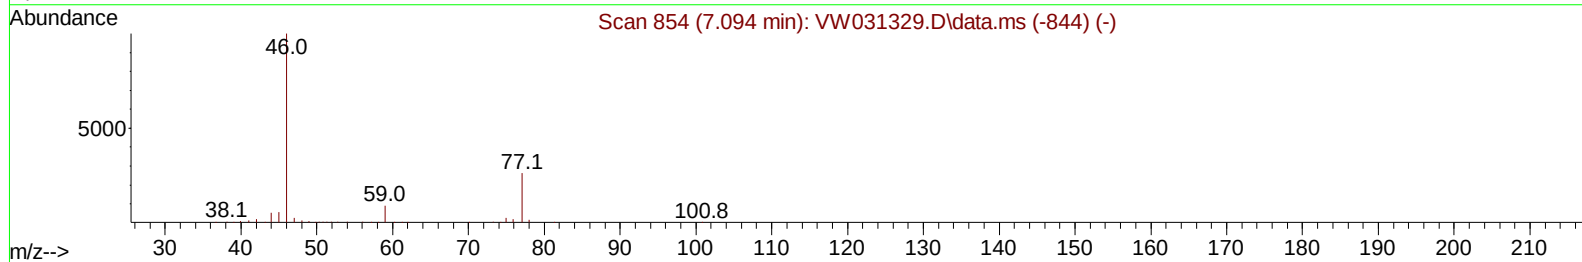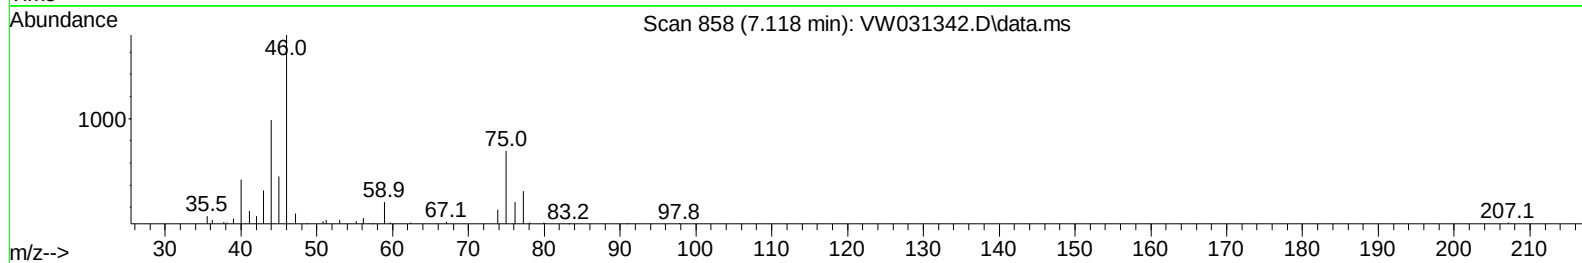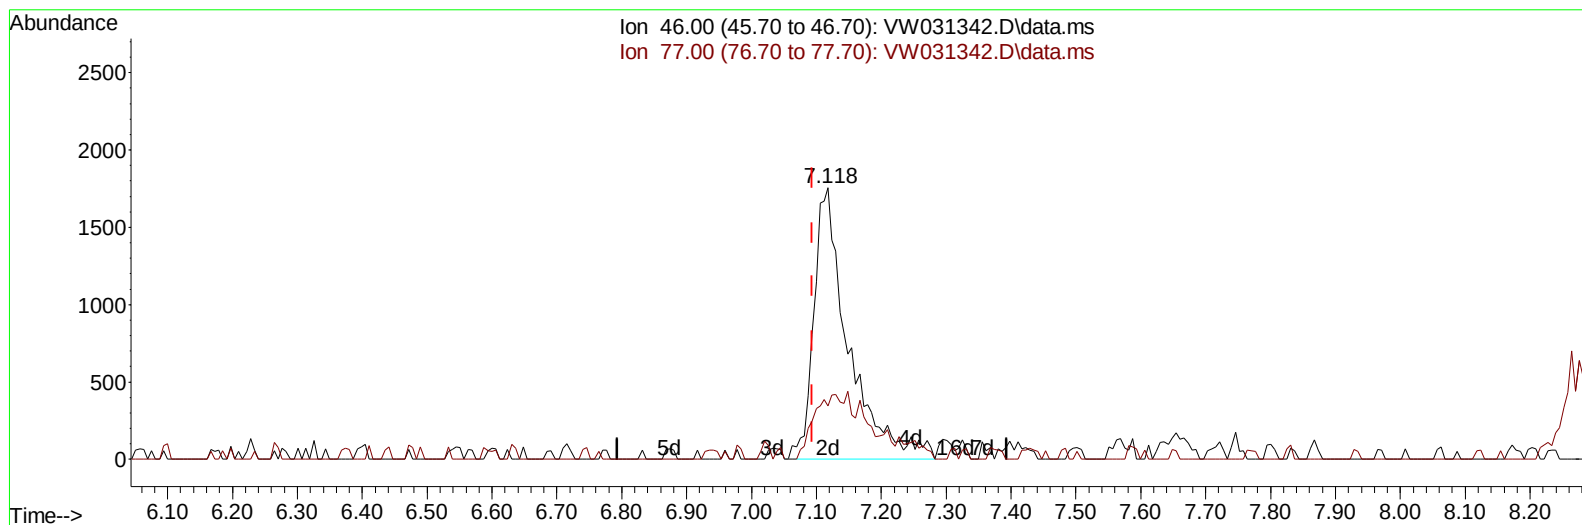

TIC: VW031342.D\data.ms

(21) 2-Butanone-d5 (S)

7.118min (+ 0.024) 2.33 ug/L m

response 6521

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	29.60	0.77#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121824\
 Data File : VW031342.D
 Acq On : 18 Dec 2024 16:03
 Operator : SY/MD
 Sample : P5265-10
 Misc : 4.97g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 19 00:24:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 19 00:20:44 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/19/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		988446	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		509827	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		108655	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		239745	16.120	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	64.480%	
7) Chloroethane-d5	2.899	69		198415	18.035	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.160%	
11) 1,1-Dichloroethene-d2	4.015	65		90691	12.855	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	51.440%	
21) 2-Butanone-d5	7.118	46		6521m	2.328	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135		Recovery	=	4.660%#	
24) Chloroform-d	7.648	84		408940	15.100	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	60.400%	
26) 1,2-Dichloroethane-d4	8.301	65		239190	17.586	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	70.360%	
32) Benzene-d6	8.270	84		656568	20.093	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	80.360%	
36) 1,2-Dichloropropane-d6	9.270	67		230380	24.190	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	96.760%	
41) Toluene-d8	10.319	98		406928	13.386	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	53.560%	
43) trans-1,3-Dichloroprop...	10.575	79		23723	5.402	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	21.600%#	
47) 2-Hexanone-d5	10.928	63		2322	1.813	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	3.620%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		118381	19.798	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	79.200%	
66) 1,2-Dichlorobenzene-d4	13.848	152		46847	11.614	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	46.440%#	
Target Compounds							Qvalue
15) Methyl Acetate	4.692	43		8536	1.927	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121824\
Data File : VW031342.D
Acq On : 18 Dec 2024 16:03
Operator : SY/MD
Sample : P5265-10
Misc : 4.97g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Z5

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 12/19/2024
Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 00:24:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 19 00:20:44 2024
Response via : Initial Calibration

