




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121824\
Data File : VW031343.D
Acq On : 18 Dec 2024 16:27
Operator : SY/MD
Sample : P5265-11
Misc : 1.51g/10mL/MSVOA_W/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Z6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 00:25:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 19 00:20:44 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/19/2024
Supervised By :Mahesh Dadoda 12/20/2024

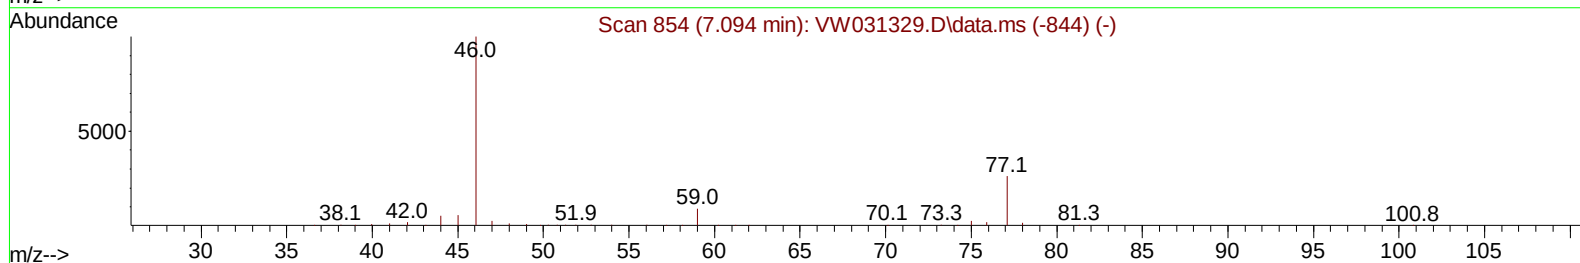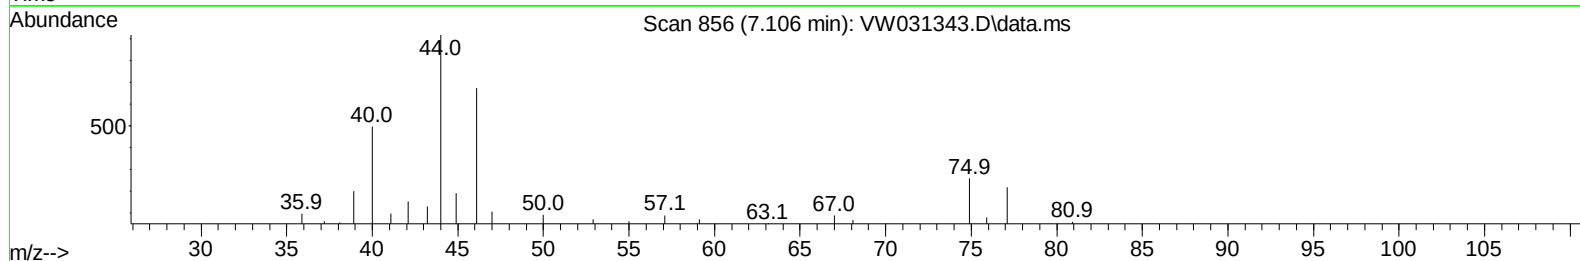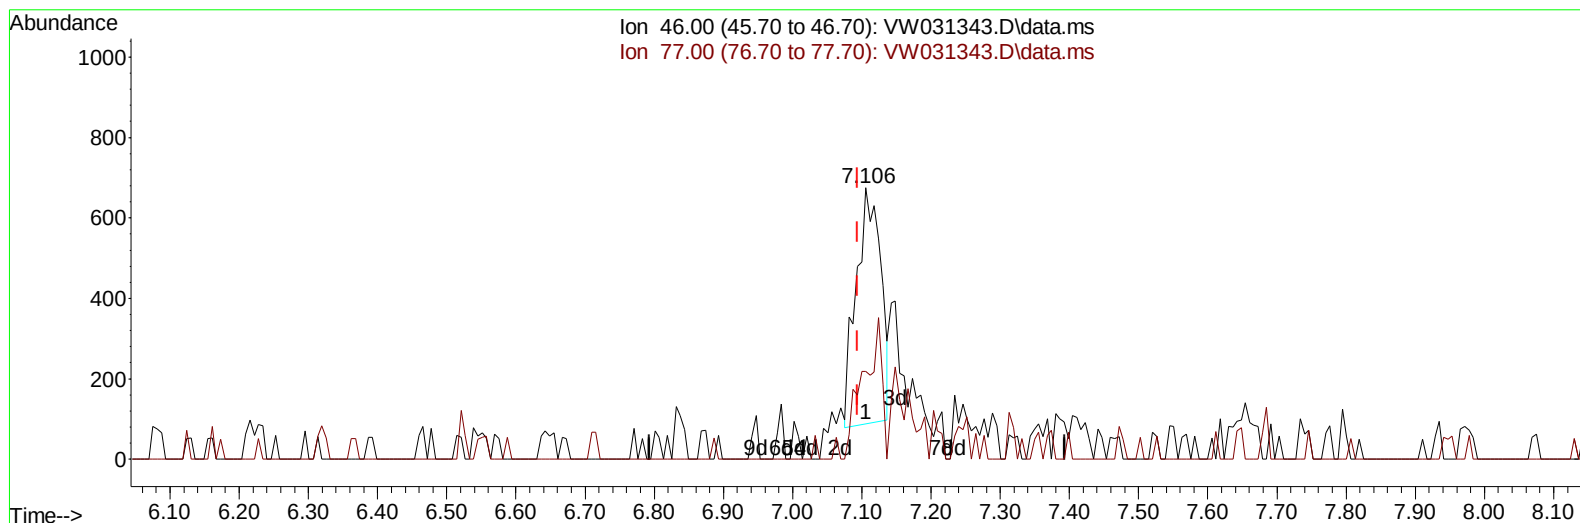

TIC: VW031343.D\data.ms

(21) 2-Butanone-d5 (S)

7.106min (+ 0.012) 1.38 ug/L

response 1445

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	29.60	26.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121824\
 Data File : VW031343.D
 Acq On : 18 Dec 2024 16:27
 Operator : SY/MD
 Sample : P5265-11
 Misc : 1.51g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Z6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 00:25:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 19 00:20:44 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/19/2024
 Supervised By :Mahesh Dadoda 12/20/2024

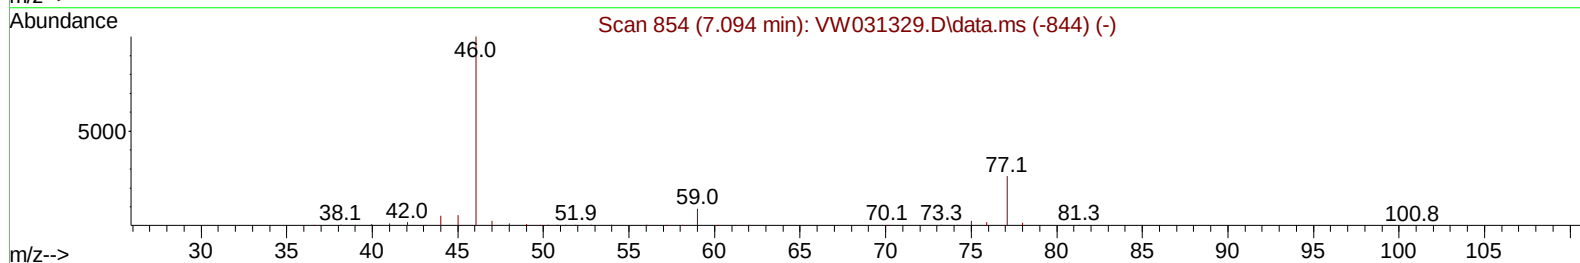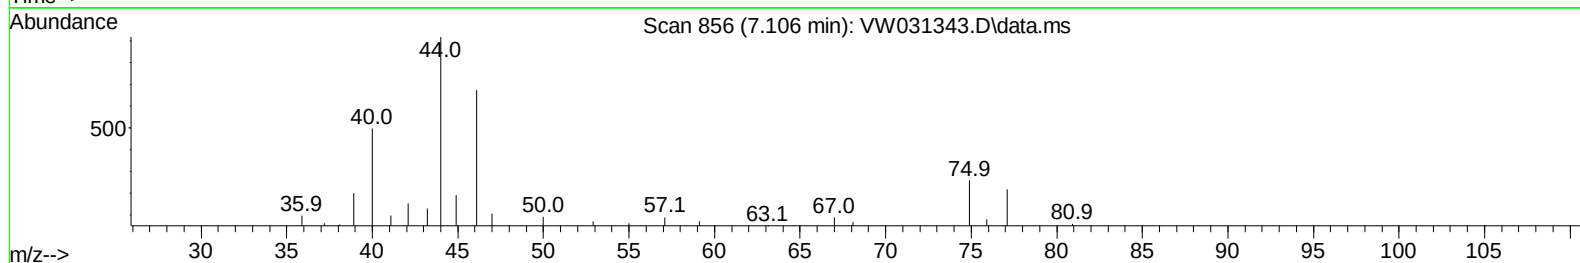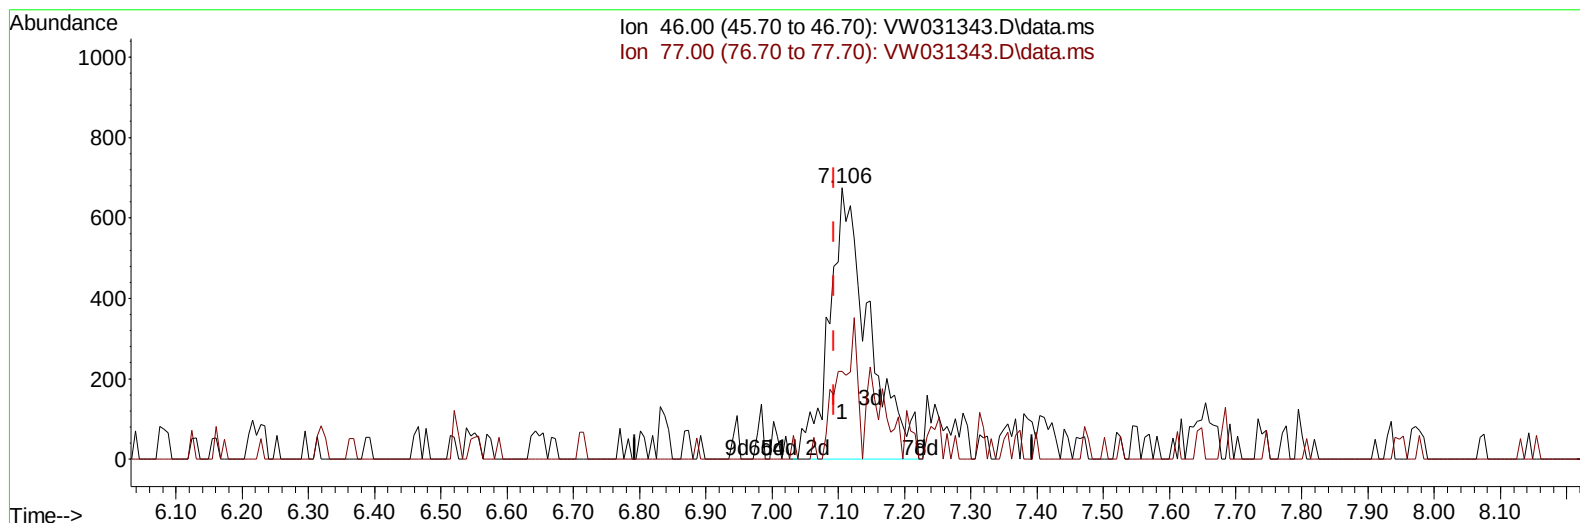

TIC: VW031343.D\data.ms

(21) 2-Butanone-d5 (S)

7.106min (+ 0.012) 2.70 ug/L m

response 2822

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	29.60	13.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121824\
 Data File : VW031343.D
 Acq On : 18 Dec 2024 16:27
 Operator : SY/MD
 Sample : P5265-11
 Misc : 1.51g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Z6

Manual IntegrationsAPPROVED

Quant Time: Dec 19 00:25:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 19 00:20:44 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/19/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	369157	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	211965	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	47201	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	65688	11.826	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	47.320%		
7) Chloroethane-d5	2.887	69	61189	14.892	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	59.560%		
11) 1,1-Dichloroethene-d2	4.015	65	27153	10.306	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	41.240%#		
21) 2-Butanone-d5	7.106	46	2822m	2.698	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery =	5.400%#		
24) Chloroform-d	7.648	84	136687	13.514	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	54.040%		
26) 1,2-Dichloroethane-d4	8.307	65	84822	16.698	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	66.800%#		
32) Benzene-d6	8.270	84	209723	15.437	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	61.760%		
36) 1,2-Dichloropropane-d6	9.270	67	81600	20.609	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	82.440%		
41) Toluene-d8	10.319	98	142734	11.293	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	45.160%		
43) trans-1,3-Dichloroprop...	10.581	79	5496	3.010	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	12.040%#		
47) 2-Hexanone-d5	10.934	63	1419	2.665	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery =	5.320%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	49139	19.766	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	79.080%		
66) 1,2-Dichlorobenzene-d4	13.849	152	20326	11.600	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	46.400%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121824\
Data File : VW031343.D
Acq On : 18 Dec 2024 16:27
Operator : SY/MD
Sample : P5265-11
Misc : 1.51g/10mL/MSVOA_W/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Z6

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 12/19/2024
Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 00:25:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 19 00:20:44 2024
Response via : Initial Calibration

