

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121824\
 Data File : VW031352.D
 Acq On : 18 Dec 2024 20:52
 Operator : SY/MD
 Sample : P5302-01
 Misc : 3.88g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E2AR0

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 12/19/2024
 Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 04:10:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 19 04:08:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	442355	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	369073	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	141690	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.351	65	126605	19.022	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	76.080%		
7) Chloroethane-d5	2.887	69	98481	20.002	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.000%		
11) 1,1-Dichloroethene-d2	4.015	65	56786	17.987	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.960%		
21) 2-Butanone-d5	7.081	46	61920	49.400	ug/L	-0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.800%		
24) Chloroform-d	7.642	84	227472	18.768	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	75.080%		
26) 1,2-Dichloroethane-d4	8.307	65	138004m	22.672	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.680%		
32) Benzene-d6	8.270	84	463021	19.574	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	78.280%		
36) 1,2-Dichloropropane-d6	9.270	67	138292	20.059	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	80.240%		
41) Toluene-d8	10.319	98	396340	18.010	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	72.040%		
43) trans-1,3-Dichloroprop...	10.575	79	59109	18.594	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	74.360%		
47) 2-Hexanone-d5	10.922	63	45563	49.143	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.280%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	107589	24.855	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	99.400%		
66) 1,2-Dichlorobenzene-d4	13.848	152	105538	20.064	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	80.240%		
Target Compounds					Qvalue	
13) Acetone	4.143	43	13635	7.811	ug/L #	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121824\
Data File : VW031352.D
Acq On : 18 Dec 2024 20:52
Operator : SY/MD
Sample : P5302-01
Misc : 3.88g/10mL/MSVOA_W/SOIL/A
ALS Vial : 28 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
E2AR0

Manual Integrations
APPROVED

Reviewed By :Romaben Patel 12/19/2024
Supervised By :Mahesh Dadoda 12/20/2024

Quant Time: Dec 19 04:10:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 19 04:08:34 2024
Response via : Initial Calibration

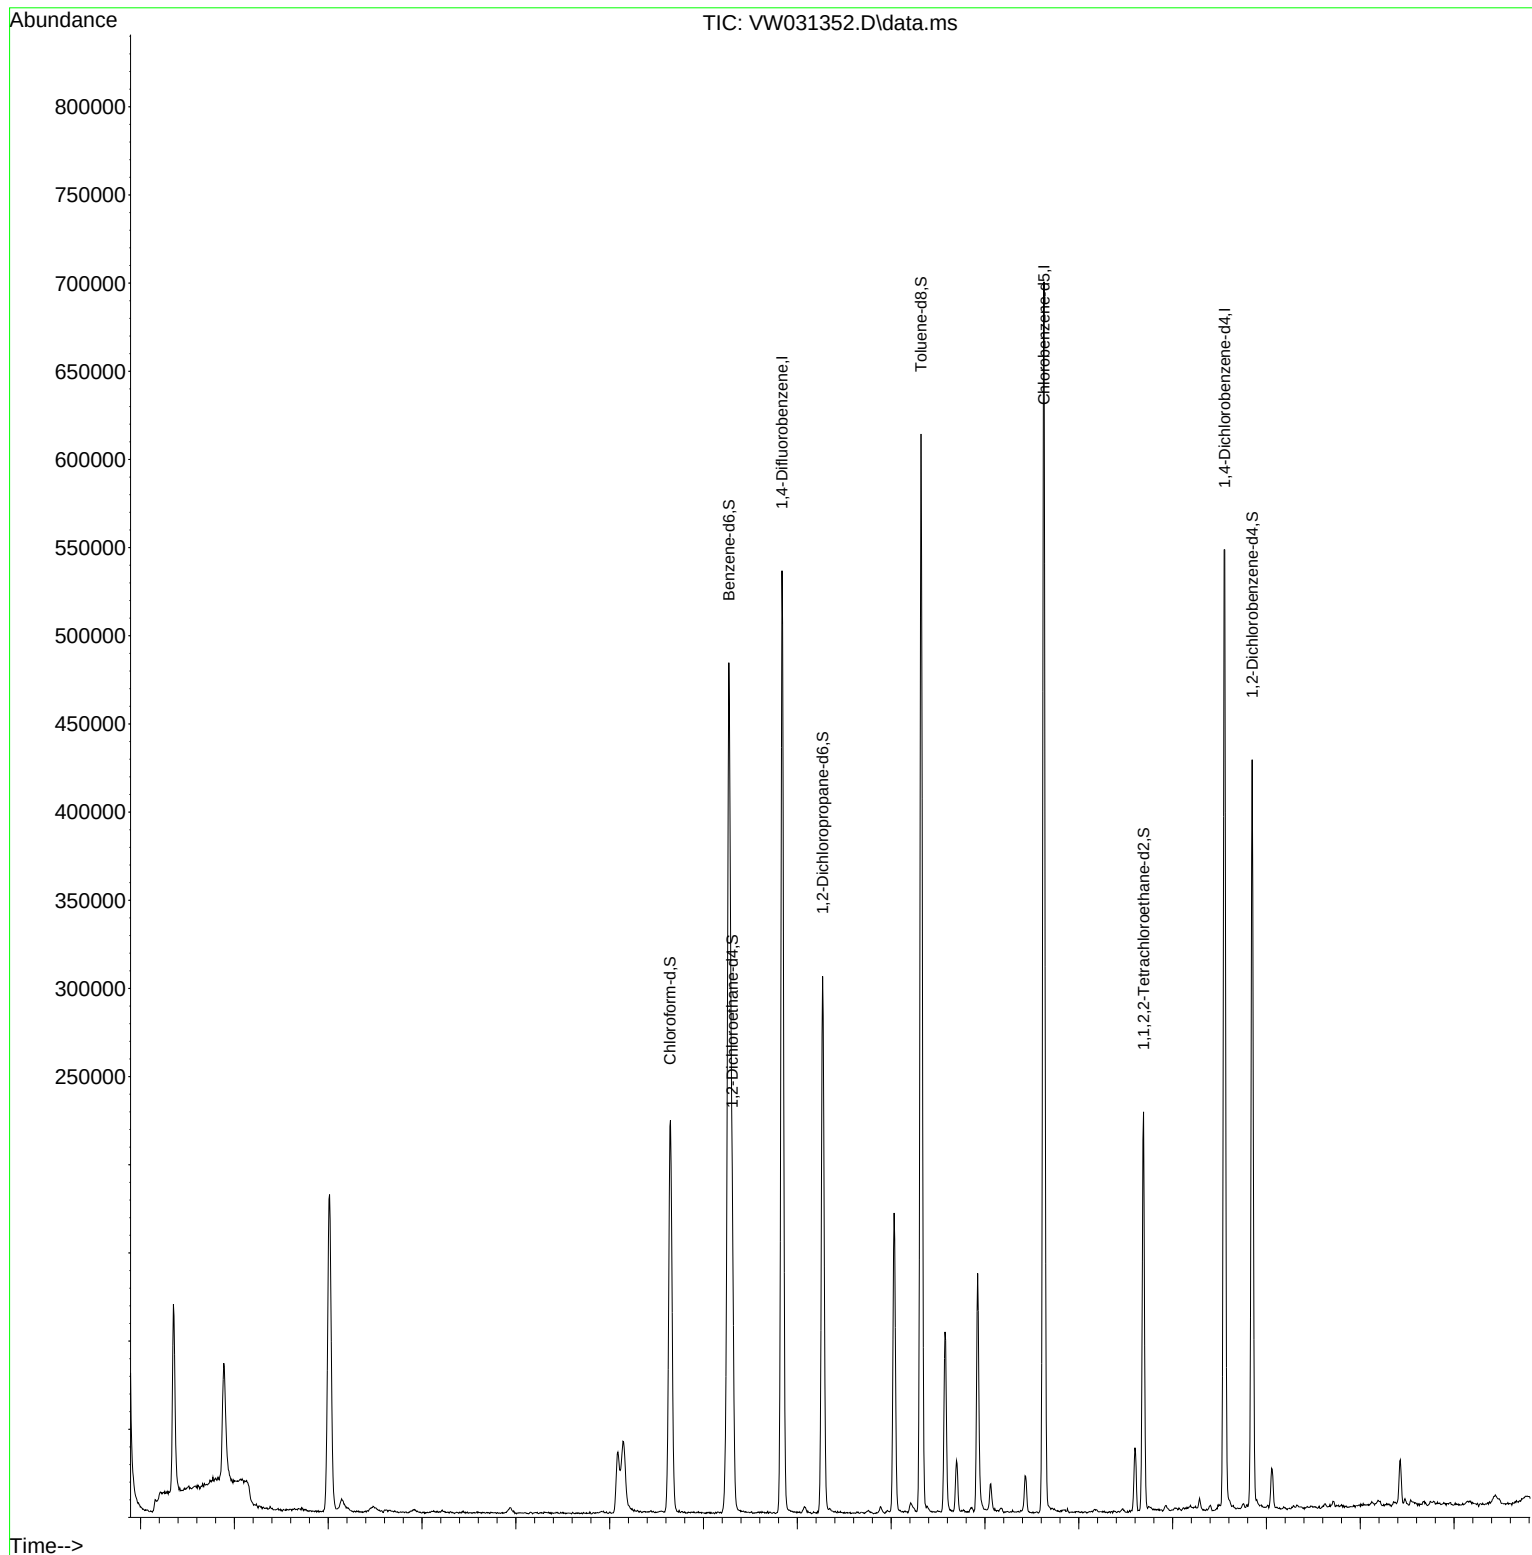

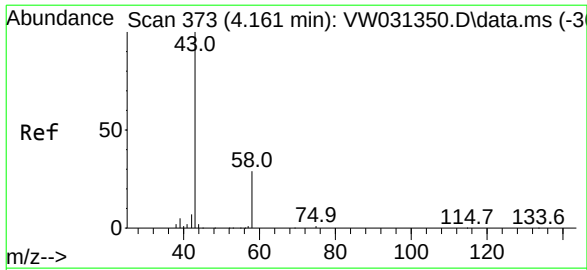

#13
 Acetone
 Concen: 7.811 ug/L
 RT: 4.143 min Scan# 373
 Delta R.T. -0.018 min
 Lab File: VW031352.D
 Acq: 18 Dec 2024 20:52

Instrument :
 MSVOA_W
 ClientSampleId :
 E2AR0

Tgt Ion: 43 Resp: 13635
 Ion Ratio Lower Upper
 43 100
 58 13.8 0.0 0.0#

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 12/19/2024
 Supervised By :Mahesh Dadoda 12/20/2024

