
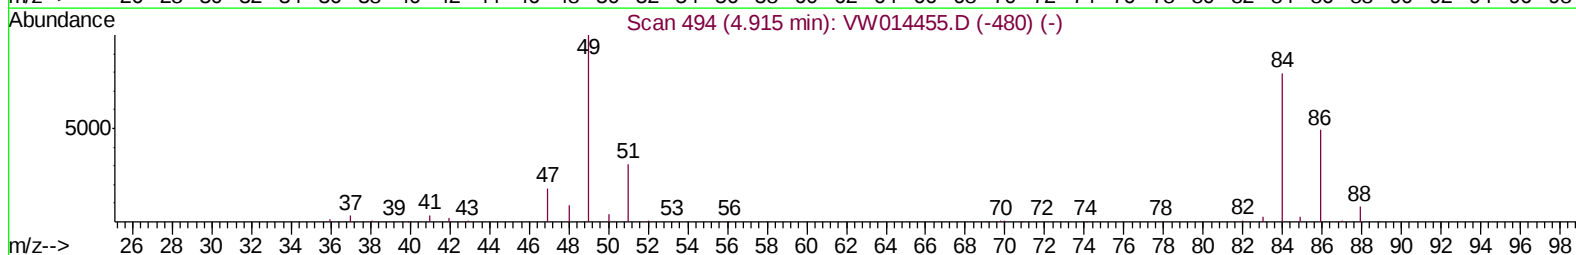
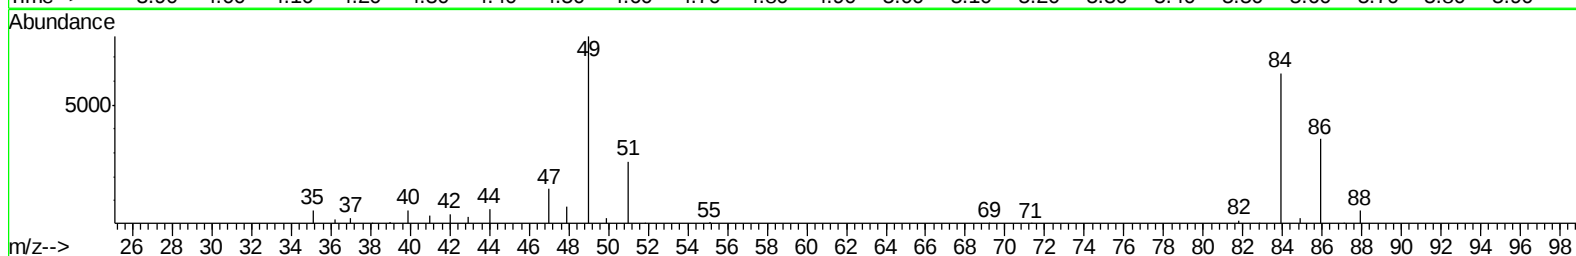


Data File : VW014460.D
Acq On : 19 Dec 2019 13:40
Operator : SY/VA
Sample : K6257-03
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 01:15:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 20 01:12:43 2019
Response via : Initial Calibration

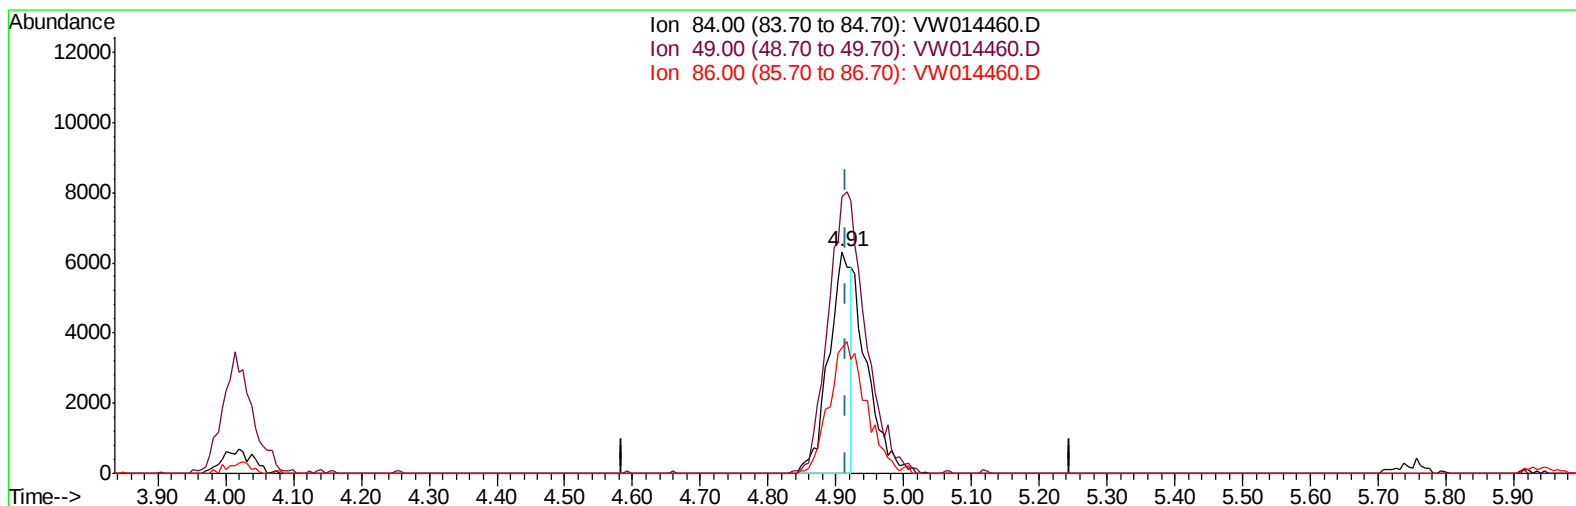

TIC: VW014460.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.01ug/L

response 14175

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	124.38
86.00	62.40	56.68
0.00	0.00	0.00