




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121924\
Data File : VW031399.D
Acq On : 19 Dec 2024 22:08
Operator : SY/MD
Sample : P5333-01
Misc : 3.16g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E2904

Manual IntegrationsAPPROVED

Quant Time: Dec 20 03:09:34 2024
Quant Title :
QLast Update : Fri Dec 20 03:08:41 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/20/2024
Supervised By :Mahesh Dadoda 12/23/2024

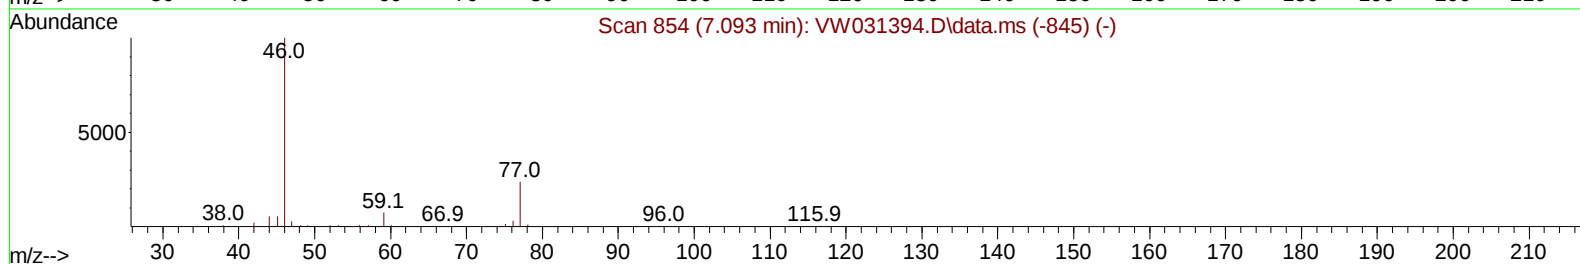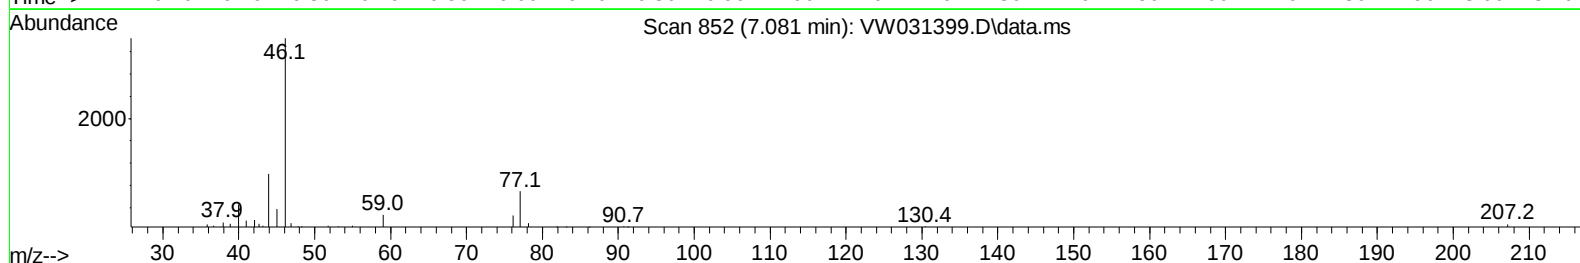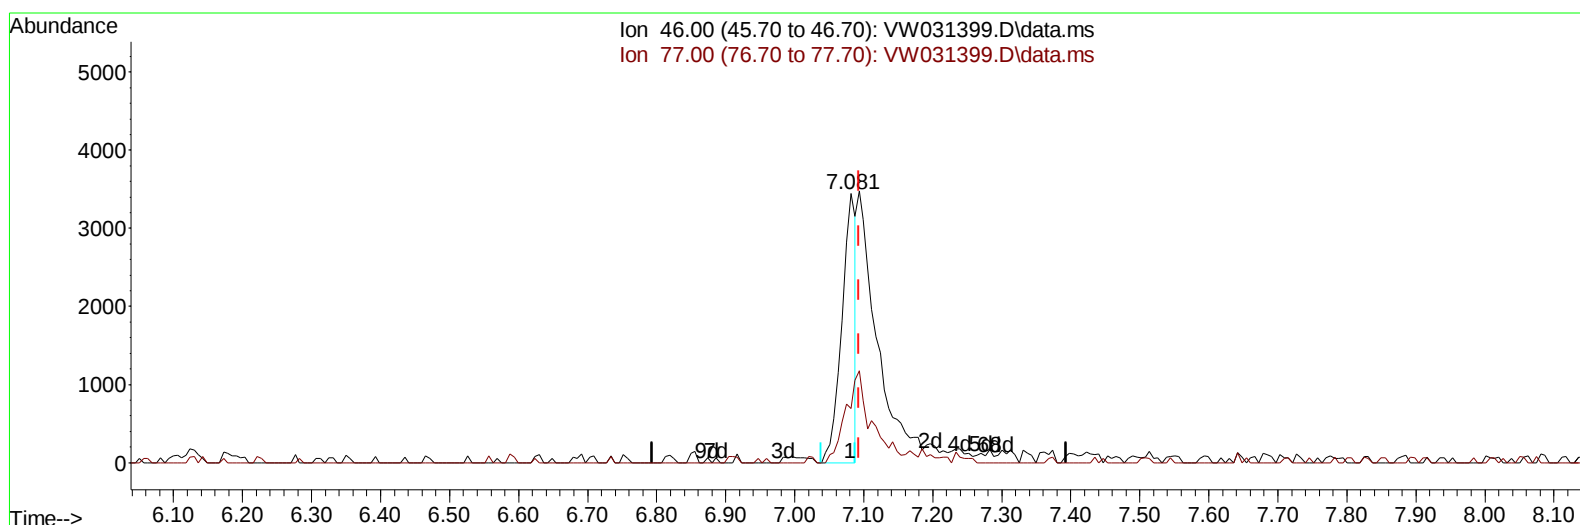

TIC: VW031399.D\data.ms

(21) 2-Butanone-d5 (S)

7.081min (-0.012) 7.14 ug/L

response 4867

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	29.60	44.61#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121924\
Data File : VW031399.D
Acq On : 19 Dec 2024 22:08
Operator : SY/MD
Sample : P5333-01
Misc : 3.16g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E2904

Manual IntegrationsAPPROVED

Quant Time: Dec 20 03:09:34 2024
Quant Title :
QLast Update : Fri Dec 20 03:08:41 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/20/2024
Supervised By :Mahesh Dadoda 12/23/2024

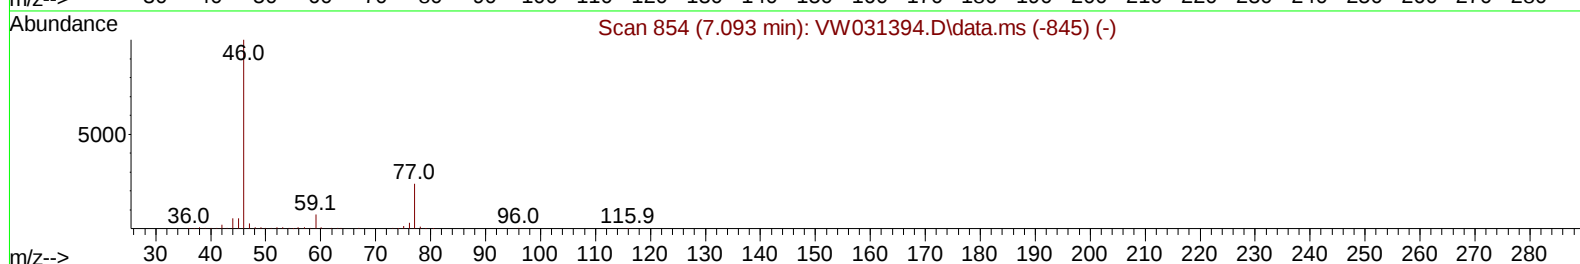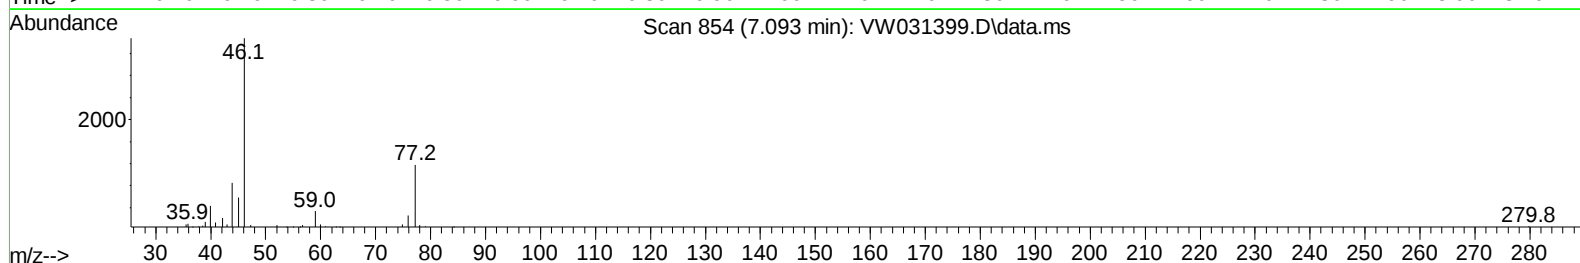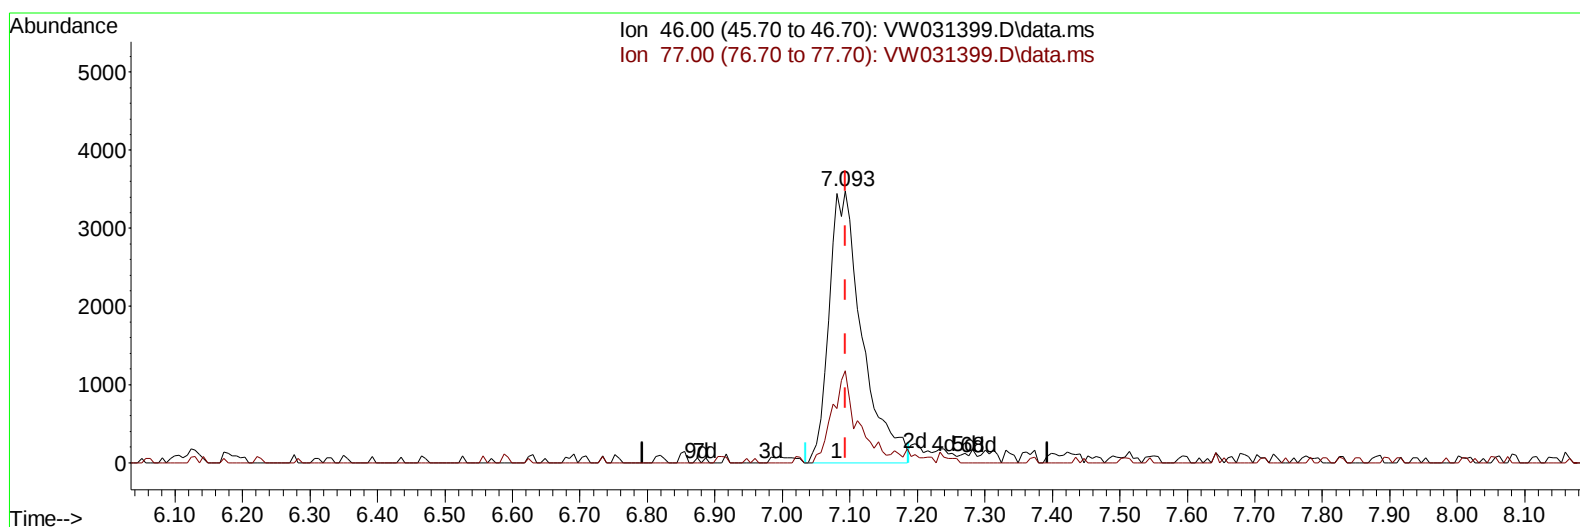

TIC: VW031399.D\data.ms

(21) 2-Butanone-d5 (S)

7.093min (+ 0.000) 17.23 ug/L m

response 11754

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	29.60	18.47#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121924\
 Data File : VW031399.D
 Acq On : 19 Dec 2024 22:08
 Operator : SY/MD
 Sample : P5333-01
 Misc : 3.16g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E2904

Manual IntegrationsAPPROVED

Quant Time: Dec 20 04:41:53 2024
 Quant Title :
 QLast Update : Fri Dec 20 03:08:41 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/20/2024
 Supervised By :Mahesh Dadoda 12/23/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	240702	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	185853	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	69196	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	67620	18.671	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	74.680%	
7) Chloroethane-d5	2.881	69	50424	18.822	ug/L	-0.01
Spiked Amount	25.000	Range 30 - 150	Recovery	=	75.280%	
11) 1,1-Dichloroethene-d2	4.015	65	28314	16.482	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	65.920%	
21) 2-Butanone-d5	7.093	46	11754m	17.233	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	34.460%	
24) Chloroform-d	7.648	84	93870	14.233	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	56.920%	
26) 1,2-Dichloroethane-d4	8.300	65	44912	13.560	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	54.240%#	
32) Benzene-d6	8.276	84	196364	16.484	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	65.920%	
36) 1,2-Dichloropropane-d6	9.270	67	53434	15.391	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	61.560%#	
41) Toluene-d8	10.318	98	173994	15.701	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	62.800%	
43) trans-1,3-Dichloroprop...	10.574	79	14186	8.862	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	35.440%	
47) 2-Hexanone-d5	10.928	63	7974	17.079	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	34.160%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	29573	13.567	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	54.280%	
66) 1,2-Dichlorobenzene-d4	13.848	152	39142	15.237	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	60.960%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121924\
Data File : VW031399.D
Acq On : 19 Dec 2024 22:08
Operator : SY/MD
Sample : P5333-01
Misc : 3.16g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E2904

Manual IntegrationsAPPROVED

Quant Time: Dec 20 04:41:53 2024
Quant Title :
QLast Update : Fri Dec 20 03:08:41 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 12/20/2024
Supervised By :Mahesh Dadoda 12/23/2024

