

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW122018\
 Data File : VW007692.D
 Acq On : 19 Dec 2018 08:00
 Operator : SY/AP
 Sample : J6386-15
 Misc : 5.83G/5ML/MSVOA_W/SOIL
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS007-0006-01

Quant Time: Dec 19 10:04:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W121118S.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 11 02:58:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	63143	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	108559	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	84709	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	28714	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	31706	45.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.52%	
35) Dibromofluoromethane	7.88	113	27581	41.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	83.94%	
50) Toluene-d8	10.32	98	86931	35.28	ug/l	0.00
Spiked Amount	50.000		Recovery	=	70.56%	
62) 4-Bromofluorobenzene	12.62	95	26262	28.99	ug/l	0.00
Spiked Amount	50.000		Recovery	=	57.98%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW122018\
Data File : VW007692.D
Acq On : 19 Dec 2018 08:00
Operator : SY/AP
Sample : J6386-15
Misc : 5.83G/5ML/MSVOA_W/SOIL
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
P001-SS007-0006-01

Quant Time: Dec 19 10:04:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W121118S.M
Quant Title : SW846 8260
QLast Update : Tue Dec 11 02:58:16 2018
Response via : Initial Calibration

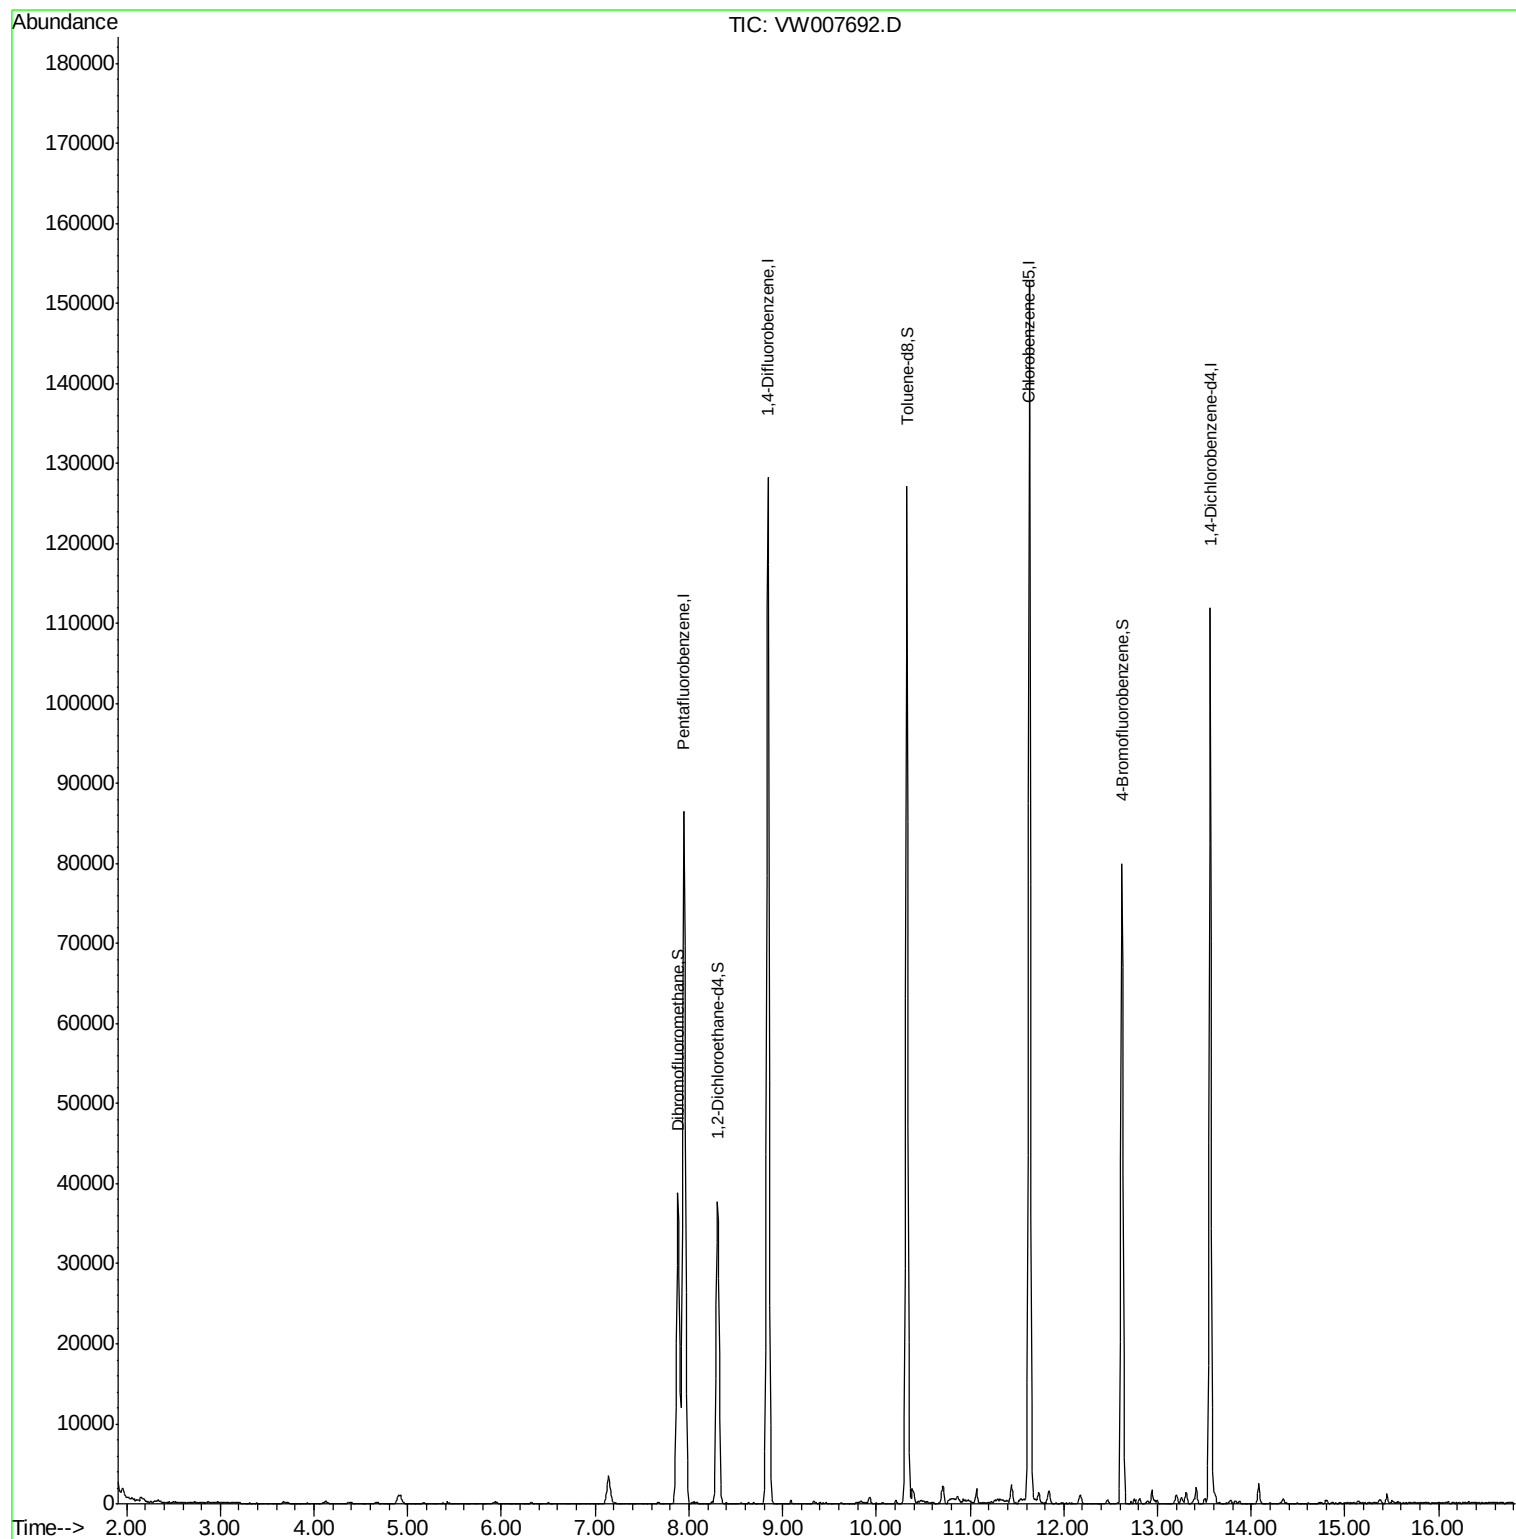

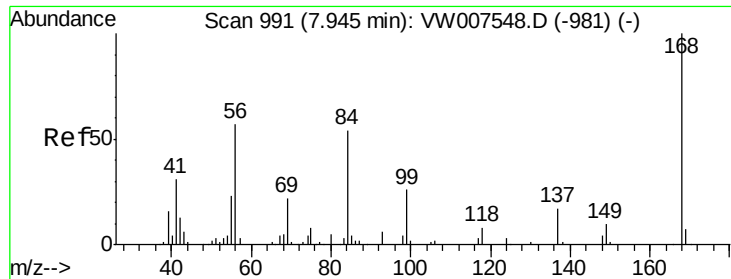

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW007692.D

Acq: 19 Dec 2018 08:00

Instrument :

MSVOA_W

ClientSampleId :


P001-SS007-0006-01

Tgt Ion:168 Resp: 63143

Ion Ratio Lower Upper

168 100

99 60.3 48.3 72.5

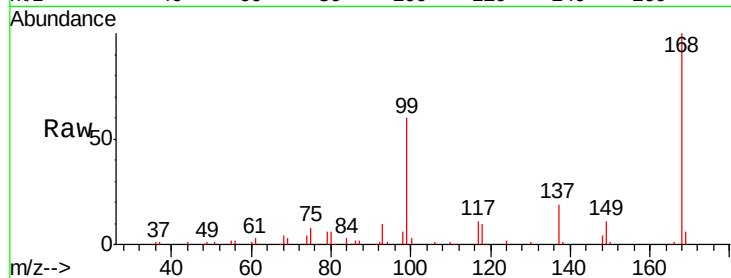

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

30000

25000

20000



15000

10000

5000

0

Time-->

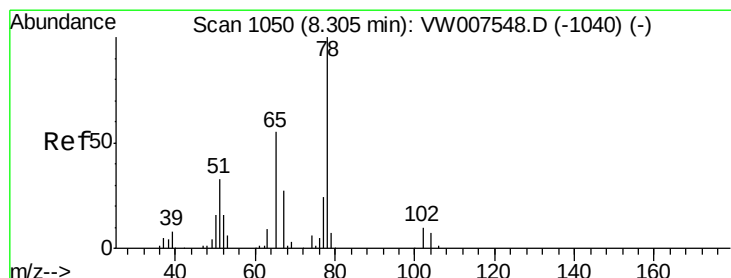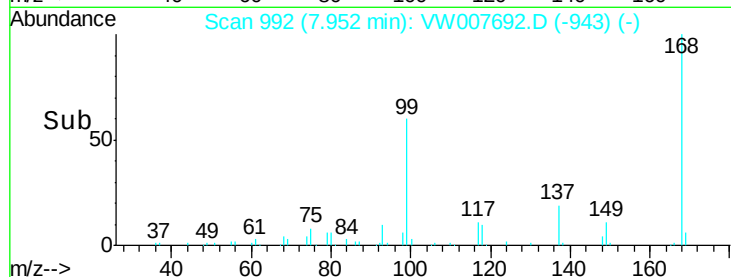

#33

1,2-Dichloroethane-d4

Concen: 45.261 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW007692.D


Acq: 19 Dec 2018 08:00

Tgt Ion: 65 Resp: 31706

Ion Ratio Lower Upper

65 100

67 48.4 0.0 101.6

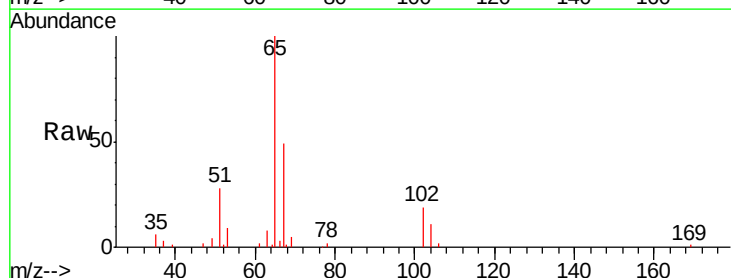

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31


15000


10000

5000

0

Time-->

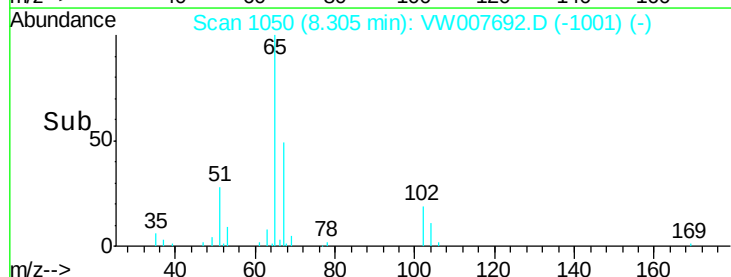


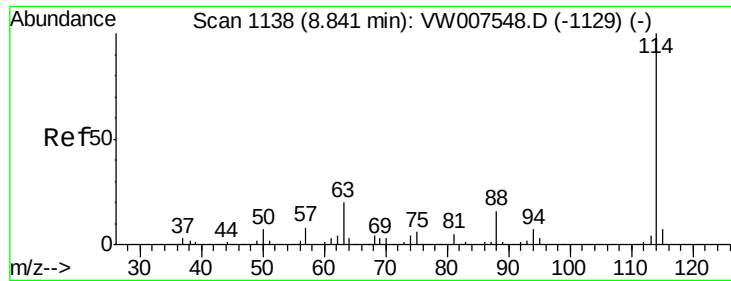




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW007692.D
 Acq: 19 Dec 2018 08:00

Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS007-0006-01

Tgt Ion:114 Resp: 108559
 Ion Ratio Lower Upper
 114 100
 63 19.0 0.0 39.6
 88 16.4 0.0 31.4

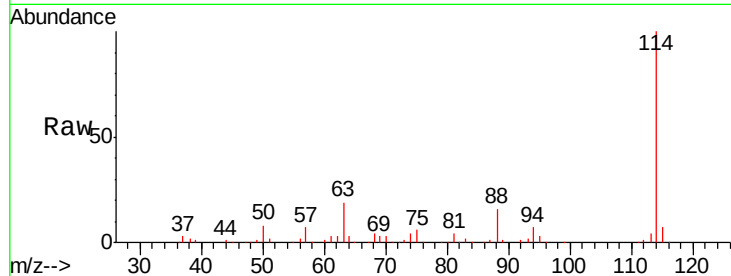


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

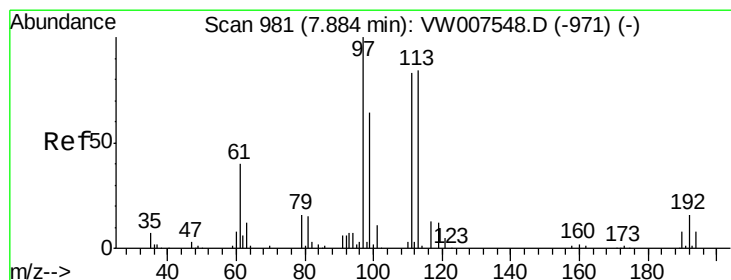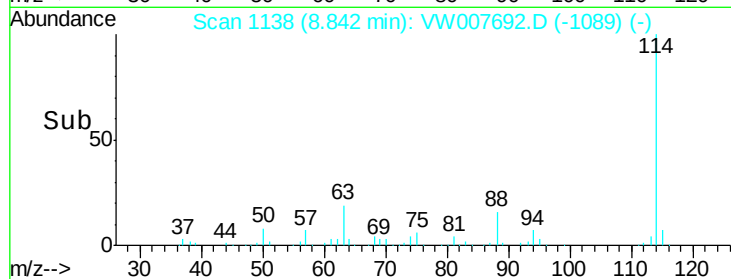
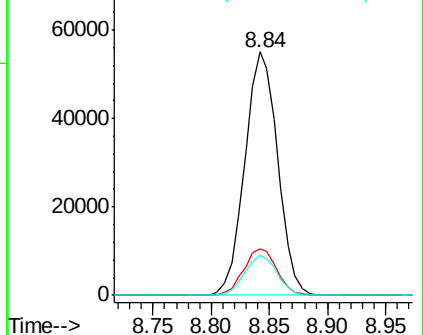



#35
 Dibromofluoromethane
 Concen: 41.971 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. 0.00 min
 Lab File: VW007692.D
 Acq: 19 Dec 2018 08:00

Tgt Ion:113 Resp: 27581
 Ion Ratio Lower Upper
 113 100
 111 105.9 81.1 121.7
 192 18.7 14.6 21.8

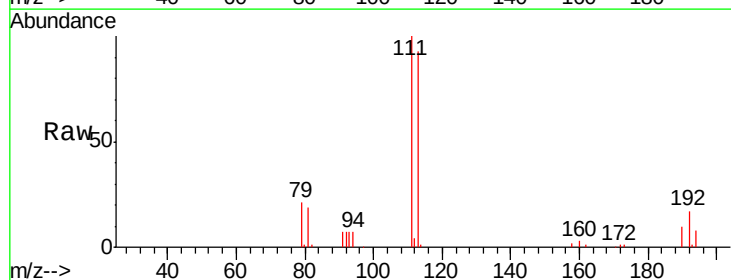

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

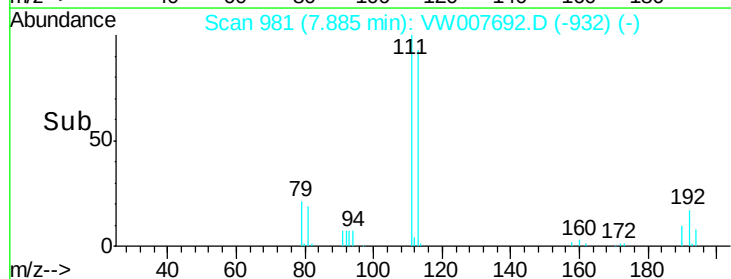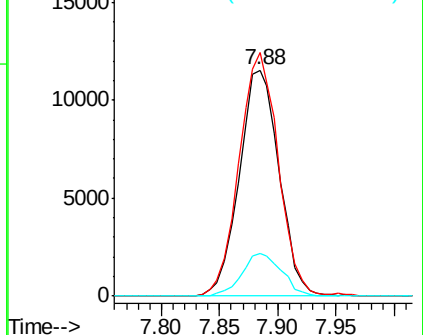

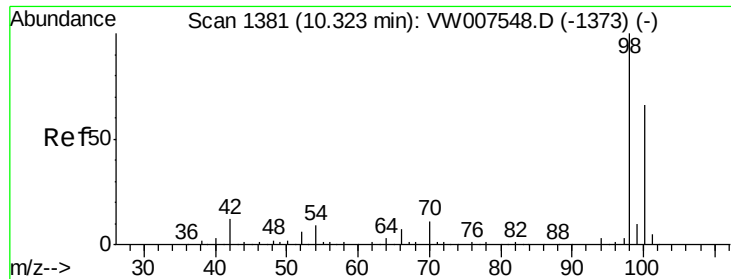

#50

Toluene-d8

Concen: 35.281 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW007692.D

Acq: 19 Dec 2018 08:00

Instrument :

MSVOA_W

ClientSampleId :


P001-SS007-0006-01

Tgt Ion: 98 Resp: 86931

Ion Ratio Lower Upper




98 100

100 65.1 51.8 77.8

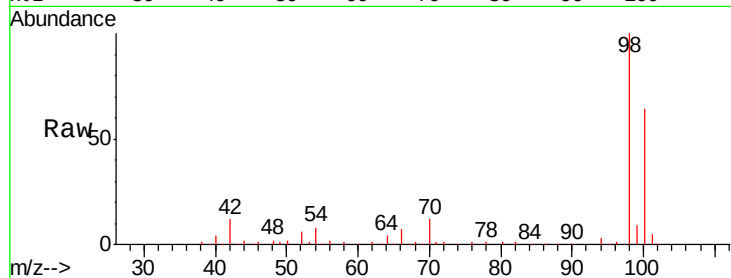

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

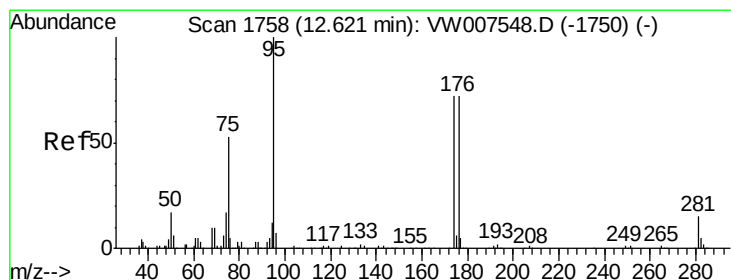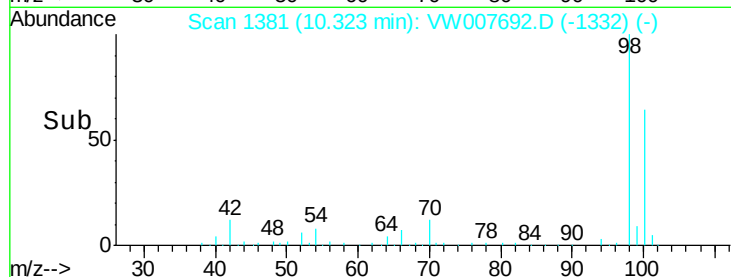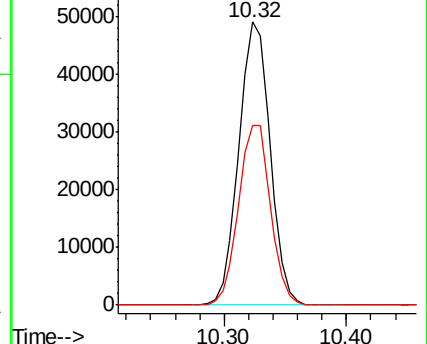

#62

4-Bromofluorobenzene

Concen: 28.989 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW007692.D

Acq: 19 Dec 2018 08:00


Tgt Ion: 95 Resp: 26262

Ion Ratio Lower Upper

95 100

174 79.8 0.0 147.2



176 72.9 0.0 138.8

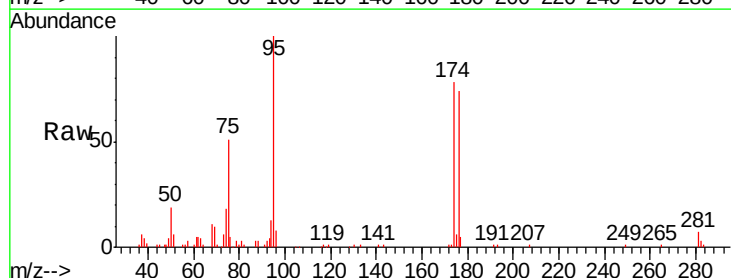


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW



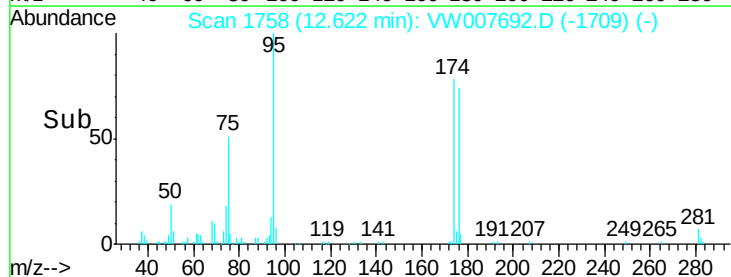
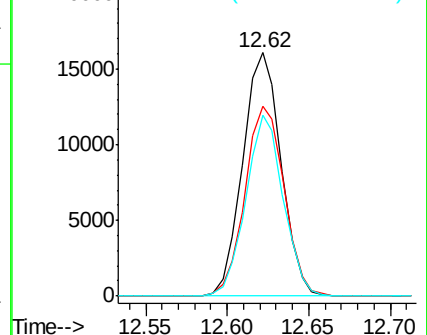


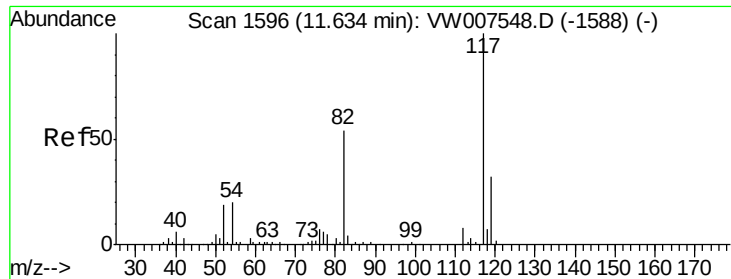

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW007692.D
Acq: 19 Dec 2018 08:00

Instrument :
MSVOA_W
ClientSampleId :
P001-SS007-0006-01

Tgt Ion:117 Resp: 84709
Ion Ratio Lower Upper
117 100
82 52.6 42.3 63.5
119 31.4 23.0 34.6

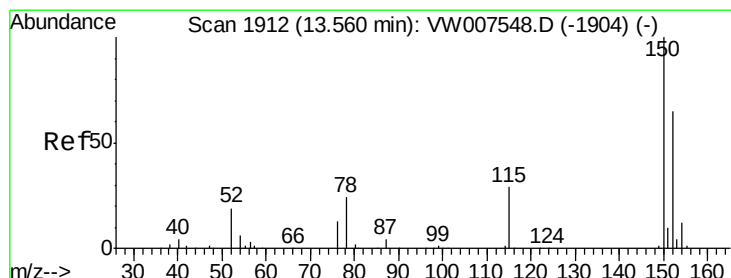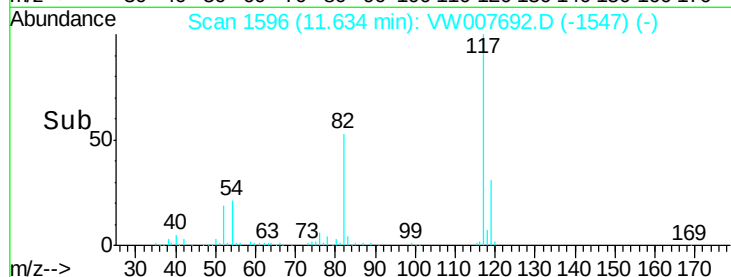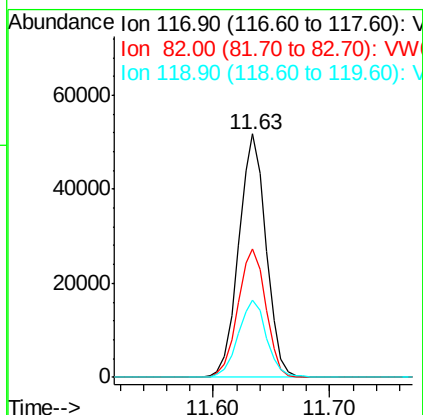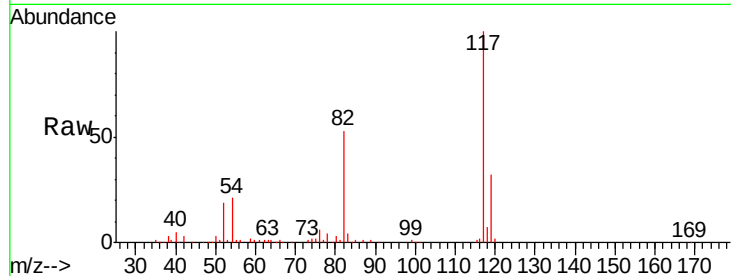

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.00 min
Lab File: VW007692.D
Acq: 19 Dec 2018 08:00

Tgt Ion:152 Resp: 28714
Ion Ratio Lower Upper
152 100
115 61.6 31.4 94.2
150 156.9 0.0 358.4

