

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122019\
 Data File : VW014471.D
 Acq On : 20 Dec 2019 11:41
 Operator : SY/VA
 Sample : VIBLK20
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VIBLK20

Manual Integrations
APPROVED

apatel
 12/23/2019 11:44:11 AM

Quant Time: Dec 21 04:37:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 21 04:34:48 2019
 Response via : Initial Calibration

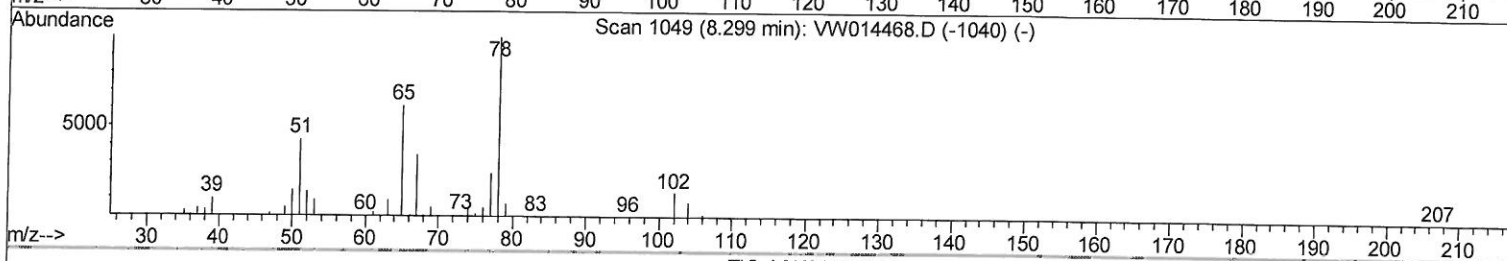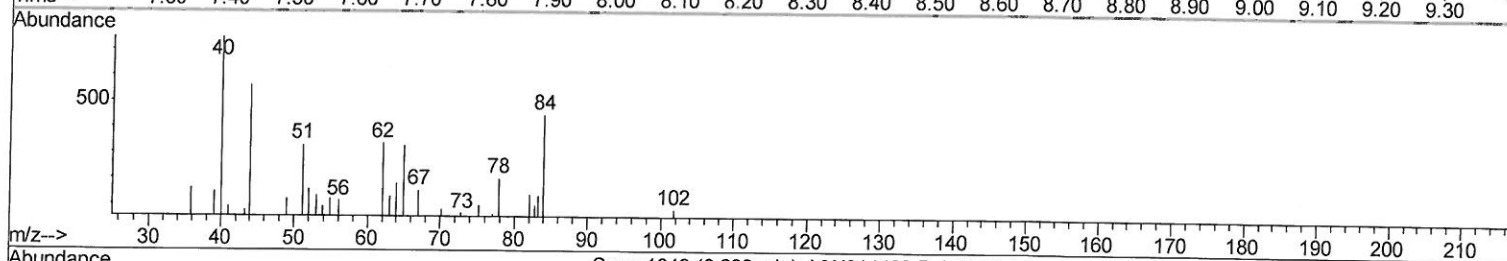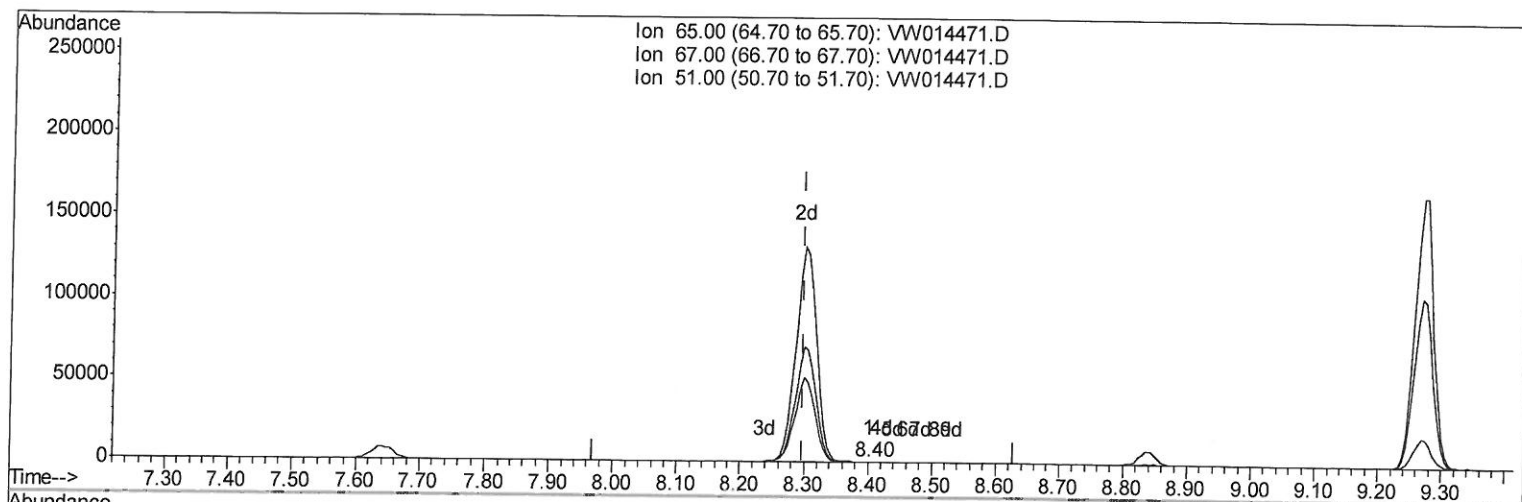

(26) 1,2-Dichloroethane-d4 (S)

8.403min (+0.104) 0.03ug/L

response 371

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	50.67
51.00	107.20	87.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122019\
 Data File : VW014471.D
 Acq On : 20 Dec 2019 11:41
 Operator : SY/VA
 Sample : VIBLK20
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VIBLK20

Manual Integrations
APPROVED

apatel
 12/23/2019 11:44:11 AM

Quant Time: Dec 21 04:37:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 21 04:34:48 2019
 Response via : Initial Calibration

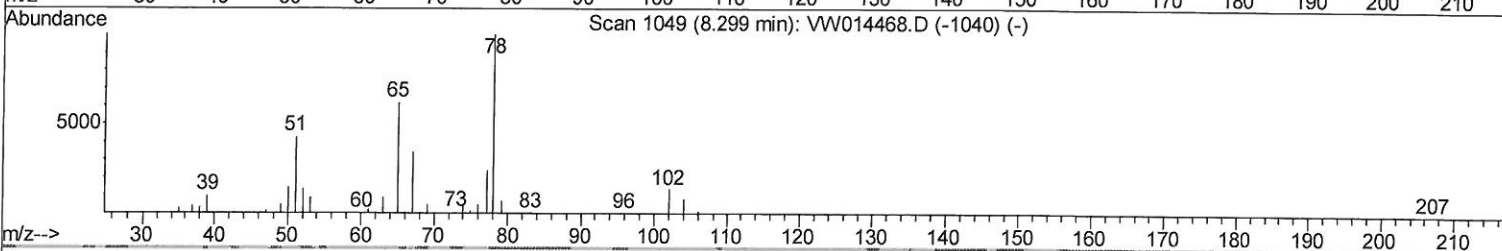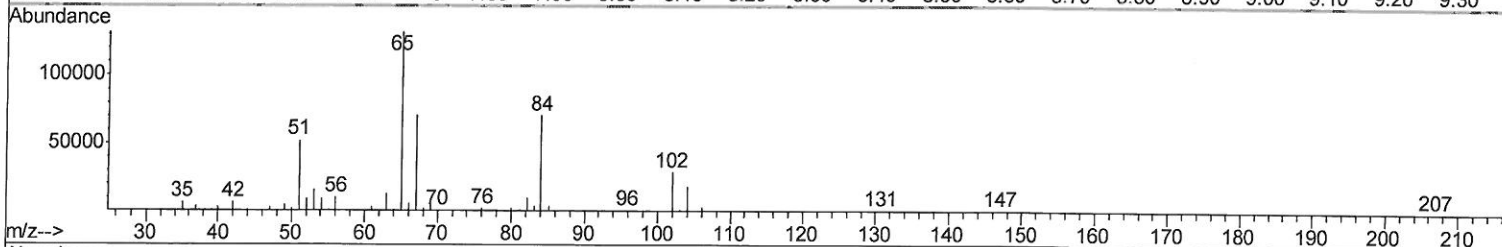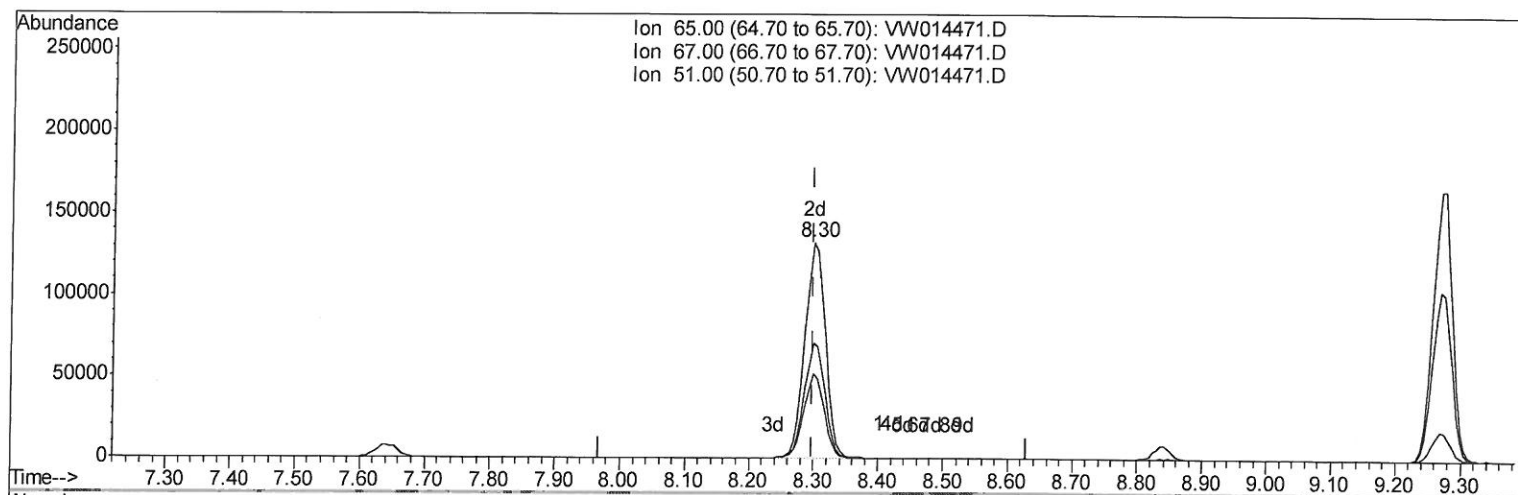

TIC: VW014471.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (+0.000) 25.16ug/L m

response 291887

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	0.06#
51.00	107.20	0.11#
0.00	0.00	0.00

12/23/19 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122019\
 Data File : VW014471.D
 Acq On : 20 Dec 2019 11:41
 Operator : SY/VA
 Sample : VIBLK20
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK20

Manual Integrations
 APPROVED

apatel
 12/23/2019 11:44:11 AM

Quant Time: Dec 21 04:48:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 21 04:34:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	869138	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	781652	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	335161	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	228490	17.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.44%
7) Chloroethane-d5	2.88	69	200844	20.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.08%
10) 1,1-Dichloroethene-d2	4.01	63	350107	15.06	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.24%
20) 2-Butanone-d5	7.07	46	223454	65.15	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	130.30%
24) Chloroform-d	7.64	84	511169	23.10	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	8.30	65	291887m	25.16	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.64%
29) Benzene-d6	8.27	84	1019561	22.26	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.04%
33) 1,2-Dichloropropane-d6	9.27	67	332800	23.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.44%
37) Toluene-d8	10.32	98	881882	21.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.16%
38) trans-1,3-Dichloropropene-	10.58	79	128777	21.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.12%
39) 2-Hexanone-d5	10.92	63	162505	57.99	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.98%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	305938	26.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.56%
61) 1,2-Dichlorobenzene-d4	13.85	152	299235	23.36	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.44%

Target Compounds				Ovalue	
13) Acetone	4.12	43	13865	4.193	ug/L 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

12/23/19 Sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122019\
Data File : VW014471.D
Acq On : 20 Dec 2019 11:41
Operator : SY/VA
Sample : VIBLK20
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VIBLK20

Manual Integrations
APPROVED

apatel
12/23/2019 11:44:11 AM

Quant Time: Dec 21 04:48:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 21 04:34:48 2019
Response via : Initial Calibration

