

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122019\
 Data File : VW014469.D
 Acq On : 20 Dec 2019 10:48
 Operator : SY/VA
 Sample : VW1220SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK16

Quant Time: Dec 21 04:40:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 21 04:34:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1053763	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	978416	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	432669	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	290975	18.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.96%
7) Chloroethane-d5	2.89	69	264166	22.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.08%
10) 1,1-Dichloroethene-d2	4.01	63	446443	15.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.36%
20) 2-Butanone-d5	7.07	46	225848	54.31	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.62%
24) Chloroform-d	7.65	84	664998	24.79	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.16%
26) 1,2-Dichloroethane-d4	8.30	65	367099	26.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.40%
29) Benzene-d6	8.27	84	1329400	23.18	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.72%
33) 1,2-Dichloropropane-d6	9.27	67	432274	24.50	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.00%
37) Toluene-d8	10.32	98	1174398	22.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.60%
38) trans-1,3-Dichloropropene-	10.58	79	164659	22.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.00%
39) 2-Hexanone-d5	10.92	63	170157	48.51	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.02%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	352507	24.52	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.08%
61) 1,2-Dichlorobenzene-d4	13.85	152	405975	24.55	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.20%


Target Compounds					Ovalue
13) Acetone	4.13	43	11727	2.925 ug/L	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW122019\
Data File : VW014469.D
Acq On : 20 Dec 2019 10:48
Operator : SY/VA
Sample : VW1220SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK16

Quant Time: Dec 21 04:40:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 21 04:34:48 2019
Response via : Initial Calibration

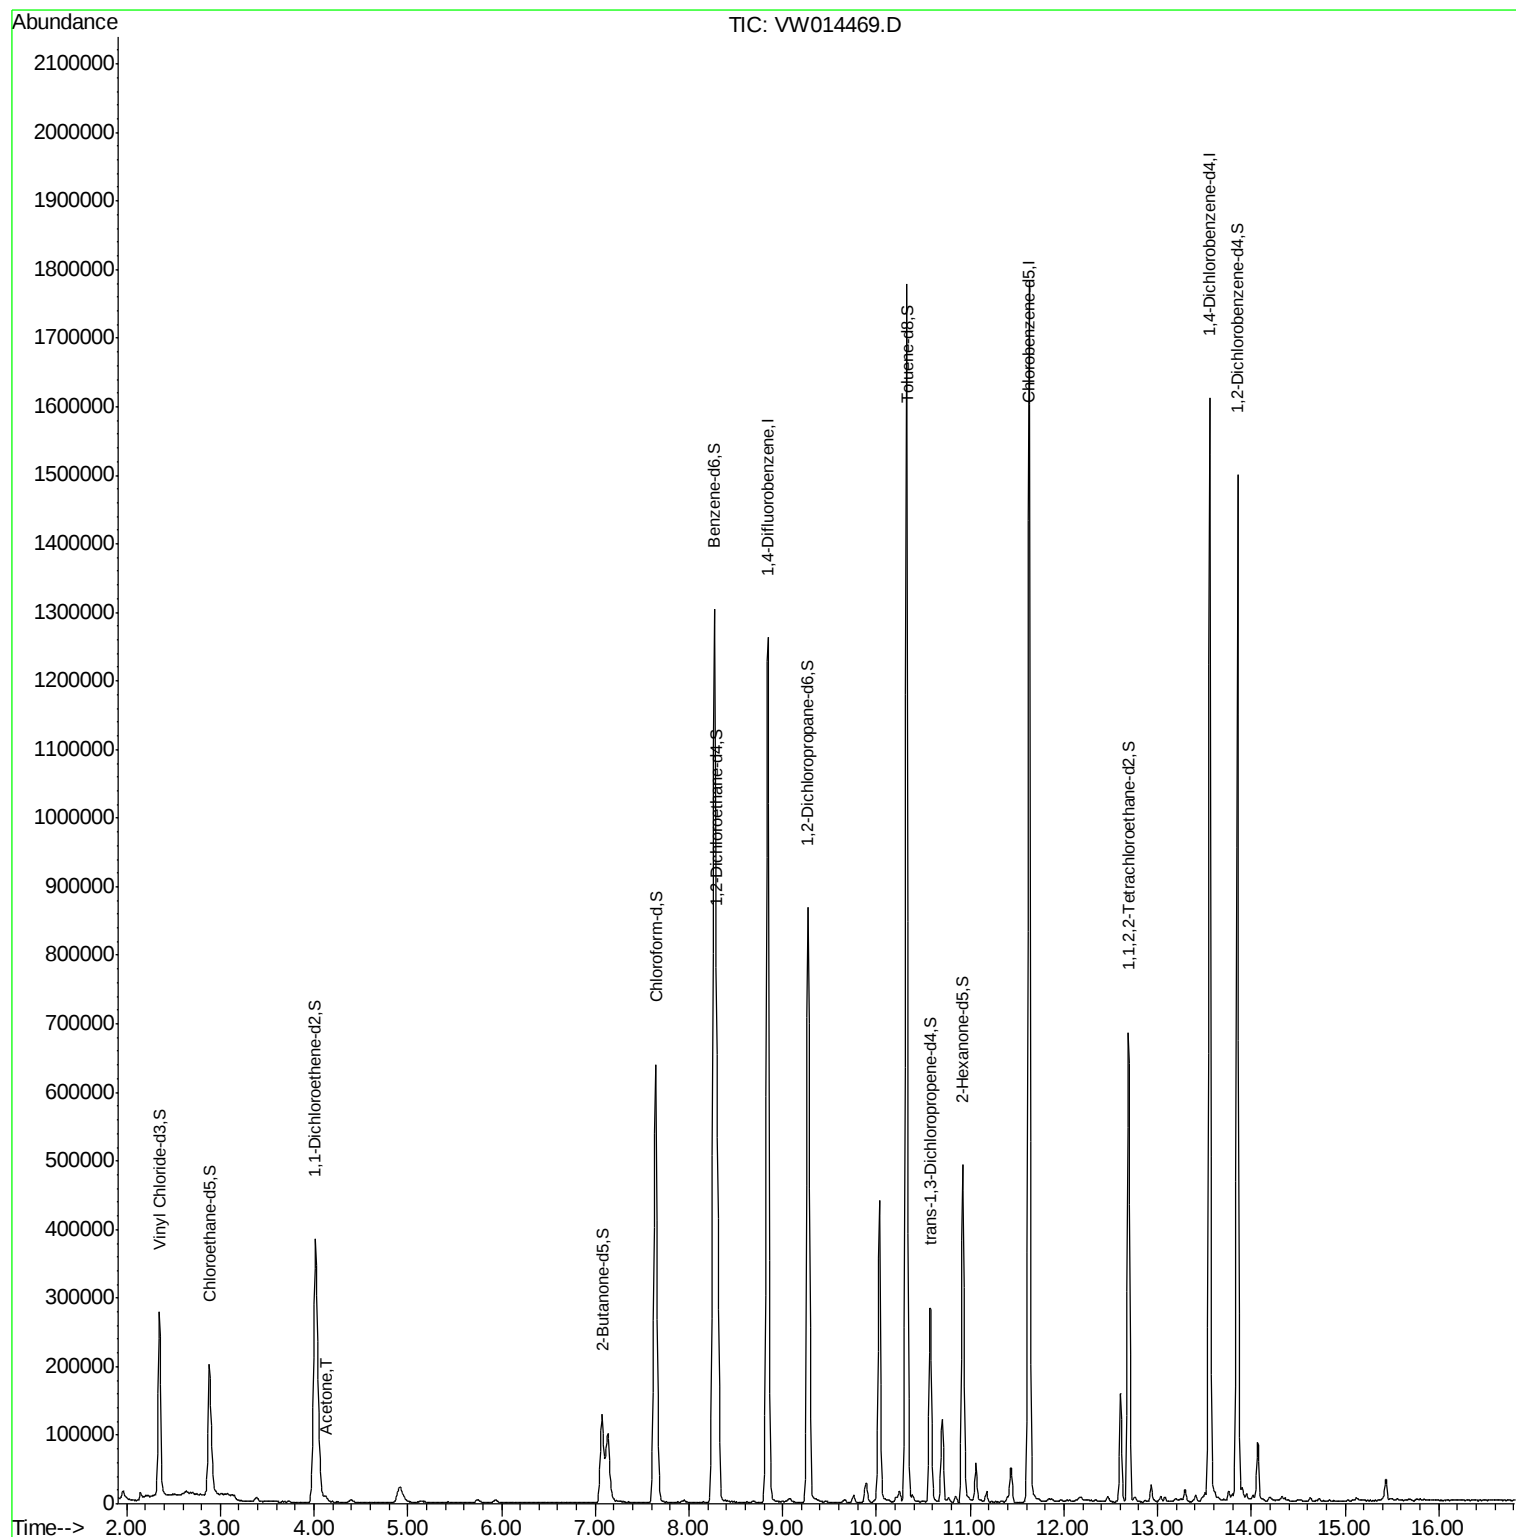

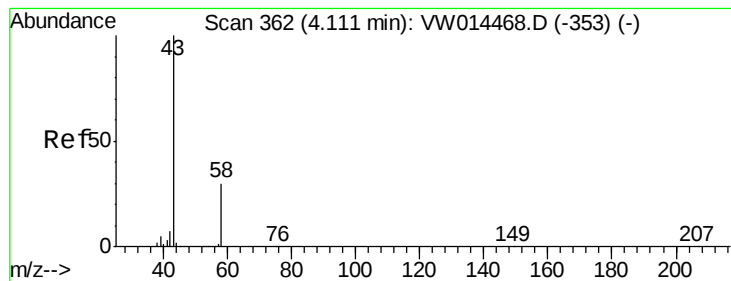

#13
 Acetone
 Concen: 2.925 ug/L
 RT: 4.13 min Scan# 365
 Delta R.T. 0.02 min
 Lab File: VW014469.D
 Acq: 20 Dec 2019 10:48

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK16

Tot Ion: 43 Resp: 11727
 Ion Ratio Lower Upper
 43 100
 58 11.2 0.0 65.4

