


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122320\
 Data File : VW017703.D
 Acq On : 23 Dec 2020 09:17
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W121420S.M
 Title : Sw846 8260
 Last Update : Mon Dec 14 12:39:23 2020

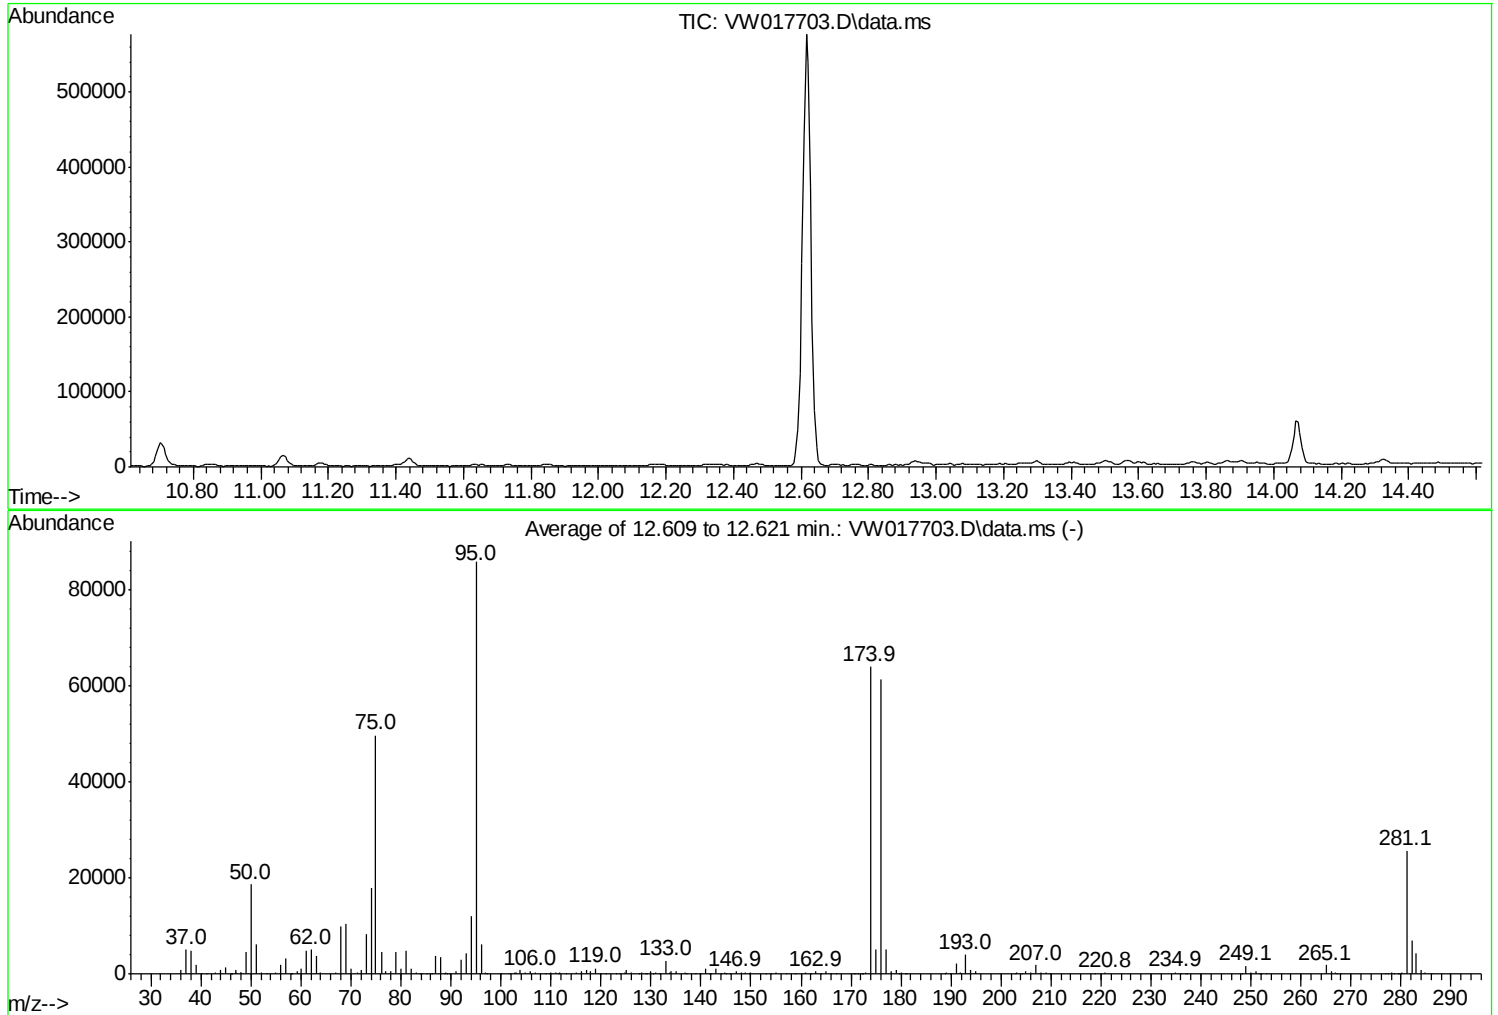

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	18633	PASS
75	95	30	60	57.8	49632	PASS
95	95	100	100	100.0	85813	PASS
96	95	5	9	7.1	6096	PASS
173	174	0.00	2	0.4	233	PASS
174	95	50	100	74.4	63880	PASS
175	174	5	9	8.1	5196	PASS
176	174	95	101	96.1	61389	PASS
177	176	5	9	8.3	5084	PASS