

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122322\
 Data File : VW025184.D
 Acq On : 23 Dec 2022 09:59
 Operator : SY/MD
 Sample : VW1223SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 23 21:59:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 23 21:59:05 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	606832	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	535298	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	255968	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	125497	17.940	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.760%
7) Chloroethane-d5	2.885	69	86089	19.059	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.240%
11) 1,1-Dichloroethene-d2	4.013	63	246309	16.072	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.280%
21) 2-Butanone-d5	7.074	46	87766	49.975	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.960%
24) Chloroform-d	7.647	84	328922	20.998	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.000%
26) 1,2-Dichloroethane-d4	8.305	65	171583	21.600	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.400%
32) Benzene-d6	8.275	84	718689	22.894	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.560%
36) 1,2-Dichloropropane-d6	9.274	67	210646	23.061	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.240%
41) Toluene-d8	10.323	98	651208	22.879	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.520%
43) trans-1,3-Dichloroprop...	10.579	79	83752	21.706	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.840%
47) 2-Hexanone-d5	10.921	63	73507	54.850	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.700%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	161733	23.977	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.920%
66) 1,2-Dichlorobenzene-d4	13.847	152	202863	23.382	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.520%
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	18819	2.167	ug/L	# 8


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122322\
Data File : VW025184.D
Acq On : 23 Dec 2022 09:59
Operator : SY/MD
Sample : VW1223SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 23 21:59:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 23 21:59:05 2022
Response via : Initial Calibration

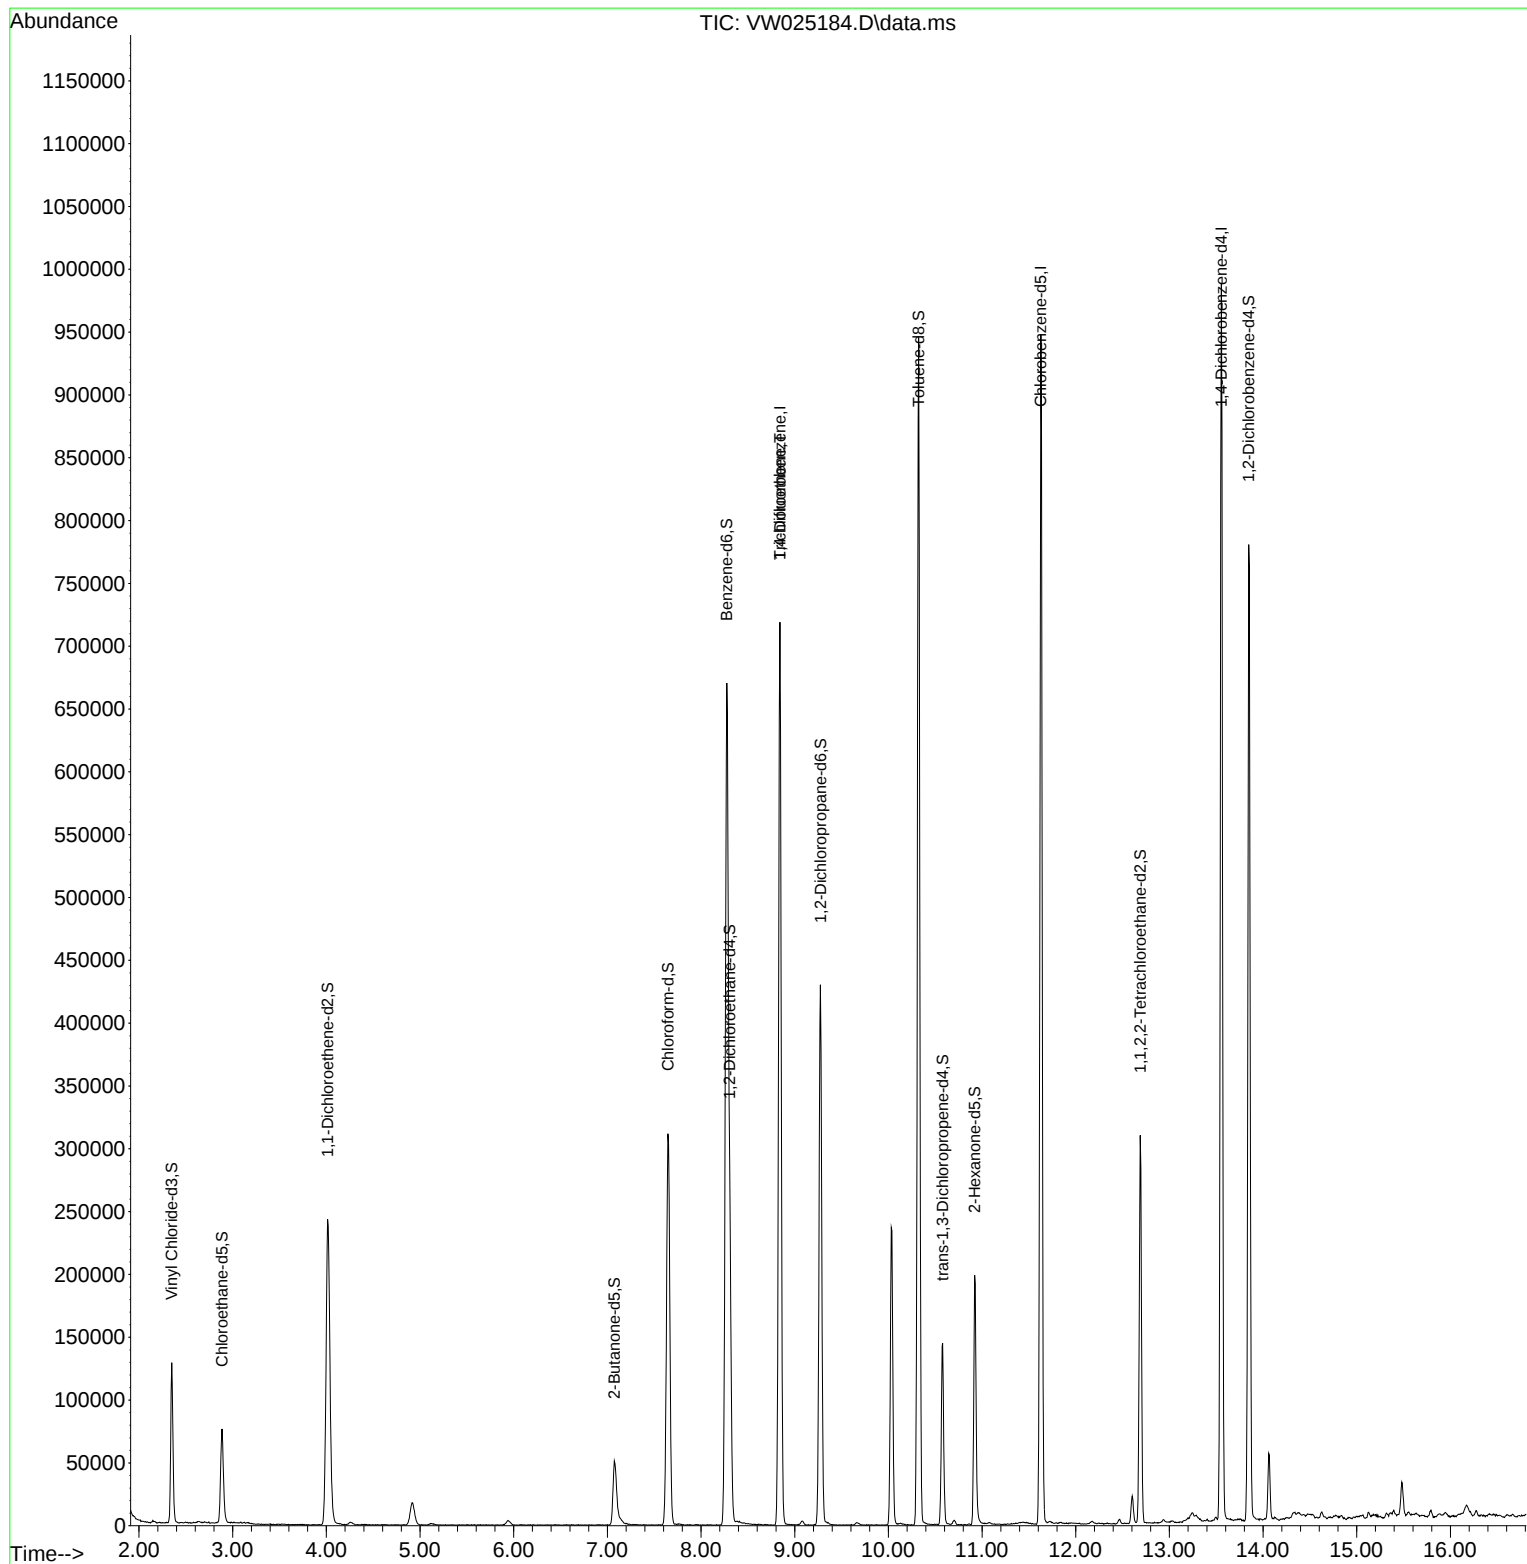

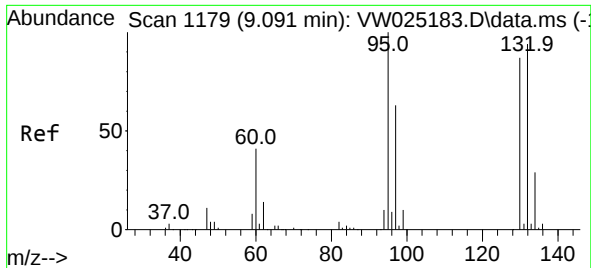

#34
 Trichloroethene
 Concen: 2.167 ug/L
 RT: 8.842 min Scan# 1179
 Delta R.T. -0.250 min
 Lab File: VW025184.D
 Acq: 23 Dec 2022 09:59

Instrument :
 MSVOA_W
 ClientSampleId :

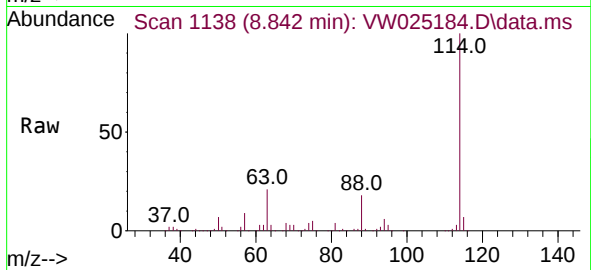

Tgt Ion: 95	Resp: 18819
Ion Ratio	Lower Upper
95	100
97	0.0 44.3 82.3#
132	0.0 63.0 117.0#
130	0.0 63.4 117.8#

