

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122322\
 Data File : VW025185.D
 Acq On : 23 Dec 2022 10:28
 Operator : SY/MD
 Sample : N6193-01RE
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 BGSL8RE

Manual IntegrationsAPPROVED

Quant Time: Dec 23 22:00:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 23 21:59:05 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

12/27/2022
 Supervised By :Mahesh
 Dadoda

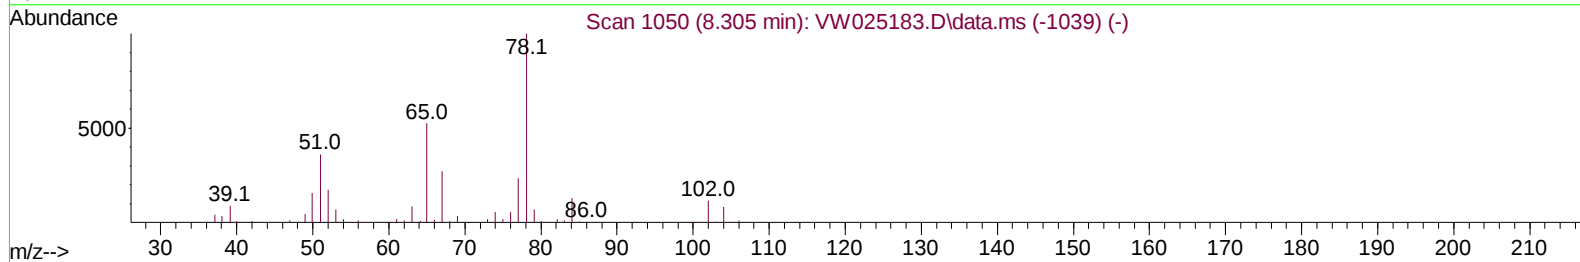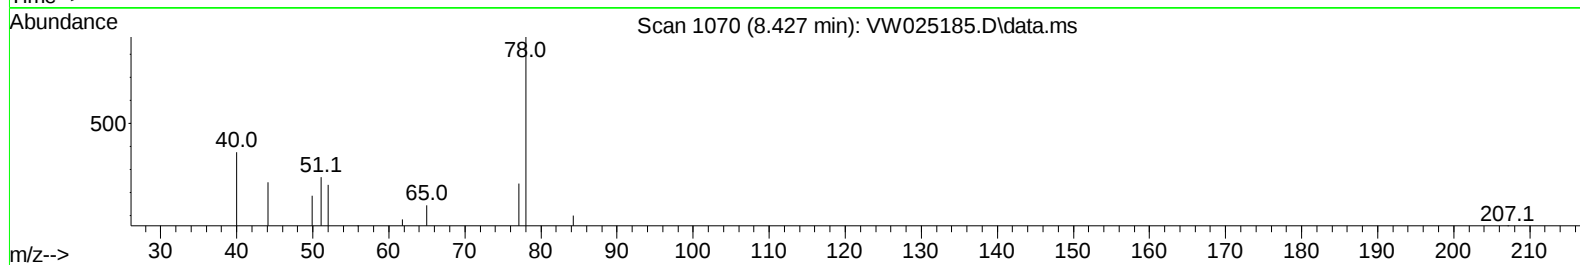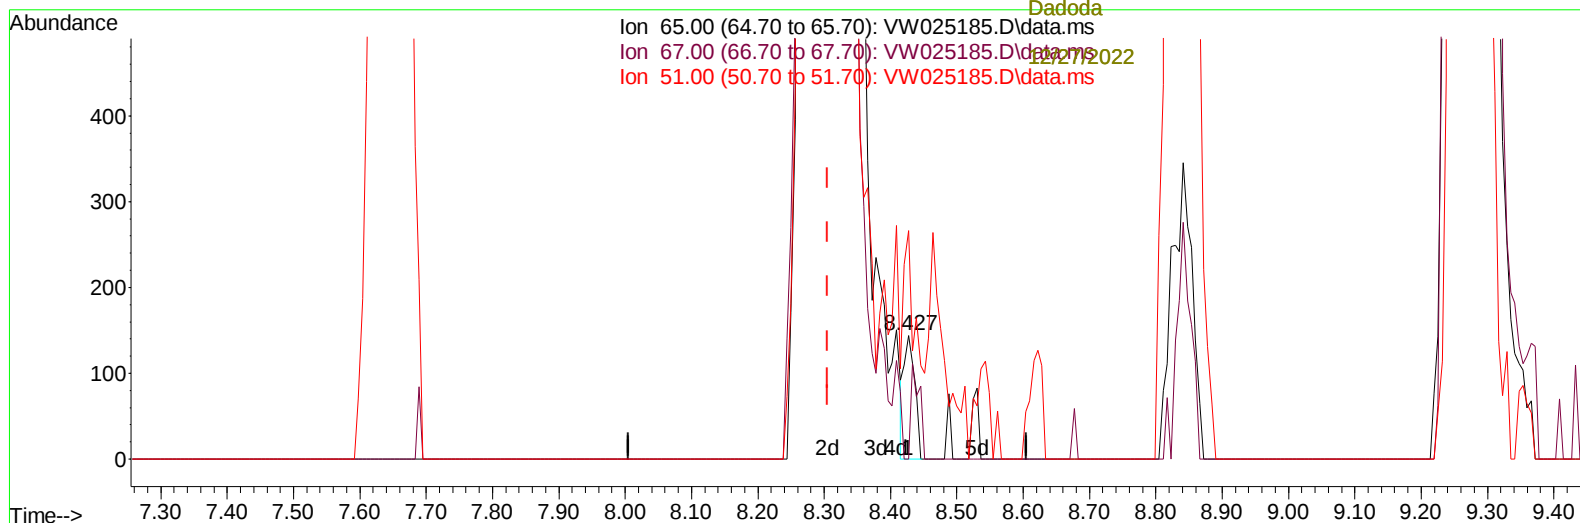

TIC: VW025185.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.427min (+ 0.122) 0.02 ug/L

response 163

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	60.12
51.00	109.90	139.26
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122322\
 Data File : VW025185.D
 Acq On : 23 Dec 2022 10:28
 Operator : SY/MD
 Sample : N6193-01RE
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGSL8RE




Manual IntegrationsAPPROVED

Reviewed By :Krupa
 Patel

12/27/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Dec 23 22:00:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 23 21:59:05 2022
 Response via : Initial Calibration

Ion 65.00 (64.70 to 65.70): VW025185.D\data.ms
 Ion 67.00 (66.70 to 67.70): VW025185.D\data.ms
 Ion 51.00 (50.70 to 51.70): VW025185.D\data.ms

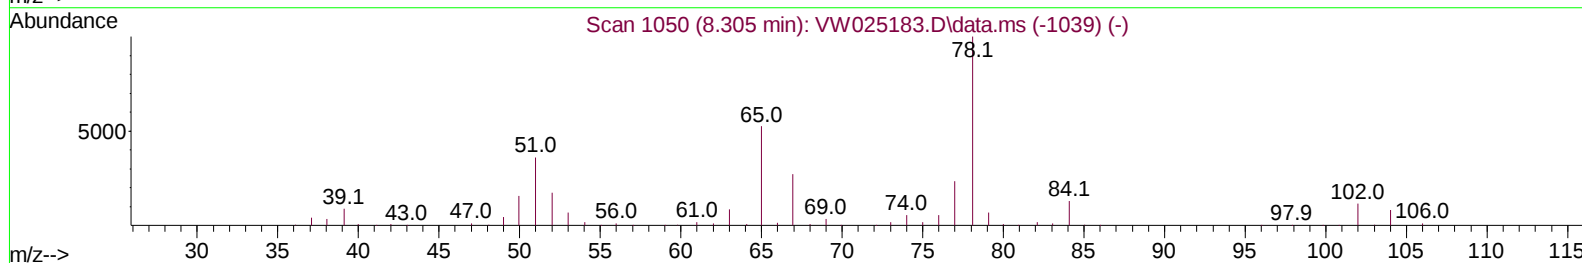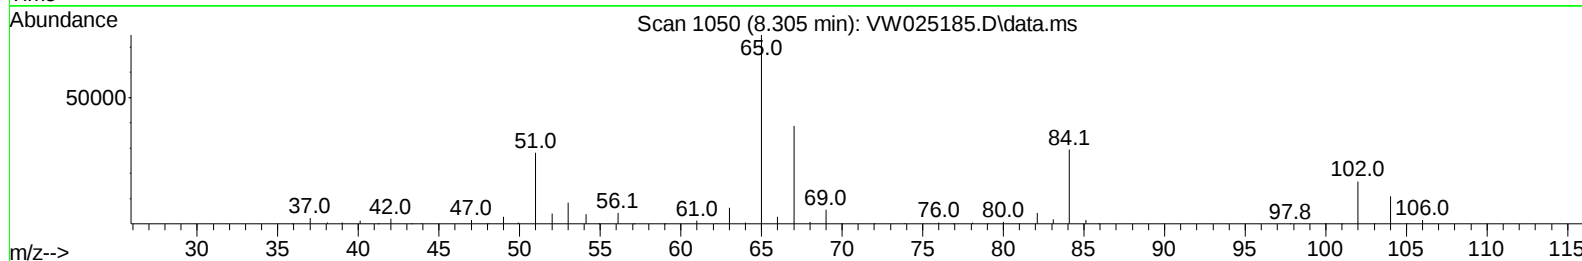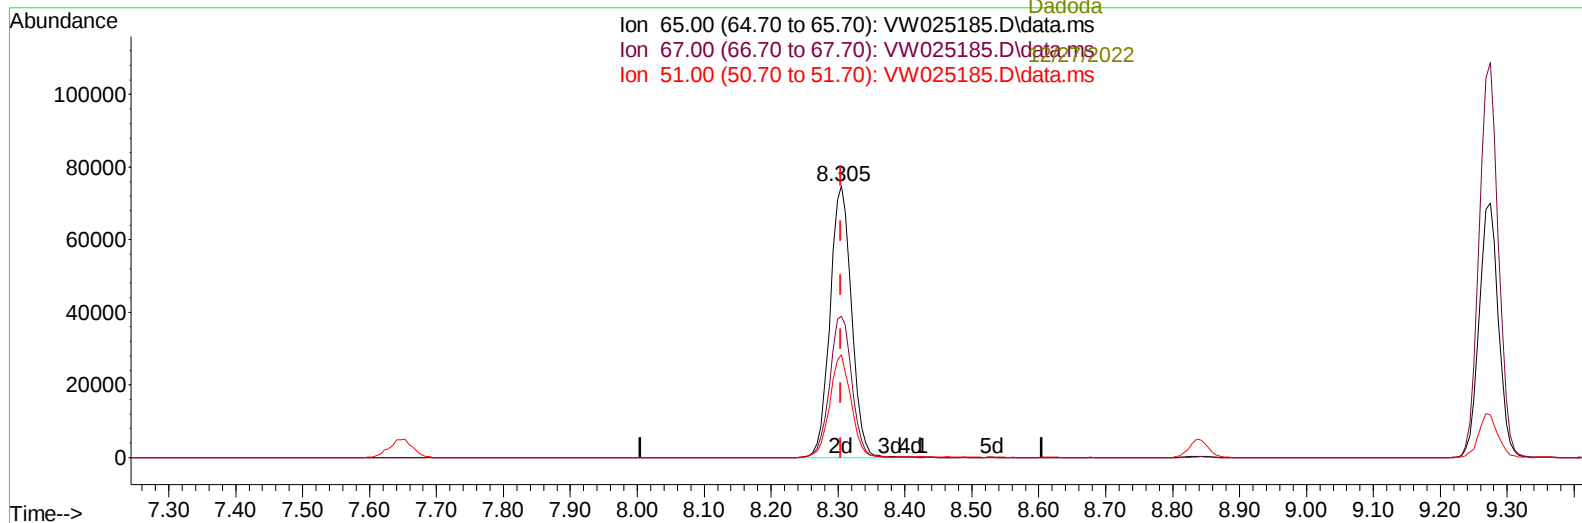

TIC: VW025185.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+ 0.000) 22.39 ug/L m

response 166578

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	0.06#
51.00	109.90	0.14#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122322\
 Data File : VW025185.D
 Acq On : 23 Dec 2022 10:28
 Operator : SY/MD
 Sample : N6193-01RE
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGSL8RE

Manual IntegrationsAPPROVED

Quant Time: Dec 23 22:00:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 23 21:59:05 2022
 Response via : Initial Calibration

Reviewed By :Krupa
 Patel

12/27/2022
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----12/27/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	568306	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	327135	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	65590	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	112384	17.155	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.600%	
7) Chloroethane-d5	2.885	69	84662	20.014	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	80.040%	
11) 1,1-Dichloroethene-d2	4.013	63	231880	16.156	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	64.640%	
21) 2-Butanone-d5	7.080	46	91644	55.721	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	111.440%	
24) Chloroform-d	7.647	84	350730	23.909	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.640%	
26) 1,2-Dichloroethane-d4	8.305	65	166578m	22.392	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	89.560%	
32) Benzene-d6	8.274	84	698645	36.417	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	145.680%#	
36) 1,2-Dichloropropane-d6	9.274	67	217882	39.031	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	156.120%#	
41) Toluene-d8	10.323	98	520981	29.951	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	119.800%	
43) trans-1,3-Dichloroprop...	10.579	79	49744	21.095	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.400%	
47) 2-Hexanone-d5	10.920	63	60821	74.262	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	148.520%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	139772	33.907	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	135.640%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	70927	31.904	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	127.600%#	
Target Compounds						
16) Methylene chloride	4.909	84	40573	4.568	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122322\
Data File : VW025185.D
Acq On : 23 Dec 2022 10:28
Operator : SY/MD
Sample : N6193-01RE
Misc : 5.00g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGSL8RE

Manual IntegrationsAPPROVED

Reviewed By :Krupa
Patel

12/27/2022
Supervised By :Mahesh
Dadoda

Quant Time: Dec 23 22:00:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120822SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 23 21:59:05 2022
Response via : Initial Calibration

