

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW122418\
 Data File : VW007854.D
 Acq On : 22 Dec 2018 20:11
 Operator : SY/AP
 Sample : J6388-16
 Misc : 5.92G/5ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS011-1218-01

Quant Time: Dec 24 03:14:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W122118S.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 20 06:30:23 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	86845	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	145585	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	113384	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	40373	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	50679	53.24	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.48%	
35) Dibromofluoromethane	7.88	113	43776	49.29	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.58%	
50) Toluene-d8	10.32	98	155643	46.49	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.98%	
62) 4-Bromofluorobenzene	12.62	95	48148	37.22	ug/l	0.00
Spiked Amount 50.000			Recovery	=	74.44%	
Target Compounds						
16) Acetone	4.12	43	11409	64.007	ug/l	99
25) 2-Butanone	7.18	43	1492	7.146	ug/l	100
52) Toluene	10.39	92	5337	2.121	ug/l	100
68) m/p-Xylenes	11.83	106	2975	1.821	ug/l	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW122418\
Data File : VW007854.D
Acq On : 22 Dec 2018 20:11
Operator : SY/AP
Sample : J6388-16
Misc : 5.92G/5ML/MSVOA_W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
P001-SS011-1218-01

Quant Time: Dec 24 03:14:12 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W122118S.M
Quant Title : SW846 8260
QLast Update : Thu Dec 20 06:30:23 2018
Response via : Initial Calibration

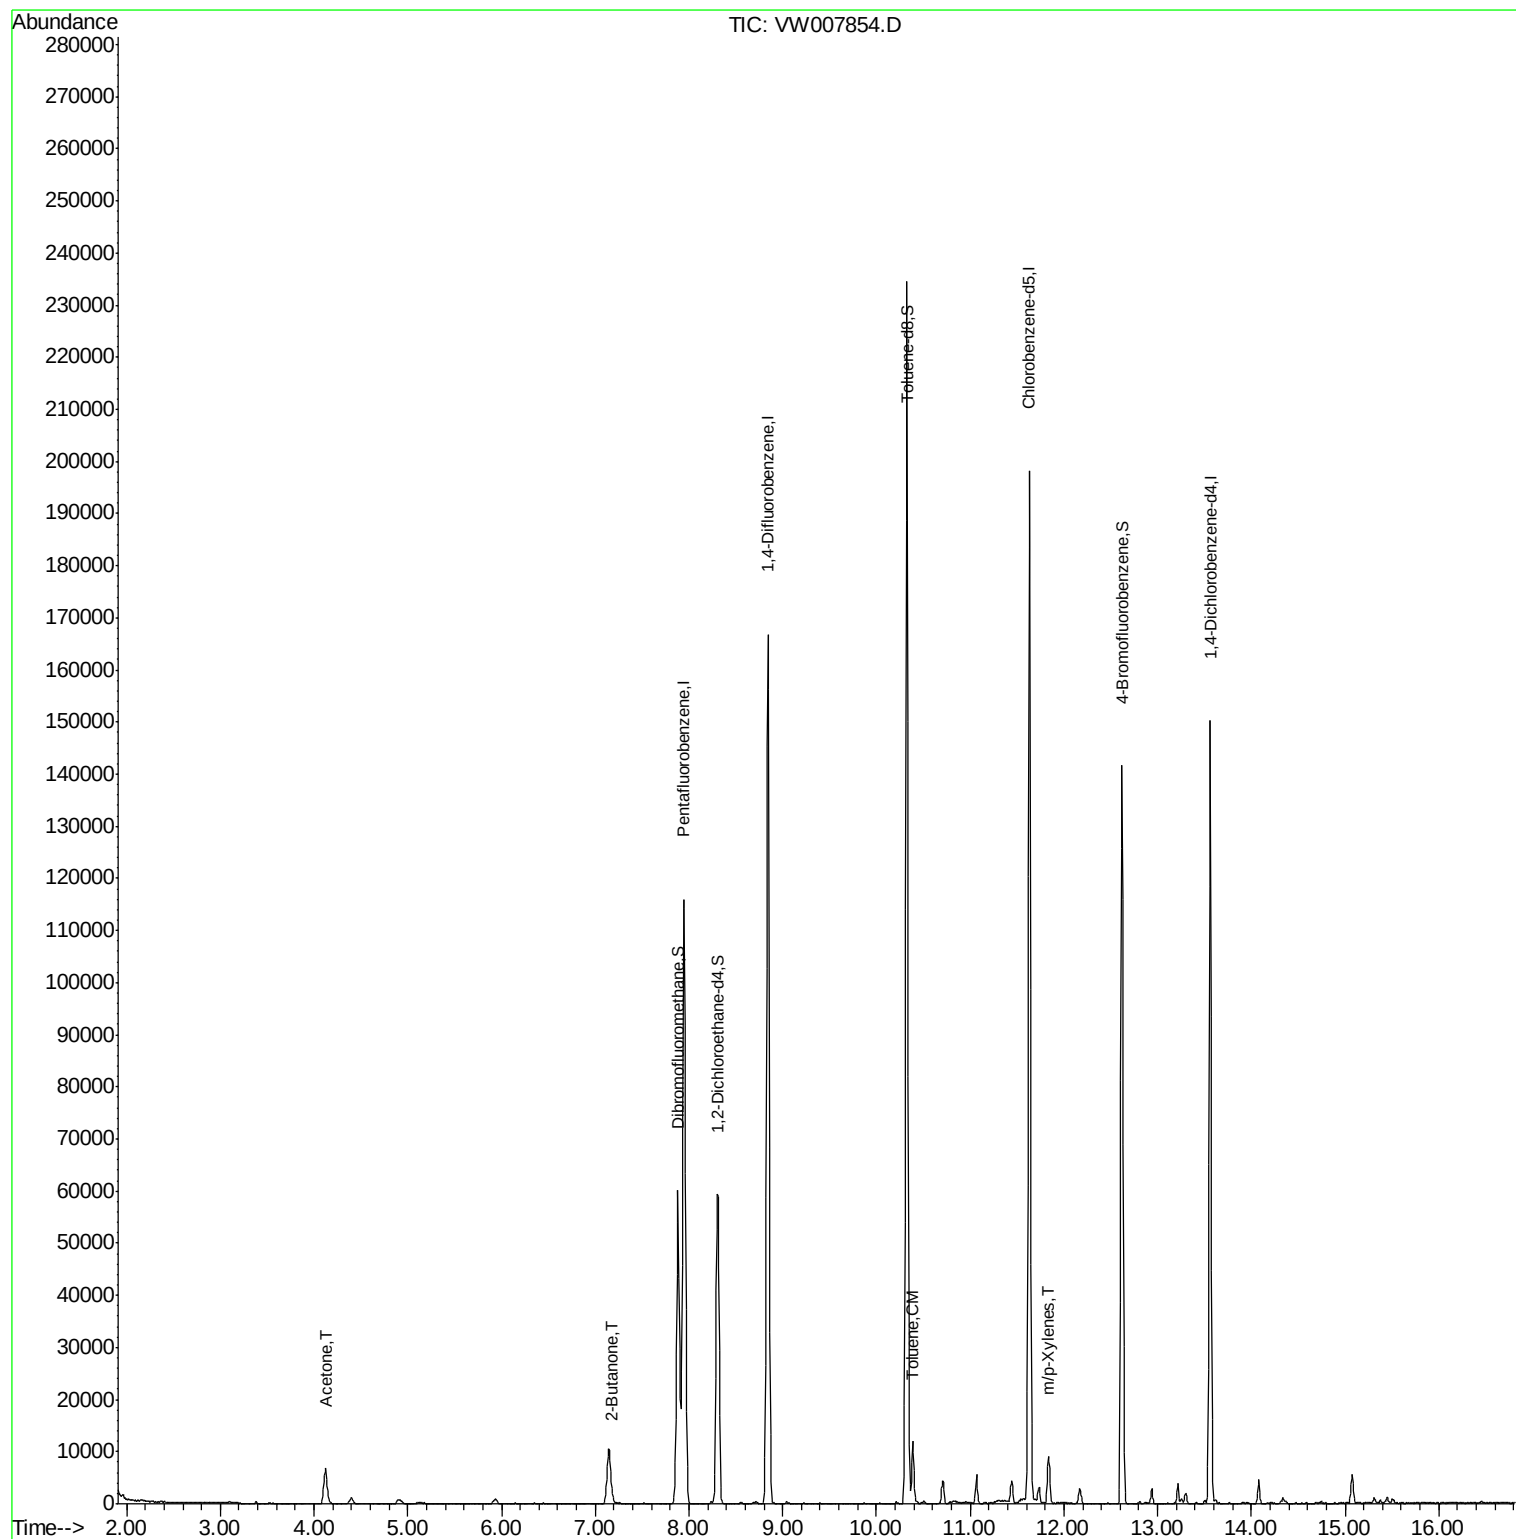

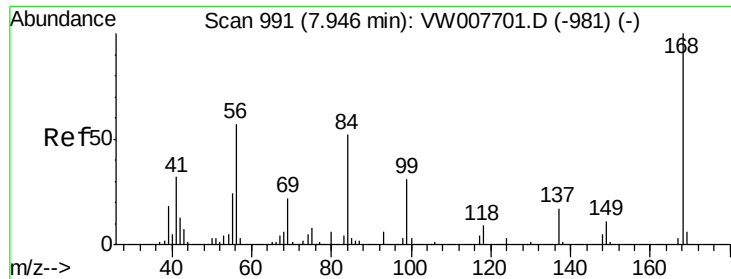

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.01 min

Lab File: VW007854.D

Acq: 22 Dec 2018 20:11

Instrument :

MSVOA_W

ClientSampleId :


P001-SS011-1218-01

Tgt Ion: 168 Resp: 86845

Ion Ratio Lower Upper




168 100

99 55.4 54.0 81.0

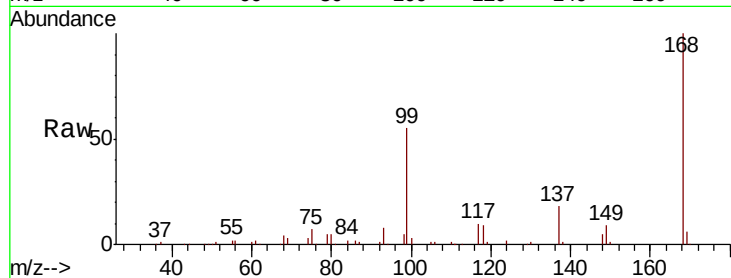

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

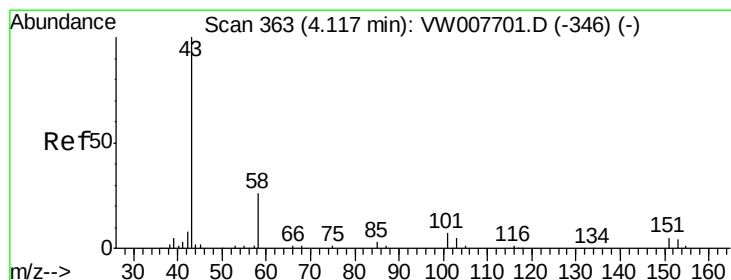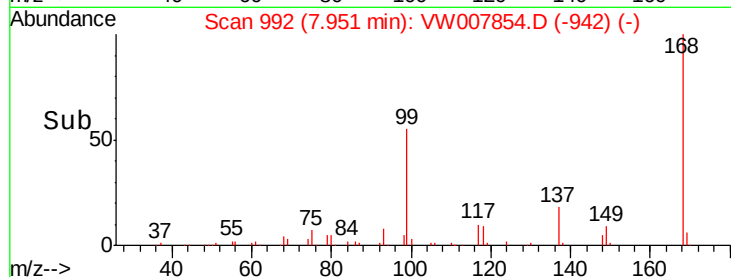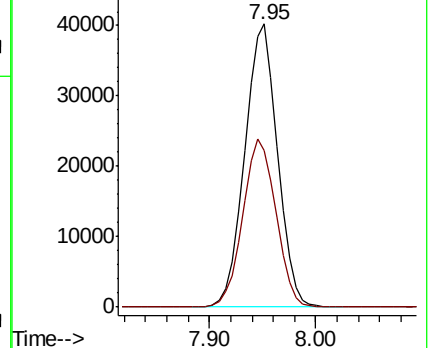

#16

Acetone

Concen: 64.007 ug/l

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW007854.D


Acq: 22 Dec 2018 20:11

Tgt Ion: 43 Resp: 11409

Ion Ratio Lower Upper



43 100


58 26.1 21.2 31.8

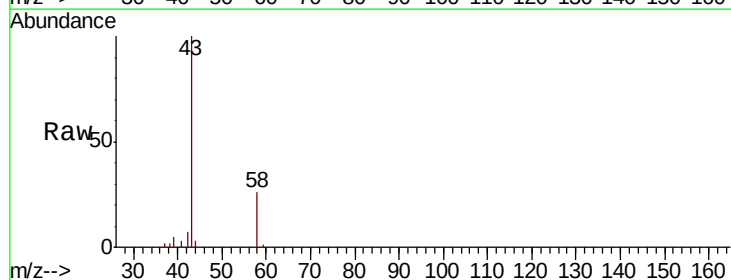

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW



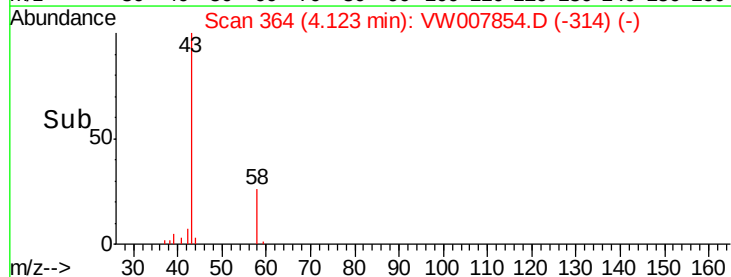
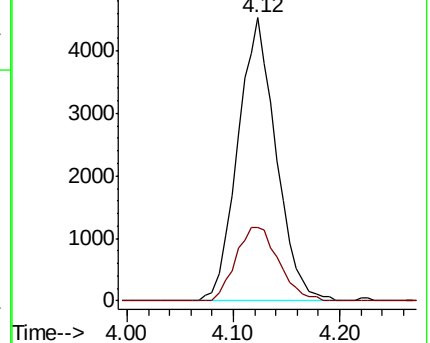


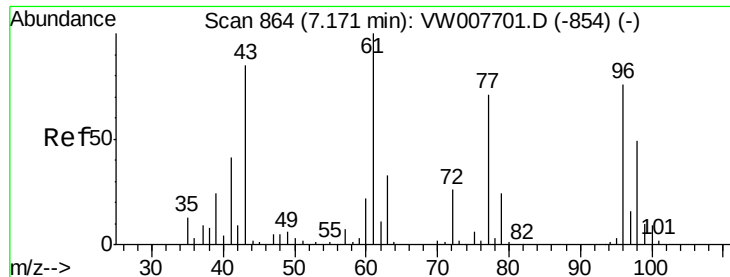

#25
 2-Butanone
 Concen: 7.146 ug/l
 RT: 7.18 min Scan# 865
 Delta R.T. 0.01 min
 Lab File: VW007854.D
 Acq: 22 Dec 2018 20:11




Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS011-1218-01


Tgt Ion: 43 Resp: 1492
 Ion Ratio Lower Upper
 43 100
 72 30.6 24.5 36.7

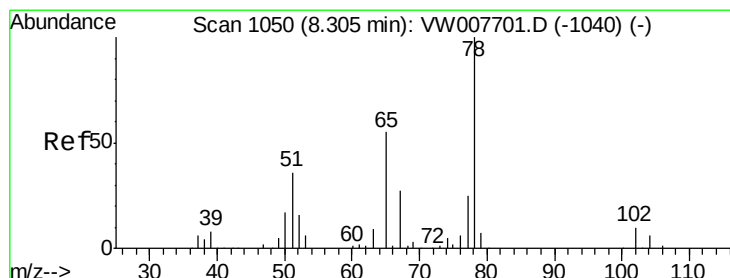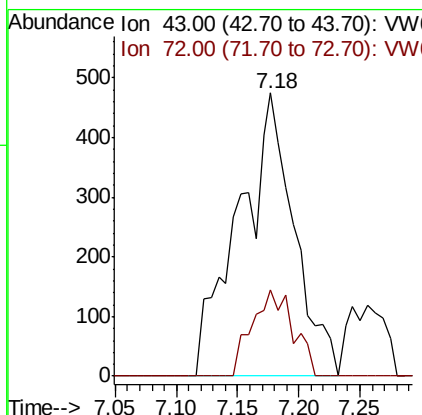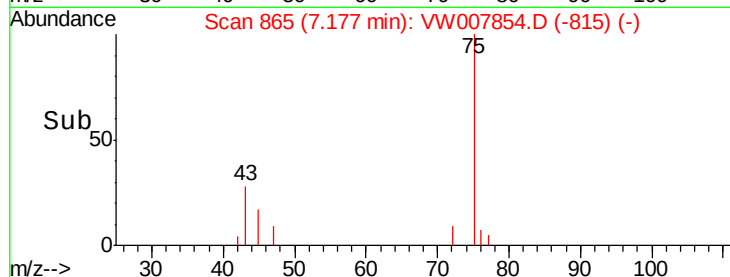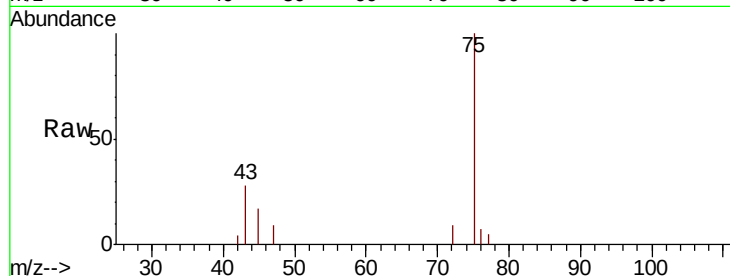

#33
 1,2-Dichloroethane-d4
 Concen: 53.242 ug/l
 RT: 8.31 min Scan# 1051
 Delta R.T. 0.01 min
 Lab File: VW007854.D
 Acq: 22 Dec 2018 20:11

Tgt Ion: 65 Resp: 50679
 Ion Ratio Lower Upper
 65 100
 67 50.6 0.0 100.6

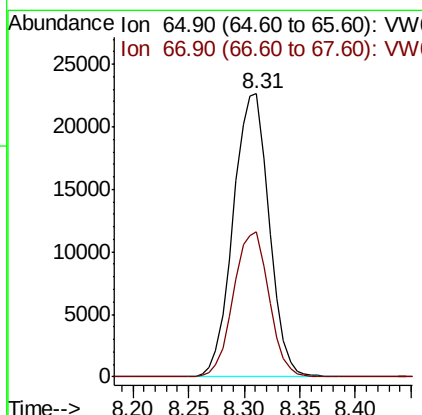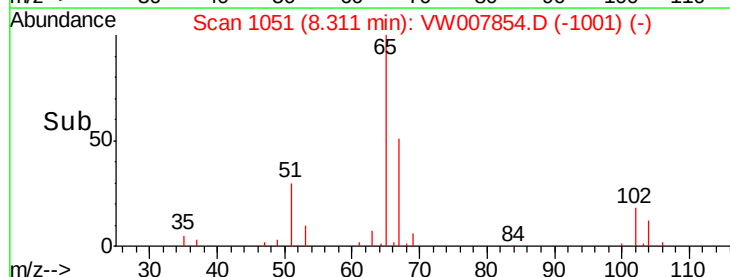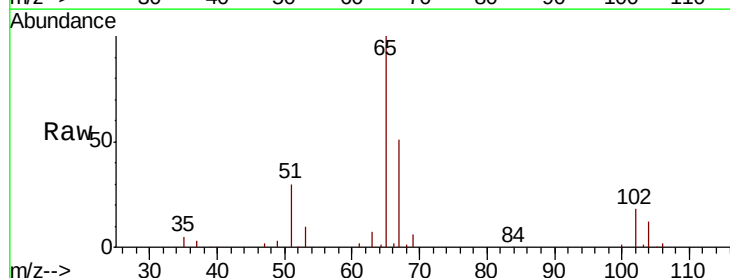


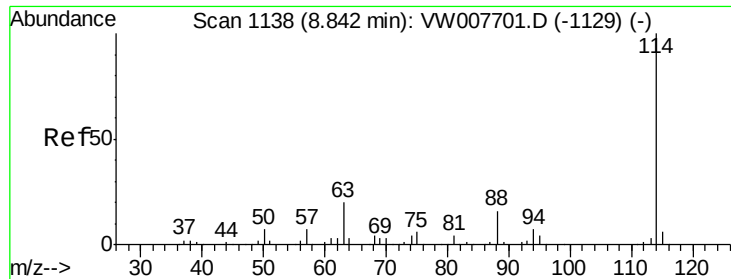




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW007854.D
 Acq: 22 Dec 2018 20:11

Instrument :
 MSVOA_W
 ClientSampleId :
 P001-SS011-1218-01

Tgt Ion:114 Resp: 145585
 Ion Ratio Lower Upper
 114 100
 63 19.4 0.0 40.0
 88 16.7 0.0 32.6

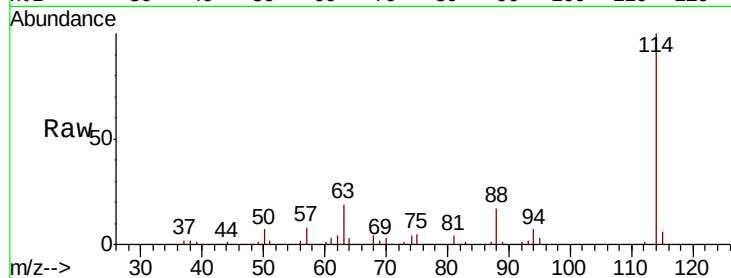


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

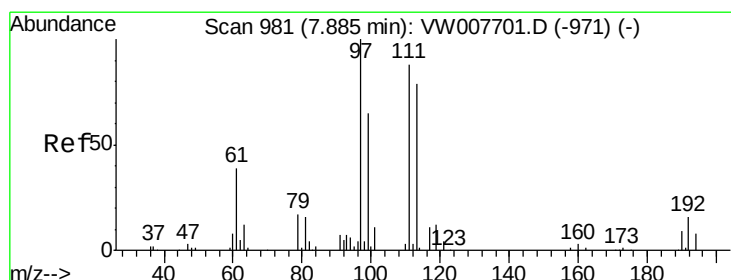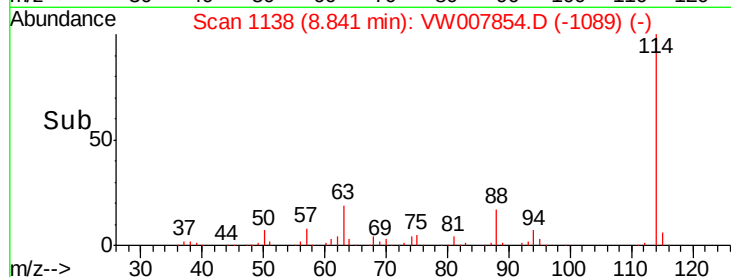
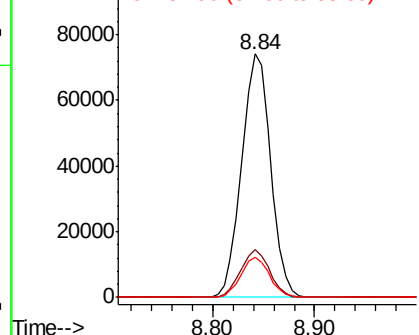



#35
 Dibromofluoromethane
 Concen: 49.289 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW007854.D
 Acq: 22 Dec 2018 20:11

Tgt Ion:113 Resp: 43776
 Ion Ratio Lower Upper
 113 100
 111 101.1 82.6 124.0
 192 18.6 15.5 23.3

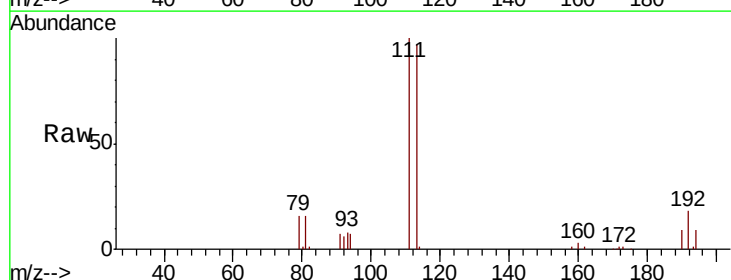

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

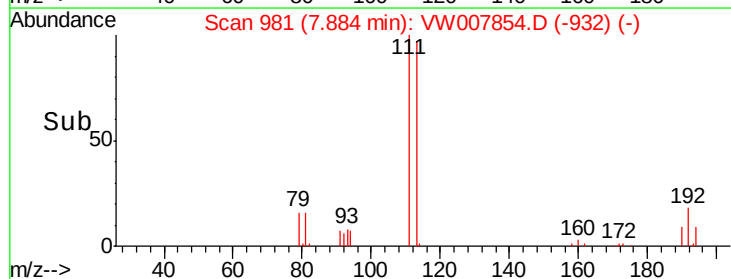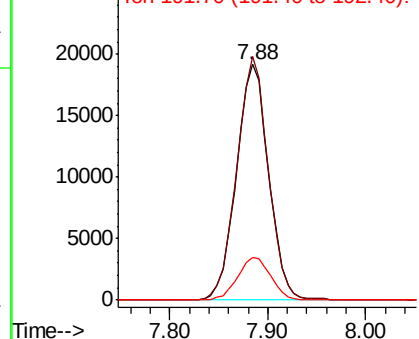

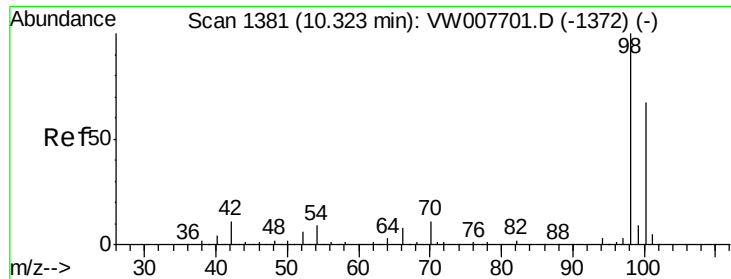

#50

Toluene-d8

Concen: 46.486 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW007854.D

Acq: 22 Dec 2018 20:11

Instrument :

MSVOA_W

ClientSampleId :


P001-SS011-1218-01

Tgt Ion: 98 Resp: 155643

Ion Ratio Lower Upper




98 100

100 65.7 52.2 78.2

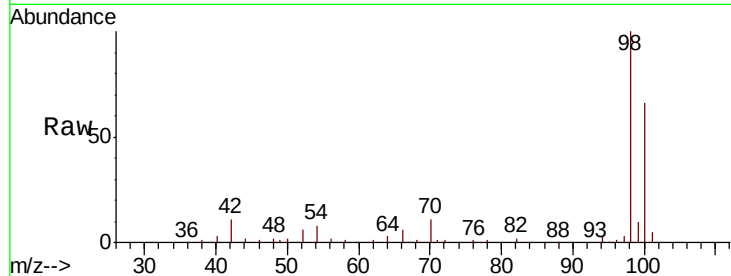

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

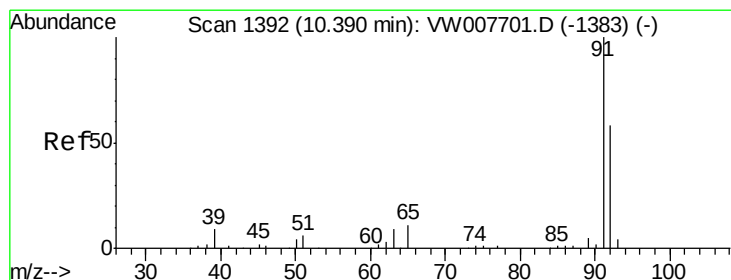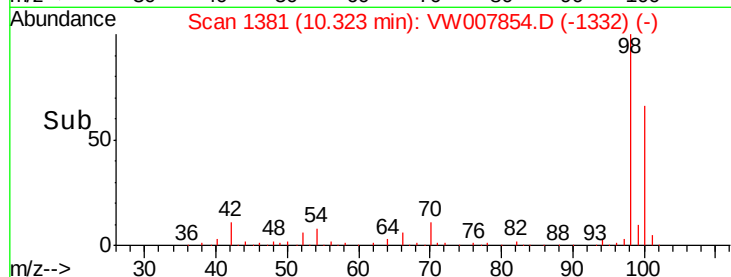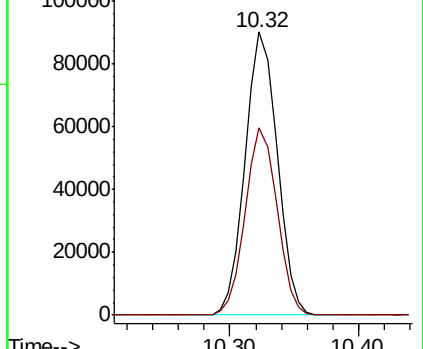

#52

Toluene

Concen: 2.121 ug/l

RT: 10.39 min Scan# 1392

Delta R.T. -0.00 min

Lab File: VW007854.D


Acq: 22 Dec 2018 20:11

Tgt Ion: 92 Resp: 5337

Ion Ratio Lower Upper



92 100


91 171.9 137.0 205.4

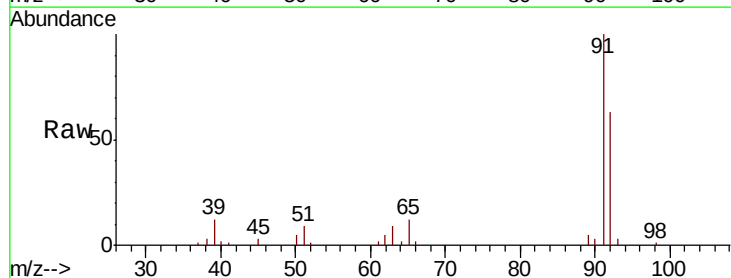

Abundance Ion 92.00 (91.70 to 92.70): VW

Ion 91.00 (90.70 to 91.70): VW

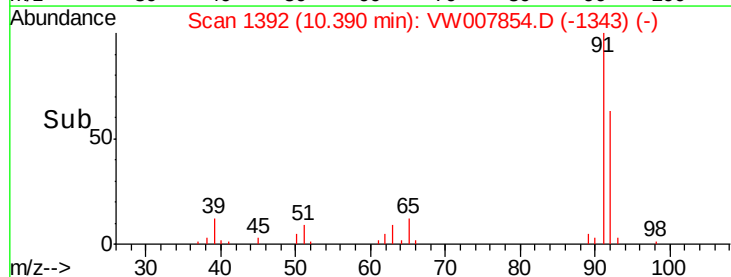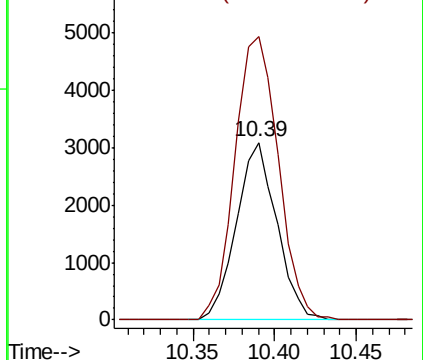

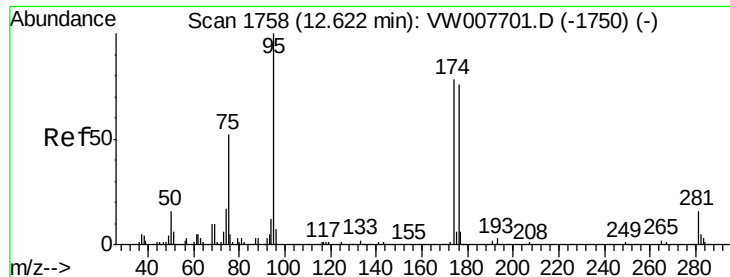

#62

4-Bromofluorobenzene

Concen: 37.224 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW007854.D

Acq: 22 Dec 2018 20:11

Instrument :

MSVOA_W

ClientSampleId :

P001-SS011-1218-01


Tgt Ion: 95 Resp: 48148

Ion Ratio Lower Upper

95 100

174 74.7 0.0 152.2




176 70.3 0.0 146.8

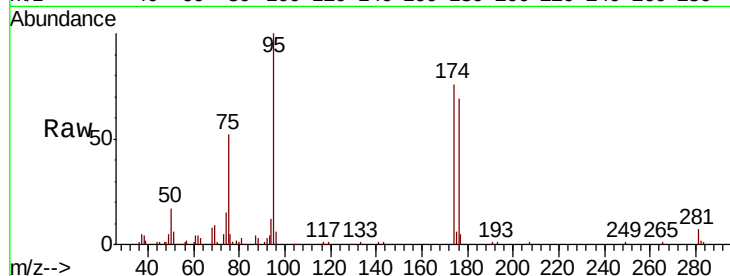

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

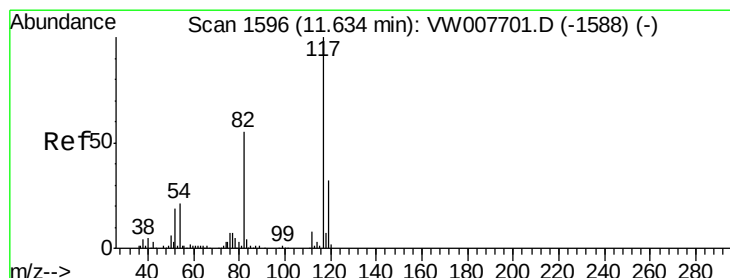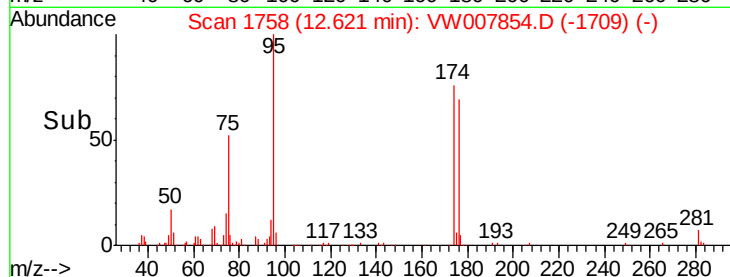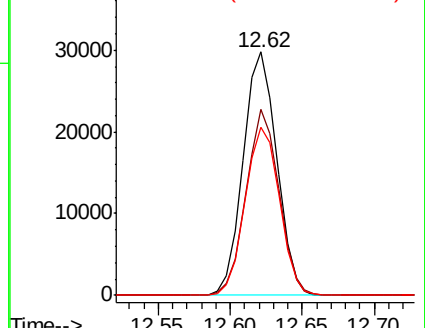

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. -0.00 min

Lab File: VW007854.D

Acq: 22 Dec 2018 20:11


Tgt Ion: 117 Resp: 113384

Ion Ratio Lower Upper

117 100

82 56.5 44.3 66.5



119 31.2 25.7 38.5

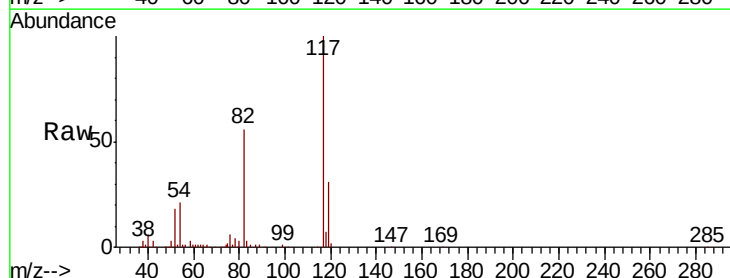


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW



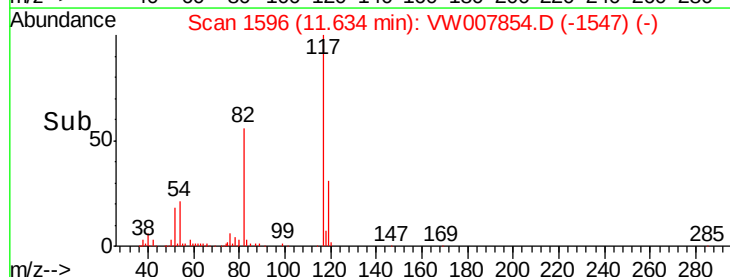
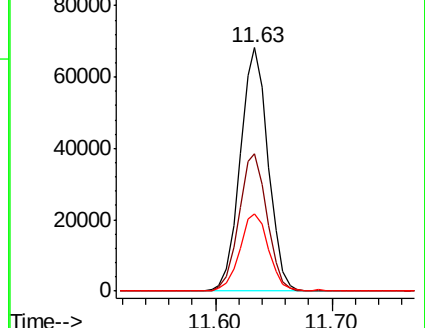


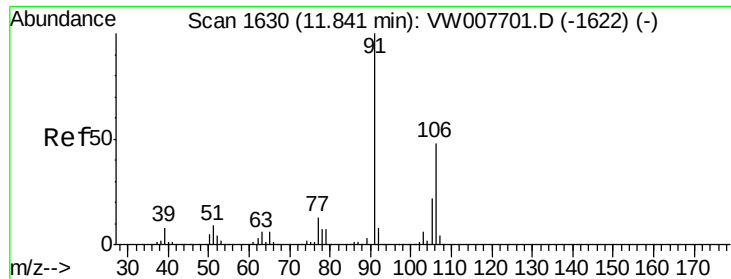

#68
m/p-Xylenes
Concen: 1.821 ug/l
RT: 11.83 min Scan# 1629
Delta R.T. -0.01 min
Lab File: VW007854.D
Acq: 22 Dec 2018 20:11

Instrument :
MSVOA_W
ClientSampleId :
P001-SS011-1218-01

Tgt Ion:106 Resp: 2975
Ion Ratio Lower Upper
106 100
91 187.9 165.2 247.8

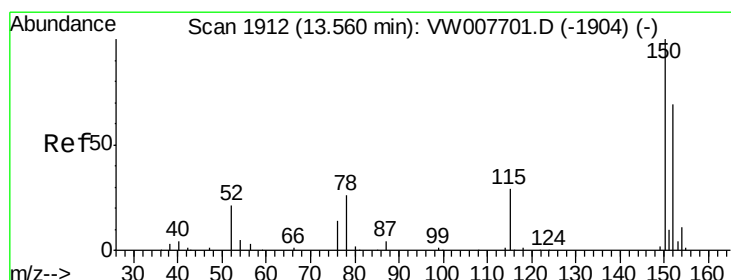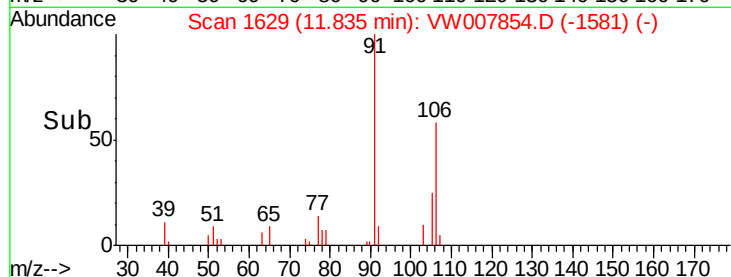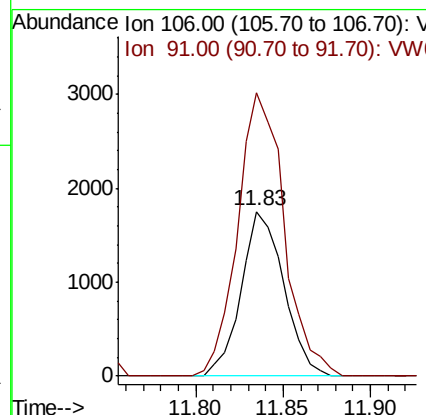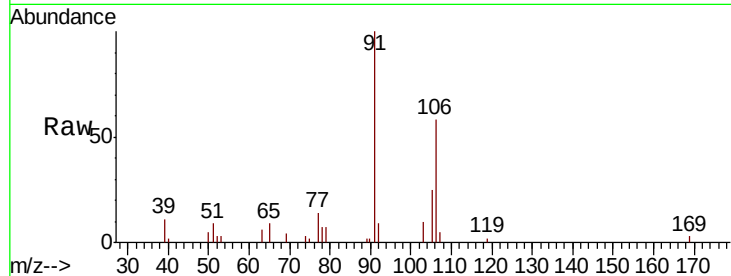

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW007854.D
Acq: 22 Dec 2018 20:11

Tgt Ion:152 Resp: 40373
Ion Ratio Lower Upper
152 100
115 61.8 31.8 95.4
150 155.6 0.0 350.8

