


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW122418\
Data File : VW007868.D
Acq On : 23 Dec 2018 03:07
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W122118S.M
Title : SW846 8260
Last Update : Thu Dec 20 06:30:23 2018

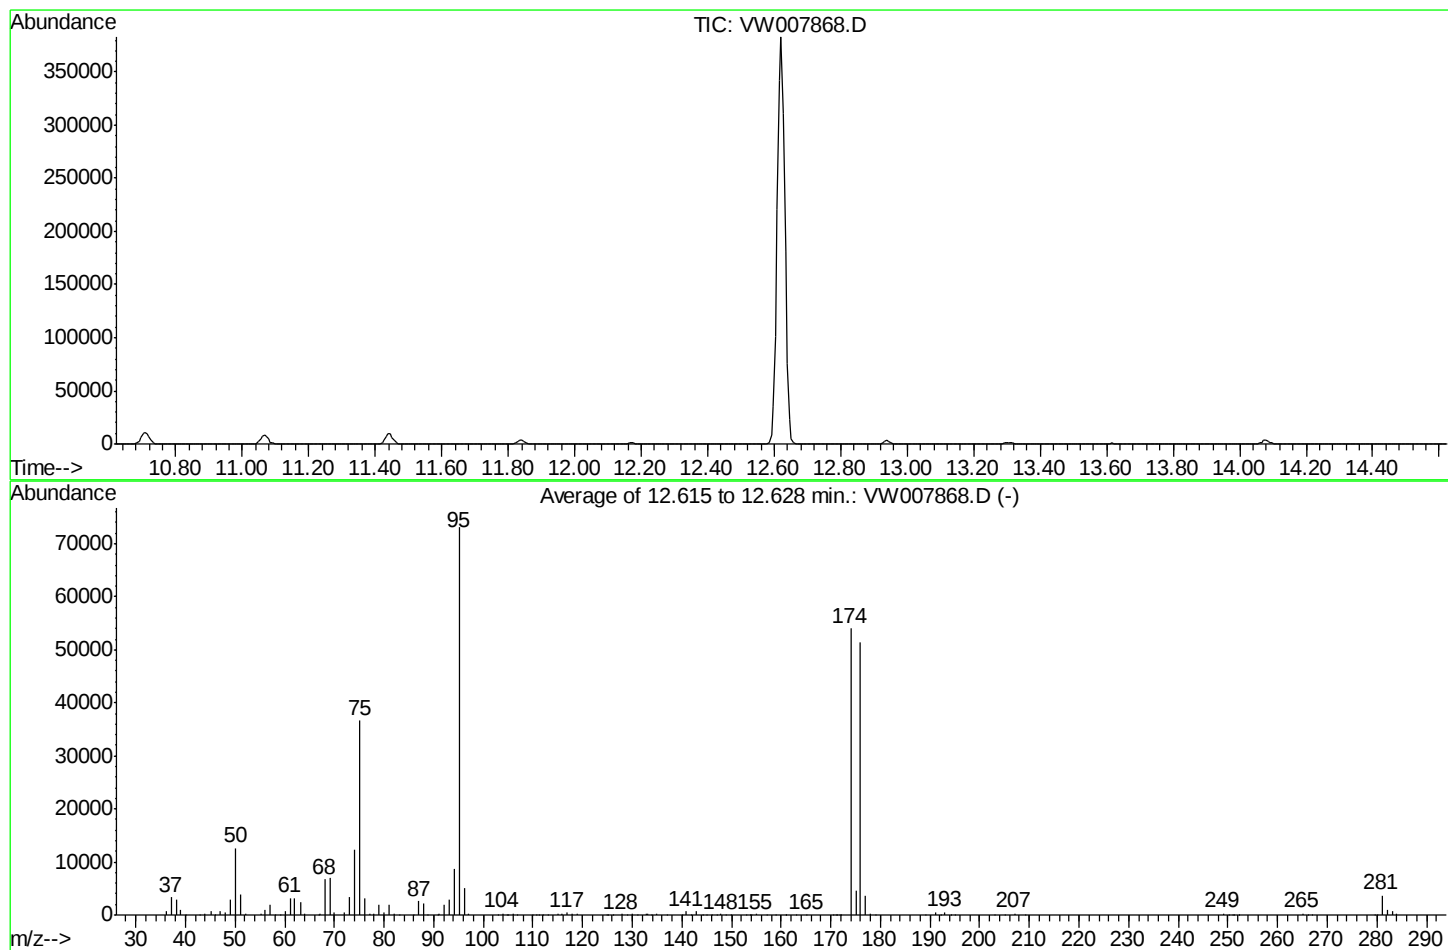

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	12612	PASS
75	95	30	60	50.1	36592	PASS
95	95	100	100	100.0	73101	PASS
96	95	5	9	6.8	4969	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.8	53968	PASS
175	174	5	9	8.5	4577	PASS
176	174	95	101	95.5	51514	PASS
177	176	5	9	7.2	3693	PASS