

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122420\
 Data File : VW017747.D
 Acq On : 24 Dec 2020 19:56
 Operator : SY/VA
 Sample : VIBLK24
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK24

Manual Integrations
 APPROVED

MMDadoda
 12/26/2020 1:37:48 PM

Quant Time: Dec 25 08:22:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 25 07:46:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	356386	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	321266	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	160282	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	124023	22.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.96%
7) Chloroethane-d5	2.89	69	103561	22.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.04%
10) 1,1-Dichloroethene-d2	4.03	63	160562	16.71	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.84%
20) 2-Butanone-d5	7.07	46	53137	59.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.92%
24) Chloroform-d	7.65	84	223026	23.95	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	8.30	65	128077	26.57	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.28%
29) Benzene-d6	8.27	84	440964	24.37	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.48%
33) 1,2-Dichloropropane-d6	9.27	67	126680	25.39	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.56%
37) Toluene-d8	10.32	98	414324	23.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.36%
38) trans-1,3-Dichloropropene-	10.58	79	54579	24.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.20%
39) 2-Hexanone-d5	10.92	63	37417	59.73	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.46%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	103323	27.90	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	111.60%
61) 1,2-Dichlorobenzene-d4	13.85	152	134507	24.10	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.40%

Target Compounds				Ovalue
16) Methylene chloride	4.93	84	6372m	1.250 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW122420\
Data File : VW017747.D
Acq On : 24 Dec 2020 19:56
Operator : SY/VA
Sample : VIBLK24
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK24

Manual Integrations
APPROVED

MMDadoda
12/26/2020 1:37:48 PM

Quant Time: Dec 25 08:22:27 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 25 07:46:43 2020
Response via : Initial Calibration

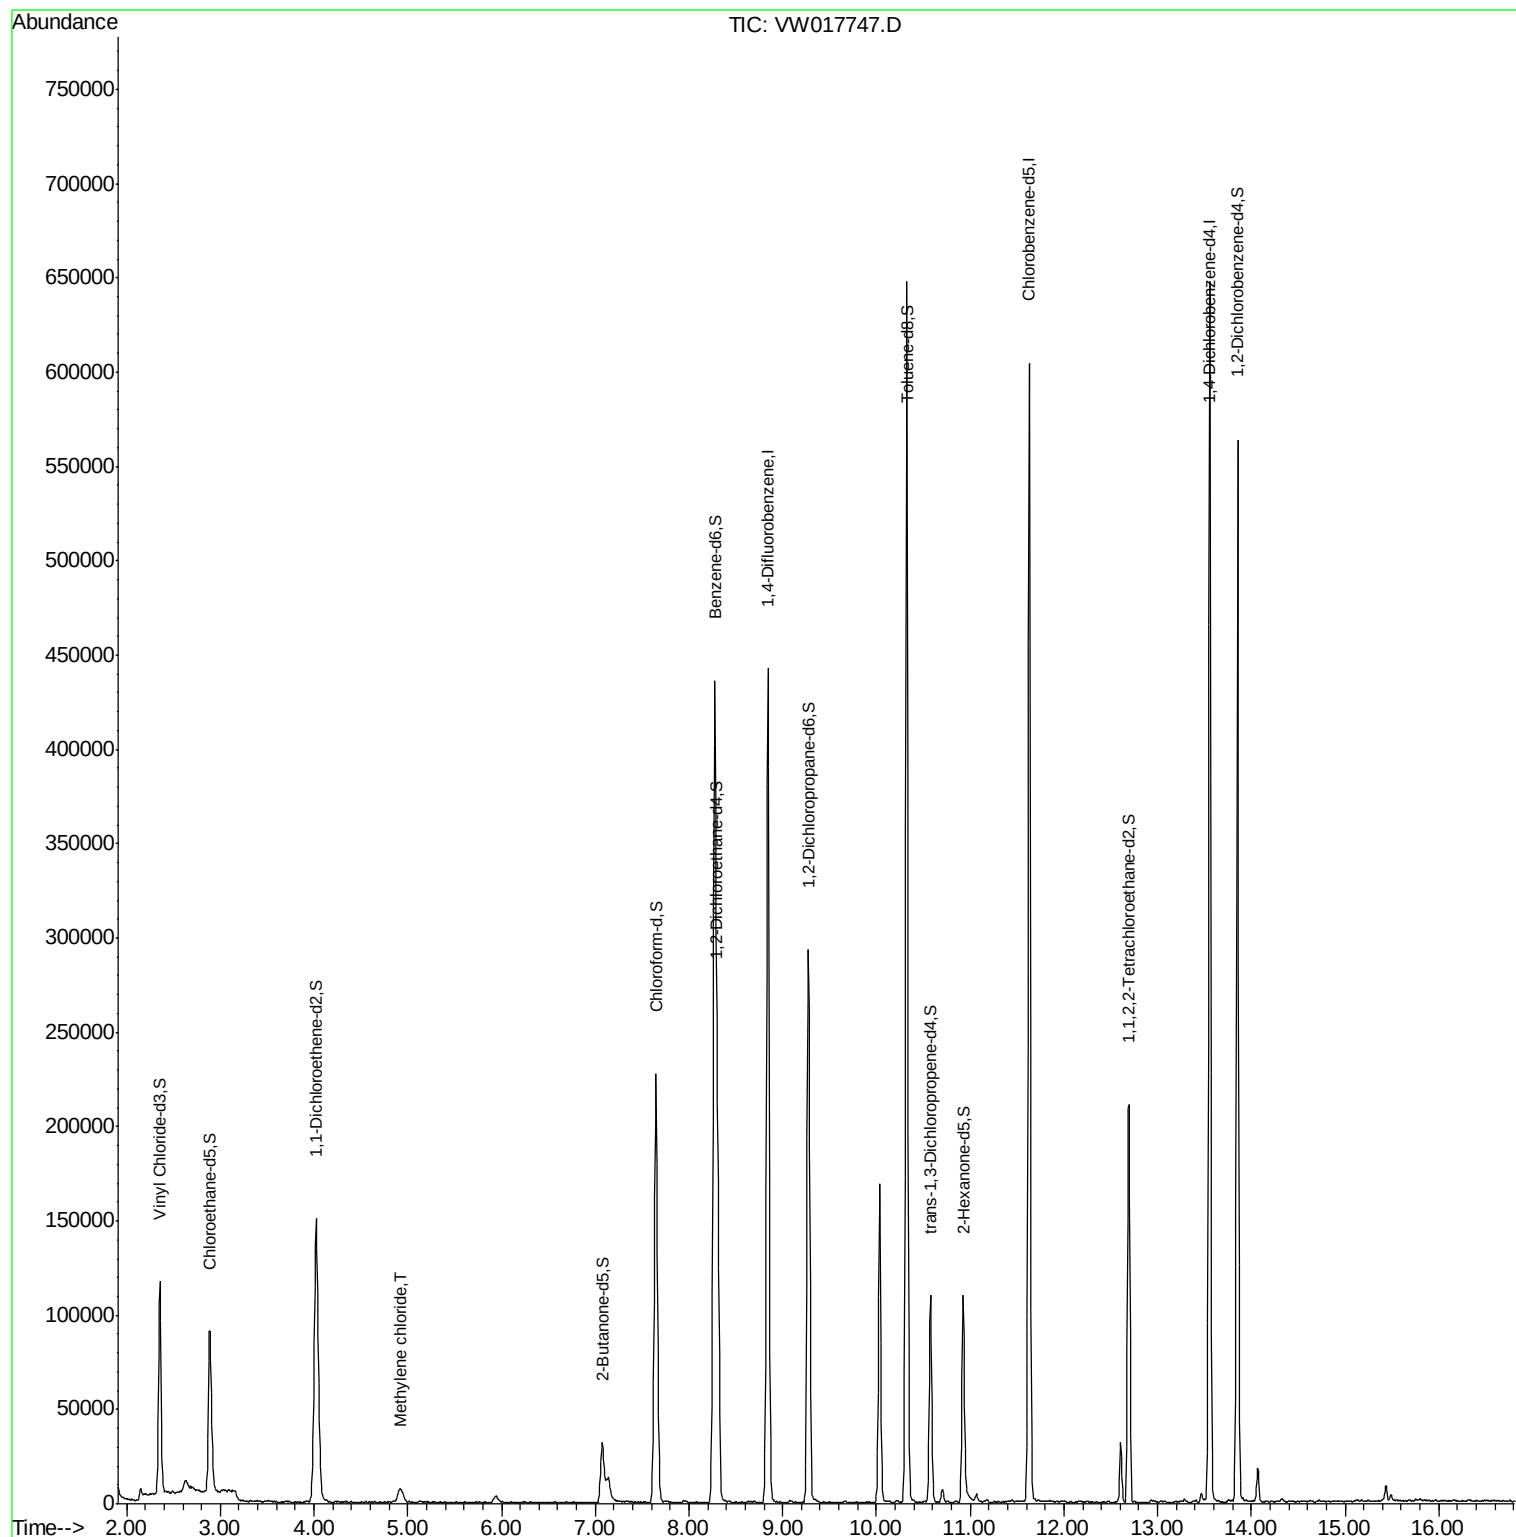

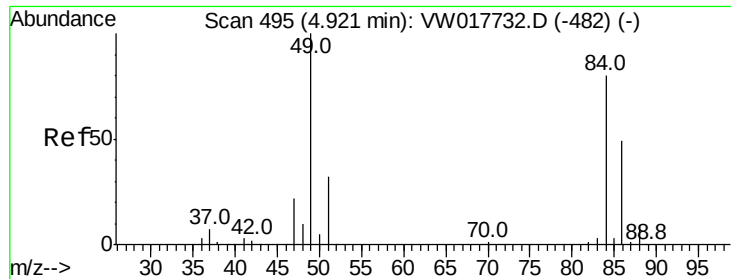

#16
 Methvlene chloride
 Concen: 1.250 ug/L m
 RT: 4.93 min Scan# 496
 Delta R.T. 0.01 min
 Lab File: VW017747.D
 Acq: 24 Dec 2020 19:56

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK24

Tot Ion	Ratio	Lower	Upper
84	100		
49	136.8	90.5	168.1
86	57.9	44.8	83.2

Manual Integrations
 APPROVED

MMDadoda
 12/26/2020 1:37:48 PM

