

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122521\
 Data File : VW021656.D
 Acq On : 25 Dec 2021 19:22
 Operator : SY/VA
 Sample : M5154-10
 Misc : 6.66g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGL90

Quant Time: Dec 27 00:42:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 24 01:43:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	127259	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.633	117	123355	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78423	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.342	65	31918	13.771	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.080%
7) Chloroethane-d5	2.879	69	22950	14.979	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.920%
11) 1,1-Dichloroethene-d2	4.007	63	37074	11.998	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.000%
21) 2-Butanone-d5	7.110	46	13984	42.803	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.600%
24) Chloroform-d	7.646	84	69961	19.727	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.920%
26) 1,2-Dichloroethane-d4	8.311	65	36937	19.580	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.320%
32) Benzene-d6	8.274	84	128991	19.077	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.320%
36) 1,2-Dichloropropane-d6	9.274	67	37332	20.587	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.360%
41) Toluene-d8	10.323	98	125946	18.231	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.920%
43) trans-1,3-Dichloroprop...	10.579	79	14756	17.673	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.680%
47) 2-Hexanone-d5	10.926	63	13019	48.552	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.100%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	34102	21.877	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	54983	18.091	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	72.360%#
Target Compounds						Qvalue
13) Acetone	4.184	43	43428	148.278	ug/L	73
14) Carbon disulfide	4.366	76	4725	1.160	ug/L	# 94
22) 2-Butanone	7.207	43	3442	8.999	ug/L	# 65
33) Benzene	8.323	78	3963	0.590	ug/L	100
35) Methylcyclohexane	9.335	83	7253	2.331	ug/L	# 69
40) 4-Methyl-2-pentanone	10.213	43	12383	15.162	ug/L	# 92
42) Toluene	10.384	91	49853	6.343	ug/L	99
51) Chlorobenzene	11.658	112	7534	1.432	ug/L	90
52) Ethylbenzene	11.731	91	1088470	121.197	ug/L	95
53) m,p-Xylene	11.835	106	184856	51.023	ug/L	83
54) o-Xylene	12.164	106	196291	57.088	ug/L	91
60) Isopropylbenzene	12.463	105	304547	28.579	ug/L	96
62) 1,3,5-Trimethylbenzene	12.938	105	121462	13.395	ug/L	95
63) 1,2,4-Trimethylbenzene	13.249	105	1285660	143.727	ug/L	95
64) 1,3-Dichlorobenzene	13.499	146	7725	1.537	ug/L	# 76
65) 1,4-Dichlorobenzene	13.578	146	13434	2.690	ug/L	# 77
67) 1,2-Dichlorobenzene	13.865	146	15498	3.502	ug/L	# 82
70) 1,2,4-trichlorobenzene	15.133	180	18121	5.997	ug/L	# 57

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122521\
Data File : VW021656.D
Acq On : 25 Dec 2021 19:22
Operator : SY/VA
Sample : M5154-10
Misc : 6.66g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGL90

Quant Time: Dec 27 00:42:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 24 01:43:02 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122521\
Data File : VW021656.D
Acq On : 25 Dec 2021 19:22
Operator : SY/VA
Sample : M5154-10
Misc : 6.66g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGL90

Quant Time: Dec 27 00:42:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 24 01:43:02 2021
Response via : Initial Calibration




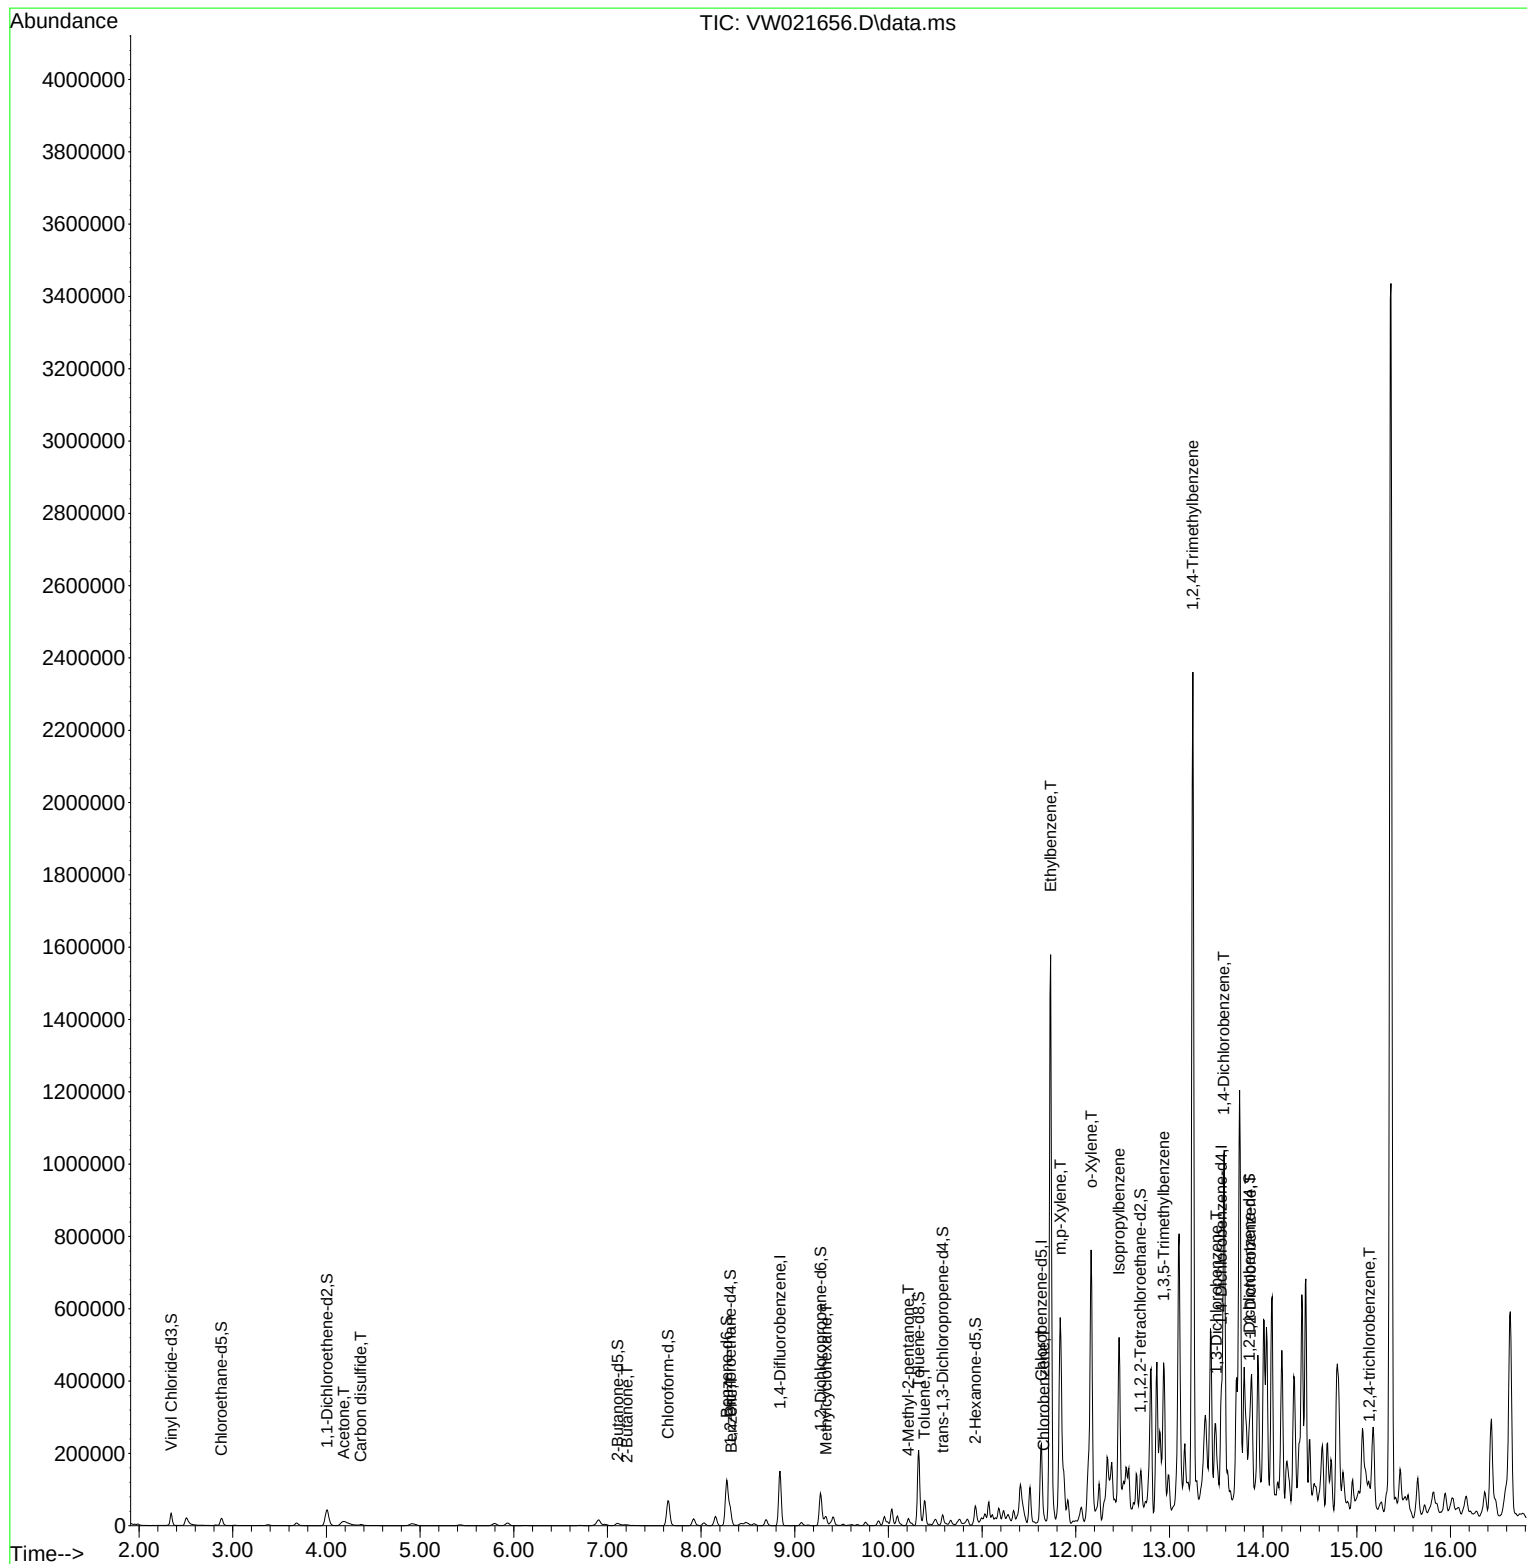




#13
Acetone
Concen: 148.278 ug/L
RT: 4.184 min Scan# 31
Delta R.T. 0.024 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22




Instrument :
MSVOA_W
ClientSampleId :
BGL90


Tgt Ion: 43 Resp: 43428
Ion Ratio Lower Upper
43 100
58 12.3 0.0 52.8

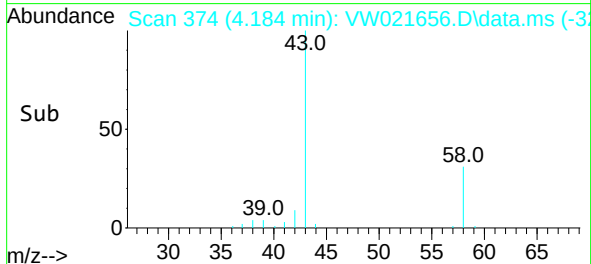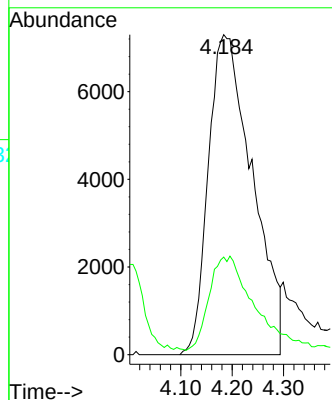

#14
Carbon disulfide
Concen: 1.160 ug/L
RT: 4.366 min Scan# 404
Delta R.T. -0.019 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22

Tgt Ion: 76 Resp: 4725
Ion Ratio Lower Upper
76 100
78 11.1 7.1 10.7#



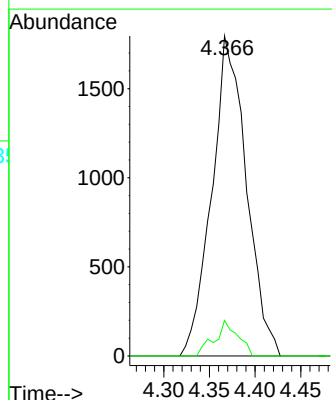
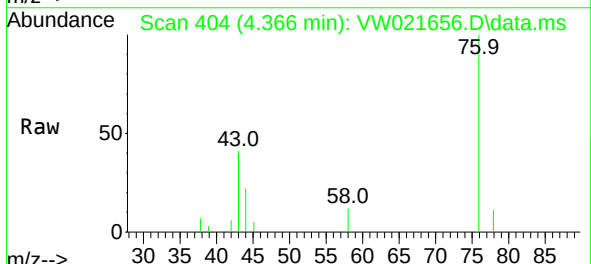


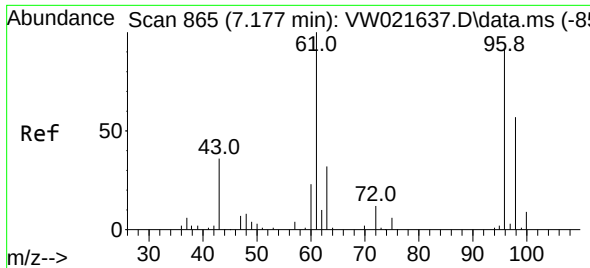

#22
2-Butanone
Concen: 8.999 ug/L
RT: 7.207 min Scan# 81
Delta R.T. 0.018 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22




Instrument :
MSVOA_W
ClientSampleId :
BGL90


Tgt Ion: 43 Resp: 3442
Ion Ratio Lower Upper
43 100
72 40.6 11.8 35.4#

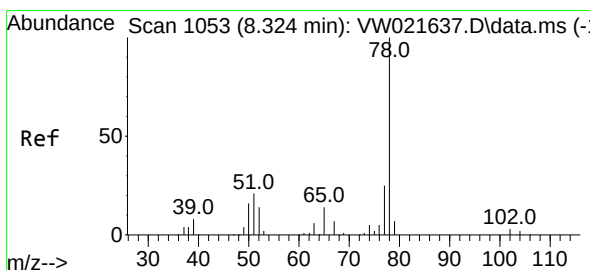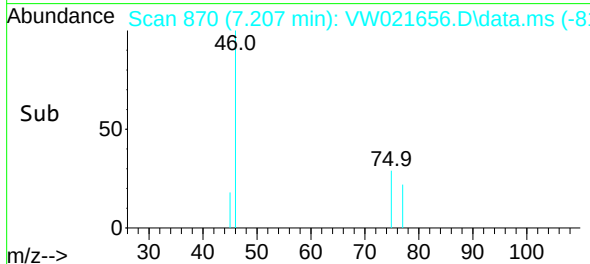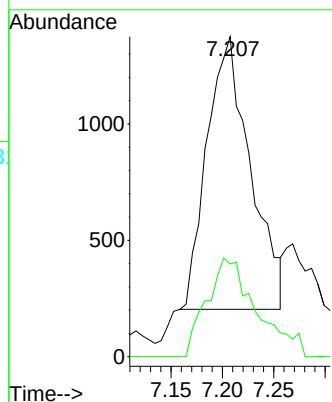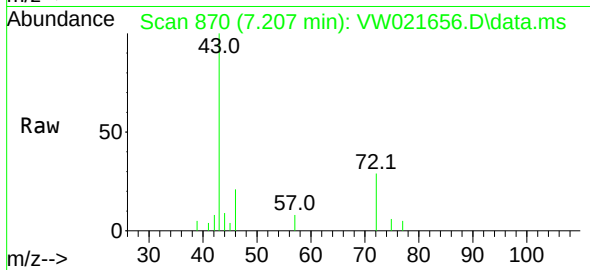

#33
Benzene
Concen: 0.590 ug/L
RT: 8.323 min Scan# 1053
Delta R.T. -0.000 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22

Tgt Ion: 78 Resp: 3963

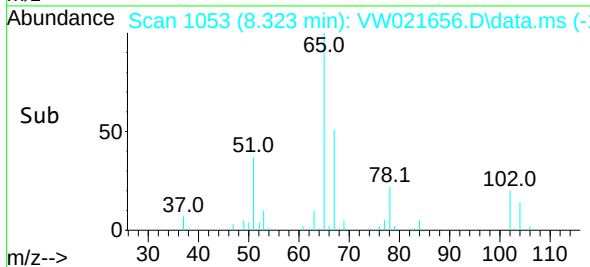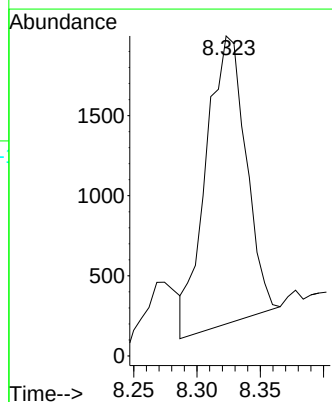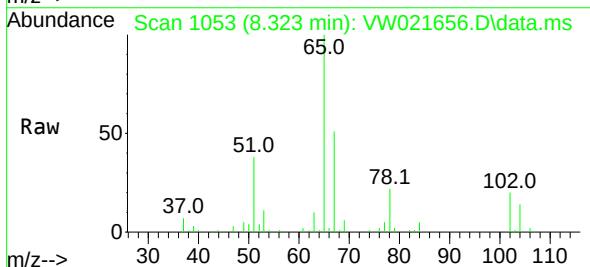



#35

Methylcyclohexane

Concen: 2.331 ug/L

RT: 9.335 min Scan# 1219

Delta R.T. -0.000 min

Lab File: VW021656.D

Acq: 25 Dec 2021 19:22

Instrument :

MSVOA_W

ClientSampleId :

BGL90





Tgt Ion: 83 Resp: 7253

Ion Ratio Lower Upper

83 100

55 126.1 70.8 106.2#

98 56.6 37.7 56.5#

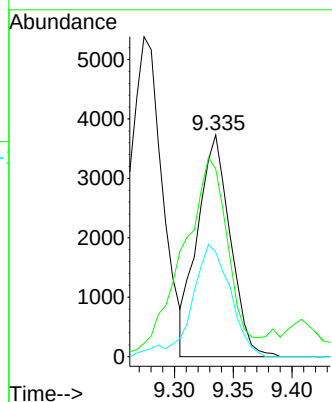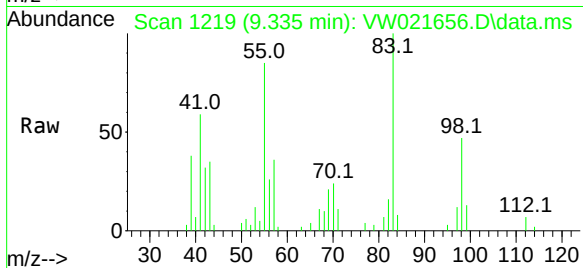

#40

4-Methyl-2-pentanone

Concen: 15.162 ug/L

RT: 10.213 min Scan# 1363

Delta R.T. -0.000 min

Lab File: VW021656.D

Acq: 25 Dec 2021 19:22




Tgt Ion: 43 Resp: 12383


Ion Ratio Lower Upper

43 100

58 39.4 28.8 43.2

100 18.4 10.0 15.0#


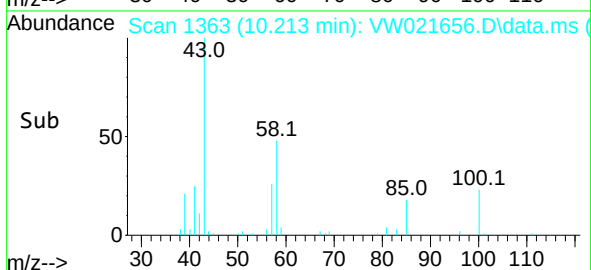
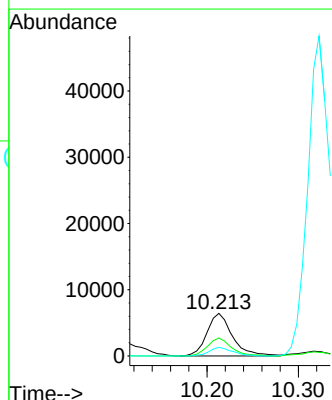
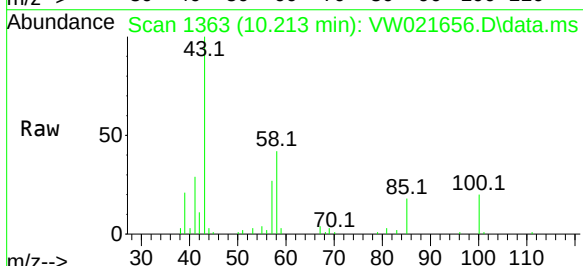




#42
Toluene
Concen: 6.343 ug/L
RT: 10.384 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22




Instrument :
MSVOA_W
ClientSampleId :
BGL90


Tgt Ion: 91 Resp: 49853
Ion Ratio Lower Upper
91 100
92 59.0 41.7 77.5

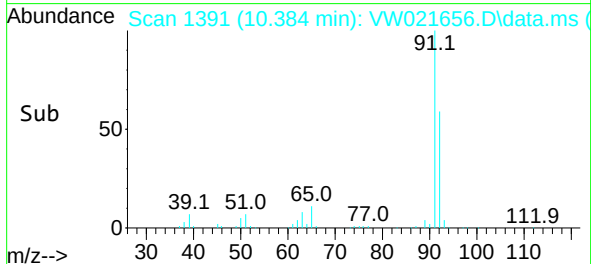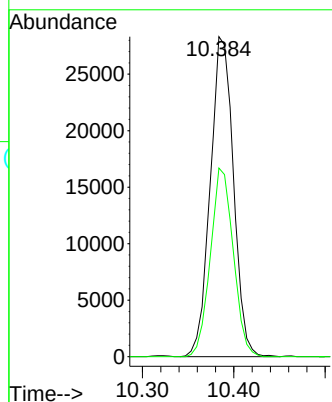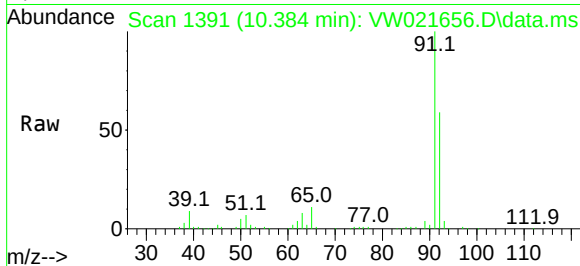

#51
Chlorobenzene
Concen: 1.432 ug/L
RT: 11.658 min Scan# 1600
Delta R.T. -0.000 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22

Tgt Ion: 112 Resp: 7534
Ion Ratio Lower Upper
112 100
114 33.7 22.4 41.6
77 52.5 50.2 75.4


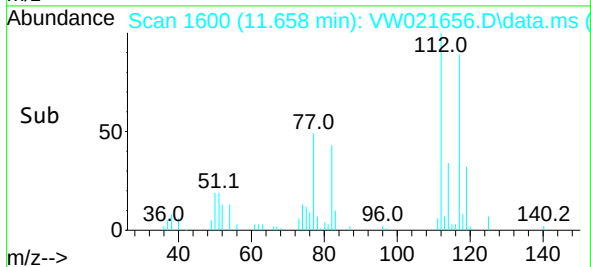
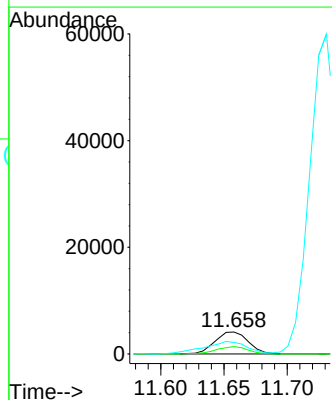
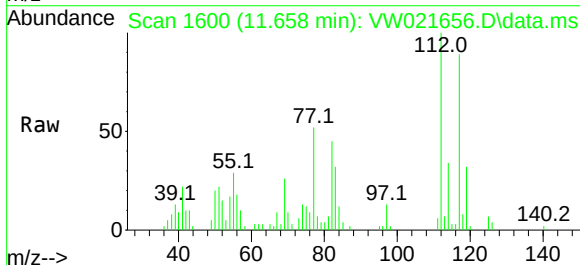




#52
Ethylbenzene
Concen: 121.197 ug/L
RT: 11.731 min Scan# 1612
Delta R.T. -0.000 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22




Instrument :
MSVOA_W
ClientSampleId :
BGL90


Tgt Ion: 91 Resp: 1088470
Ion Ratio Lower Upper
91 100
106 33.2 21.5 39.9

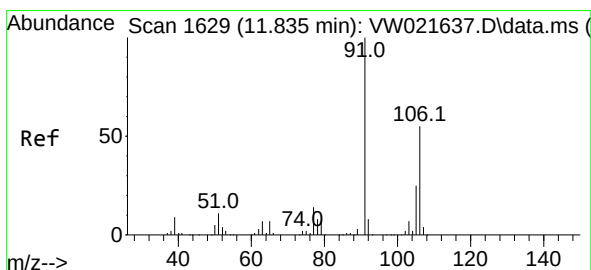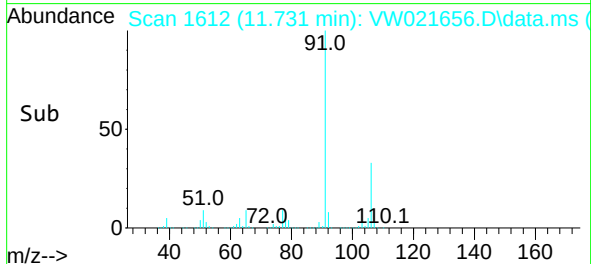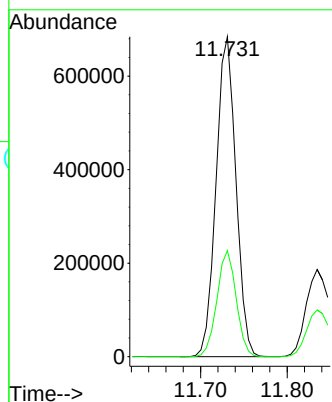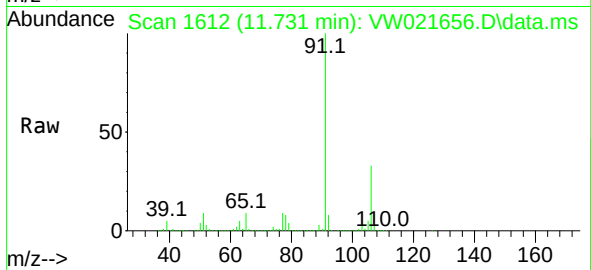

#53
m,p-Xylene
Concen: 51.023 ug/L
RT: 11.835 min Scan# 1629
Delta R.T. -0.000 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22

Tgt Ion:106 Resp: 184856
Ion Ratio Lower Upper
106 100
91 186.7 149.9 278.3

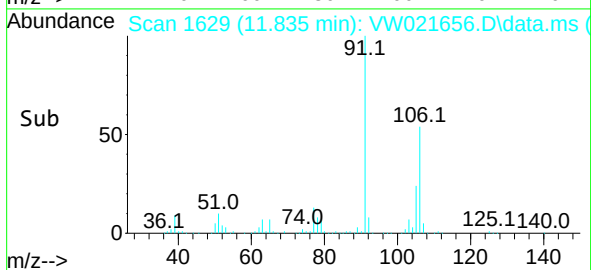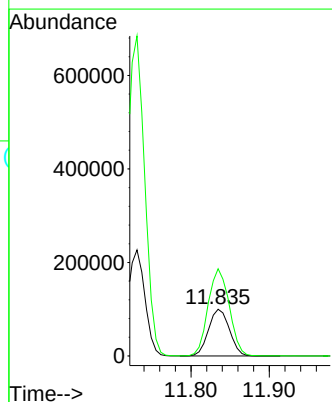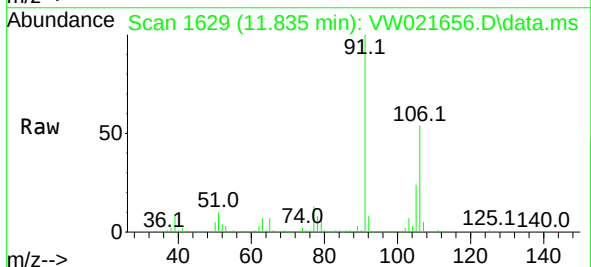



#54

o-Xylene

Concen: 57.088 ug/L

RT: 12.164 min Scan# 1

Delta R.T. -0.000 min

Lab File: VW021656.D

Acq: 25 Dec 2021 19:22

Instrument :

MSVOA_W

ClientSampleId :





BGL90

Tgt Ion:106 Resp: 196291

Ion Ratio Lower Upper

106 100

91 204.3 153.6 285.3

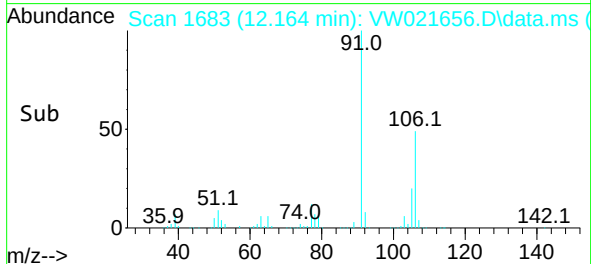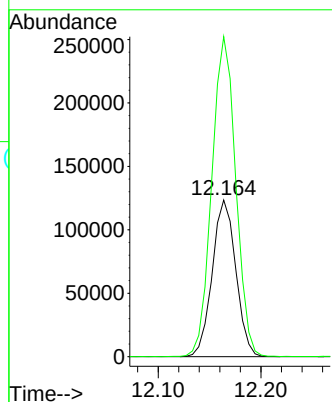

#60

Isopropylbenzene

Concen: 28.579 ug/L

RT: 12.463 min Scan# 1732

Delta R.T. -0.000 min

Lab File: VW021656.D

Acq: 25 Dec 2021 19:22




Tgt Ion:105 Resp: 304547


Ion Ratio Lower Upper

105 100

120 26.7 20.1 30.1

77 15.3 13.8 20.8

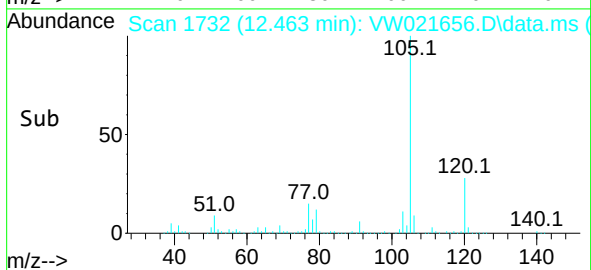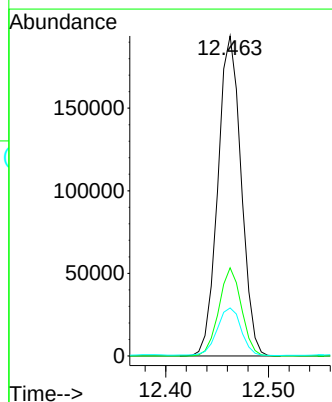



#62

1,3,5-Trimethylbenzene

Concen: 13.395 ug/L

RT: 12.938 min Scan# 1810

Delta R.T. -0.000 min

Lab File: VW021656.D

Acq: 25 Dec 2021 19:22

Instrument :

MSVOA_W

ClientSampleId :





BGL90

Tgt Ion:105 Resp: 121462

Ion Ratio Lower Upper

105 100

120 49.9 37.4 56.2

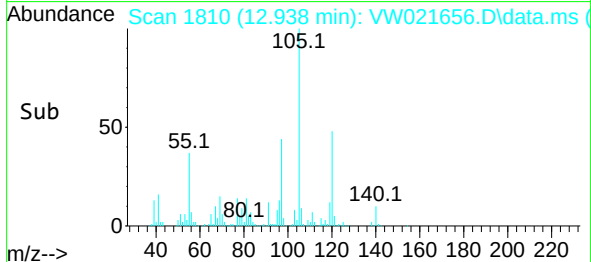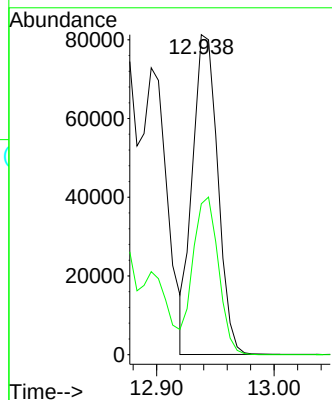

#63

1,2,4-Trimethylbenzene

Concen: 143.727 ug/L

RT: 13.249 min Scan# 1861

Delta R.T. -0.000 min

Lab File: VW021656.D




Acq: 25 Dec 2021 19:22


Tgt Ion:105 Resp: 1285660

Ion Ratio Lower Upper

105 100

120 47.2 35.0 52.6


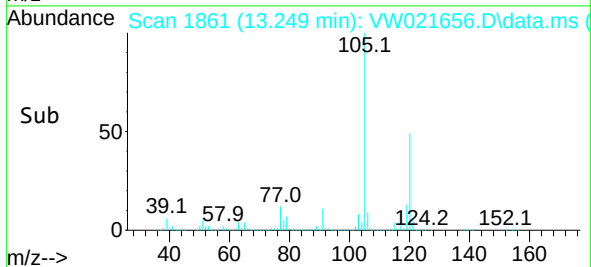
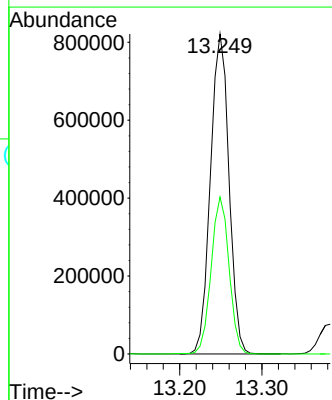
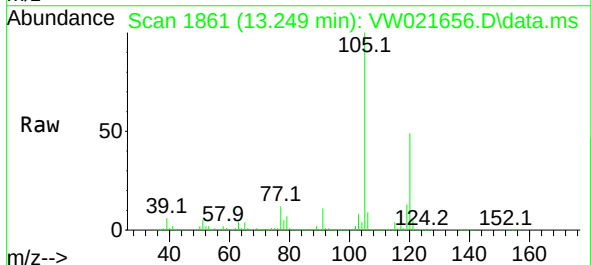




#64
1,3-Dichlorobenzene
Concen: 1.537 ug/L
RT: 13.499 min Scan# 1902
Delta R.T. -0.000 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22




Instrument :
MSVOA_W
ClientSampleId :
BGL90


Tgt Ion:146 Resp: 7725
Ion Ratio Lower Upper
146 100
111 78.4 29.8 55.3#
148 68.2 46.2 85.8

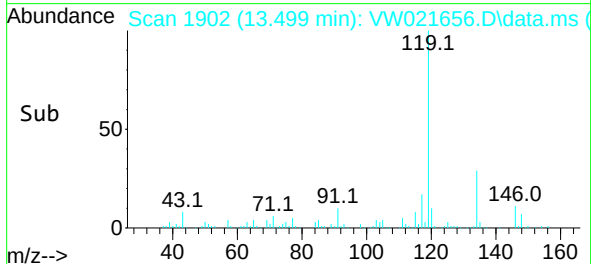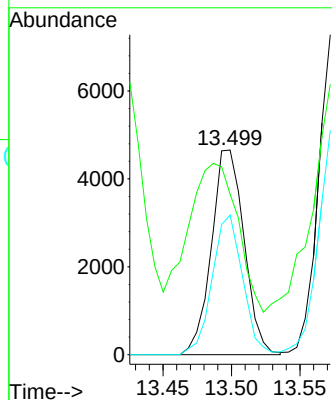

#65
1,4-Dichlorobenzene
Concen: 2.690 ug/L
RT: 13.578 min Scan# 1915
Delta R.T. -0.000 min
Lab File: VW021656.D
Acq: 25 Dec 2021 19:22

Tgt Ion:146 Resp: 13434
Ion Ratio Lower Upper
146 100
111 78.0 29.0 53.9#
148 66.3 46.9 87.1

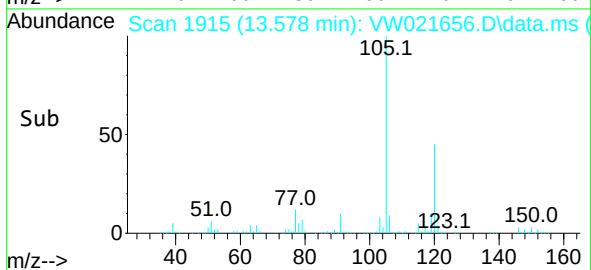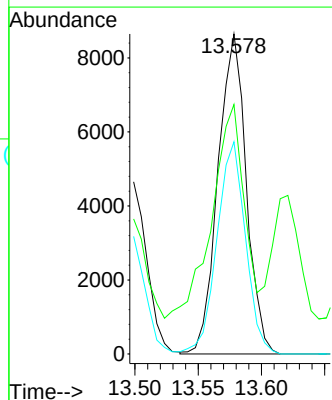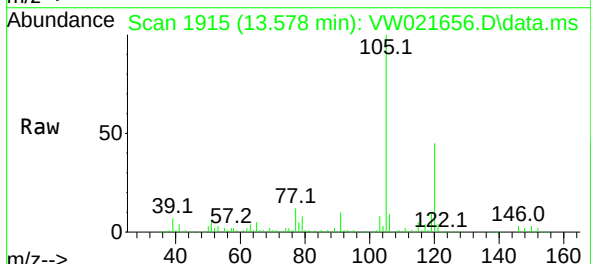



#67

1,2-Dichlorobenzene

Concen: 3.502 ug/L

RT: 13.865 min Scan# 1962

Delta R.T. -0.000 min

Lab File: VW021656.D

Acq: 25 Dec 2021 19:22

Instrument :

MSVOA_W

ClientSampleId :

BGL90





Tgt Ion:146 Resp: 15498

Ion Ratio Lower Upper

146 100

111 60.3 33.1 49.7#

148 66.0 47.4 71.2

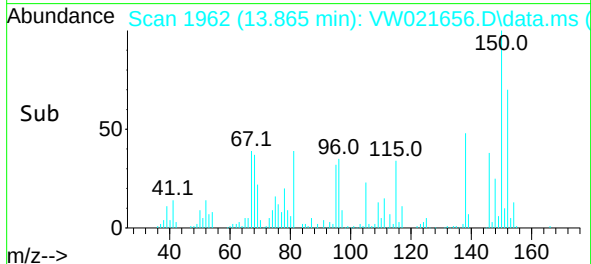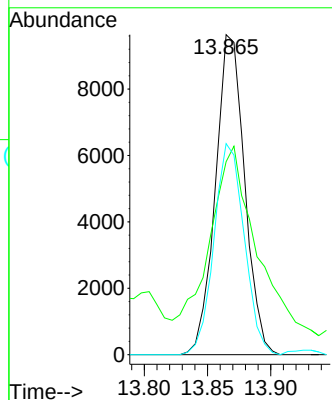

#70

1,2,4-trichlorobenzene

Concen: 5.997 ug/L

RT: 15.133 min Scan# 2170

Delta R.T. 0.006 min

Lab File: VW021656.D

Acq: 25 Dec 2021 19:22

Tgt Ion:180 Resp: 18121

Ion Ratio Lower Upper

180 100

182 96.2 79.0 118.6

145 126.1 26.0 39.0#

