


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122521\
 Data File : VW021636.D
 Acq On : 25 Dec 2021 09:14
 Operator : SY/VA
 Sample : BFB488
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB488

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Title : SFAM01.0
 Last Update : Tue Dec 28 00:40:13 2021

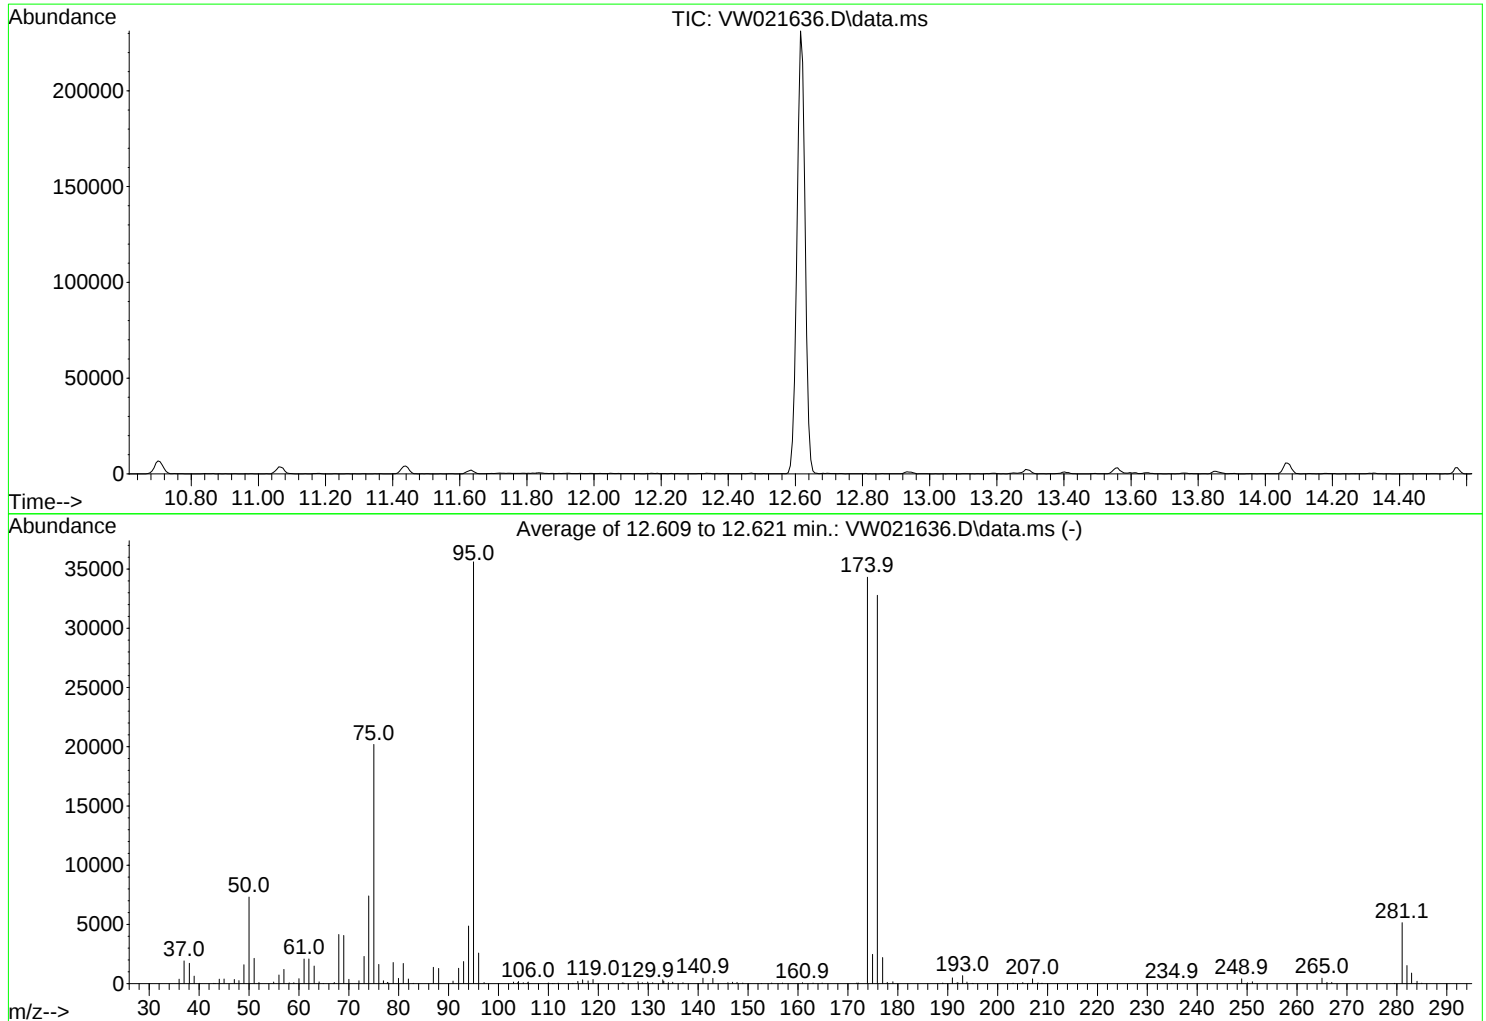

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	7314	PASS
75	95	30	80	56.7	20189	PASS
95	95	100	100	100.0	35608	PASS
96	95	5	9	7.2	2574	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.4	34309	PASS
175	174	5	9	7.2	2478	PASS
176	174	95	105	95.6	32784	PASS
177	176	5	10	6.7	2204	PASS

m/z	Abundance
36.00	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB488

m/z	Abundance
36.00	435.0
37.00	1631.0
38.00	1455.0
39.00	608.0
40.10	78.0
42.90	53.0
44.10	319.0
45.00	358.0
47.00	324.0
48.10	251.0
49.00	1370.0
50.00	6540.0
51.10	1863.0
52.00	107.0
54.90	107.0
56.00	774.0
57.00	1042.0
58.00	109.0
59.00	138.0
60.00	414.0
61.00	1846.0
62.00	1862.0
63.00	1270.0
64.10	126.0
66.90	99.0
68.00	3487.0
69.00	3455.0
70.00	317.0
72.10	201.0
73.10	2374.0
74.00	6596.0
75.00	17320.0
76.00	1491.0
77.00	173.0
77.70	89.0
78.90	1584.0
79.90	349.0
80.90	1528.0
81.90	368.0
82.90	65.0
87.00	1246.0
88.00	1209.0
91.00	198.0
92.00	1128.0
93.00	1630.0
94.00	4056.0
95.00	28704.0
96.00	2317.0
97.10	106.0
103.00	192.0
103.80	191.0
105.00	77.0
105.80	204.0
109.90	78.0
111.10	51.0
115.90	164.0
116.90	281.0
118.00	229.0
118.90	371.0
124.80	222.0
127.90	168.0
128.90	86.0
129.90	118.0
130.90	59.0
132.90	735.0
134.00	140.0
135.00	140.0
137.00	63.0
140.90	343.0
142.90	395.0
146.00	64.0
147.00	146.0
147.80	110.0
148.90	75.0
154.70	63.0
161.00	103.0
163.00	108.0
164.80	88.0
171.80	151.0
173.90	26904.0
175.00	2153.0
175.90	25656.0
177.00	1817.0
178.00	121.0
179.00	248.0
189.00	91.0
190.90	686.0
191.90	255.0
193.00	901.0
193.90	194.0
194.90	85.0
203.20	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB488

205.10	146.0
206.10	76.0
207.00	584.0
208.10	130.0
208.90	57.0
248.90	543.0
250.10	98.0
251.10	167.0
265.00	615.0
266.00	167.0
267.00	134.0
279.50	72.0
281.00	6125.0
282.00	2182.0
283.00	1148.0
284.10	264.0
285.00	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB488

m/z	Abundance
36.00	495.0
37.00	2250.0
38.10	2115.0
39.00	726.0
43.20	57.0
44.00	434.0
45.00	484.0
47.10	352.0
47.90	295.0
49.00	1879.0
50.00	8034.0
51.00	2367.0
52.00	112.0
55.00	154.0
56.00	747.0
57.00	1330.0
58.10	87.0
59.00	97.0
60.00	406.0
61.00	2341.0
62.00	2318.0
63.10	1729.0
64.00	170.0
67.10	193.0
68.00	4771.0
69.00	4598.0
70.00	403.0
72.00	291.0
73.00	2453.0
74.00	7908.0
75.00	22248.0
76.00	1776.0
77.00	330.0
77.80	250.0
78.90	1901.0
80.00	510.0
80.90	1881.0
82.00	418.0
86.90	1415.0
88.00	1437.0
90.90	232.0
92.00	1385.0
93.00	2103.0
94.00	5633.0
95.00	39512.0
96.00	2683.0
97.10	82.0
103.00	109.0
104.00	306.0
104.90	110.0
106.00	214.0
110.10	95.0
110.80	50.0
112.00	63.0
115.90	222.0
116.80	379.0
117.90	267.0
119.00	382.0
125.00	154.0
128.00	155.0
128.80	99.0
129.90	144.0
130.90	111.0
133.10	624.0
134.10	110.0
134.80	146.0
137.00	118.0
141.00	480.0
143.00	461.0
146.00	101.0
146.90	99.0
147.80	114.0
149.00	78.0
150.10	57.0
152.70	61.0
156.90	70.0
160.90	79.0
163.00	71.0
164.90	76.0
172.10	158.0
173.90	37488.0
175.00	2476.0
175.90	35872.0
176.90	2178.0
177.90	113.0
179.00	138.0
189.00	66.0
191.00	516.0
192.10	137.0
193.00	831.0
193.90	88.0
203.00	83.0

Instrument :
MSVOA_W
ClientSampleId :
BFB488

205.00	130.0
207.00	460.0
208.10	69.0
208.90	61.0
234.90	85.0
248.90	423.0
250.00	99.0
251.00	239.0
265.00	517.0
266.00	100.0
266.90	109.0
281.10	7076.0
282.00	1595.0
282.90	796.0
284.00	253.0
285.00	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB488

m/z	Abundance
36.00	411.0
37.00	1868.0
38.00	1598.0
39.00	577.0
43.00	52.0
44.00	397.0
45.00	317.0
47.00	372.0
48.00	243.0
49.00	1543.0
50.00	7368.0
51.00	2167.0
52.00	70.0
55.00	130.0
56.00	677.0
57.00	1231.0
60.00	433.0
61.10	2069.0
62.00	2067.0
63.00	1444.0
64.00	153.0
64.90	62.0
67.10	100.0
68.00	4169.0
69.00	4164.0
70.00	390.0
72.00	244.0
73.00	2076.0
74.00	7708.0
75.00	21000.0
76.00	1584.0
76.90	213.0
78.00	150.0
78.90	1848.0
79.90	485.0
80.90	1706.0
81.90	387.0
87.00	1473.0
88.00	1190.0
90.80	215.0
92.00	1383.0
93.00	1850.0
94.00	4901.0
95.00	38608.0
96.00	2722.0
97.10	95.0
103.00	98.0
104.00	206.0
104.90	75.0
105.90	210.0
110.00	59.0
111.90	52.0
114.90	74.0
115.90	178.0
116.90	297.0
117.90	205.0
118.90	302.0
125.20	92.0
127.90	170.0
128.70	69.0
129.90	166.0
130.90	98.0
132.90	225.0
134.80	76.0
136.90	76.0
140.00	54.0
140.90	575.0
142.90	482.0
145.90	97.0
146.80	113.0
147.80	109.0
154.80	85.0
156.90	82.0
160.80	71.0
173.90	38536.0
174.90	2806.0
175.90	36824.0
176.90	2616.0
177.80	80.0
178.90	92.0
190.90	263.0
192.00	65.0
193.00	313.0
193.80	112.0
195.10	51.0
207.00	180.0
248.90	269.0
251.00	72.0
265.00	247.0
266.10	62.0
267.00	65.0
281.10	2255.0

Instrument :
MSVOA_W
ClientSampleId :
BFB488

282.00	823.0
283.00	716.0
284.00	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB488