


Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

MMDadoda
12/27/2018 4:48:34 PM

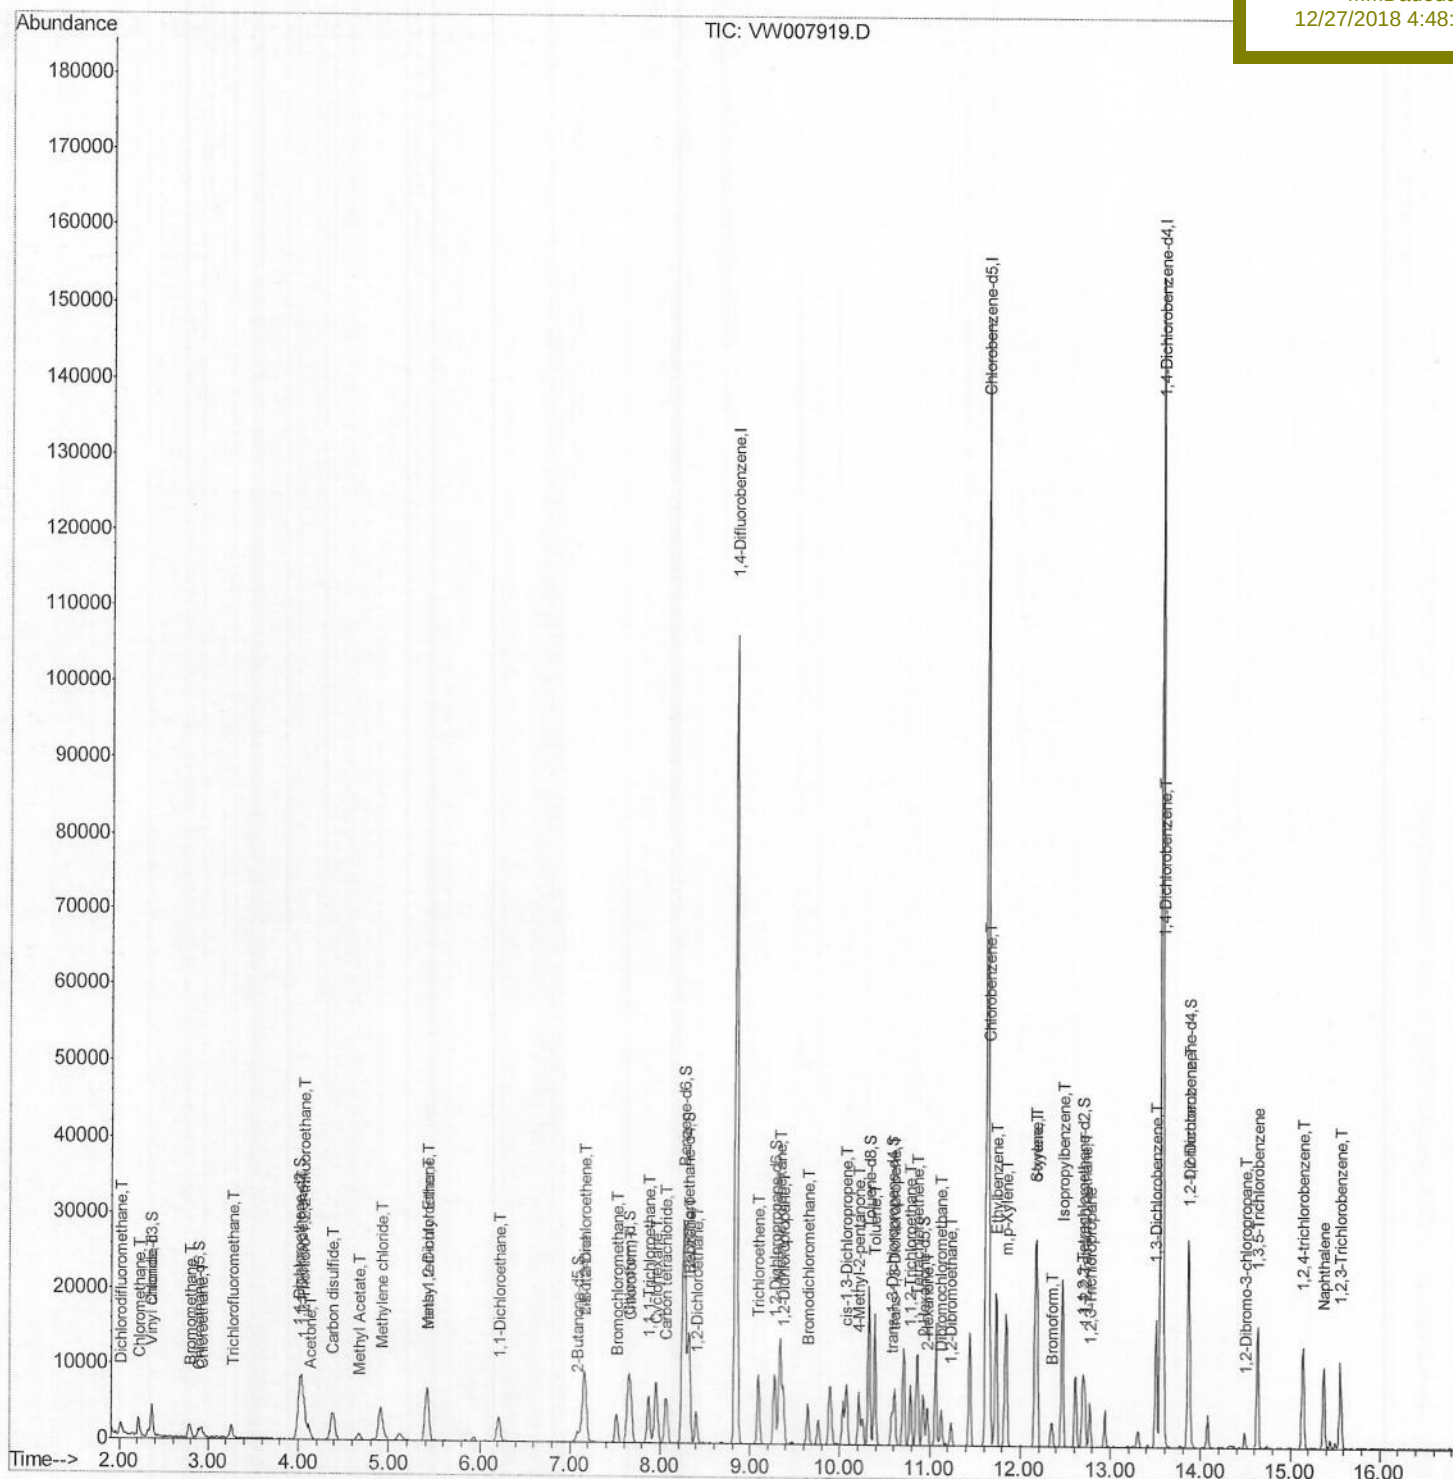

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

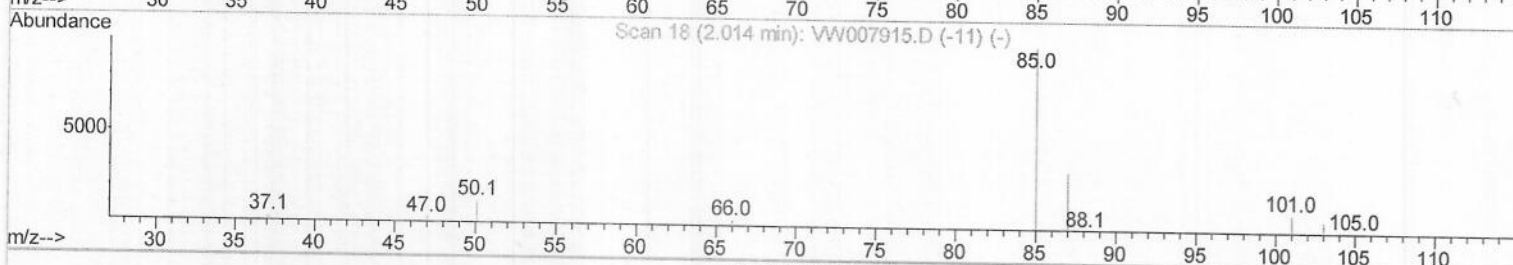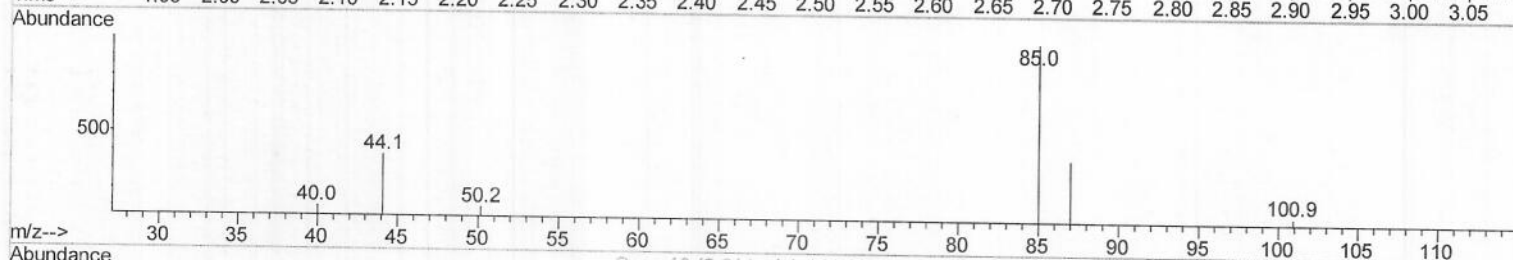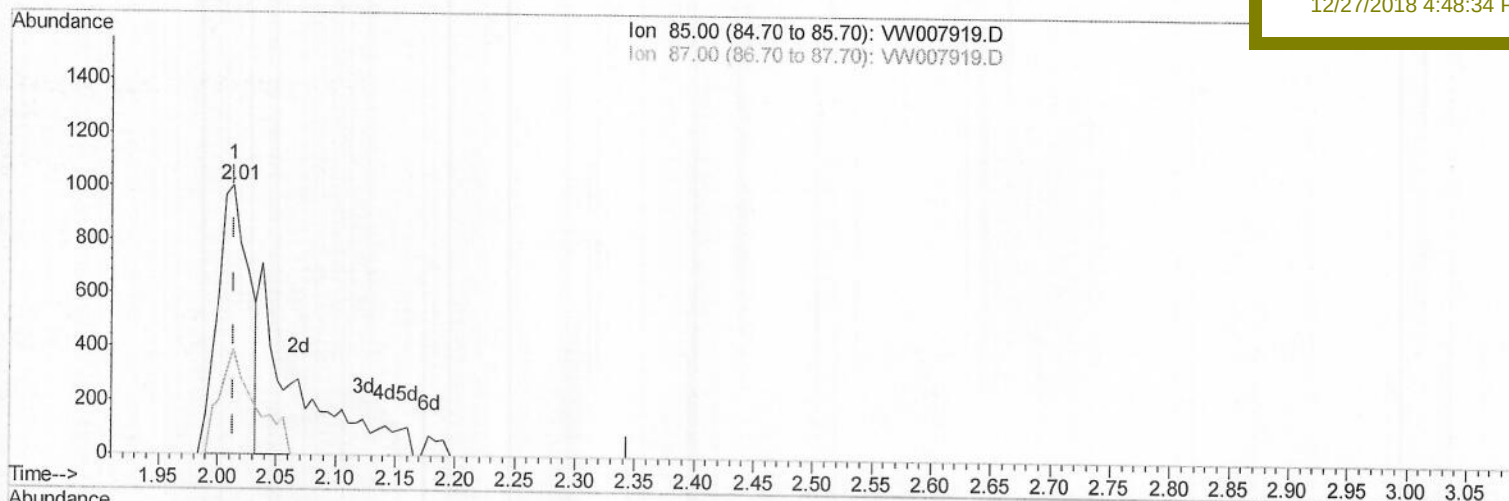

TIC: VW007919.D

(2) Dichlorodifluoromethane (T)

2.014min (-0.000) 1.93ug/L

response 1869

Ion	Exp%	Act%
85.00	100	100
87.00	29.50	41.79#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

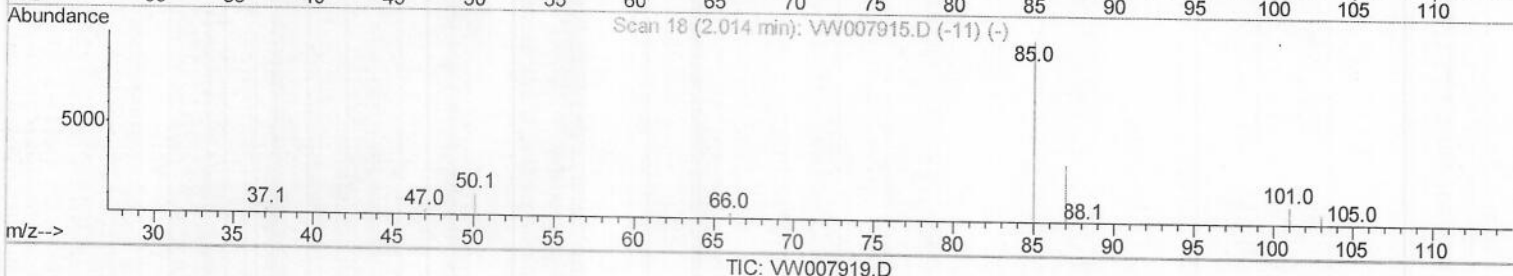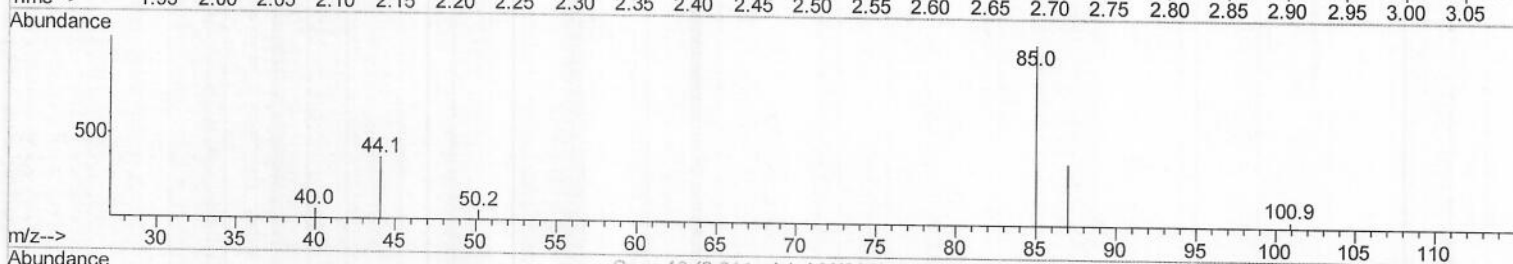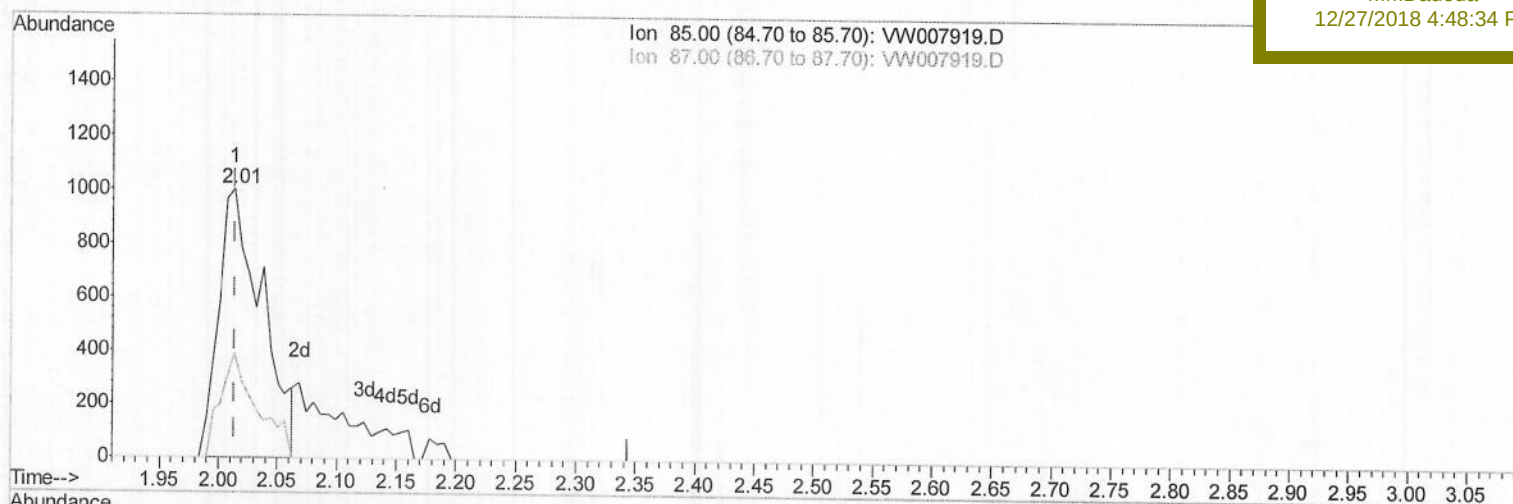

(2) Dichlorodifluoromethane (T)

2.014min (-0.000) 2.64ug/L m

response 2553

Ion	Exp%	Act%
85.00	100	100
87.00	29.50	30.59
0.00	0.00	0.00
0.00	0.00	0.00

SY
12/28/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

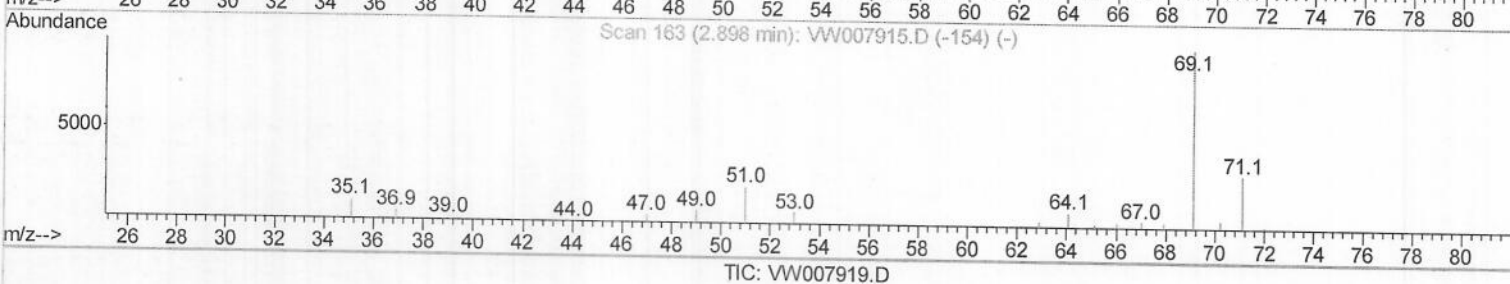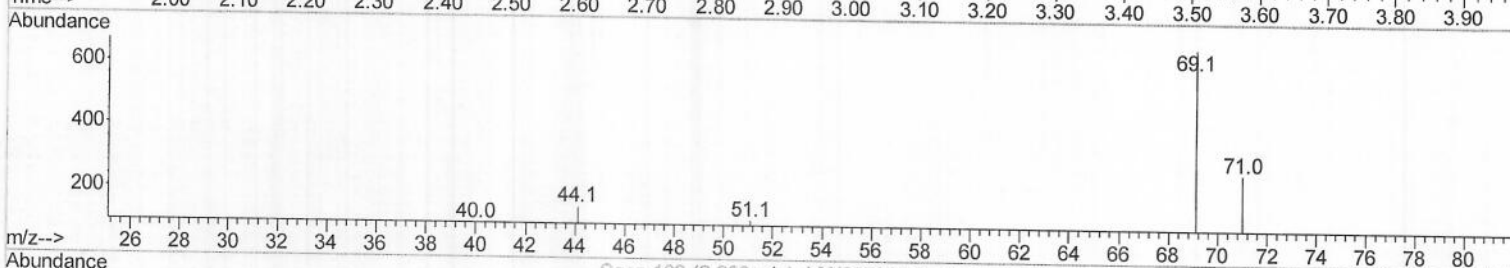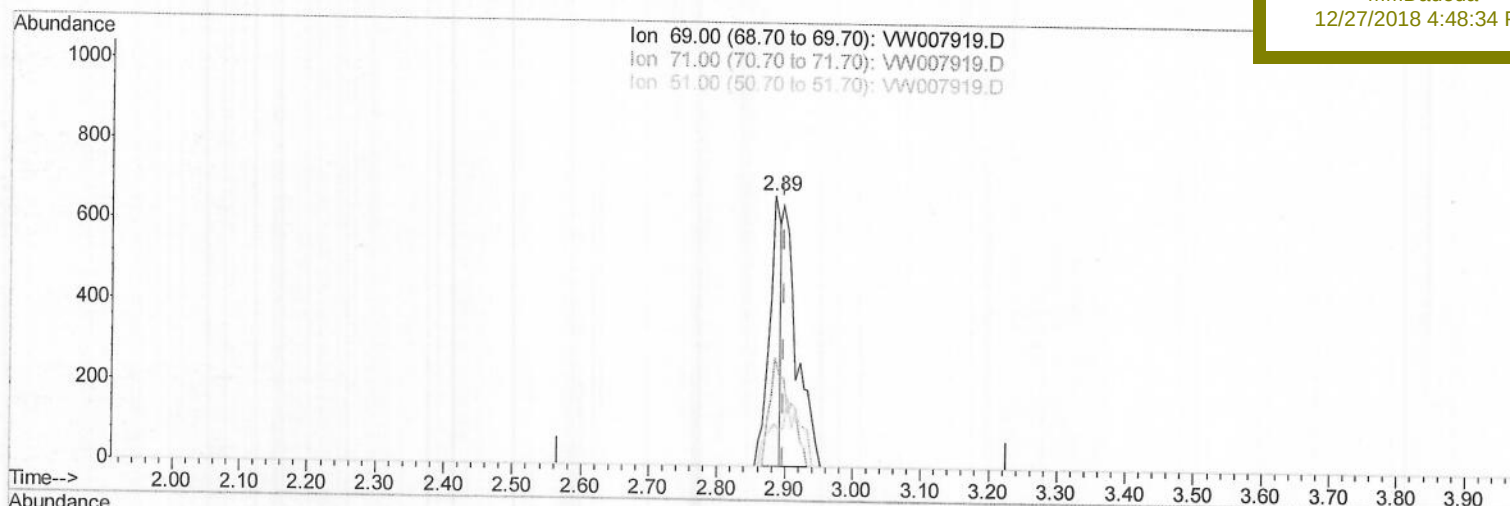

(7) Chloroethane-d5 (S)

2.885min (-0.012) 1.59ug/L

response 775

Ion	Exp%	Act%
69.00	100	100
71.00	32.40	53.55#
51.00	13.10	20.52#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

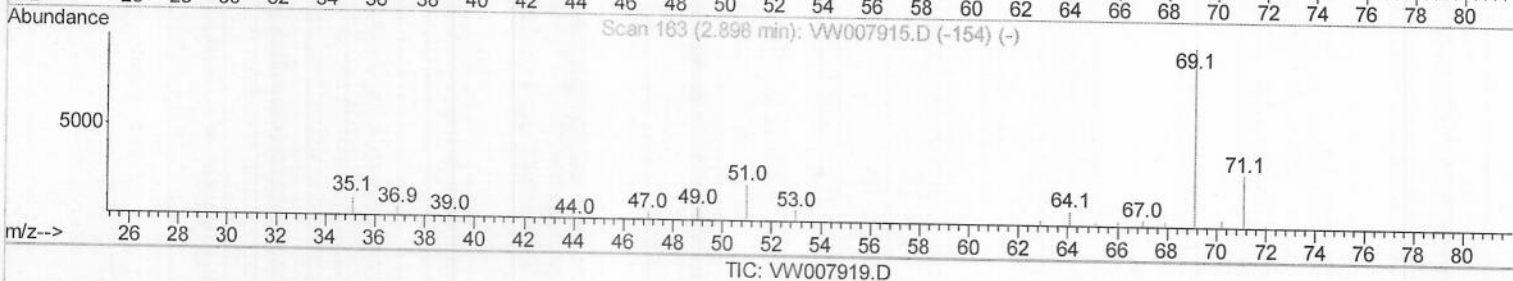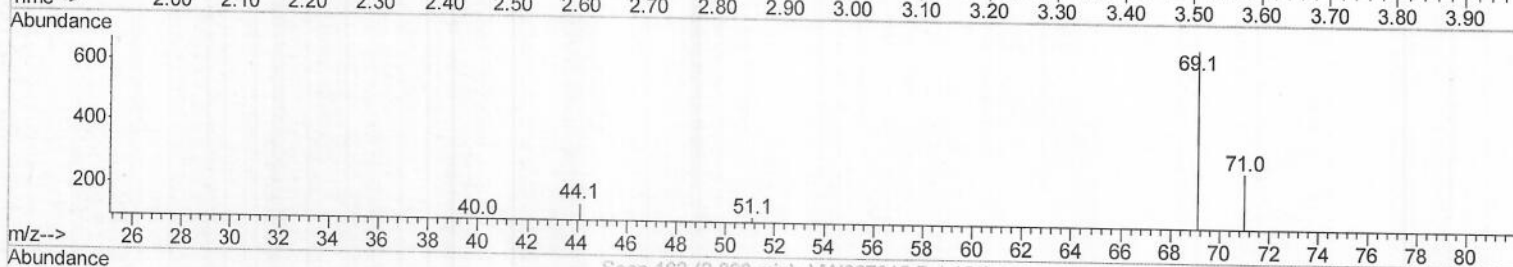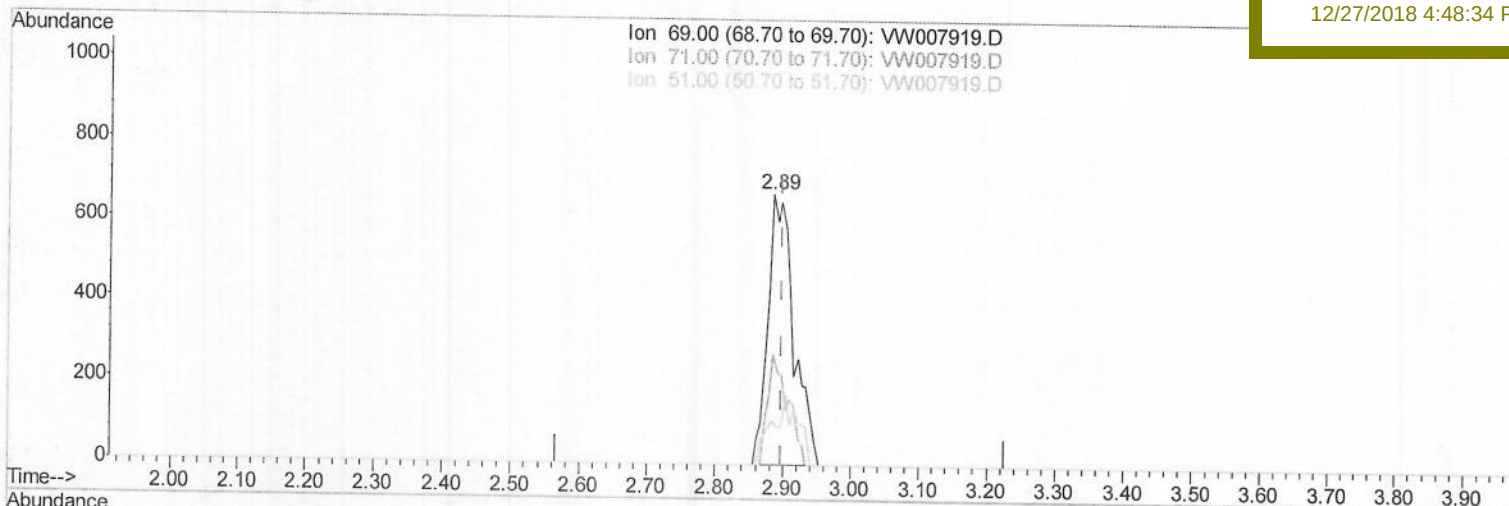

(7) Chloroethane-d5 (S)

2.885min (-0.012) 3.61ug/L m

response 1764

Ion	Exp%	Act%
69.00	100	100
71.00	32.40	23.53
51.00	13.10	9.01
0.00	0.00	0.00

SY
12/28/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

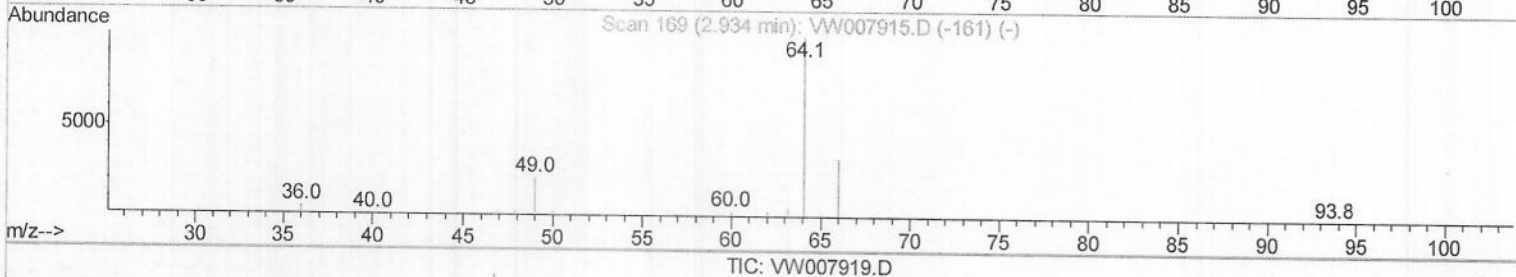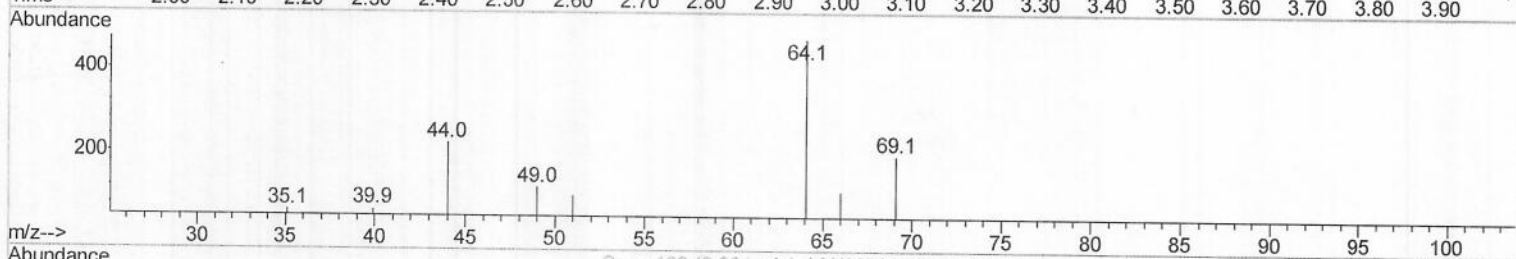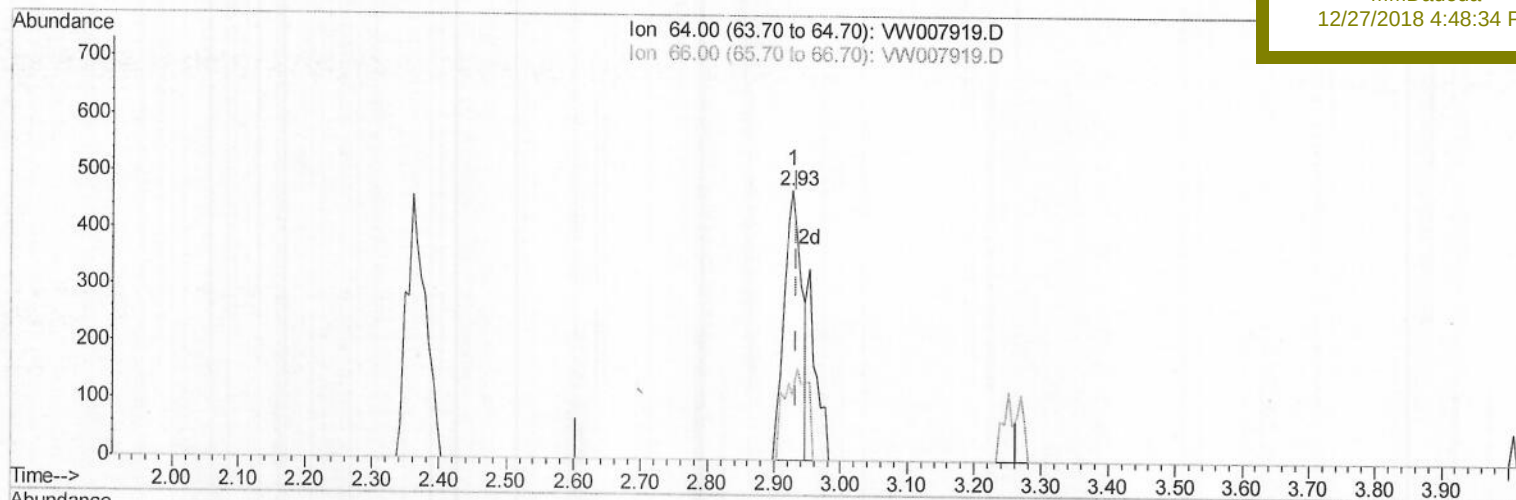

(8) Chloroethane (T)

2.928min (-0.006) 1.98ug/L

response 870

Ion	Exp%	Act%
64.00	100	100
66.00	33.30	23.78
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\

Quantitation Report (Qedit)

Data File : VW007919.D

Acq On : 26 Dec 2018 12:04

Operator : SY/AP

Sample : VSTD2.587

Misc : 5.00G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M

Quant Title : VOC Analysis

QLast Update : Wed Dec 26 10:32:54 2018

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :




VSTD2.587

Manual Integrations

APPROVED

MMDadoda

12/27/2018 4:48:34 PM

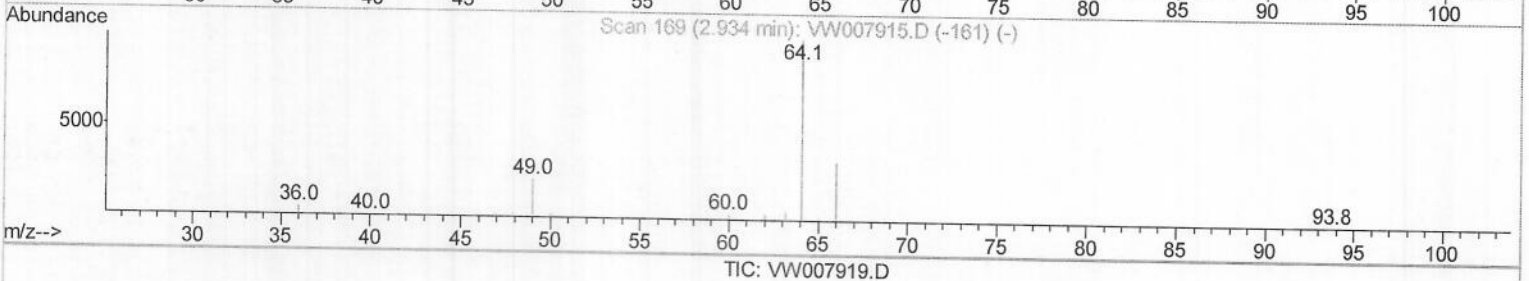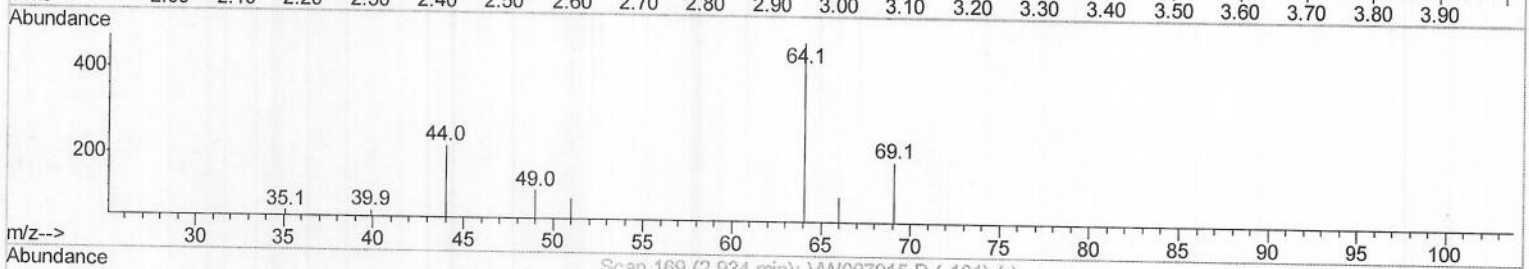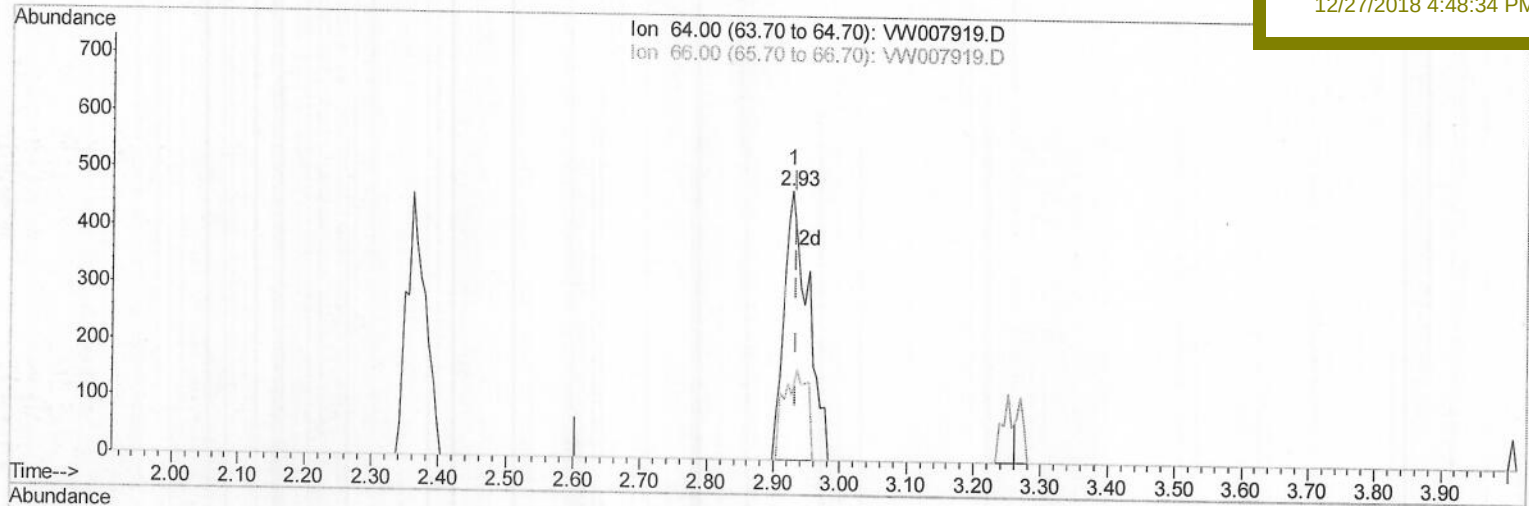

(8) Chloroethane (T)

2.928min (-0.006) 2.66ug/L m

response 1170

Ion	Exp%	Act%
64.00	100	100
66.00	33.30	23.78
0.00	0.00	0.00
0.00	0.00	0.00

SY
12/28/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
VSTD2.587

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

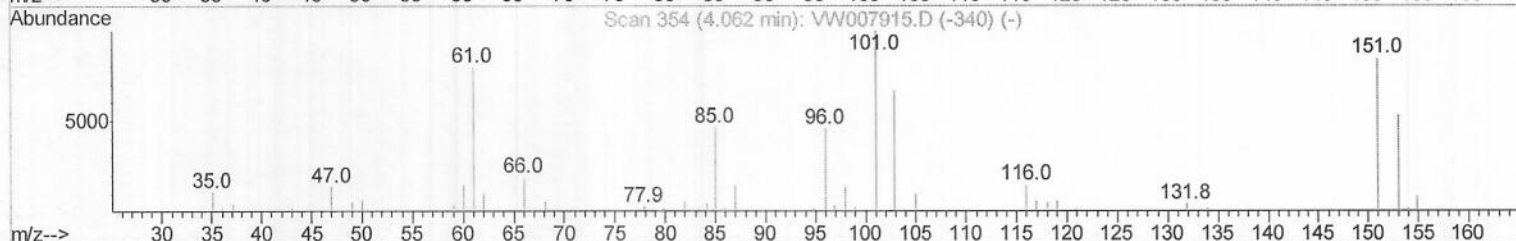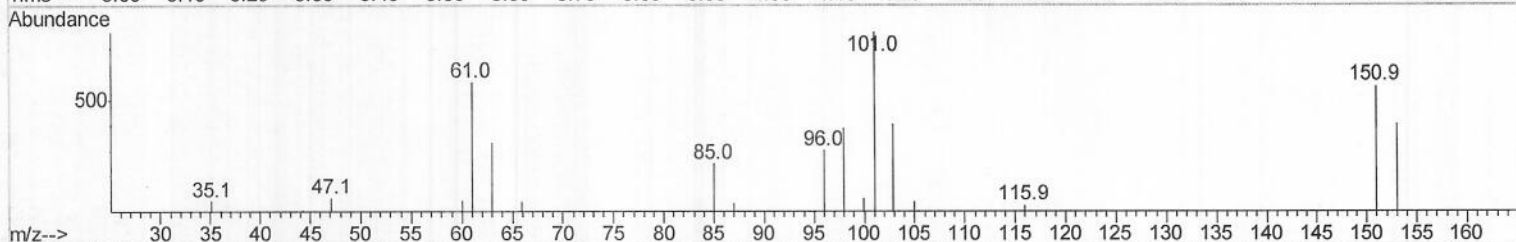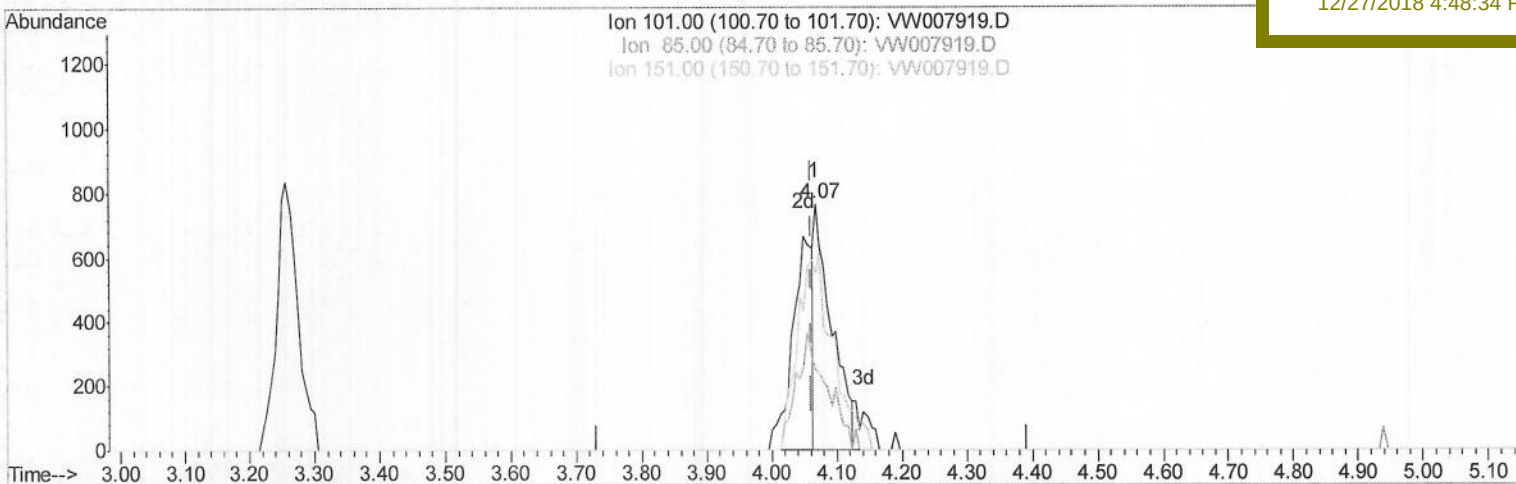

TIC: VW007919.D

(11) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.068min (+0.006) 1.31ug/L

response 1459

Ion	Exp%	Act%
101.00	100	100
85.00	41.80	0.00#
151.00	79.00	85.26
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)


Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

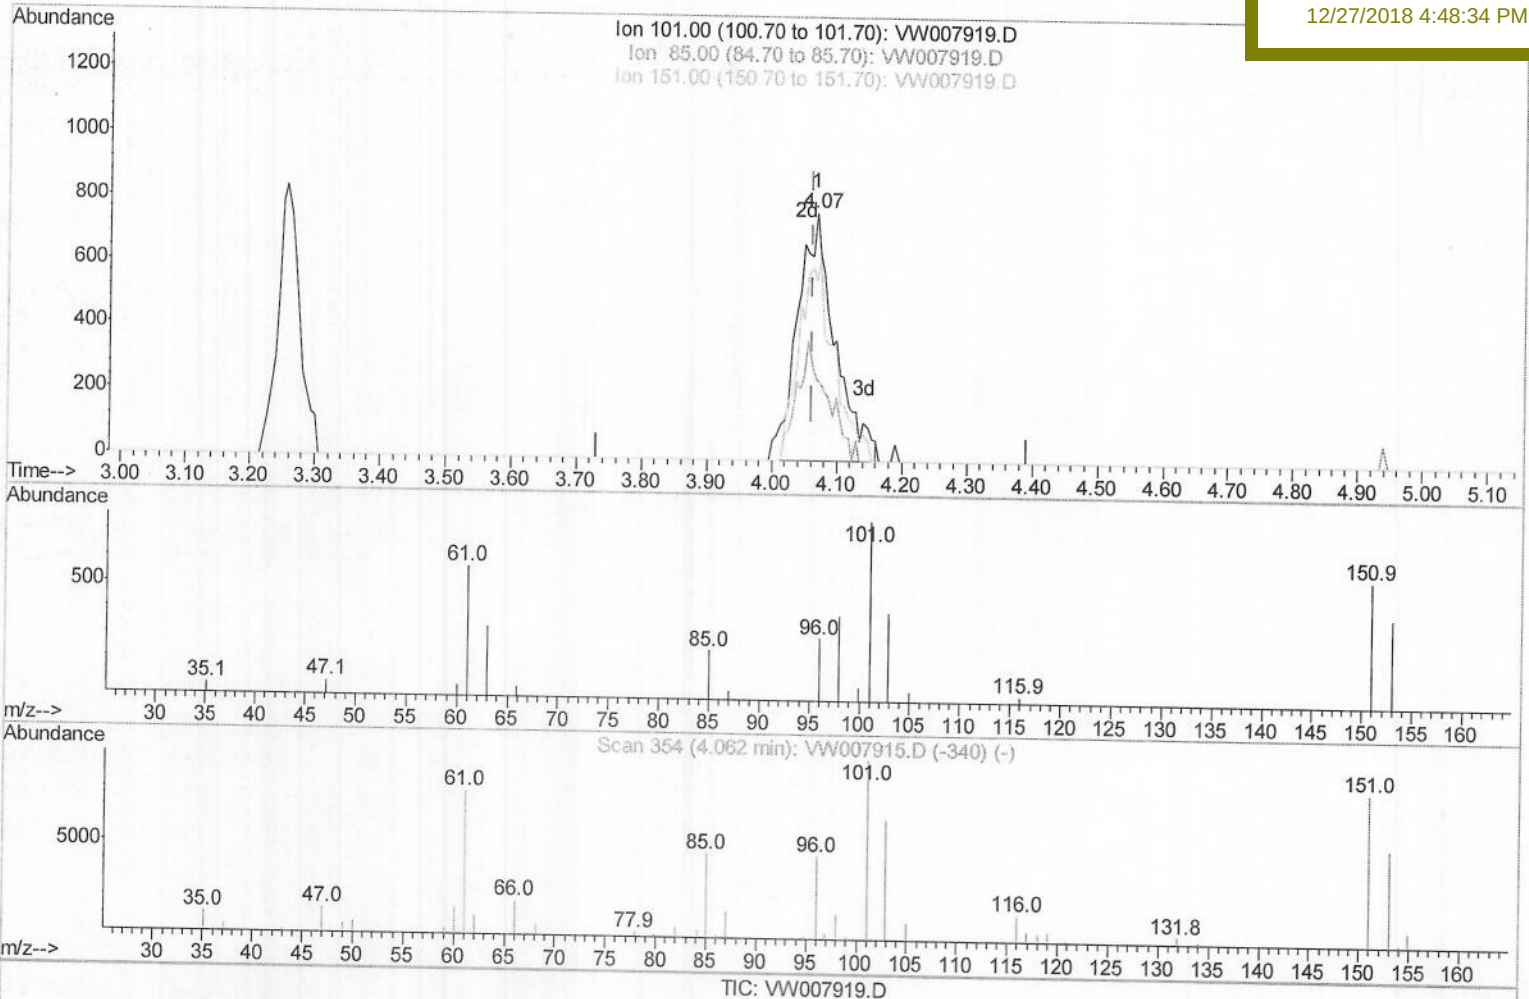

(11) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.068min (+0.006) 2.74ug/L m

response 3061

Ion	Exp%	Act%
101.00	100	100
85.00	41.80	0.00#
151.00	79.00	40.64#
0.00	0.00	0.00

SY
12/28/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

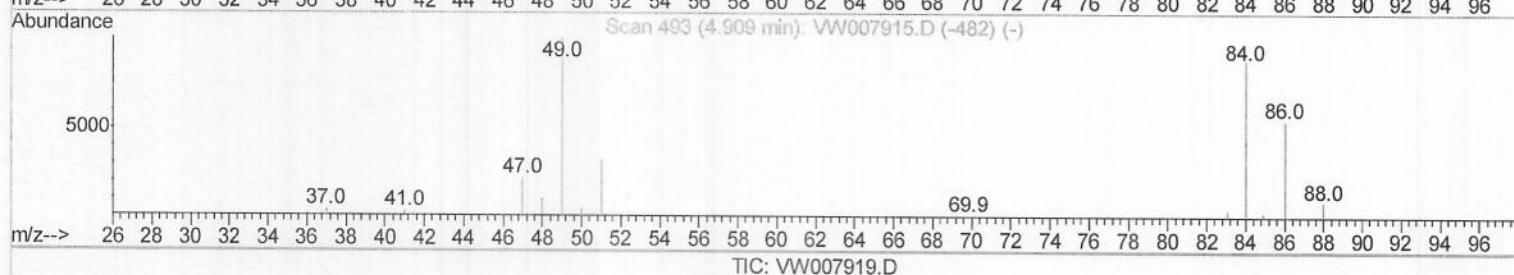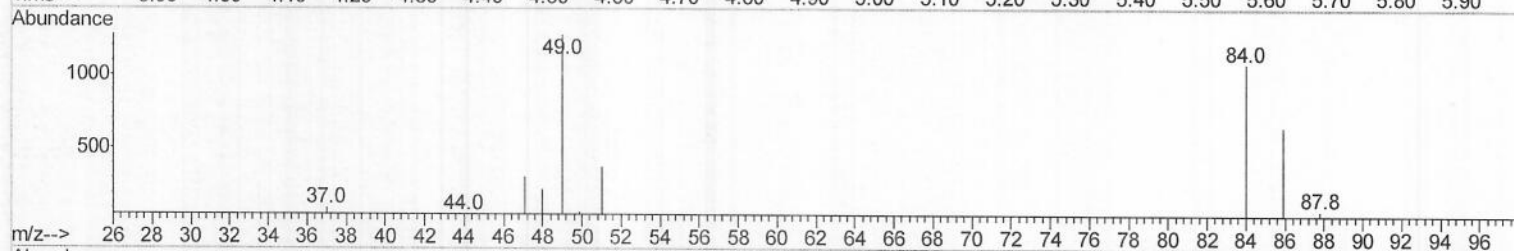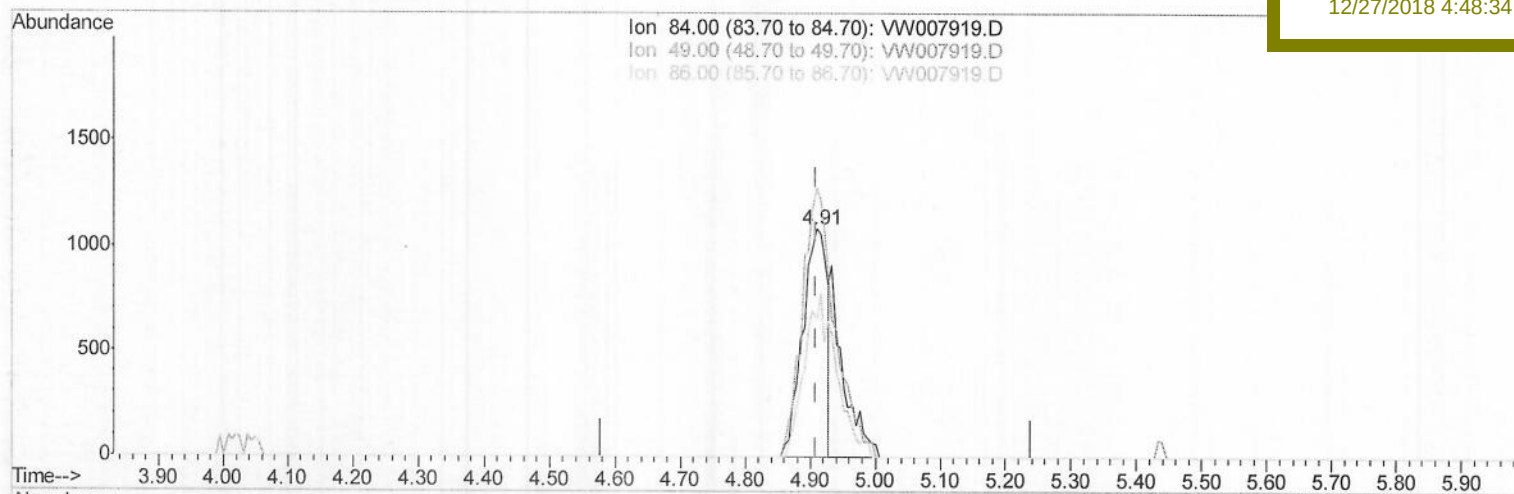

(16) Methylene chloride (T)

4.909min (-0.000) 1.97ug/L

response 2824

Ion	Exp%	Act%
84.00	100	100
49.00	113.10	117.91
86.00	61.70	60.20
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

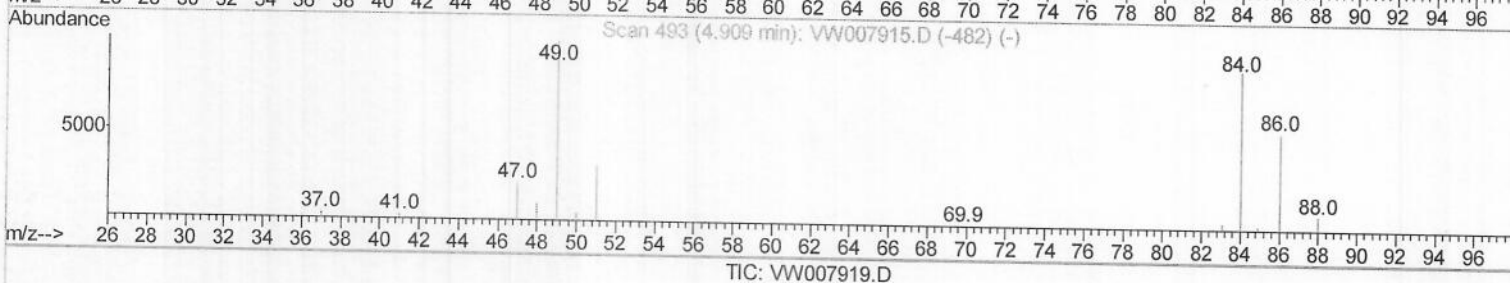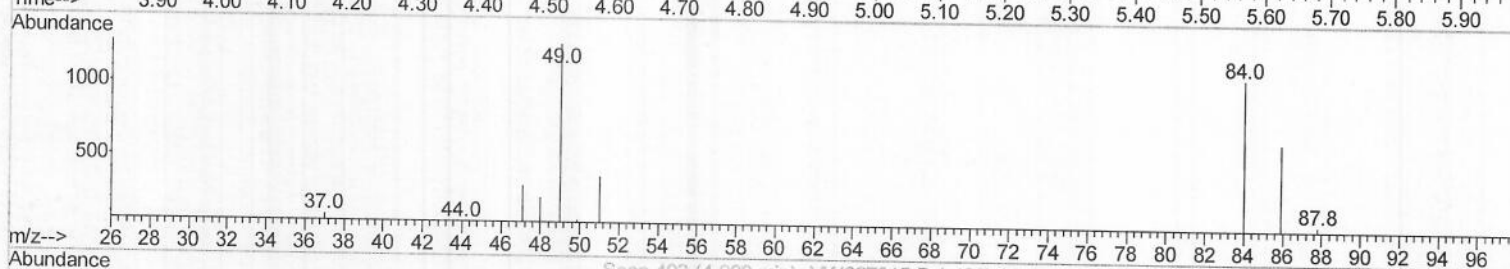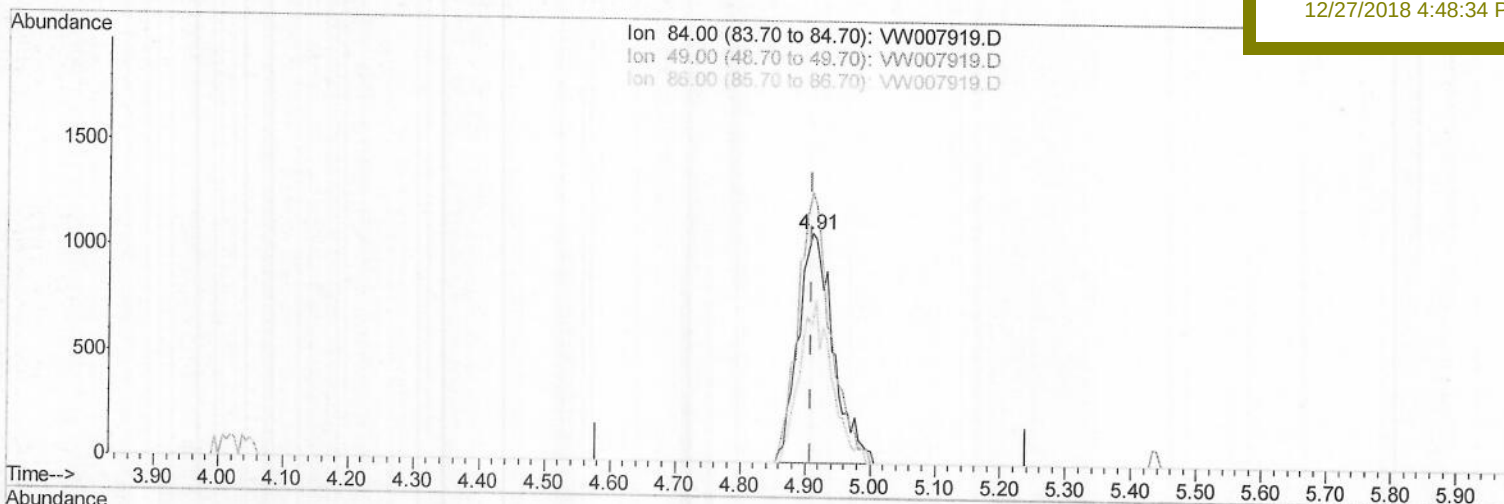

(16) Methylene chloride (T)

4.909min (-0.000) 2.85ug/L m

response 4073

Ion	Exp%	Act%
84.00	100	100
49.00	113.10	117.91
86.00	61.70	60.20
0.00	0.00	0.00

SY
12/28/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)


Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

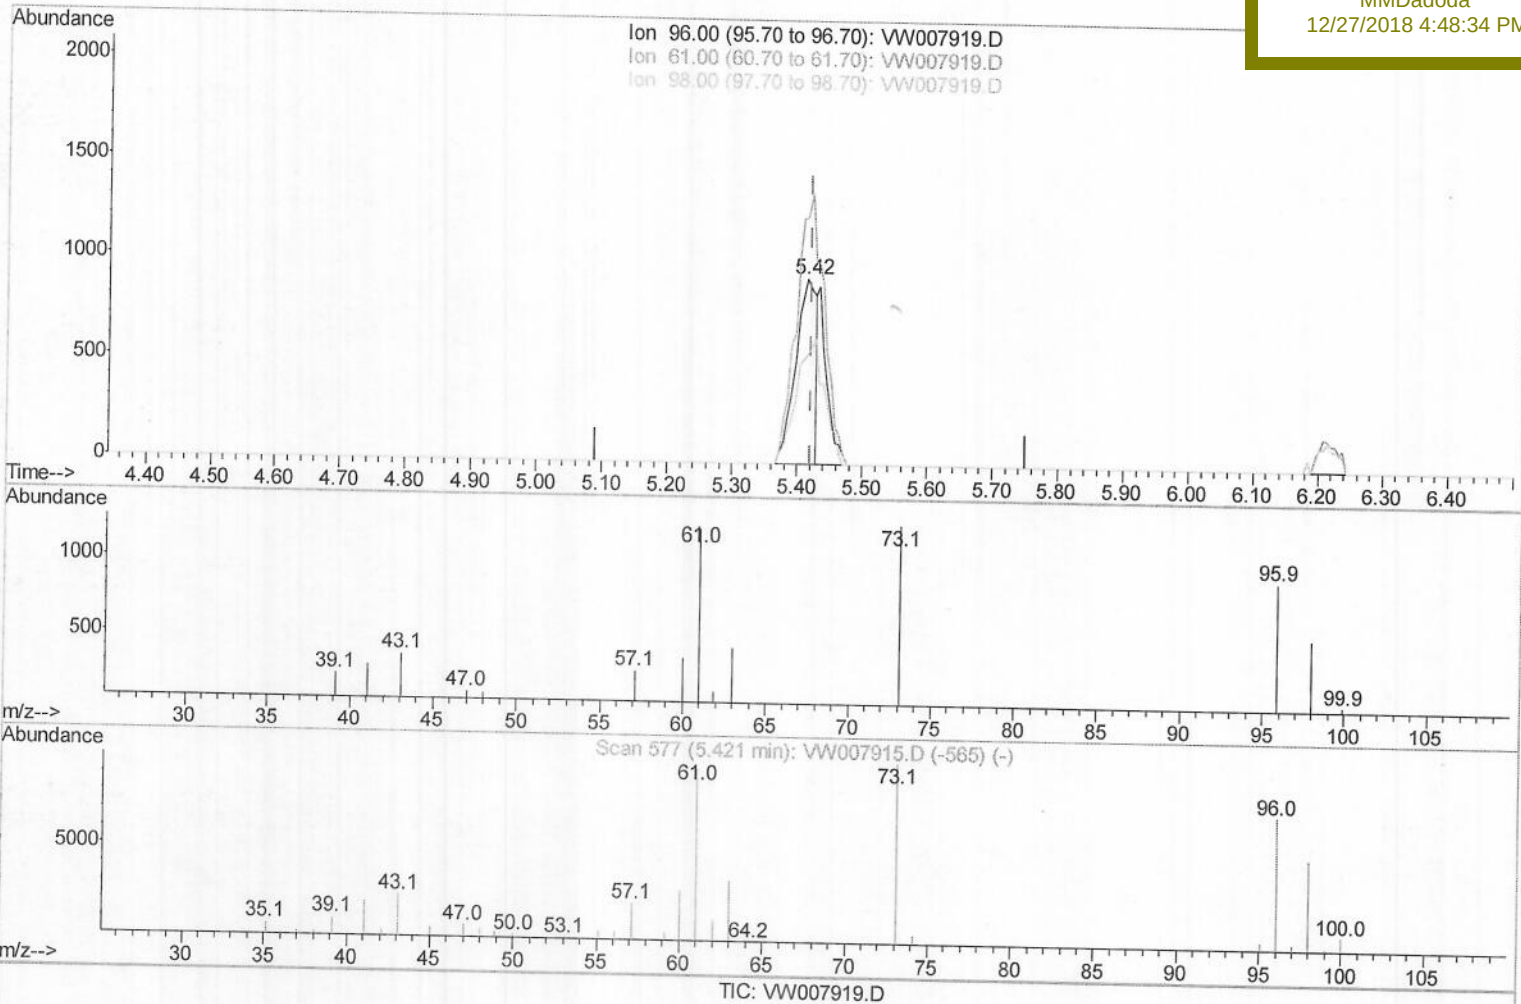

(18) trans-1,2-Dichloroethene (T)

5.415min (-0.006) 1.79ug/L

response 1991

Ion	Exp%	Act%
96.00	100	100
61.00	130.60	132.90
98.00	68.60	58.91
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

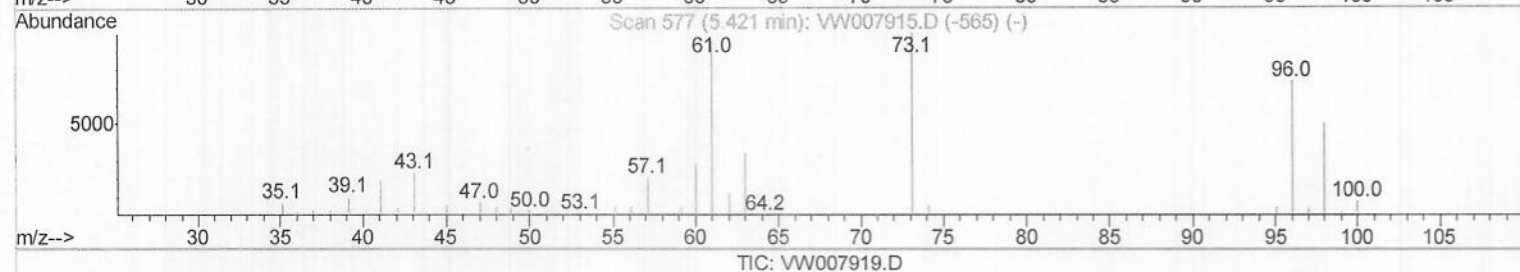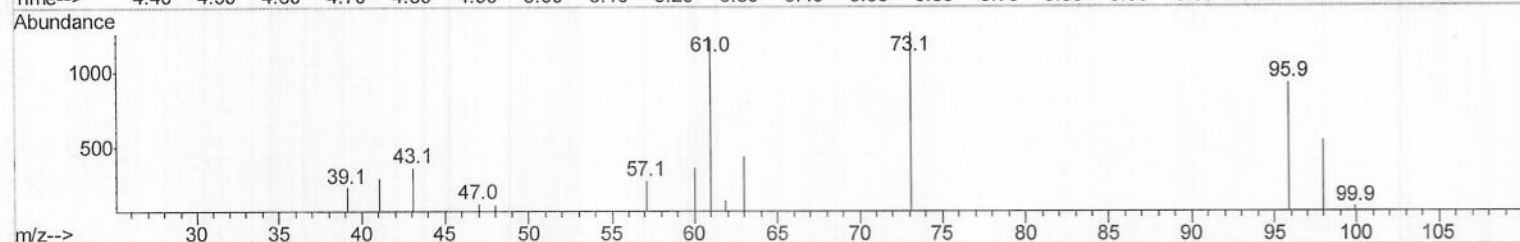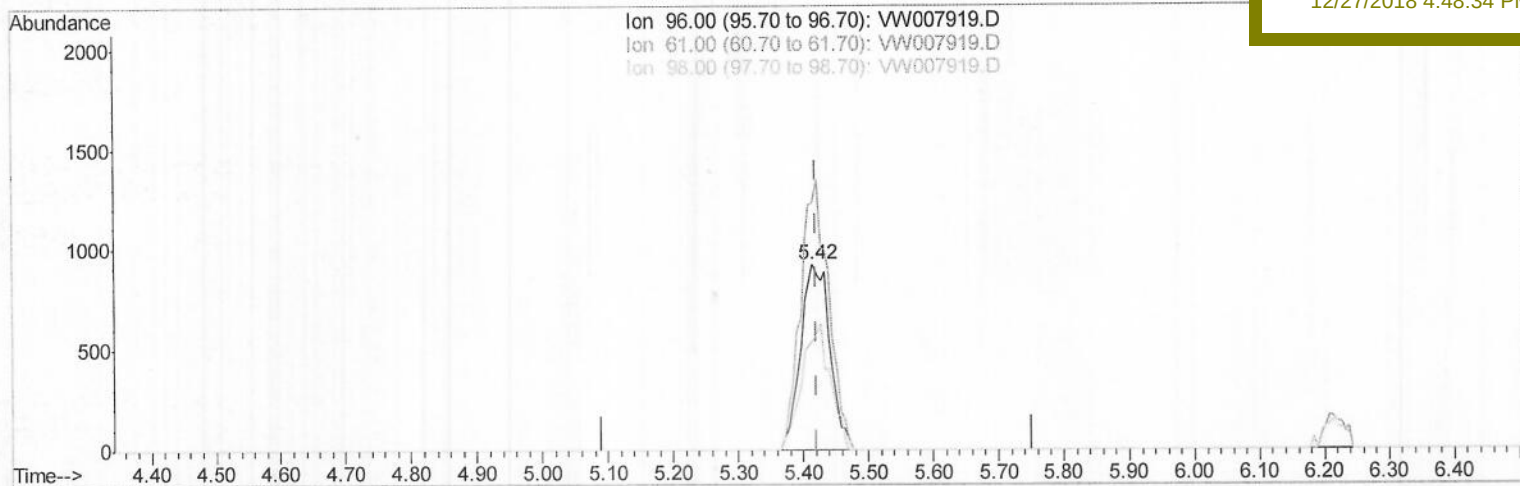

TIC: VW007919.D

(18) trans-1,2-Dichloroethene (T)

5.415min (-0.006) 2.55ug/L m

response 2844

Ion	Exp%	Act%
96.00	100	100
61.00	130.60	132.90
98.00	68.60	58.91
0.00	0.00	0.00

SY
12/28/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

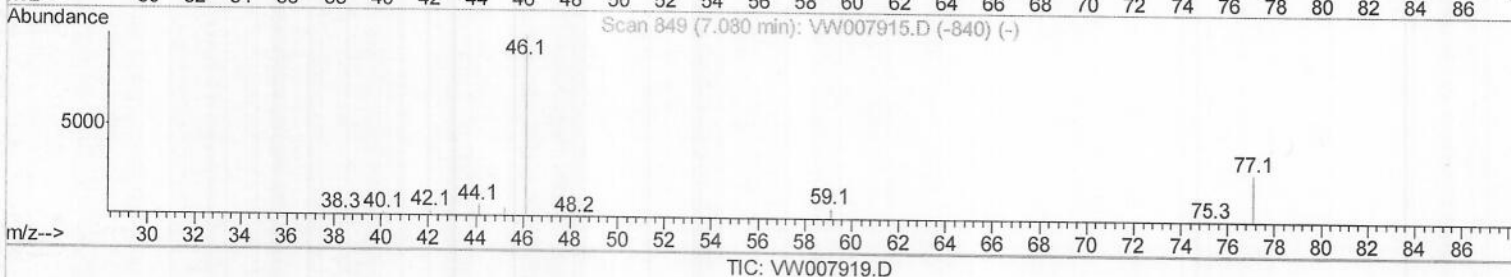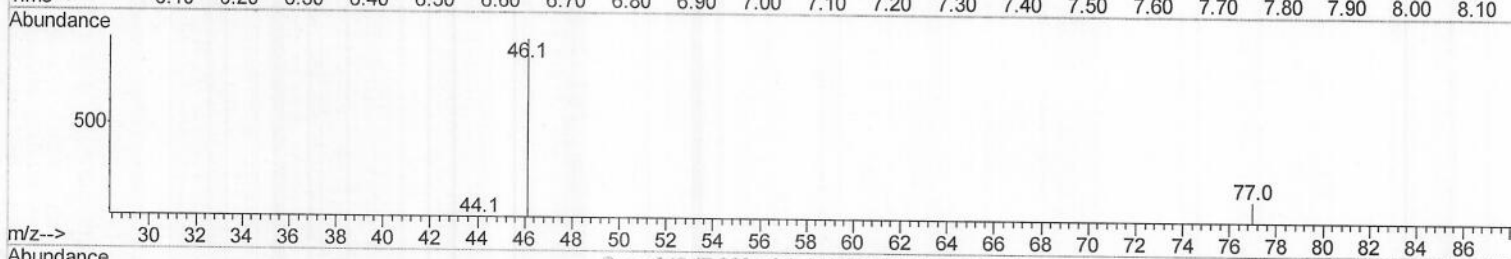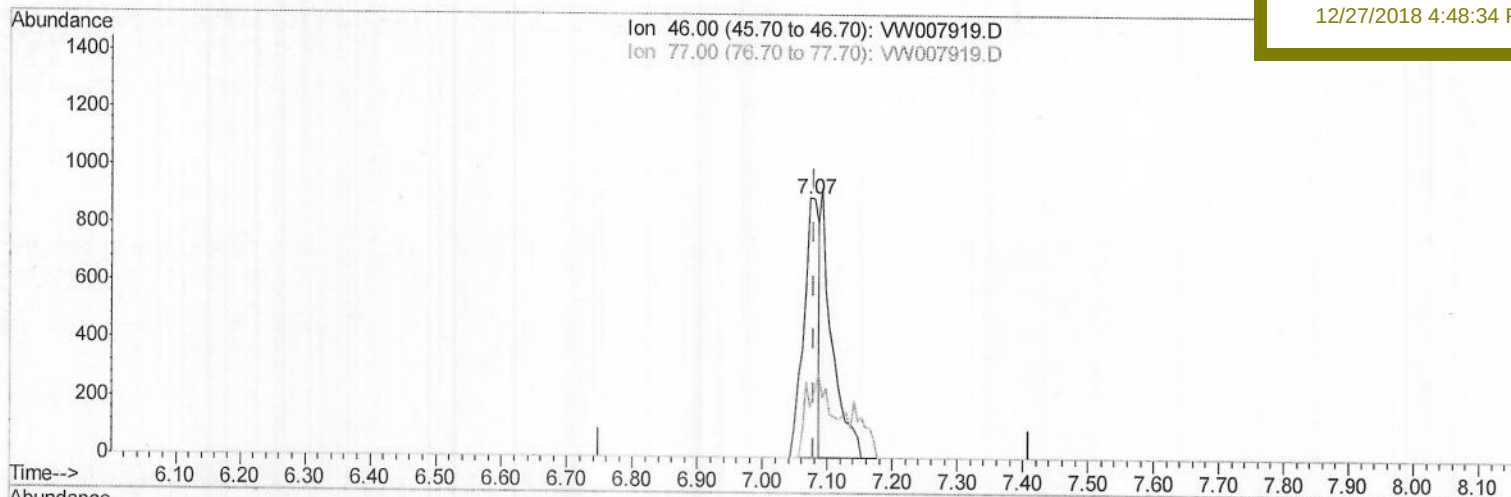

(20) 2-Butanone-d5 (S)

7.074min (-0.006) 3.95ug/L

response 1437

Ion	Exp%	Act%
46.00	100	100
77.00	26.90	13.29#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)

Data File : VW007919.D

Acq On : 26 Dec 2018 12:04

Operator : SY/AP

Sample : VSTD2.587

Misc : 5.00G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Instrument :

MSVOA_W

ClientSampleId :

VSTD2.587

Quant Time: Dec 26 12:29:01 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M




Quant Title : VOC Analysis

QLast Update : Wed Dec 26 10:32:54 2018

Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

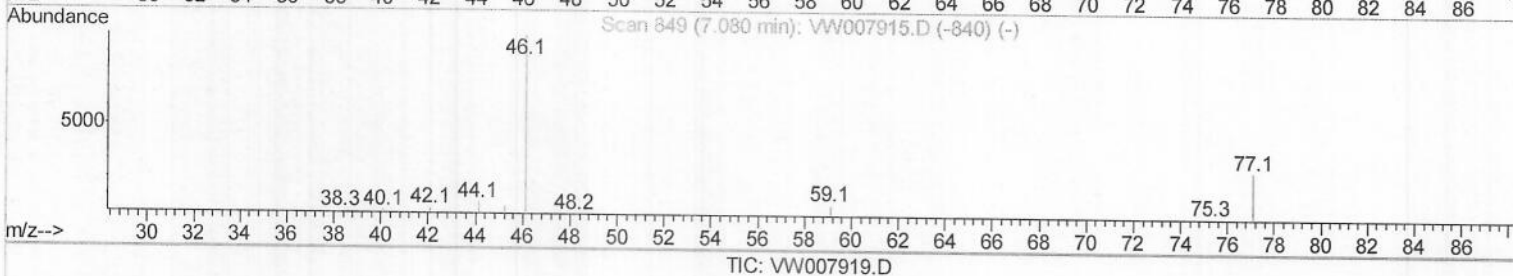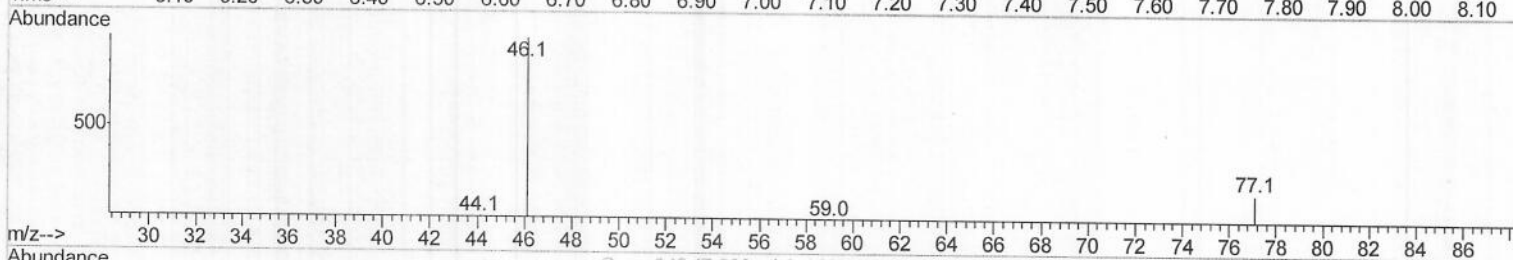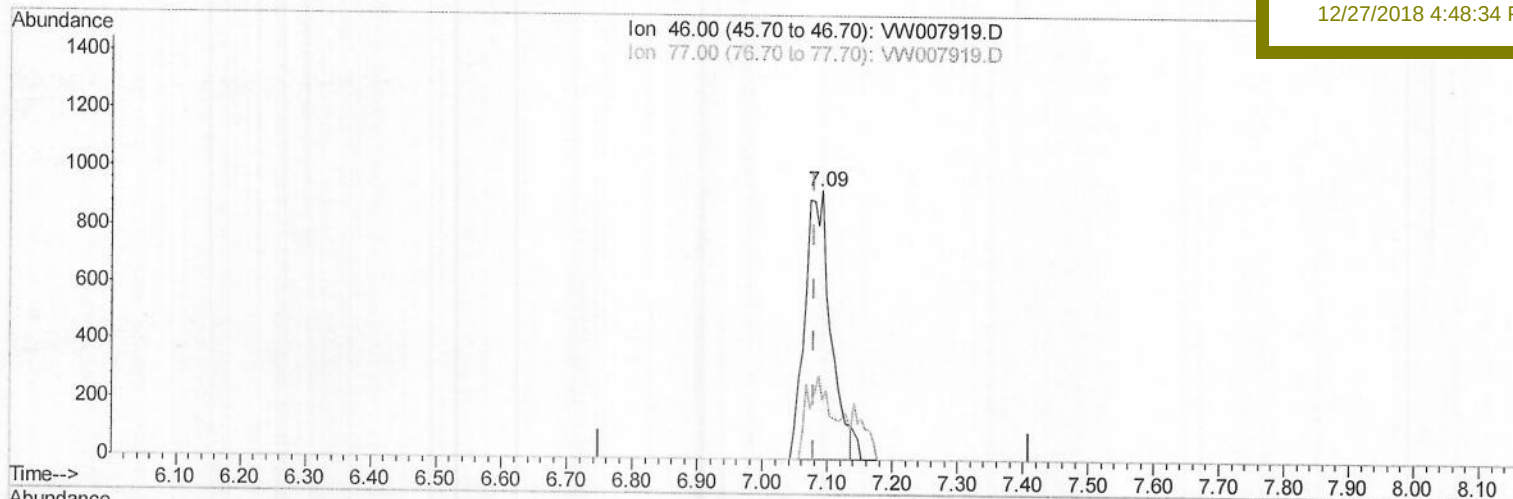

(20) 2-Butanone-d5 (S)

7.092min (+0.012) 6.92ug/L m

response 2514

Ion Exp% Act%

46.00 100 100

77.00 26.90 7.60#

0.00 0.00 0.00

0.00 0.00 0.00

SY
12/28/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

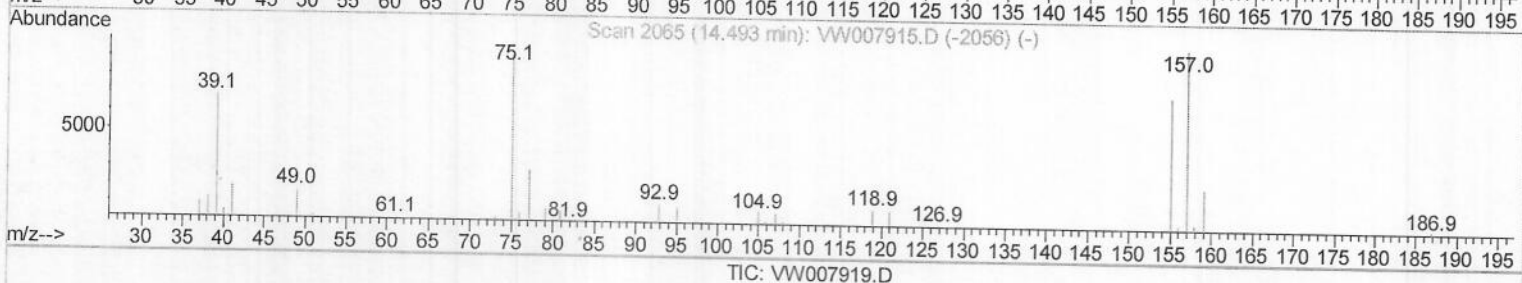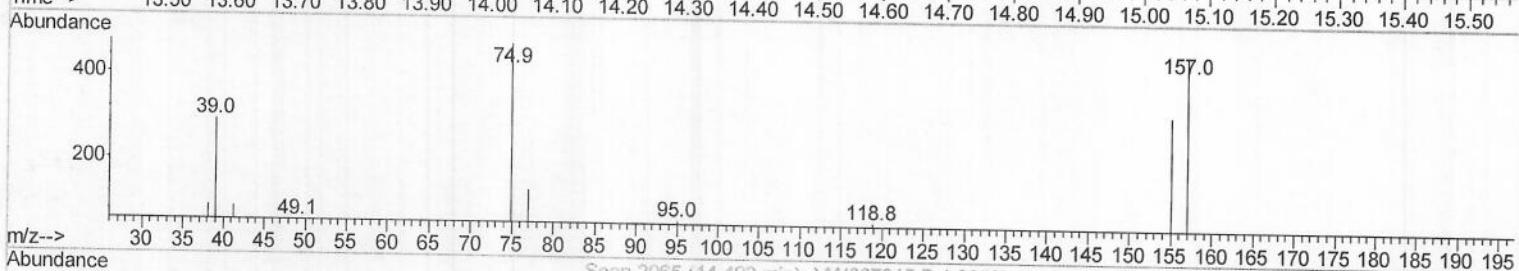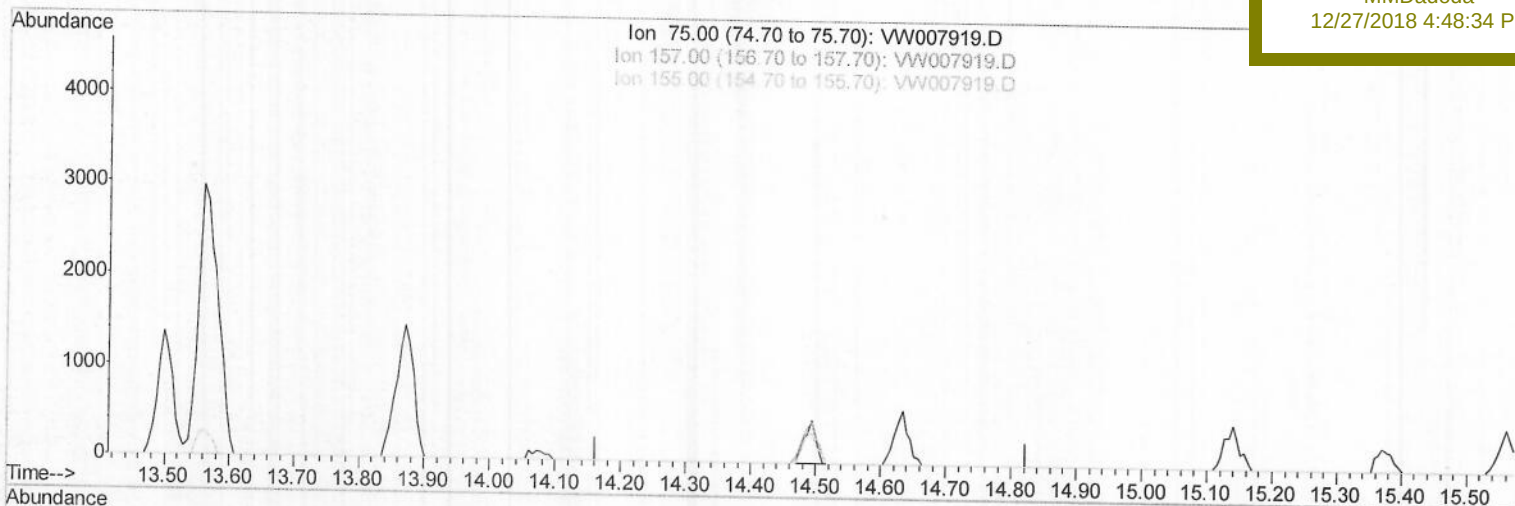

(66) 1,2-Dibromo-3-chloropropane (T)

14.493min (-14.493) 0.00ug/L

response 0

Ion	Exp%	Act%
75.00	100	0.00
157.00	107.00	0.00#
155.00	79.20	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (Qedit)




Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:29:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

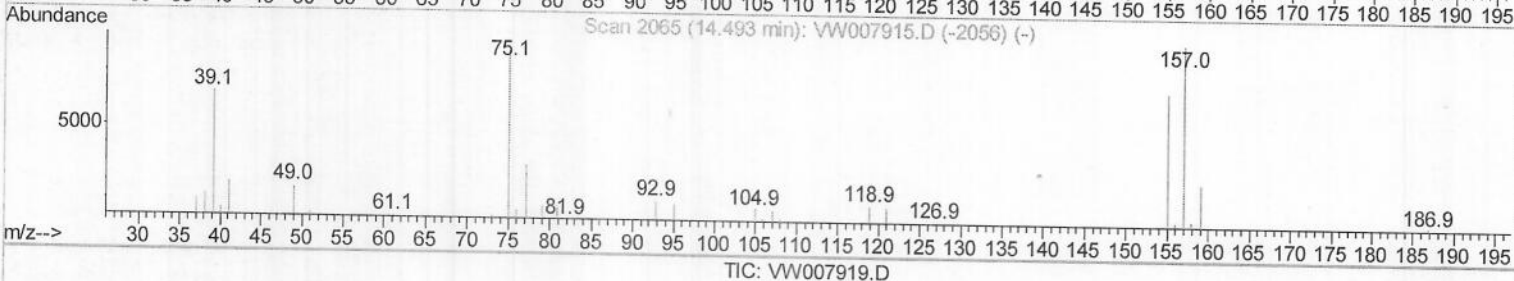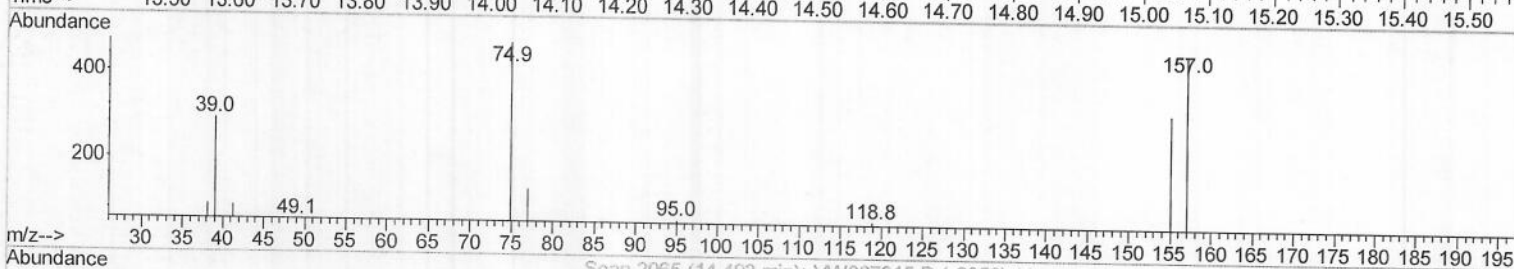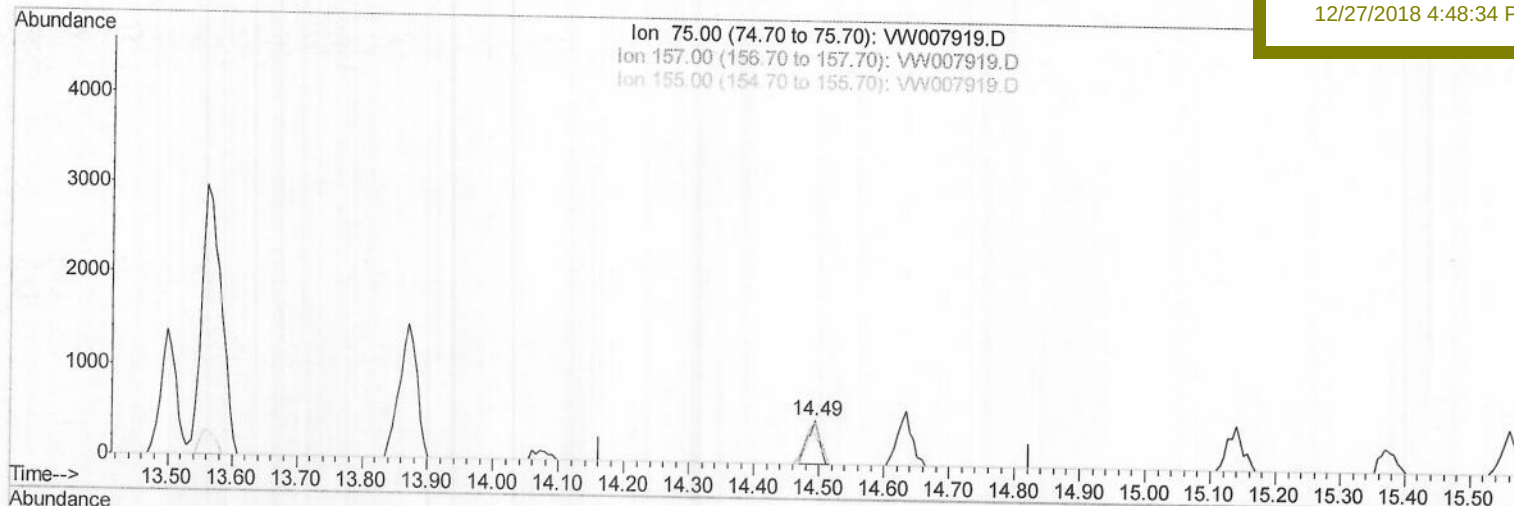

(66) 1,2-Dibromo-3-chloropropane (T)

14.493min (-0.000) 2.48ug/L m

response 599

Ion	Exp%	Act%
75.00	100	100
157.00	107.00	97.05
155.00	79.20	68.35
0.00	0.00	0.00

SY
12/28/18

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\

Quantitation Report (QT Reviewed)

Data File : VW007919.D

Acq On : 26 Dec 2018 12:04

Operator : SY/AP

Sample : VSTD2.587

Misc : 5.00G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:36:13 2018

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M

Quant Title : VOC Analysis

QLast Update : Wed Dec 26 10:32:54 2018

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :

VSTD2.587

Manual Integrations
APPROVEDMMDadoda
12/27/2018 4:48:34 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	88510	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	80827	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	39689	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	2635	4.57	ug/L	0.00
7) Chloroethane-d5	2.89	69	1764m	3.61	ug/L	-0.01
10) 1,1-Dichloroethene-d2	4.01	63	7431	3.74	ug/L	0.00
20) 2-Butanone-d5	7.09	46	2514m	6.92	ug/L	0.01
24) Chloroform-d	7.65	84	7698	3.69	ug/L	0.00
26) 1,2-Dichloroethane-d4	8.31	65	4702	3.96	ug/L	0.00
29) Benzene-d6	8.27	84	14654	3.34	ug/L	0.00
33) 1,2-Dichloropropane-d6	9.27	67	4019	3.21	ug/L	0.00
37) Toluene-d8	10.32	98	14253	3.46	ug/L	0.00
38) trans-1,3-Dichloropropene-	10.58	79	2251	3.51	ug/L	0.00
39) 2-Hexanone-d5	10.93	63	2160	7.16	ug/L	0.00
48) 1,1,2,2-Tetrachloroethane-	12.69	84	4119	3.61	ug/L	0.00
61) 1,2-Dichlorobenzene-d4	13.86	152	5608	4.02	ug/L	0.00

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	2.01	85	2553m	2.641	ug/L	
3) Chloromethane	2.21	50	2234	2.887	ug/L	86
5) Vinyl chloride	2.36	62	2468	3.381	ug/L	86
6) Bromomethane	2.79	94	1422	2.816	ug/L	90
8) Chloroethane	2.93	64	1170m	2.662	ug/L	
9) Trichlorofluoromethane	3.26	101	1905	2.273	ug/L	100
11) 1,1,2-Trichloro-1,2,2-trif	4.07	101	3061m	2.740	ug/L	
12) 1,1-Dichloroethene	4.04	96	2572	2.474	ug/L	92
13) Acetone	4.12	43	2144	5.074	ug/L	86
14) Carbon disulfide	4.38	76	7974	2.627	ug/L	99
15) Methyl Acetate	4.67	43	1575	2.486	ug/L #	68
16) Methylene chloride	4.91	84	4073m	2.848	ug/L	
17) Methyl tert-butyl Ether	5.43	73	4910	2.905	ug/L #	87
18) trans-1,2-Dichloroethene	5.42	96	2844m	2.550	ug/L	
19) 1,1-Dichloroethane	6.21	63	4817	2.534	ug/L	97
21) 2-Butanone	7.17	43	2617	5.762	ug/L	82
22) cis-1,2-Dichloroethene	7.17	96	3210	2.616	ug/L	95
23) Bromochloromethane	7.51	128	1459	2.608	ug/L	94
25) Chloroform	7.67	83	5299	2.576	ug/L	95
27) 1,2-Dichloroethane	8.40	62	3948	2.685	ug/L	97
30) Cyclohexane	7.96	56	4388	2.263	ug/L	95
31) 1,1,1-Trichloroethane	7.87	97	5023	2.640	ug/L	96
32) Carbon tetrachloride	8.07	117	4777	2.599	ug/L	100
34) Benzene	8.32	78	11178	2.413	ug/L	100
35) Trichloroethene	9.09	95	3337	2.512	ug/L	96
36) Methylcyclohexane	9.34	83	5546	2.418	ug/L	97
40) 1,2-Dichloropropane	9.37	63	2661	2.348	ug/L #	91
41) Bromodichloromethane	9.64	83	3710	2.280	ug/L	100
42) cis-1,3-Dichloropropene	10.07	75	4482	2.355	ug/L	97
43) 4-Methyl-2-pentanone	10.21	43	4820	5.373	ug/L	98

SOM2WLM122618S.M Wed Dec 26 12:34:22 2018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122718\
Quantitation Report (QT Reviewed)

Data File : VW007919.D
Acq On : 26 Dec 2018 12:04
Operator : SY/AP
Sample : VSTD2.587
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 12:36:13 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 26 10:32:54 2018
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
VSTD2.587

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:48:34 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
44) Toluene	10.39	91	12653	2.534	ug/L	98
45) trans-1,3-Dichloropropene	10.61	75	4162	2.490	ug/L	95
46) 1,1,2-Trichloroethane	10.79	97	2230	2.390	ug/L	94
47) Tetrachloroethene	10.86	164	2564	2.555	ug/L	95
49) 2-Hexanone	10.98	43	3233	5.128	ug/L #	97
50) Dibromochloromethane	11.13	129	2800	2.442	ug/L	91
51) 1,2-Dibromoethane	11.24	107	2233	2.383	ug/L #	98
52) Chlorobenzene	11.66	112	8305	2.563	ug/L	95
53) Ethylbenzene	11.73	91	14142	2.519	ug/L	100
54) m,p-Xylene	11.84	106	5378	2.521	ug/L	88
55) o-xylene	12.17	106	5097	2.529	ug/L	97
56) Styrene	12.18	104	8414	2.435	ug/L	100
57) Isopropylbenzene	12.47	105	14409	2.561	ug/L	97
58) 1,1,2,2-Tetrachloroethane	12.72	83	3031	2.620	ug/L	98
59) 1,2,3-Trichloropropane	12.77	75	2321	2.535	ug/L	92
62) Bromoform	12.35	173	1627	2.394	ug/L #	96
63) 1,3-Dichlorobenzene	13.50	146	6788	2.662	ug/L	96
64) 1,4-Dichlorobenzene	13.58	146	6731	2.648	ug/L	96
65) 1,2-Dichlorobenzene	13.88	146	6390	2.800	ug/L	95
66) 1,2-Dibromo-3-chloropropan	14.49	75	599m	2.478	ug/L	
67) 1,3,5-Trichlorobenzene	14.64	180	4969	2.690	ug/L	97
68) 1,2,4-trichlorobenzene	15.14	180	4326	2.717	ug/L	94
69) Naphthalene	15.37	128	9668	2.456	ug/L	99
70) 1,2,3-Trichlorobenzene	15.56	180	3845	2.656	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

57
12/28/18