

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007927.D
 Acq On : 26 Dec 2018 17:06
 Operator : SY/AP
 Sample : J6468-18
 Misc : 5.82G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0JH4

Manual Integrations
 APPROVED

MMDadoda
 12/27/2018 4:49:10 PM

Quant Time: Dec 28 06:51:58 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 27 00:43:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	98478	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	80887	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	31616	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	22115	22.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.16%
7) Chloroethane-d5	2.89	69	14894	22.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.12%
10) 1,1-Dichloroethene-d2	4.01	63	45460	17.30	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.20%
20) 2-Butanone-d5	7.07	46	17685	42.73	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.46%
24) Chloroform-d	7.65	84	57995	22.14	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.56%
26) 1,2-Dichloroethane-d4	8.31	65	35635	22.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.76%
29) Benzene-d6	8.27	84	114791	25.30	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.20%
33) 1,2-Dichloropropane-d6	9.27	67	31571	25.58	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.32%
37) Toluene-d8	10.32	98	106412	24.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.32%
38) trans-1,3-Dichloropropene-	10.58	79	14673	20.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.84%
39) 2-Hexanone-d5	10.93	63	14231	45.09	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.18%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	26844	22.60	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.40%
61) 1,2-Dichlorobenzene-d4	13.86	152	29929	23.44	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.76%

Target Compounds					Ovalue
5) Vinyl chloride	2.36	62	1032	0.970 ug/L	# 19
13) Acetone	4.12	43	8281m	20.478 ug/L	
21) 2-Butanone	7.18	43	2689	5.844 ug/L	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW122718\
Data File : VW007927.D
Acq On : 26 Dec 2018 17:06
Operator : SY/AP
Sample : J6468-18
Misc : 5.82G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0JH4

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:49:10 PM

Quant Time: Dec 28 06:51:58 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 27 00:43:27 2018
Response via : Initial Calibration

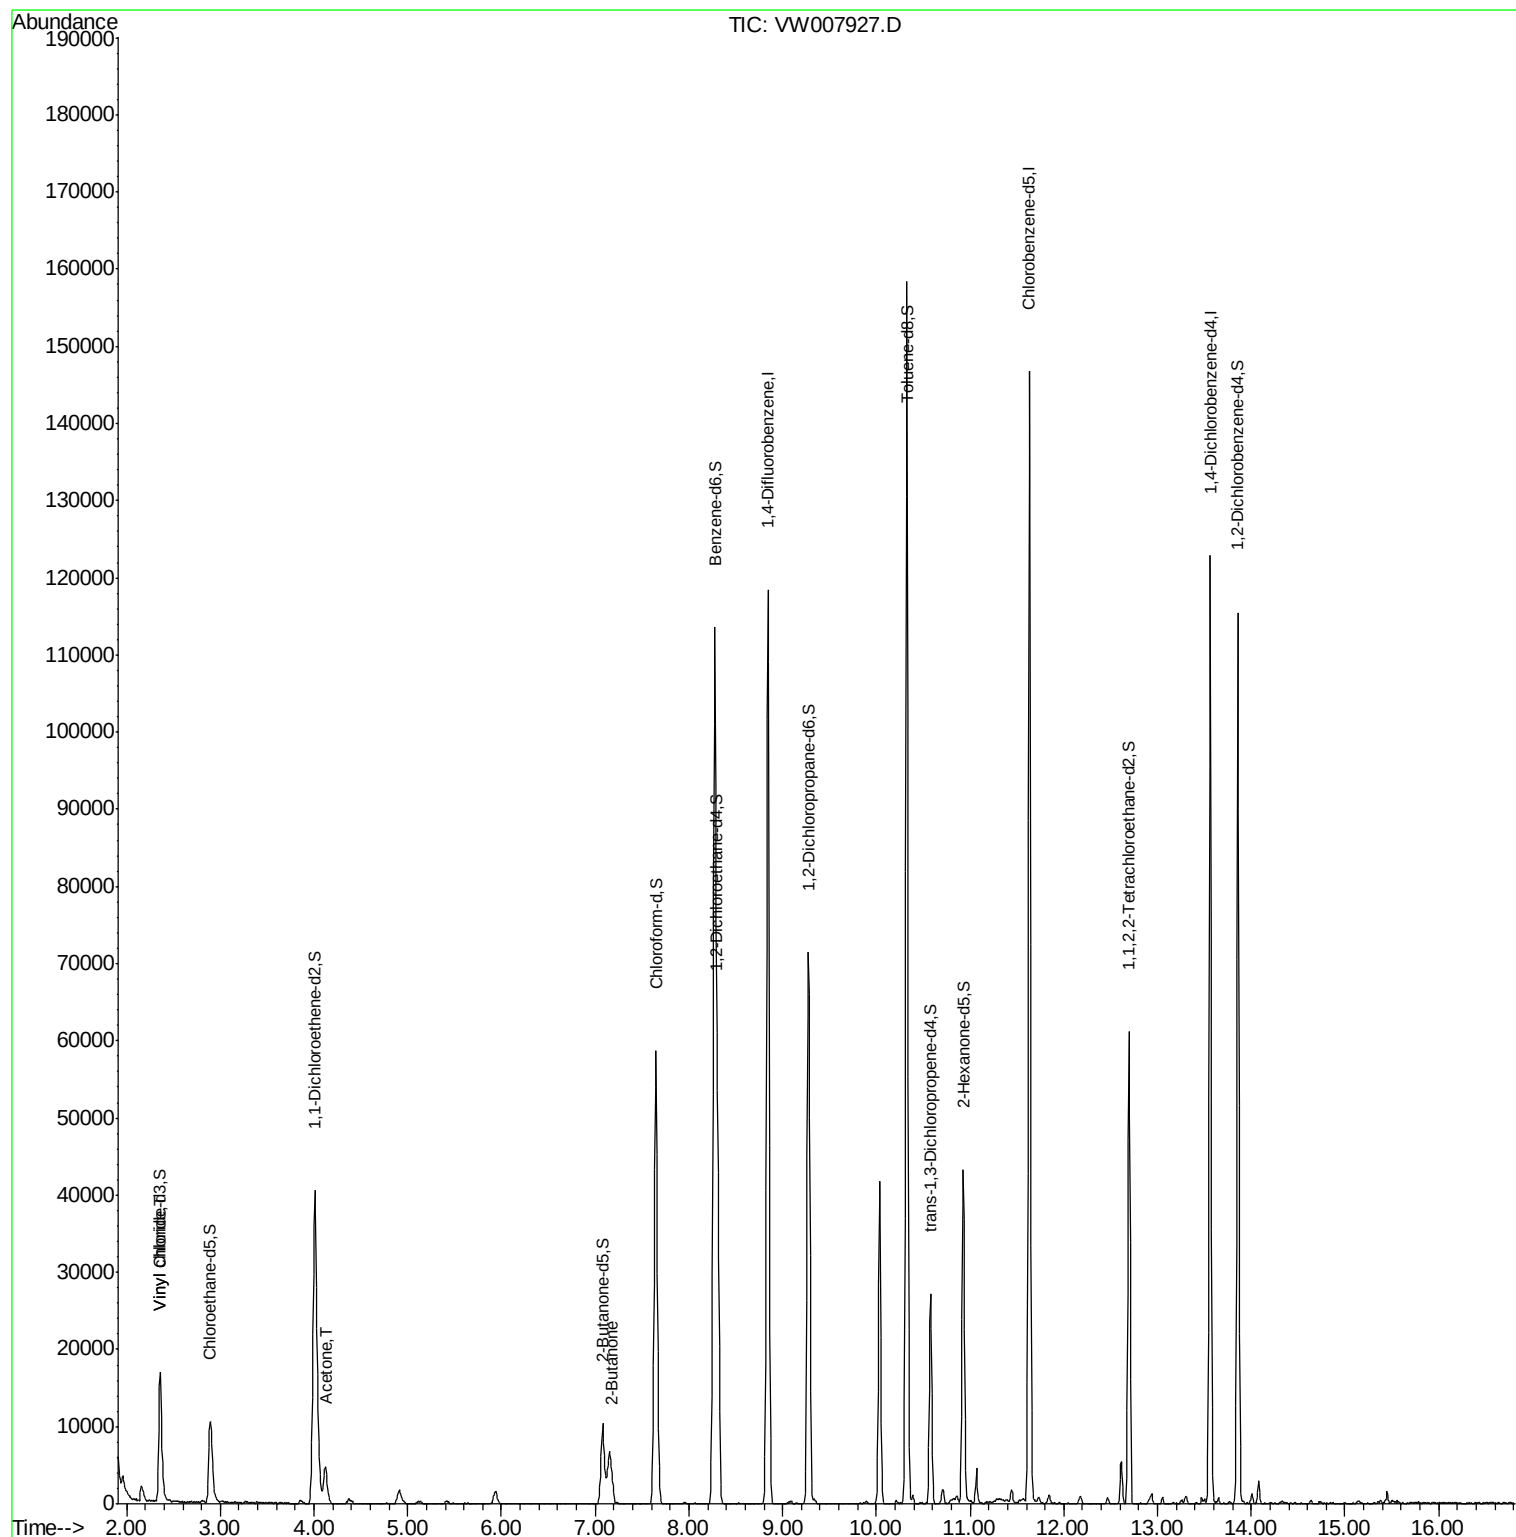

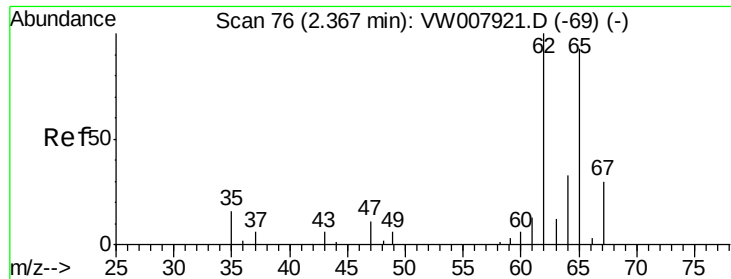

#5

Vinyl chloride

Concen: 0.970 ug/L

RT: 2.36 min Scan# 75

Delta R.T. -0.01 min

Lab File: VW007927.D

Acq: 26 Dec 2018 17:06

Instrument :

MSVOA_W

ClientSampled :

C0JH4

Tot Ion: 62 Resp: 1032

Ion Ratio Lower Upper

62 100


64 76.2 22.0 41.0#

Manual Integrations

APPROVED

MMDadoda

12/27/2018 4:49:10 PM

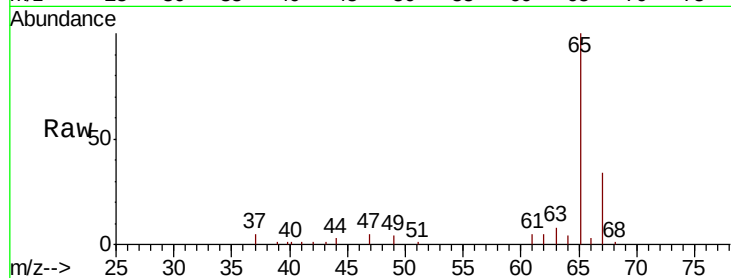


Abundance Ion 62.00 (61.70 to 62.70): VW


Ion 64.00 (63.70 to 64.70): VW

2.36

2.40

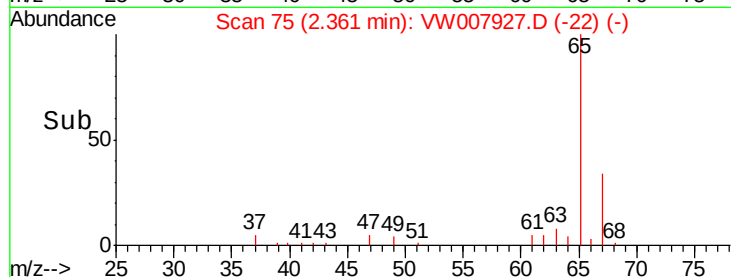

Time-->

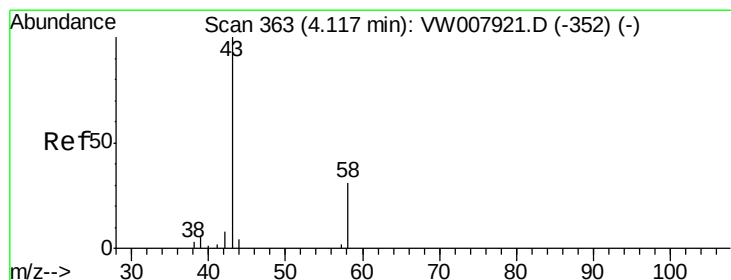

#13

Acetone

Concen: 20.478 ug/L m

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW007927.D


Acq: 26 Dec 2018 17:06

Tgt Ion: 43 Resp: 8281

Ion Ratio Lower Upper

43 100

58 29.5 0.0 58.6

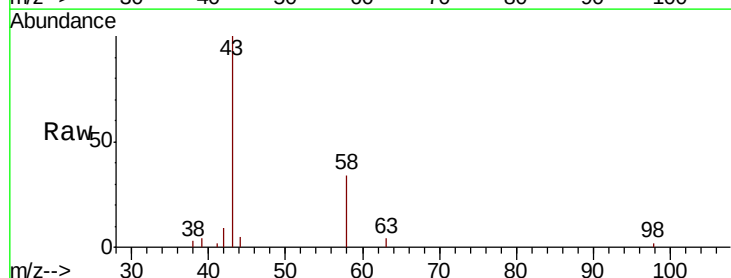


Abundance Ion 43.00 (42.70 to 43.70): VW


Ion 58.00 (57.70 to 58.70): VW

4.12

4.20

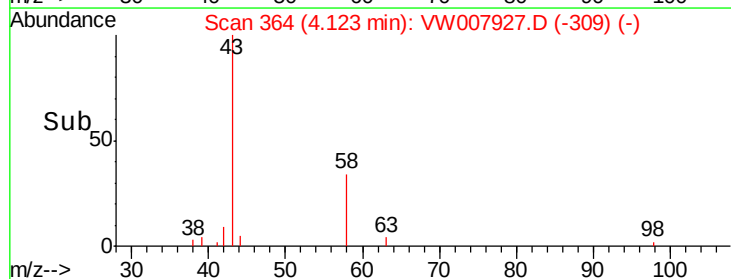

Time-->

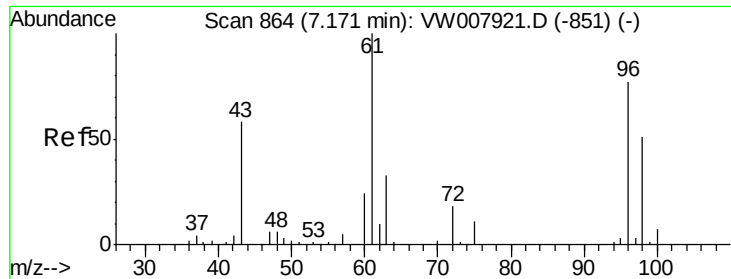

#21
 2-Butanone
 Concen: 5.844 ug/L
 RT: 7.18 min Scan# 865
 Delta R.T. 0.01 min
 Lab File: VW007927.D
 Acq: 26 Dec 2018 17:06

Instrument :
 MSVOA_W
 ClientSampleId :
 C0JH4

Tot Ion: 43 Resp: 2689
 Ion Ratio Lower Upper
 43 100
 72 16.1 14.4 43.4

Manual Integrations
 APPROVED

MMDadoda
 12/27/2018 4:49:10 PM

