

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007930.D
 Acq On : 26 Dec 2018 18:24
 Operator : SY/AP
 Sample : VIBLK82
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK82

Manual Integrations
 APPROVED

MMDadoda
 12/27/2018 4:49:15 PM

Quant Time: Dec 27 02:03:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 27 00:43:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	101940	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	92802	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	45967	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	21173	21.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.32%
7) Chloroethane-d5	2.90	69	14937	22.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.28%
10) 1,1-Dichloroethene-d2	4.01	63	45465	16.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.88%
20) 2-Butanone-d5	7.08	46	17147	40.02	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.04%
24) Chloroform-d	7.65	84	58495	21.57	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.28%
26) 1,2-Dichloroethane-d4	8.31	65	36721	22.58	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.32%
29) Benzene-d6	8.27	84	114654	22.03	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.12%
33) 1,2-Dichloropropane-d6	9.27	67	31953	22.57	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.28%
37) Toluene-d8	10.32	98	111993	22.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.36%
38) trans-1,3-Dichloropropene-	10.58	79	17706	21.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.12%
39) 2-Hexanone-d5	10.93	63	14300	39.49	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.98%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	28404	20.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.40%
61) 1,2-Dichlorobenzene-d4	13.86	152	40532	21.83	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.32%

Target Compounds				Ovalue
16) Methylene chloride	4.90	84	6358m	3.854 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW122718\
Data File : VW007930.D
Acq On : 26 Dec 2018 18:24
Operator : SY/AP
Sample : VIBLK82
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleID :
VIBLK82

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:49:15 PM

Quant Time: Dec 27 02:03:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 27 00:43:27 2018
Response via : Initial Calibration

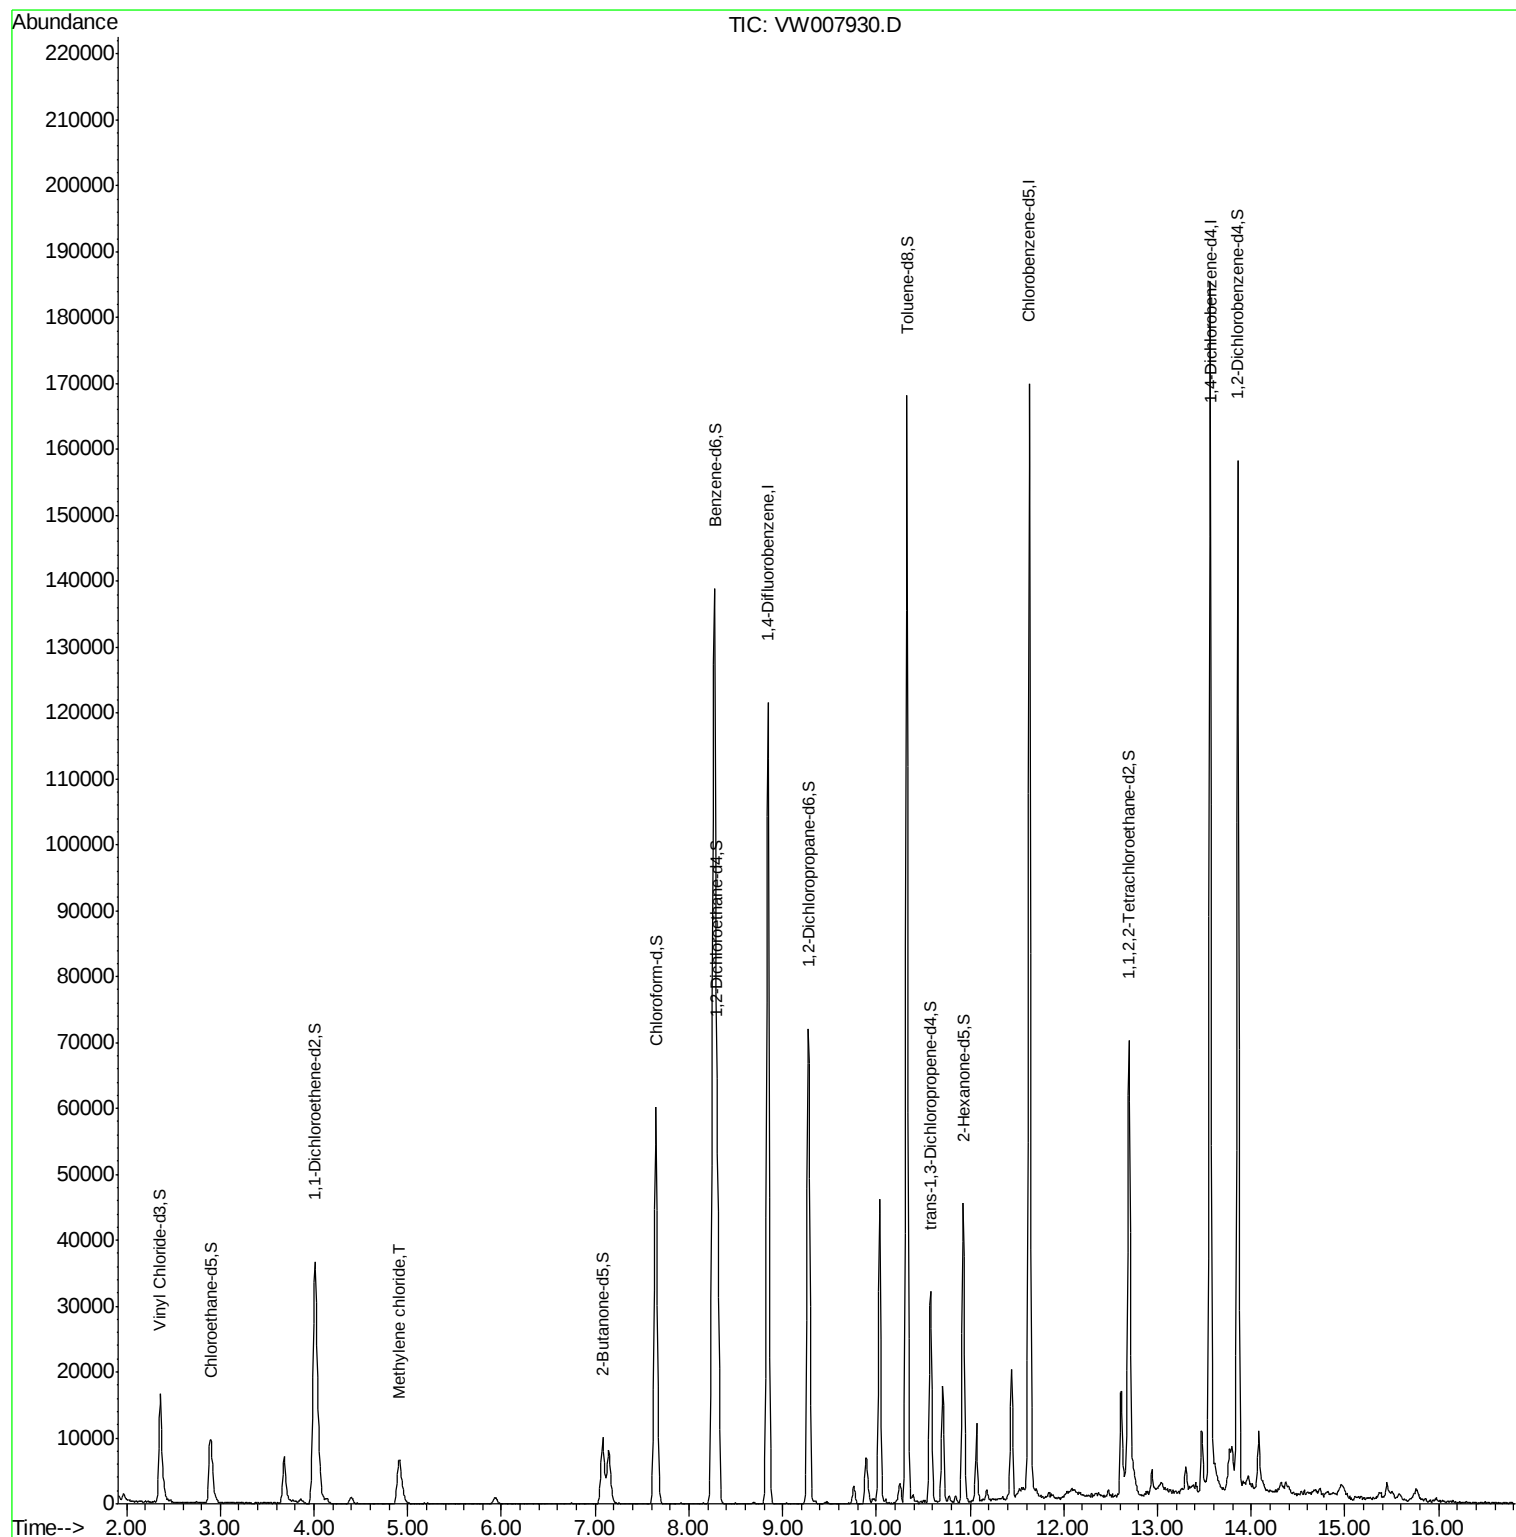

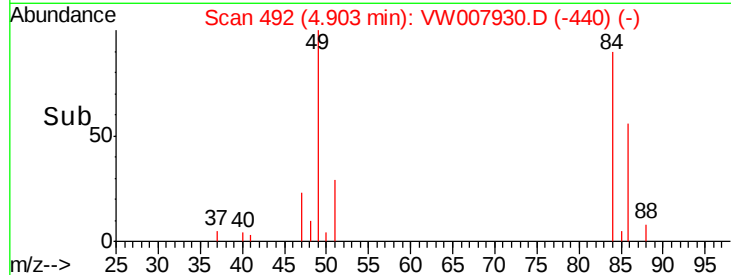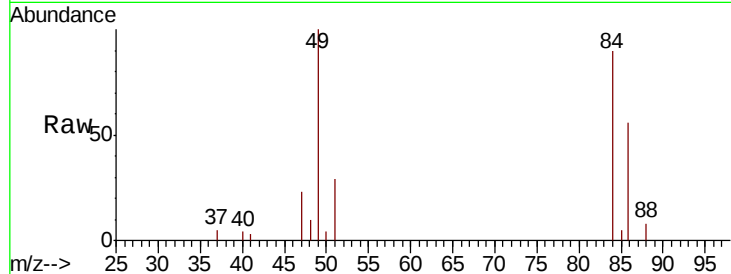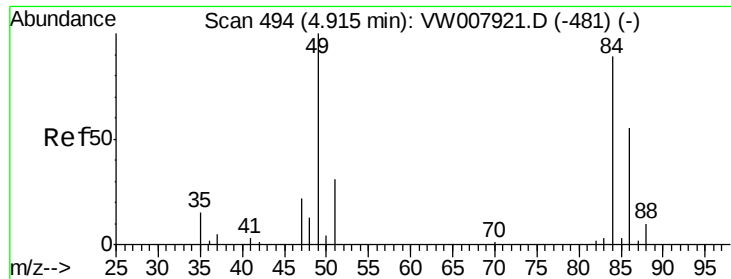

#16
Methvlene chloride
Concen: 3.854 ug/L m
RT: 4.90 min Scan# 492
Delta R.T. -0.01 min
Lab File: VW007930.D
Acq: 26 Dec 2018 18:24

Tot Ion	Ratio	Lower	Upper
84	100		
49	111.7	79.2	147.0
86	62.4	43.2	80.2

Instrument :
MSVOA_W
ClientSampleId :
VIBLK82

Manual Integrations
APPROVED

MMDadoda
12/27/2018 4:49:15 PM

