

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007980.D
 Acq On : 27 Dec 2018 20:03
 Operator : SY/AP
 Sample : J6540-02
 Misc : 4.97G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAEN5

Quant Time: Dec 28 06:31:08 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 28 05:56:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	104045	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	97461	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	48102	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	22888	22.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.28%
7) Chloroethane-d5	2.89	69	15760	22.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.24%
10) 1,1-Dichloroethene-d2	4.01	63	45917	16.54	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.16%
20) 2-Butanone-d5	7.07	46	22649	51.79	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.58%
24) Chloroform-d	7.65	84	67298	24.31	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.24%
26) 1,2-Dichloroethane-d4	8.31	65	44206	26.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.56%
29) Benzene-d6	8.27	84	124326	22.75	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.00%
33) 1,2-Dichloropropane-d6	9.27	67	35241	23.70	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.80%
37) Toluene-d8	10.32	98	120134	22.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.24%
38) trans-1,3-Dichloropropene-	10.58	79	20466	23.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.92%
39) 2-Hexanone-d5	10.93	63	20510	53.93	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.86%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	37895	26.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.92%
61) 1,2-Dichlorobenzene-d4	13.86	152	47970	24.69	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.76%


Target Compounds					Ovalue
13) Acetone	4.12	43	3286	7.691 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007980.D
 Acq On : 27 Dec 2018 20:03
 Operator : SY/AP
 Sample : J6540-02
 Misc : 4.97G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 GAEN5

Quant Time: Dec 28 06:31:08 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 28 05:56:01 2018
 Response via : Initial Calibration

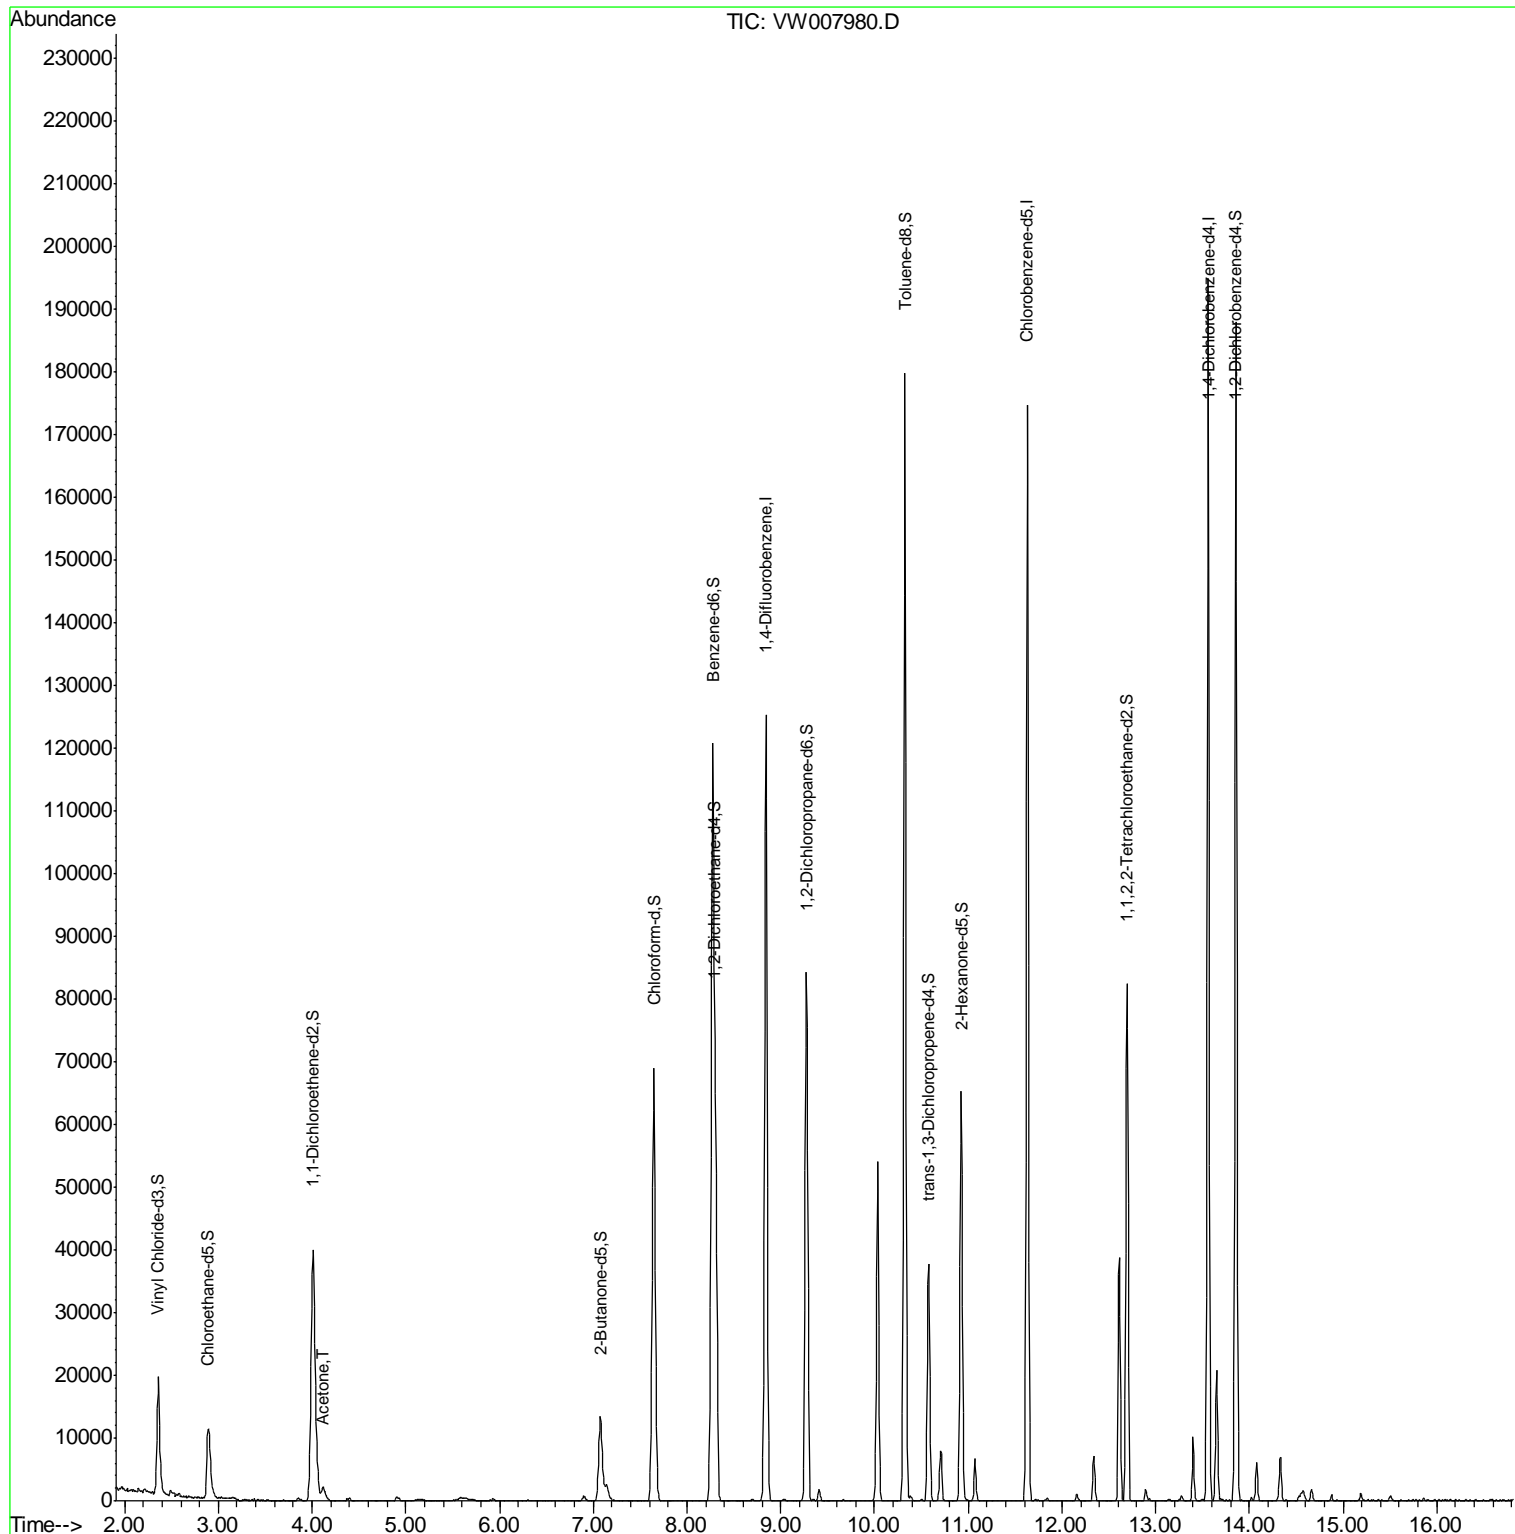

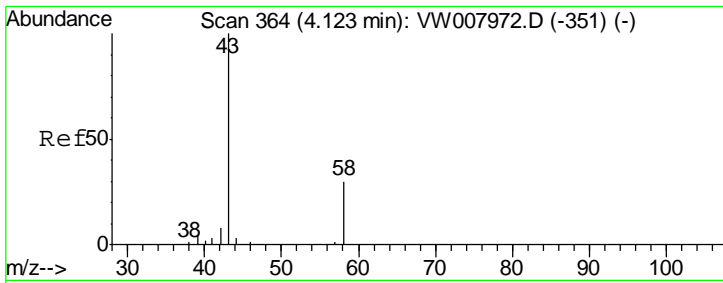

#13
 Acetone
 Concen: 7.691 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. -0.00 min
 Lab File: VW007980.D
 Acq: 27 Dec 2018 20:03

Instrument :
 MSVOA_W
ClientSampled :
 GAEN5

Tot Ion: 43 Resp: 3286

Ion	Ratio	Lower	Upper
43	100		
58	25.0	0.0	58.6

