

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007981.D
 Acq On : 27 Dec 2018 20:29
 Operator : SY/AP
 Sample : J6540-03
 Misc : 4.06G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAEN6

Quant Time: Dec 28 06:32:40 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 28 05:56:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	102145	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	96335	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	46965	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	22775	22.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.52%
7) Chloroethane-d5	2.90	69	16927	24.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.84%
10) 1,1-Dichloroethene-d2	4.01	63	48385	17.75	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.00%
20) 2-Butanone-d5	7.07	46	21358	49.75	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.50%
24) Chloroform-d	7.65	84	68935	25.37	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.48%
26) 1,2-Dichloroethane-d4	8.30	65	44467	27.29	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.16%
29) Benzene-d6	8.27	84	127513	23.60	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.40%
33) 1,2-Dichloropropane-d6	9.27	67	36152	24.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.40%
37) Toluene-d8	10.32	98	122879	23.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.36%
38) trans-1,3-Dichloropropene-	10.58	79	20318	24.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.32%
39) 2-Hexanone-d5	10.93	63	19217	51.12	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.24%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	36393	25.73	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.92%
61) 1,2-Dichlorobenzene-d4	13.86	152	47899	25.25	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.00%


Target Compounds					Ovalue
13) Acetone	4.12	43	2453	5.848 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW122718\
Data File : VW007981.D
Acq On : 27 Dec 2018 20:29
Operator : SY/AP
Sample : J6540-03
Misc : 4.06G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAEN6

Quant Time: Dec 28 06:32:40 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 28 05:56:01 2018
Response via : Initial Calibration

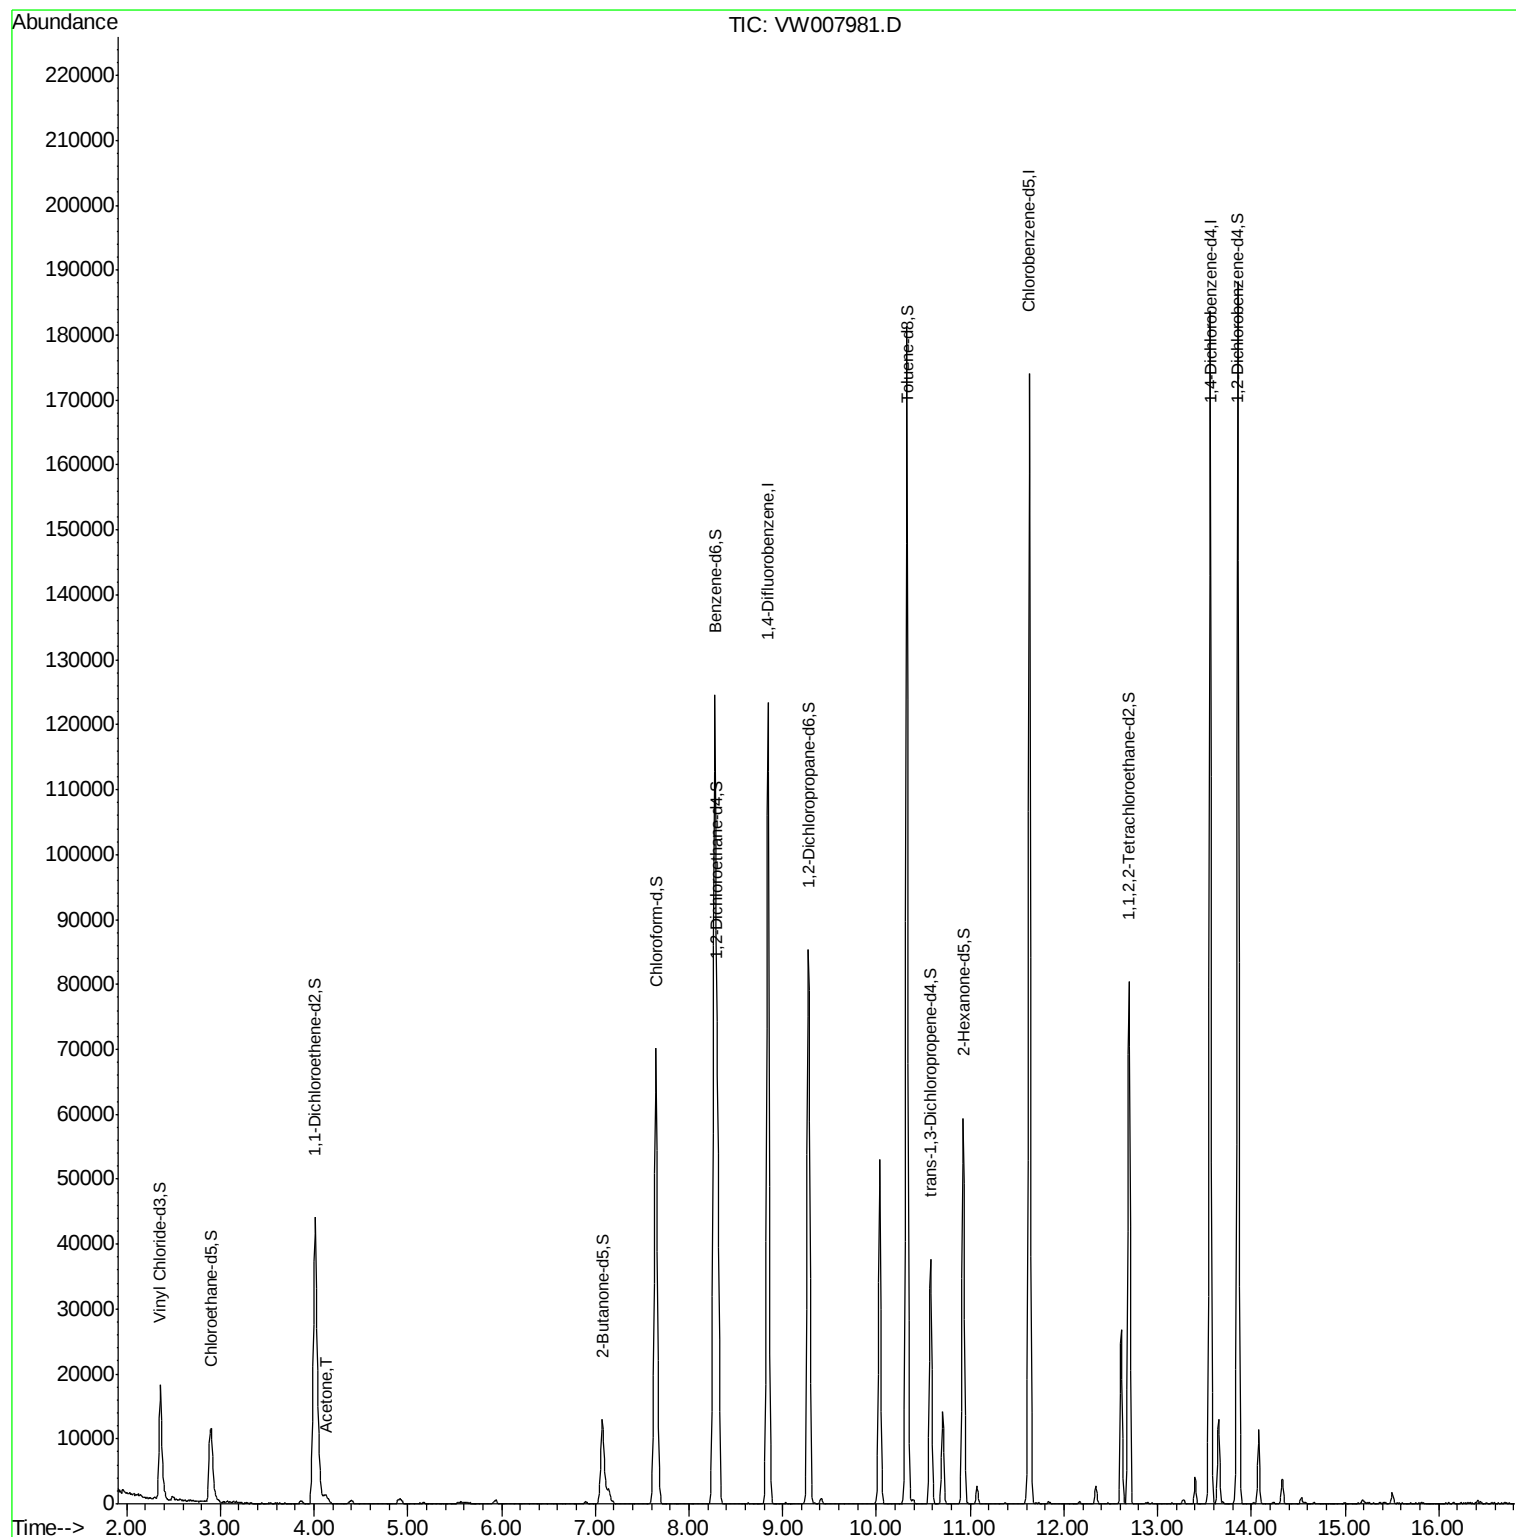

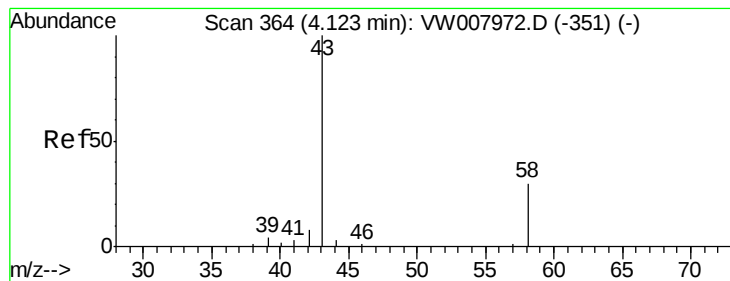

#13
 Acetone
 Concen: 5.848 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. -0.00 min
 Lab File: VW007981.D
 Acq: 27 Dec 2018 20:29

Instrument :
 MSVOA_W
 ClientSampleId :
 GAEN6

Tot Ion: 43 Resp: 2453
 Ion Ratio Lower Upper
 43 100
 58 21.2 0.0 58.6

