

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007984.D
 Acq On : 27 Dec 2018 21:46
 Operator : SY/AP
 Sample : J6540-09
 Misc : 6.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAEP0

Quant Time: Dec 28 06:40:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 28 05:56:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	96104	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	92085	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	44628	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	20087	21.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.84%
7) Chloroethane-d5	2.89	69	15343	24.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.20%
10) 1,1-Dichloroethene-d2	4.01	63	41742	16.28	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.12%
20) 2-Butanone-d5	7.08	46	21004	52.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.00%
24) Chloroform-d	7.65	84	60720	23.75	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	8.31	65	40453	26.39	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.56%
29) Benzene-d6	8.27	84	111464	21.58	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.32%
33) 1,2-Dichloropropane-d6	9.27	67	32698	23.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.12%
37) Toluene-d8	10.32	98	108274	21.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.08%
38) trans-1,3-Dichloropropene-	10.58	79	18815	23.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.32%
39) 2-Hexanone-d5	10.93	63	18644	51.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.78%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	33929	25.10	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.40%
61) 1,2-Dichlorobenzene-d4	13.86	152	43749	24.27	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.08%


Target Compounds					Ovalue
13) Acetone	4.12	43	4872	12.346 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW122718\
Data File : VW007984.D
Acq On : 27 Dec 2018 21:46
Operator : SY/AP
Sample : J6540-09
Misc : 6.36G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAEP0

Quant Time: Dec 28 06:40:00 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 28 05:56:01 2018
Response via : Initial Calibration

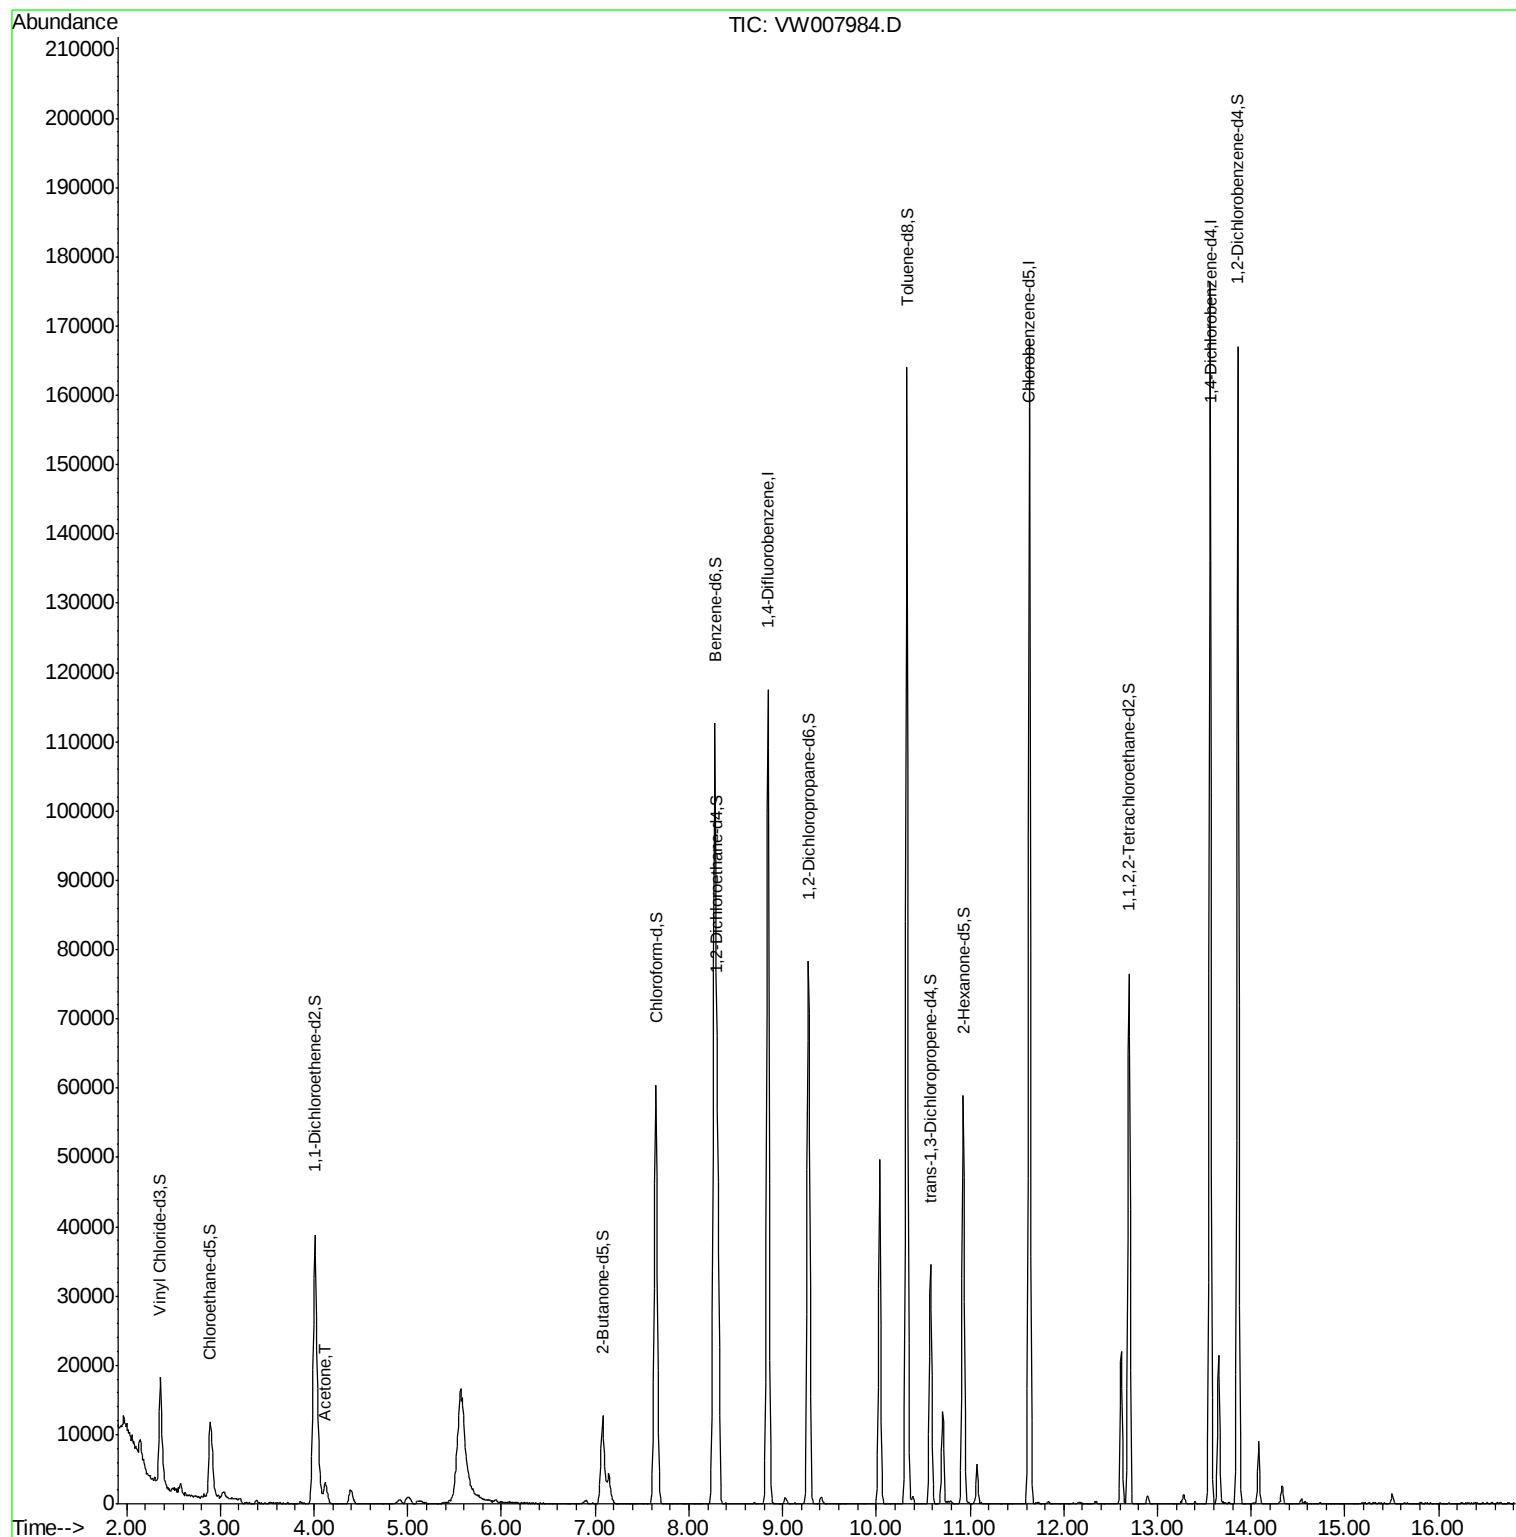

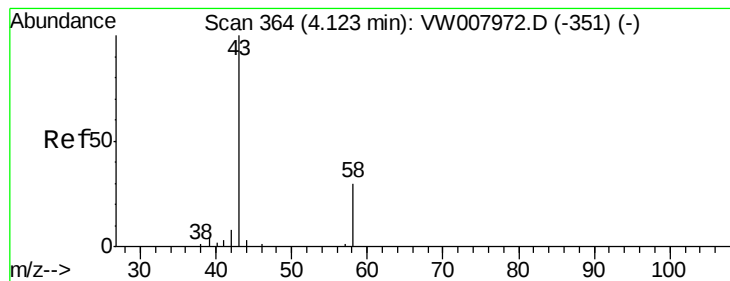

#13

Acetone

Concen: 12.346 ug/L

RT: 4.12 min Scan# 363

Delta R.T. -0.01 min

Lab File: VW007984.D

Acq: 27 Dec 2018 21:46

Instrument :
MSVOA_W
ClientSampleId :
GAEP0

Tot Ion: 43 Resp: 4872

Ion Ratio Lower Upper

43 100

58 27.9 0.0 58.6

