

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007989.D
 Acq On : 27 Dec 2018 23:56
 Operator : SY/AP
 Sample : J6540-14
 Misc : 6.15G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAEP5

Quant Time: Dec 28 06:54:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 28 05:56:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	85005	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	79443	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	39041	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	18994	22.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.68%
7) Chloroethane-d5	2.90	69	12766	22.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.48%
10) 1,1-Dichloroethene-d2	4.01	63	38202	16.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.36%
20) 2-Butanone-d5	7.07	46	23653	66.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	132.40%
24) Chloroform-d	7.65	84	53488	23.65	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	8.31	65	35696	26.33	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.32%
29) Benzene-d6	8.27	84	99389	22.31	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.24%
33) 1,2-Dichloropropane-d6	9.27	67	28043	23.14	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.56%
37) Toluene-d8	10.32	98	95065	21.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.60%
38) trans-1,3-Dichloropropene-	10.58	79	16226	23.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.28%
39) 2-Hexanone-d5	10.93	63	20569	66.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	132.70%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	34238	29.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	117.44%
61) 1,2-Dichlorobenzene-d4	13.86	152	37613	23.85	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.40%


Target Compounds					Ovalue
13) Acetone	4.12	43	3887	11.136 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
Data File : VW007989.D
Acq On : 27 Dec 2018 23:56
Operator : SY/AP
Sample : J6540-14
Misc : 6.15G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAEP5

Quant Time: Dec 28 06:54:00 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 28 05:56:01 2018
Response via : Initial Calibration

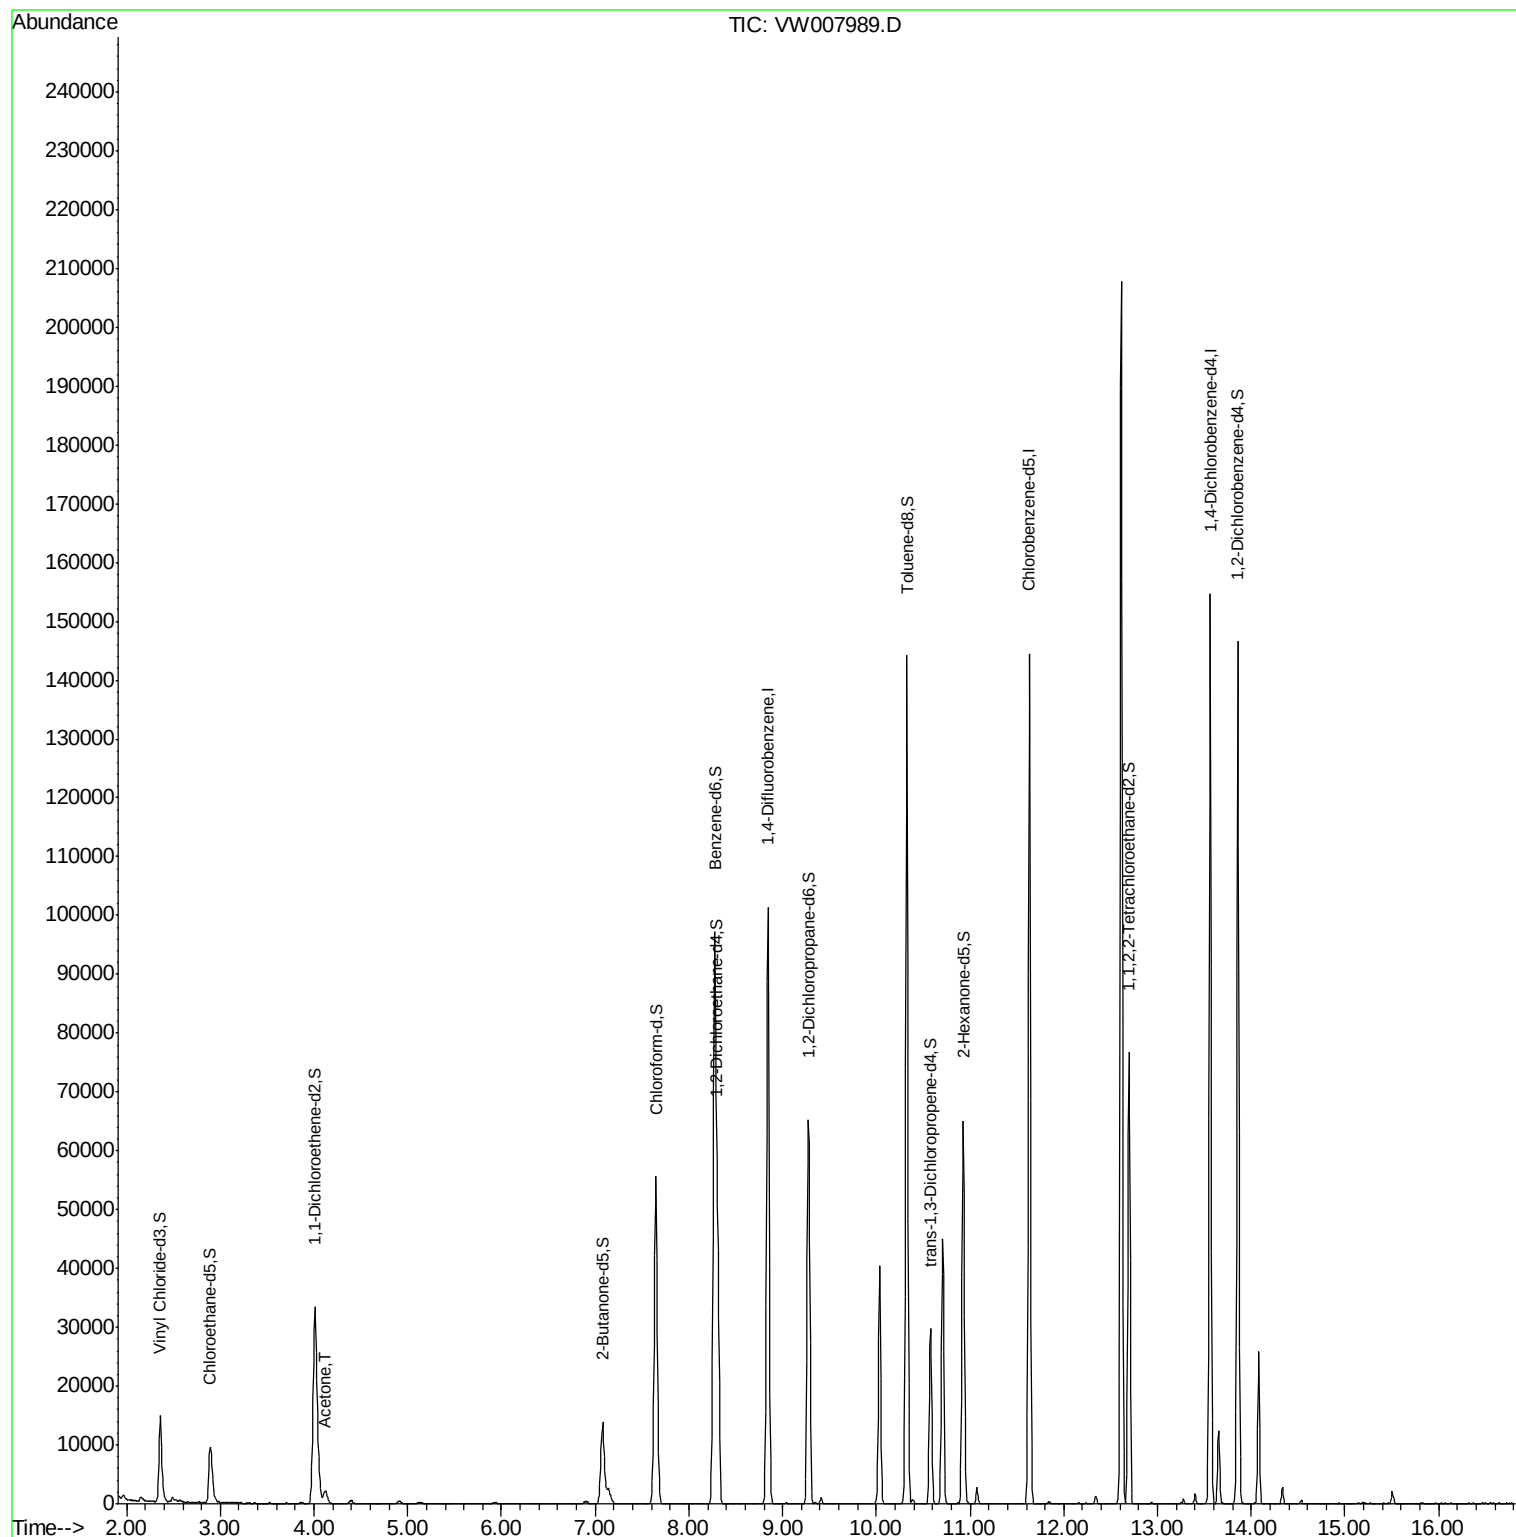

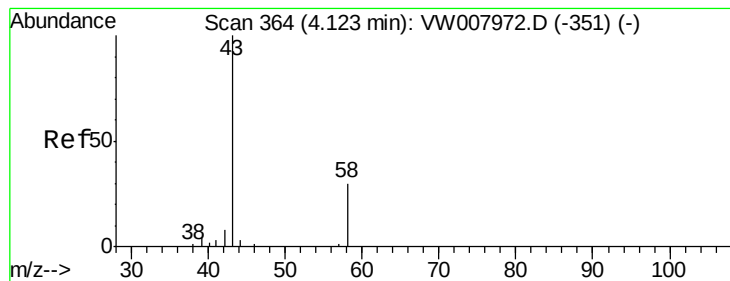

#13

Acetone

Concen: 11.136 ug/L

RT: 4.12 min Scan# 363

Delta R.T. -0.01 min

Lab File: VW007989.D

Acq: 27 Dec 2018 23:56

Instrument :
MSVOA_W
ClientSampleId :
GAEP5

Tot Ion: 43 Resp: 3887

Ion Ratio Lower Upper

43 100

58 27.7 0.0 58.6

