

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007990.D
 Acq On : 28 Dec 2018 00:22
 Operator : SY/AP
 Sample : J6540-15
 Misc : 5.9G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAEP6

Quant Time: Dec 28 06:55:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 28 05:56:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	98107	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	92689	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	45107	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	20524	21.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.92%
7) Chloroethane-d5	2.89	69	15658	24.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.16%
10) 1,1-Dichloroethene-d2	4.01	63	43044	16.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.80%
20) 2-Butanone-d5	7.08	46	21371	51.83	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.66%
24) Chloroform-d	7.65	84	64884	24.86	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.44%
26) 1,2-Dichloroethane-d4	8.31	65	43787	27.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.92%
29) Benzene-d6	8.27	84	120593	23.20	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.80%
33) 1,2-Dichloropropane-d6	9.27	67	35385	25.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.08%
37) Toluene-d8	10.32	98	114156	22.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.16%
38) trans-1,3-Dichloropropene-	10.58	79	20057	24.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.84%
39) 2-Hexanone-d5	10.93	63	18858	52.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.28%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	36761	27.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.04%
61) 1,2-Dichlorobenzene-d4	13.86	152	44951	24.67	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.68%


Target Compounds					Ovalue
13) Acetone	4.12	43	1832	4.548 ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW122718\
Data File : VW007990.D
Acq On : 28 Dec 2018 00:22
Operator : SY/AP
Sample : J6540-15
Misc : 5.9G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAEP6

Quant Time: Dec 28 06:55:46 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 28 05:56:01 2018
Response via : Initial Calibration

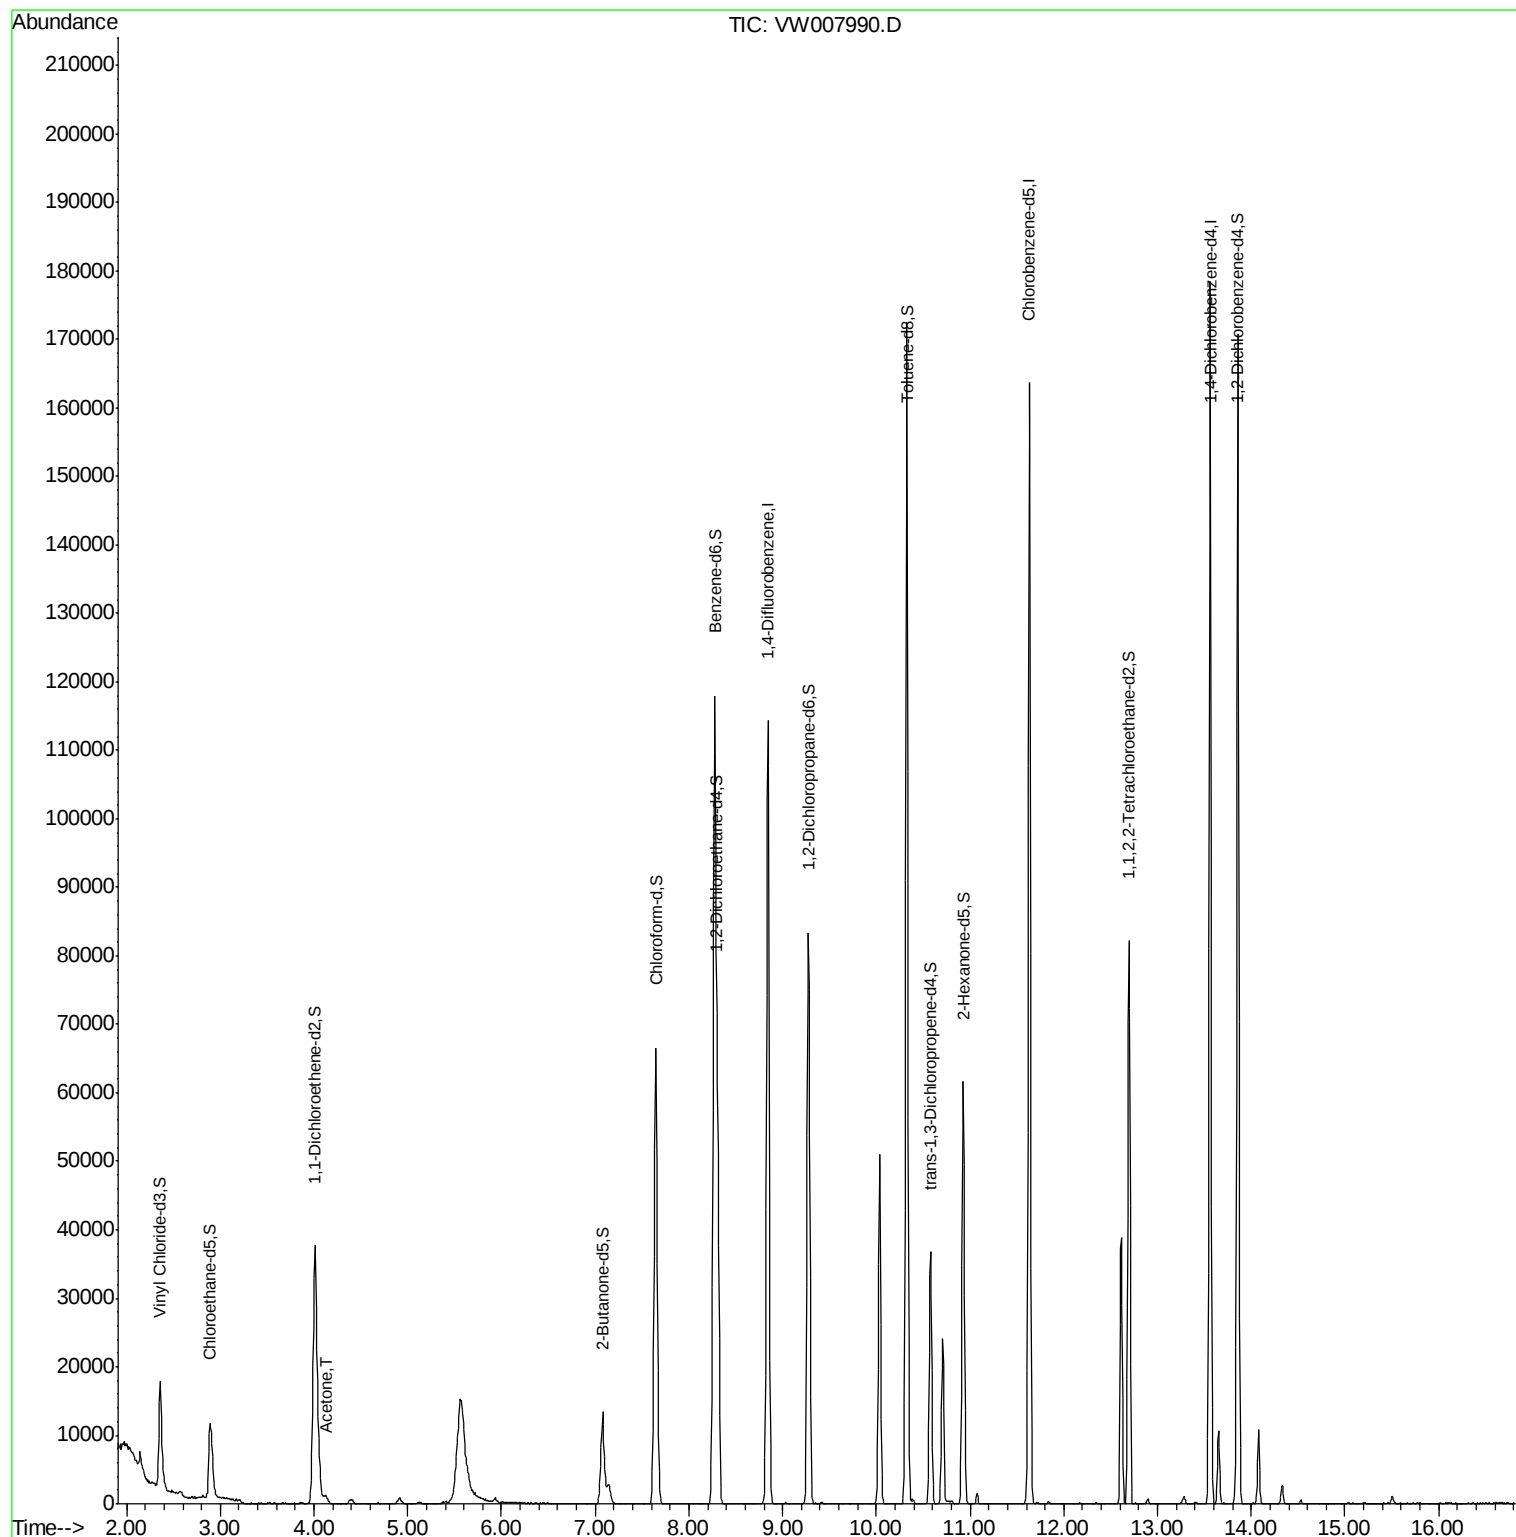

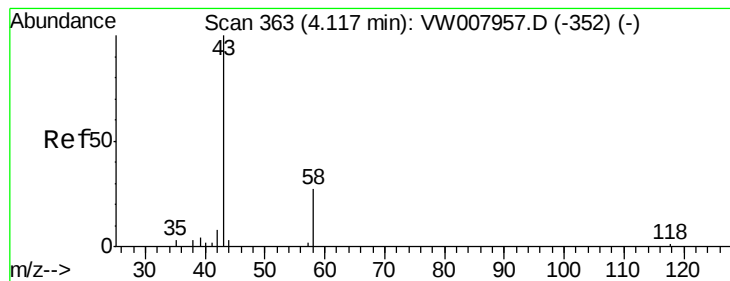

#13

Acetone

Concen: 4.548 ug/L

RT: 4.12 min Scan# 364

Delta R.T. -0.00 min

Lab File: VW007990.D

Acq: 28 Dec 2018 00:22

Instrument :
MSVOA_W
ClientSampleId :
GAEP6

Tot Ion: 43 Resp: 1832

Ion Ratio Lower Upper

43 100

58 15.8 0.0 58.6

