


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122718\
 Data File : VW007912.D
 Acq On : 26 Dec 2018 07:19
 Operator : SY/AP
 Sample : BFB81
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122618S.M
 Title : VOC Analysis
 Last Update : Thu Dec 27 03:06:17 2018

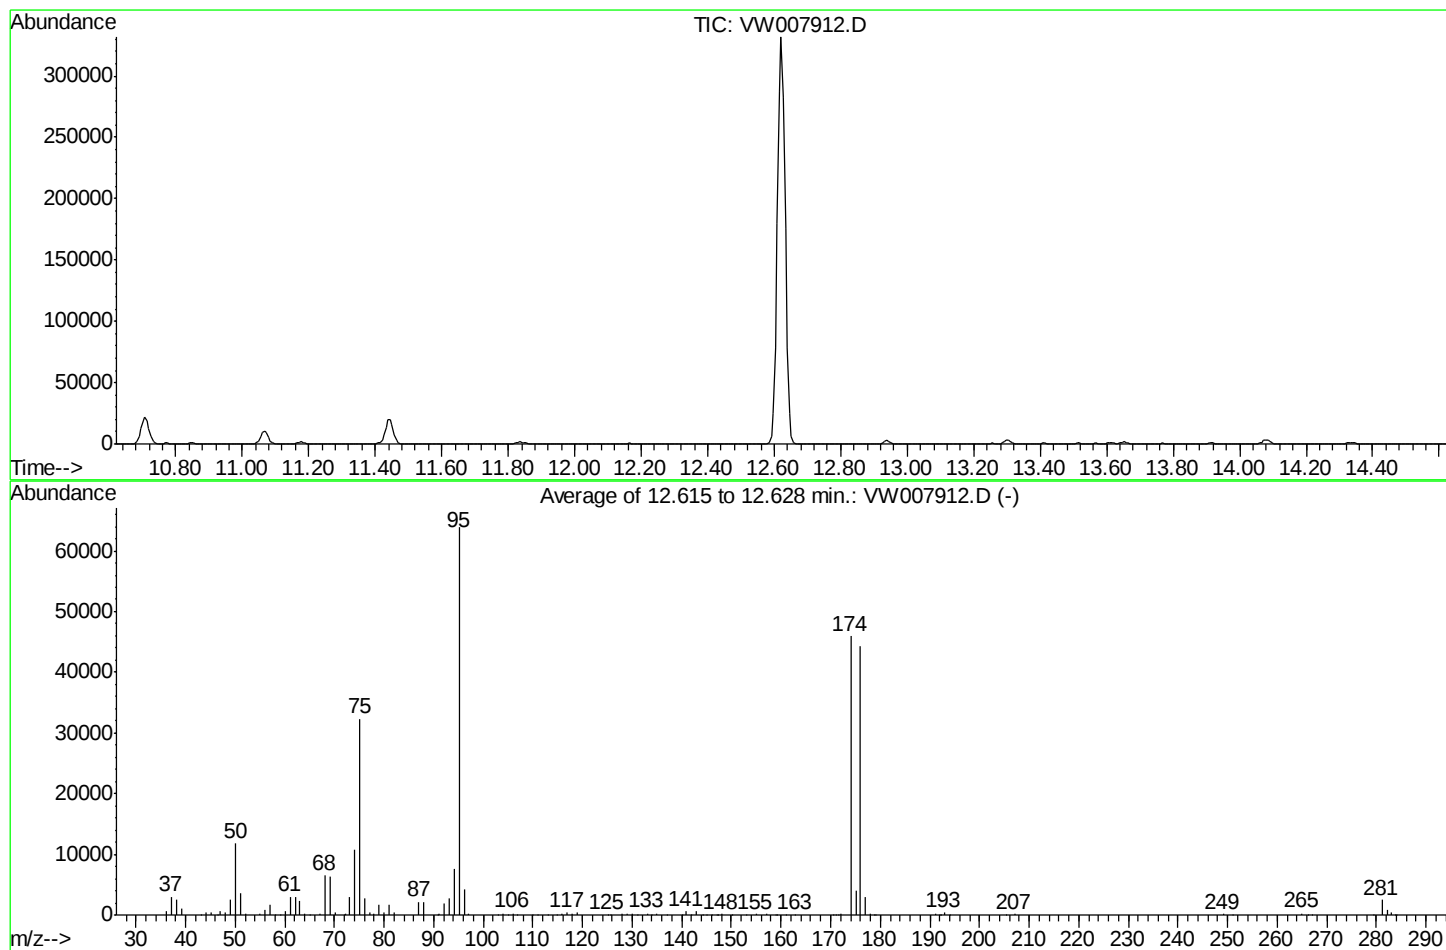

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	11802	PASS
75	95	30	80	50.6	32309	PASS
95	95	100	100	100.0	63880	PASS
96	95	5	9	6.7	4290	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.9	45912	PASS
175	174	5	9	8.8	4031	PASS
176	174	95	101	96.4	44250	PASS
177	176	5	9	6.7	2950	PASS

m/z	Abundance
40.00	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

m/z	Abundance
36.00	520.0
37.10	3246.0
38.10	2560.0
39.10	1004.0
40.10	119.0
43.00	57.0
44.10	332.0
45.00	486.0
47.00	659.0
48.10	365.0
49.10	2532.0
50.10	11554.0
51.10	3641.0
52.00	201.0
55.00	202.0
56.00	876.0
57.00	1597.0
58.10	57.0
59.00	91.0
60.10	671.0
61.00	2985.0
62.00	2729.0
63.00	2140.0
64.10	275.0
64.90	89.0
67.00	166.0
68.00	6484.0
69.10	6690.0
70.10	463.0
72.10	341.0
73.10	2974.0
74.10	10690.0
75.10	31888.0
76.10	2583.0
77.10	302.0
79.00	1584.0
79.90	441.0
80.90	1707.0
81.90	427.0
87.00	2205.0
88.00	2034.0
90.80	283.0
92.10	1744.0
93.00	2608.0
94.10	7307.0
95.10	61072.0
96.10	4371.0
97.20	110.0
103.10	84.0
104.00	282.0
104.90	111.0
105.90	376.0
106.90	91.0
110.00	61.0
114.90	78.0
116.00	276.0
116.90	417.0
117.90	280.0
118.90	385.0
125.00	148.0
125.70	100.0
128.00	213.0
128.90	101.0
130.00	265.0
130.90	70.0
133.10	427.0
133.80	90.0
135.10	141.0
136.80	81.0
140.90	536.0
141.90	130.0
142.90	601.0
145.00	66.0
146.00	60.0
146.90	87.0
147.30	76.0
147.90	152.0
150.00	80.0
153.00	64.0
155.00	108.0
157.00	106.0
160.90	121.0
162.80	71.0
170.60	56.0
171.00	66.0
172.10	298.0
174.00	40608.0
175.00	3600.0
176.00	38824.0
177.00	2986.0
177.90	121.0
178.90	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

191.10	389.0
192.30	145.0
192.90	440.0
193.90	117.0
205.30	85.0
207.10	220.0
249.10	172.0
250.90	80.0
265.10	314.0
266.10	74.0
279.50	56.0
281.10	2996.0
282.10	1021.0
283.10	517.0
284.10	131.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

m/z	Abundance
36.10	590.0
37.10	3278.0
38.10	2871.0
39.10	1178.0
40.00	87.0
43.90	293.0
45.10	586.0
46.40	56.0
47.00	635.0
48.10	455.0
49.10	2963.0
50.10	13409.0
51.10	3998.0
52.10	212.0
55.10	190.0
56.00	896.0
57.00	1689.0
58.10	72.0
60.00	682.0
61.00	3389.0
62.10	3532.0
63.10	2514.0
64.00	218.0
65.00	61.0
67.10	242.0
68.00	7034.0
69.10	6750.0
70.00	460.0
72.20	417.0
73.10	3399.0
74.10	12015.0
75.10	35504.0
76.10	3303.0
77.00	427.0
77.90	299.0
79.00	1831.0
80.00	482.0
81.00	1869.0
81.90	452.0
87.00	2388.0
88.00	2377.0
91.00	248.0
92.00	2154.0
93.10	2838.0
94.10	8298.0
95.10	70312.0
96.10	4613.0
97.10	178.0
103.10	65.0
104.00	350.0
105.00	115.0
106.00	263.0
109.90	53.0
110.90	107.0
112.90	87.0
114.80	106.0
115.90	247.0
116.90	476.0
117.90	283.0
118.90	377.0
125.00	83.0
125.60	102.0
128.00	225.0
129.00	106.0
129.90	302.0
131.00	100.0
133.00	221.0
133.80	101.0
134.90	202.0
136.90	120.0
141.00	796.0
141.90	96.0
142.90	657.0
145.00	78.0
146.00	111.0
147.00	94.0
148.00	196.0
150.10	65.0
155.00	125.0
157.00	128.0
158.80	87.0
159.10	98.0
160.90	81.0
170.90	81.0
171.50	103.0
174.00	50656.0
175.10	4525.0
176.00	49240.0
177.00	3033.0
178.00	110.0
179.10	77.0
191.00	264.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

191.90	59.0
193.00	403.0
193.90	73.0
207.00	130.0
249.10	217.0
265.00	248.0
266.20	60.0
267.10	63.0
281.10	2758.0
282.20	781.0
283.10	458.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

m/z	Abundance
36.10	511.0
37.10	2631.0
38.10	2148.0
39.10	926.0
44.00	415.0
45.00	516.0
47.10	467.0
48.00	339.0
49.10	2309.0
50.10	10443.0
51.10	3117.0
52.00	116.0
55.00	209.0
56.10	816.0
57.10	1497.0
60.00	527.0
61.10	2800.0
62.10	2357.0
63.10	2022.0
64.00	156.0
66.90	183.0
68.00	5903.0
69.00	5816.0
70.00	429.0
71.90	265.0
73.00	2483.0
74.10	9497.0
75.10	29536.0
76.10	2570.0
77.00	285.0
78.00	239.0
79.00	1472.0
79.90	385.0
80.90	1688.0
82.00	339.0
86.90	2016.0
88.00	1841.0
90.90	350.0
92.00	1981.0
93.00	2583.0
94.10	7095.0
95.10	60256.0
96.10	3886.0
97.00	117.0
102.90	66.0
103.80	199.0
104.80	53.0
106.10	214.0
112.90	78.0
114.80	80.0
115.90	200.0
117.00	363.0
118.00	176.0
119.00	396.0
127.90	170.0
129.00	167.0
129.90	193.0
131.00	88.0
132.90	243.0
135.00	138.0
136.80	91.0
140.10	78.0
141.00	543.0
142.00	113.0
142.90	616.0
144.10	54.0
145.00	77.0
146.00	124.0
146.90	78.0
148.10	102.0
150.00	73.0
154.90	168.0
157.10	149.0
159.00	110.0
160.90	60.0
170.90	57.0
171.90	170.0
174.00	46472.0
175.10	3970.0
176.00	44688.0
177.00	2833.0
177.90	123.0
191.00	124.0
191.90	59.0
193.10	148.0
207.10	163.0
249.10	132.0
265.10	101.0
266.20	64.0
267.00	59.0
281.10	1796.0
282.10	575.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

283.10411.0

283.8093.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81