

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122719\

Data File : VW014484.D

Acq On : 28 Dec 2019 01:17

Operator : SY/VA

Sample : K6397-01

Misc : 5.28G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 04:01:38 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M

Quant Title : VOC Analysis

QLast Update : Sat Dec 28 03:24:24 2019

Response via : Initial Calibration

Instrument :

MSVOA_W


ClientSampleId :

ETK90

Manual Integrations
APPROVED

apatel

12/30/2019 11:02:10 AM

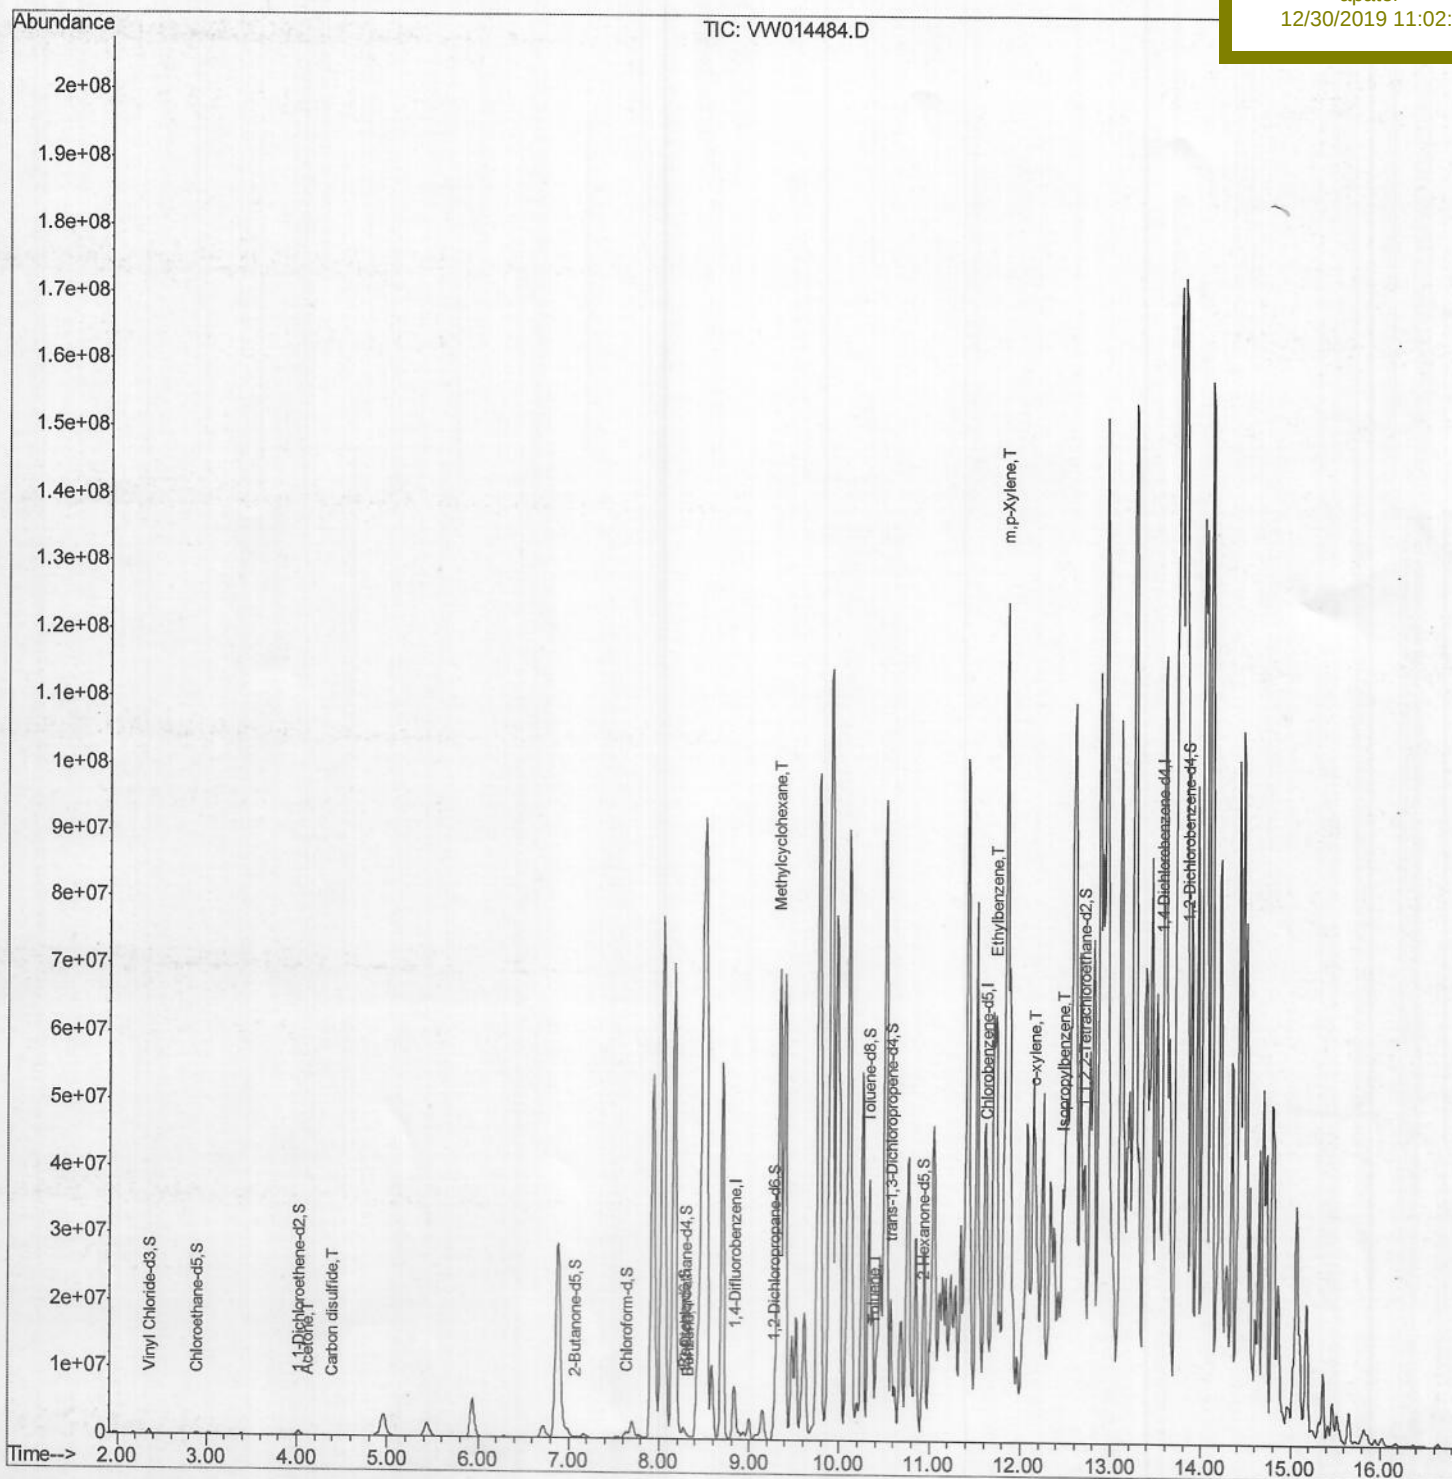

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122719\

Data File : VW014484.D

Acq On : 28 Dec 2019 01:17

Operator : SY/VA

Sample : K6397-01

Misc : 5.28G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 03:27:13 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M

Quant Title : VOC Analysis

QLast Update : Sat Dec 28 03:24:24 2019

Response via : Initial Calibration

Instrument :

MSVOA_W




ClientSampled :

ETK90

Manual Integrations
APPROVED

apatel

12/30/2019 11:02:10 AM

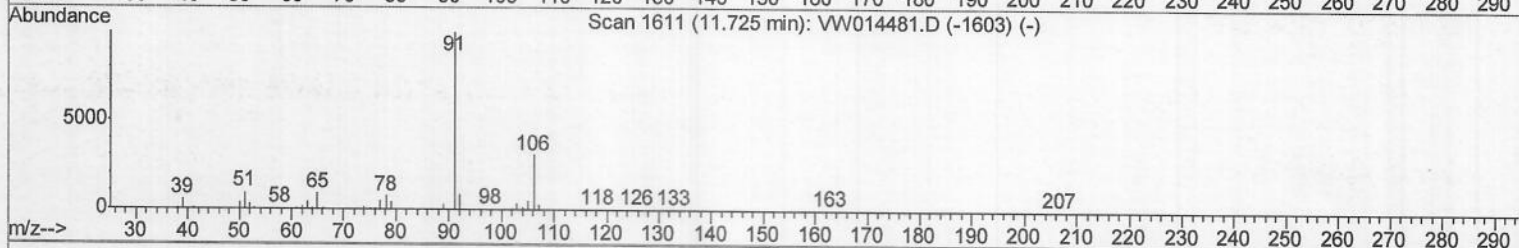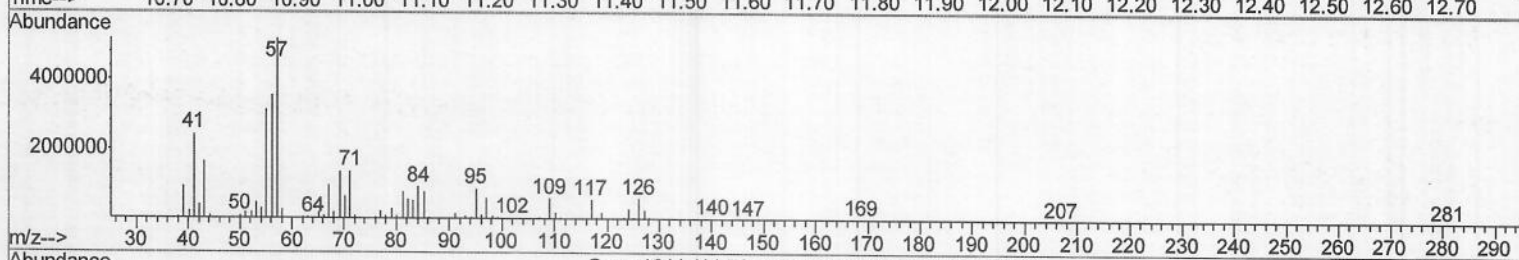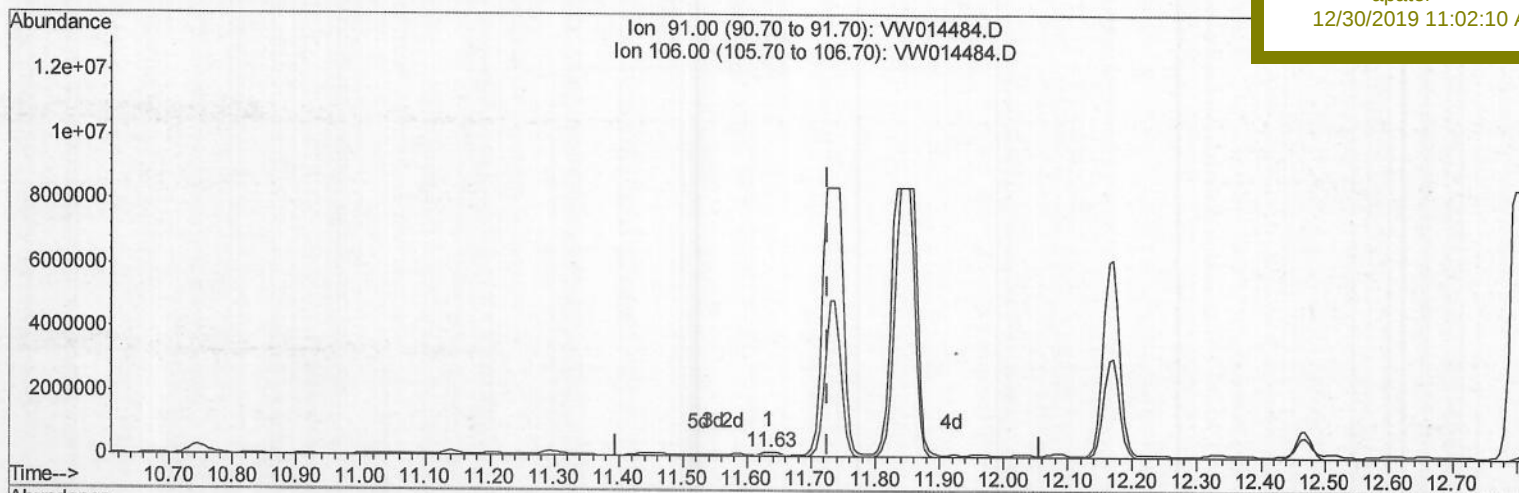

TIC: VW014484.D

(53) Ethylbenzene (T)

11.634min (-0.092) 2.33ug/L

response 160037

Ion	Exp%	Act%
91.00	100	100
106.00	31.20	1.70#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122719\

Data File : VW014484.D

Acq On : 28 Dec 2019 01:17

Operator : SY/VA

Sample : K6397-01

Misc : 5.28G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 03:27:13 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M

Quant Title : VOC Analysis

QLast Update : Sat Dec 28 03:24:24 2019

Response via : Initial Calibration

Instrument :

MSVOA_W




ClientSampled :

ETK90

Manual Integrations
APPROVED

apatel

12/30/2019 11:02:10 AM

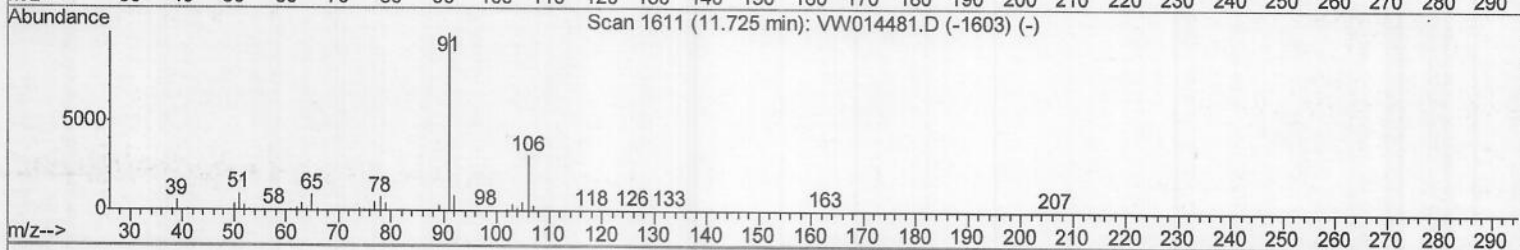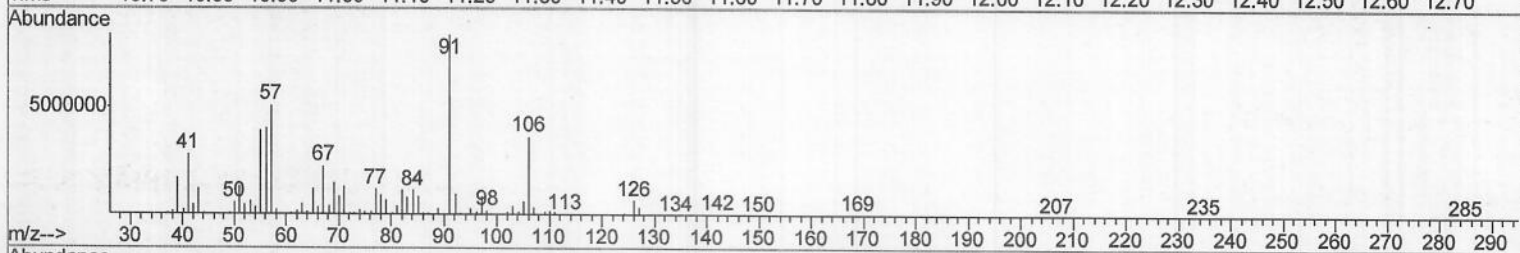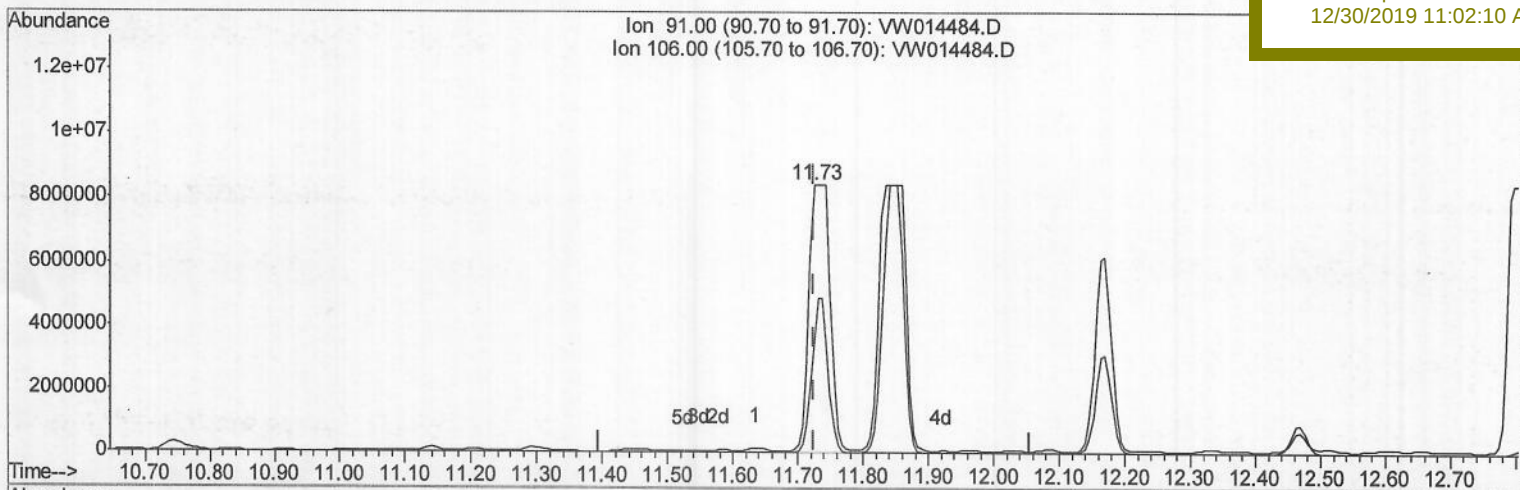

TIC: VW014484.D

(53) Ethylbenzene (T)

11.725min (-0.000) 278.05ug/L m

response 19058433

Ion	Exp%	Act%
91.00	100	100
106.00	31.20	43.37#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122719\

Data File : VW014484.D

Acq On : 28 Dec 2019 01:17

Operator : SY/VA

Sample : K6397-01

Misc : 5.28G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 03:27:13 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M

Quant Title : VOC Analysis

QLast Update : Sat Dec 28 03:24:24 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :




ETK90

Manual Integrations

APPROVED

apatel

12/30/2019 11:02:10 AM

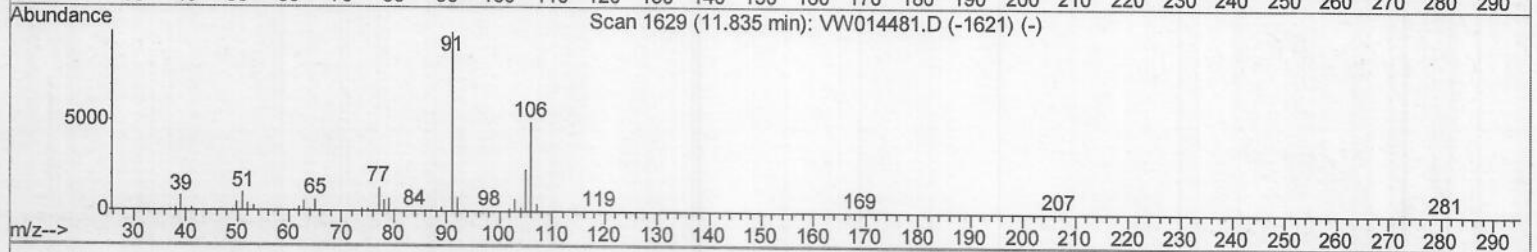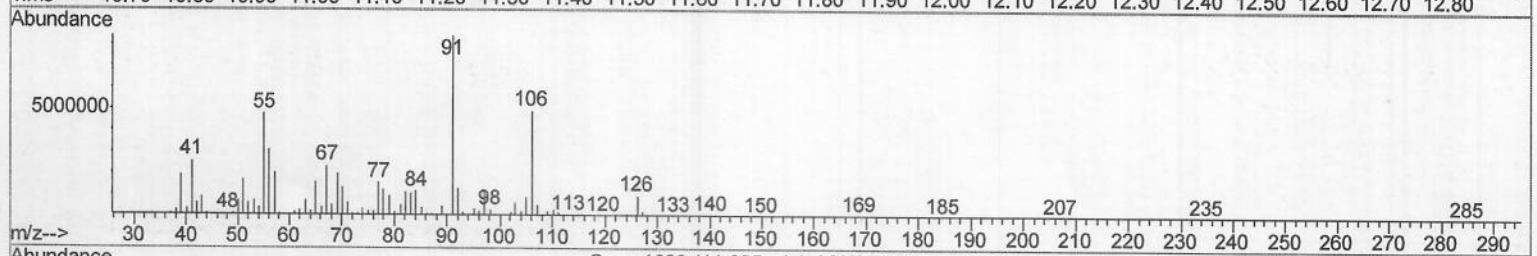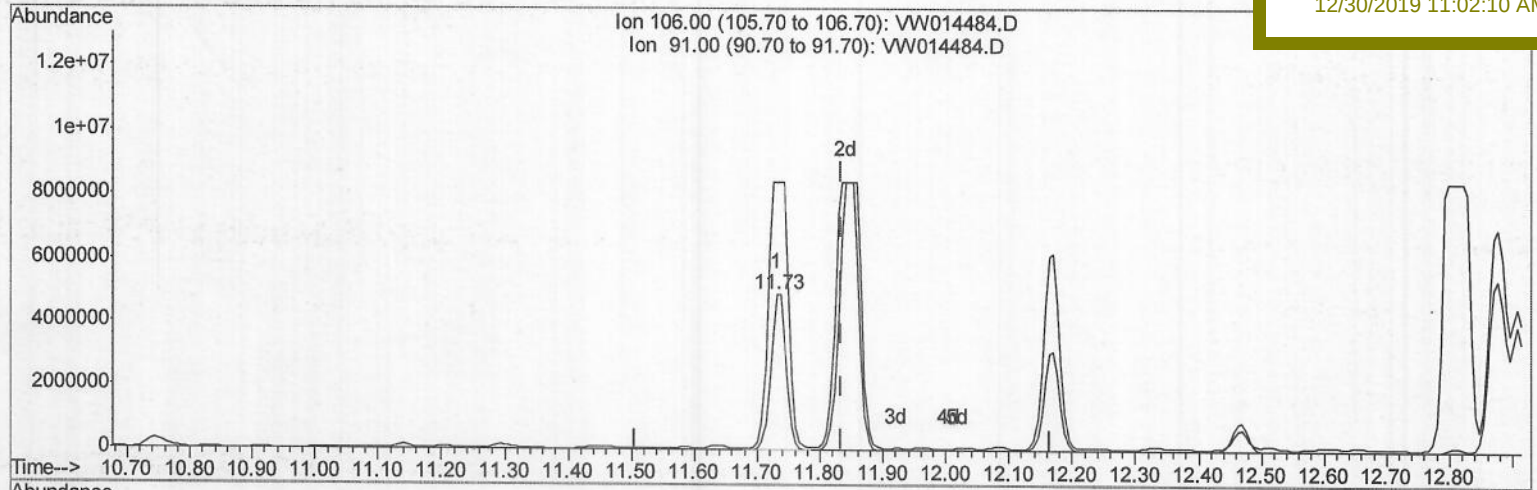

TIC: VW014484.D

(54) m,p-Xylene (T)

11.731min (-0.104) 320.62ug/L

response 8316550

Ion	Exp%	Act%
106.00	100	100
91.00	203.10	171.48
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122719\

Data File : VW014484.D

Acq On : 28 Dec 2019 01:17

Operator : SY/VA

Sample : K6397-01

Misc : 5.28G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 03:27:13 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M

Quant Title : VOC Analysis

QLast Update : Sat Dec 28 03:24:24 2019

Response via : Initial Calibration

Instrument :

MSVOA_W


ClientSampled :

ETK90

Manual Integrations
APPROVED

apatel

12/30/2019 11:02:10 AM

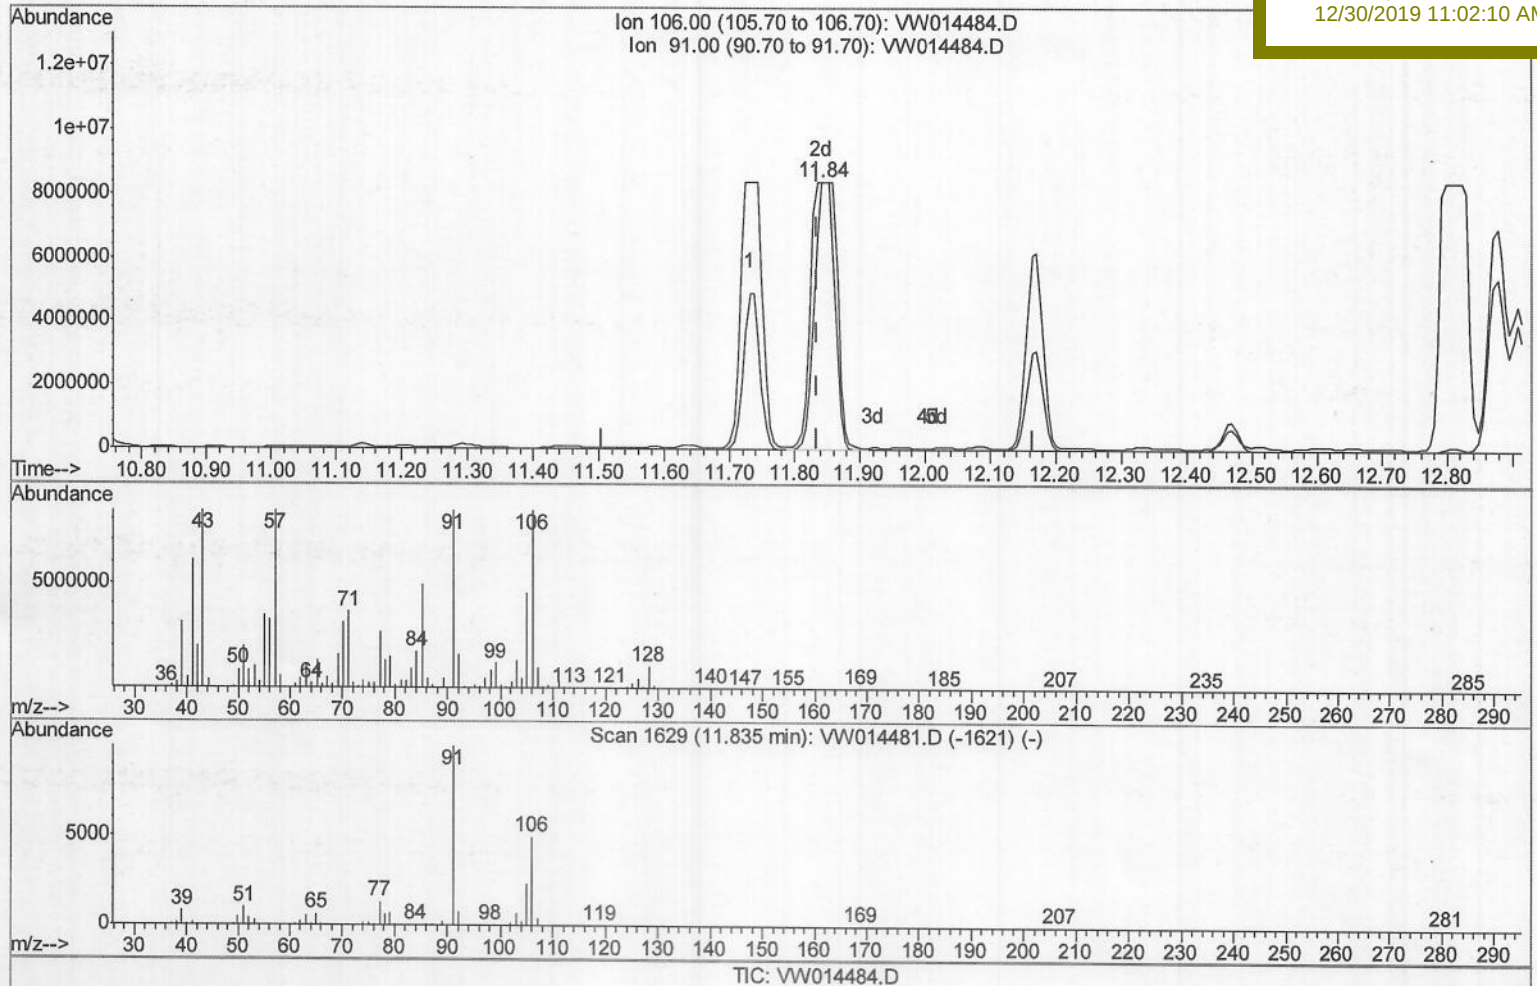

(54) m,p-Xylene (T)

11.841min (+0.006) 693.92ug/L m

response 17999237

Ion	Exp%	Act%
106.00	100	100
91.00	203.10	100.00#
0.00	0.00	0.00
0.00	0.00	0.00

> 12/28/19 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW122719\
 Data File : VW014484.D
 Acq On : 28 Dec 2019 01:17
 Operator : SY/VA
 Sample : K6397-01
 Misc : 5.28G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 ETK90

Quant Time: Dec 28 04:01:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 28 03:24:24 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 12/30/2019 11:02:10 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1263994	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	991304	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	451885	25.00	ug/L	0.01

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	418371	23.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.92%
7) Chloroethane-d5	2.89	69	345685	26.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.32%
10) 1,1-Dichloroethene-d2	4.03	63	586659	18.00	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.00%
20) 2-Butanone-d5	7.07	46	205848	48.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.10%
24) Chloroform-d	7.65	84	754916	25.96	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.84%
26) 1,2-Dichloroethane-d4	8.30	65	359313	23.81	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.24%
29) Benzene-d6	8.27	84	1531654	29.05	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	116.20%
33) 1,2-Dichloropropane-d6	9.27	67	597397	37.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	150.76%#
37) Toluene-d8	10.32	98	2338829	48.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	195.76%#
38) trans-1,3-Dichloropropene-	10.57	79	332190	50.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	202.96%#
39) 2-Hexanone-d5	10.92	63	224133	82.70	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	165.40%#
48) 1,1,2,2-Tetrachloroethane-	12.71	84	827483	69.52	ug/L	0.02
Spiked Amount	25.000	Range	45 - 120	Recovery	=	278.08%#
61) 1,2-Dichlorobenzene-d4	13.86	152	408194	27.41	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.64%

Target Compounds

					Ovalue
13) Acetone	4.12	43	69894	11.906	ug/L 92
14) Carbon disulfide	4.38	76	61456	1.231	ug/L 96
34) Benzene	8.32	78	84210	1.412	ug/L 100
36) Methylcyclohexane	9.34	83	13263554	491.046	ug/L # 67
44) Toluene	10.39	91	394199	6.323	ug/L 98
53) Ethylbenzene	11.73	91	19058433m	278.047	ug/L
54) m,p-Xylene	11.84	106	17999237m	693.917	ug/L
55) o-xylene	12.17	106	5280516	215.527	ug/L 91
57) Isopropylbenzene	12.47	105	14961416	229.569	ug/L 94

12/28/195y

(#) = qualifier out of range (m) = manual integration (+) = signals summed