
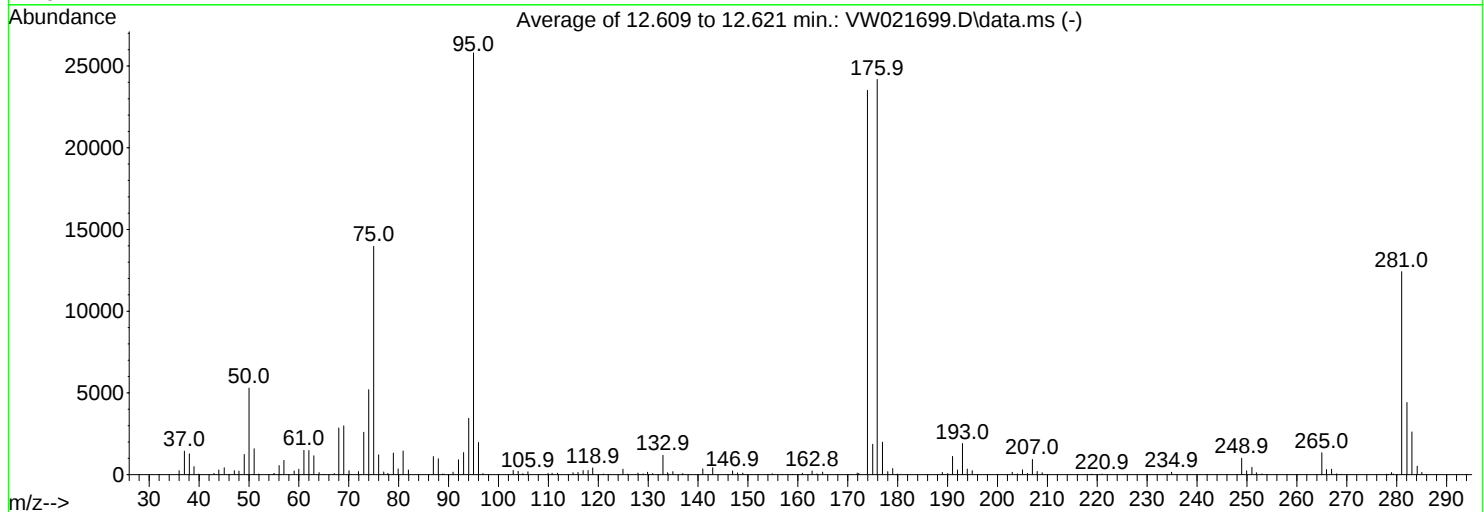


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW123021\
Data File : VW021699.D
Acq On : 30 Dec 2021 07:44
Operator : SY/VA
Sample : BFB492
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB492

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Title : SFAM01.0
Last Update : Fri Dec 31 00:51:50 2021

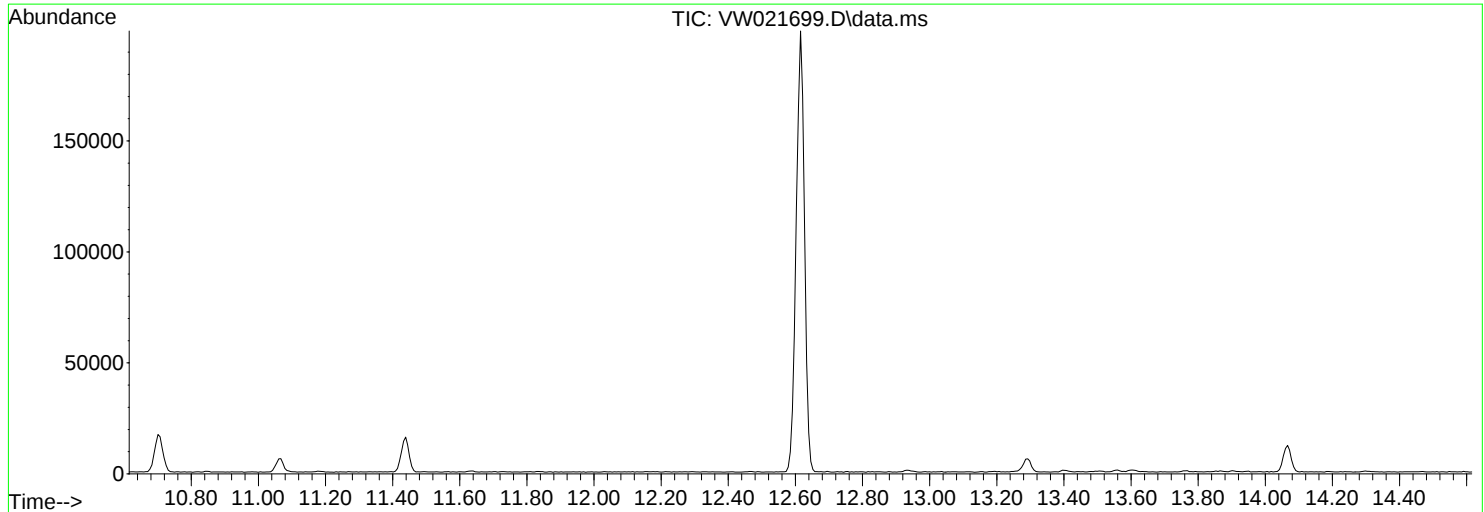

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	5293	PASS
75	95	30	80	54.1	13971	PASS
95	95	100	100	100.0	25808	PASS
96	95	5	9	7.6	1970	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.1	23520	PASS
175	174	5	9	7.9	1857	PASS
176	174	95	105	102.8	24179	PASS
177	176	5	10	8.2	1986	PASS

m/z	Abundance
40.00	808.0
73.00	54.0
132.90	54.0
281.00	151.0

Instrument :
MSVOA_W
ClientSampleId :
BFB492

m/z	Abundance
36.10	225.0
37.00	1217.0
38.10	1190.0
39.00	406.0
39.90	844.0
43.00	154.0
43.90	286.0
45.10	570.0
46.00	61.0
47.00	235.0
48.10	189.0
49.10	1010.0
50.00	4869.0
51.10	1495.0
52.00	65.0
54.90	122.0
56.10	434.0
57.00	751.0
59.00	365.0
60.00	338.0
61.00	1340.0
62.00	1164.0
63.00	960.0
64.10	120.0
65.00	64.0
68.00	2511.0
69.00	2581.0
70.00	203.0
72.00	182.0
73.10	3203.0
74.00	4566.0
75.00	11716.0
76.00	1090.0
77.00	153.0
79.00	1151.0
79.90	347.0
80.90	1164.0
81.90	283.0
86.00	54.0
86.90	988.0
87.90	731.0
88.80	120.0
90.90	154.0
92.00	755.0
93.00	1218.0
94.00	2698.0
95.00	22608.0
96.00	1781.0
96.80	107.0
103.00	451.0
104.00	243.0
104.80	136.0
106.00	166.0
109.90	97.0
110.70	142.0
111.90	121.0
115.00	134.0
115.90	145.0
116.90	254.0
118.00	367.0
118.90	539.0
121.10	60.0
125.00	512.0
128.00	102.0
130.00	115.0
130.90	93.0
132.00	69.0
133.00	1797.0
133.90	360.0
134.90	245.0
136.90	73.0
140.90	270.0
142.90	386.0
146.80	358.0
147.80	88.0
149.00	118.0
158.90	59.0
160.90	184.0
162.90	371.0
163.80	103.0
164.90	223.0
171.90	172.0
174.00	16600.0
175.00	1396.0
175.90	18536.0
177.00	1747.0
178.00	264.0
179.00	559.0
180.00	117.0
189.00	208.0
190.10	138.0
191.00	1882.0

Instrument :
MSVOA_W
ClientSampleId :
BFB492

192.00	427.0
193.00	2796.0
194.00	479.0
194.90	371.0
203.00	256.0
204.00	87.0
205.00	446.0
206.00	143.0
207.00	1188.0
208.00	272.0
209.00	155.0
221.00	69.0
234.90	182.0
249.00	1319.0
250.00	297.0
251.00	765.0
252.00	196.0
253.00	84.0
265.00	1950.0
266.00	413.0
267.00	455.0
268.00	97.0
268.90	52.0
278.00	88.0
279.00	240.0
281.00	13730.0
282.10	5516.0
283.10	3158.0
284.10	931.0
285.10	158.0

Instrument :
MSVOA_W
ClientSampleId :
BFB492

m/z	Abundance
36.00	234.0
37.00	1608.0
38.10	1263.0
39.00	561.0
40.00	824.0
43.00	91.0
43.90	295.0
45.00	398.0
47.00	224.0
47.90	226.0
49.00	1490.0
50.00	6178.0
51.00	1742.0
51.90	60.0
55.10	134.0
56.00	665.0
57.00	1047.0
59.10	241.0
60.00	395.0
61.00	1693.0
62.00	1679.0
63.00	1292.0
64.00	160.0
67.10	106.0
68.00	3178.0
69.00	3411.0
70.10	244.0
72.00	187.0
73.00	2737.0
74.00	5711.0
75.00	15762.0
76.00	1418.0
77.10	204.0
77.80	91.0
78.90	1445.0
79.90	413.0
80.90	1646.0
81.90	290.0
86.90	1361.0
87.90	1101.0
89.10	85.0
90.90	175.0
92.00	1010.0
93.00	1508.0
94.00	3959.0
95.00	28712.0
96.00	2215.0
96.90	50.0
102.90	223.0
103.90	225.0
105.00	91.0
105.80	215.0
110.00	139.0
110.80	65.0
111.80	75.0
114.90	115.0
115.90	139.0
117.00	275.0
118.00	182.0
118.90	403.0
121.00	59.0
124.90	256.0
125.90	127.0
128.00	108.0
129.00	68.0
129.80	137.0
130.90	61.0
133.00	1370.0
135.00	192.0
137.00	74.0
140.90	382.0
143.00	450.0
146.90	162.0
147.90	145.0
148.90	101.0
154.80	99.0
156.90	54.0
160.90	87.0
162.80	198.0
163.80	54.0
165.00	157.0
172.20	221.0
173.90	26008.0
175.00	2112.0
175.90	27240.0
177.00	2293.0
178.00	201.0
179.00	385.0
179.70	61.0
188.90	117.0
189.90	77.0
191.00	939.0

Instrument :
MSVOA_W
ClientSampleId :
BFB492

192.00	289.0
193.00	2009.0
193.90	393.0
195.00	274.0
202.90	117.0
204.00	58.0
205.00	309.0
206.10	91.0
207.00	1125.0
207.90	192.0
209.00	156.0
218.90	99.0
220.90	50.0
235.00	158.0
248.90	1148.0
249.90	281.0
251.00	351.0
251.80	147.0
253.00	62.0
265.00	1493.0
265.90	338.0
266.90	332.0
268.00	59.0
278.90	154.0
281.10	14930.0
282.00	5378.0
283.00	3328.0
284.10	386.0
285.10	163.0

Instrument :
MSVOA_W
ClientSampleId :
BFB492

m/z	Abundance
35.90	275.0
37.10	1487.0
38.00	1374.0
39.00	495.0
40.00	875.0
44.00	260.0
45.10	299.0
47.10	264.0
48.00	219.0
49.00	1186.0
50.00	4833.0
51.00	1508.0
55.00	100.0
56.00	567.0
57.00	812.0
59.00	82.0
60.00	272.0
61.00	1444.0
62.00	1600.0
63.00	1204.0
64.00	101.0
67.10	89.0
68.00	2880.0
69.00	2980.0
70.00	290.0
71.90	179.0
73.00	1992.0
74.00	5311.0
75.00	14435.0
76.00	1145.0
76.90	129.0
77.90	142.0
78.90	1371.0
79.90	299.0
80.90	1528.0
82.00	271.0
87.00	969.0
88.00	1085.0
90.90	141.0
92.00	958.0
93.00	1318.0
94.10	3688.0
95.00	26104.0
96.00	1914.0
97.00	54.0
103.10	119.0
104.00	157.0
105.90	162.0
110.80	52.0
111.90	57.0
115.00	116.0
116.00	129.0
116.90	241.0
117.90	202.0
118.90	293.0
125.00	246.0
127.80	91.0
129.00	79.0
129.90	192.0
130.90	62.0
133.00	537.0
134.10	99.0
135.00	133.0
136.90	63.0
141.00	396.0
142.90	417.0
147.00	163.0
148.00	100.0
148.90	83.0
154.90	81.0
162.90	98.0
165.00	80.0
171.90	128.0
174.00	27952.0
175.00	2064.0
175.90	26760.0
176.90	1918.0
178.00	105.0
178.90	169.0
189.00	76.0
191.00	536.0
191.90	151.0
192.90	919.0
194.00	164.0
195.00	80.0
202.90	78.0
205.10	135.0
207.00	485.0
208.00	117.0
208.80	55.0
234.80	92.0
248.90	538.0

Instrument :
MSVOA_W
ClientSampleId :
BFB492

250.00	124.0
251.00	231.0
265.10	595.0
266.00	191.0
267.00	218.0
278.30	62.0
279.30	110.0
281.00	9065.0
282.00	2355.0
283.00	1362.0
284.00	229.0
284.90	100.0

Instrument :
MSVOA_W
ClientSampleId :
BFB492