



Dichlorodifluoromethane

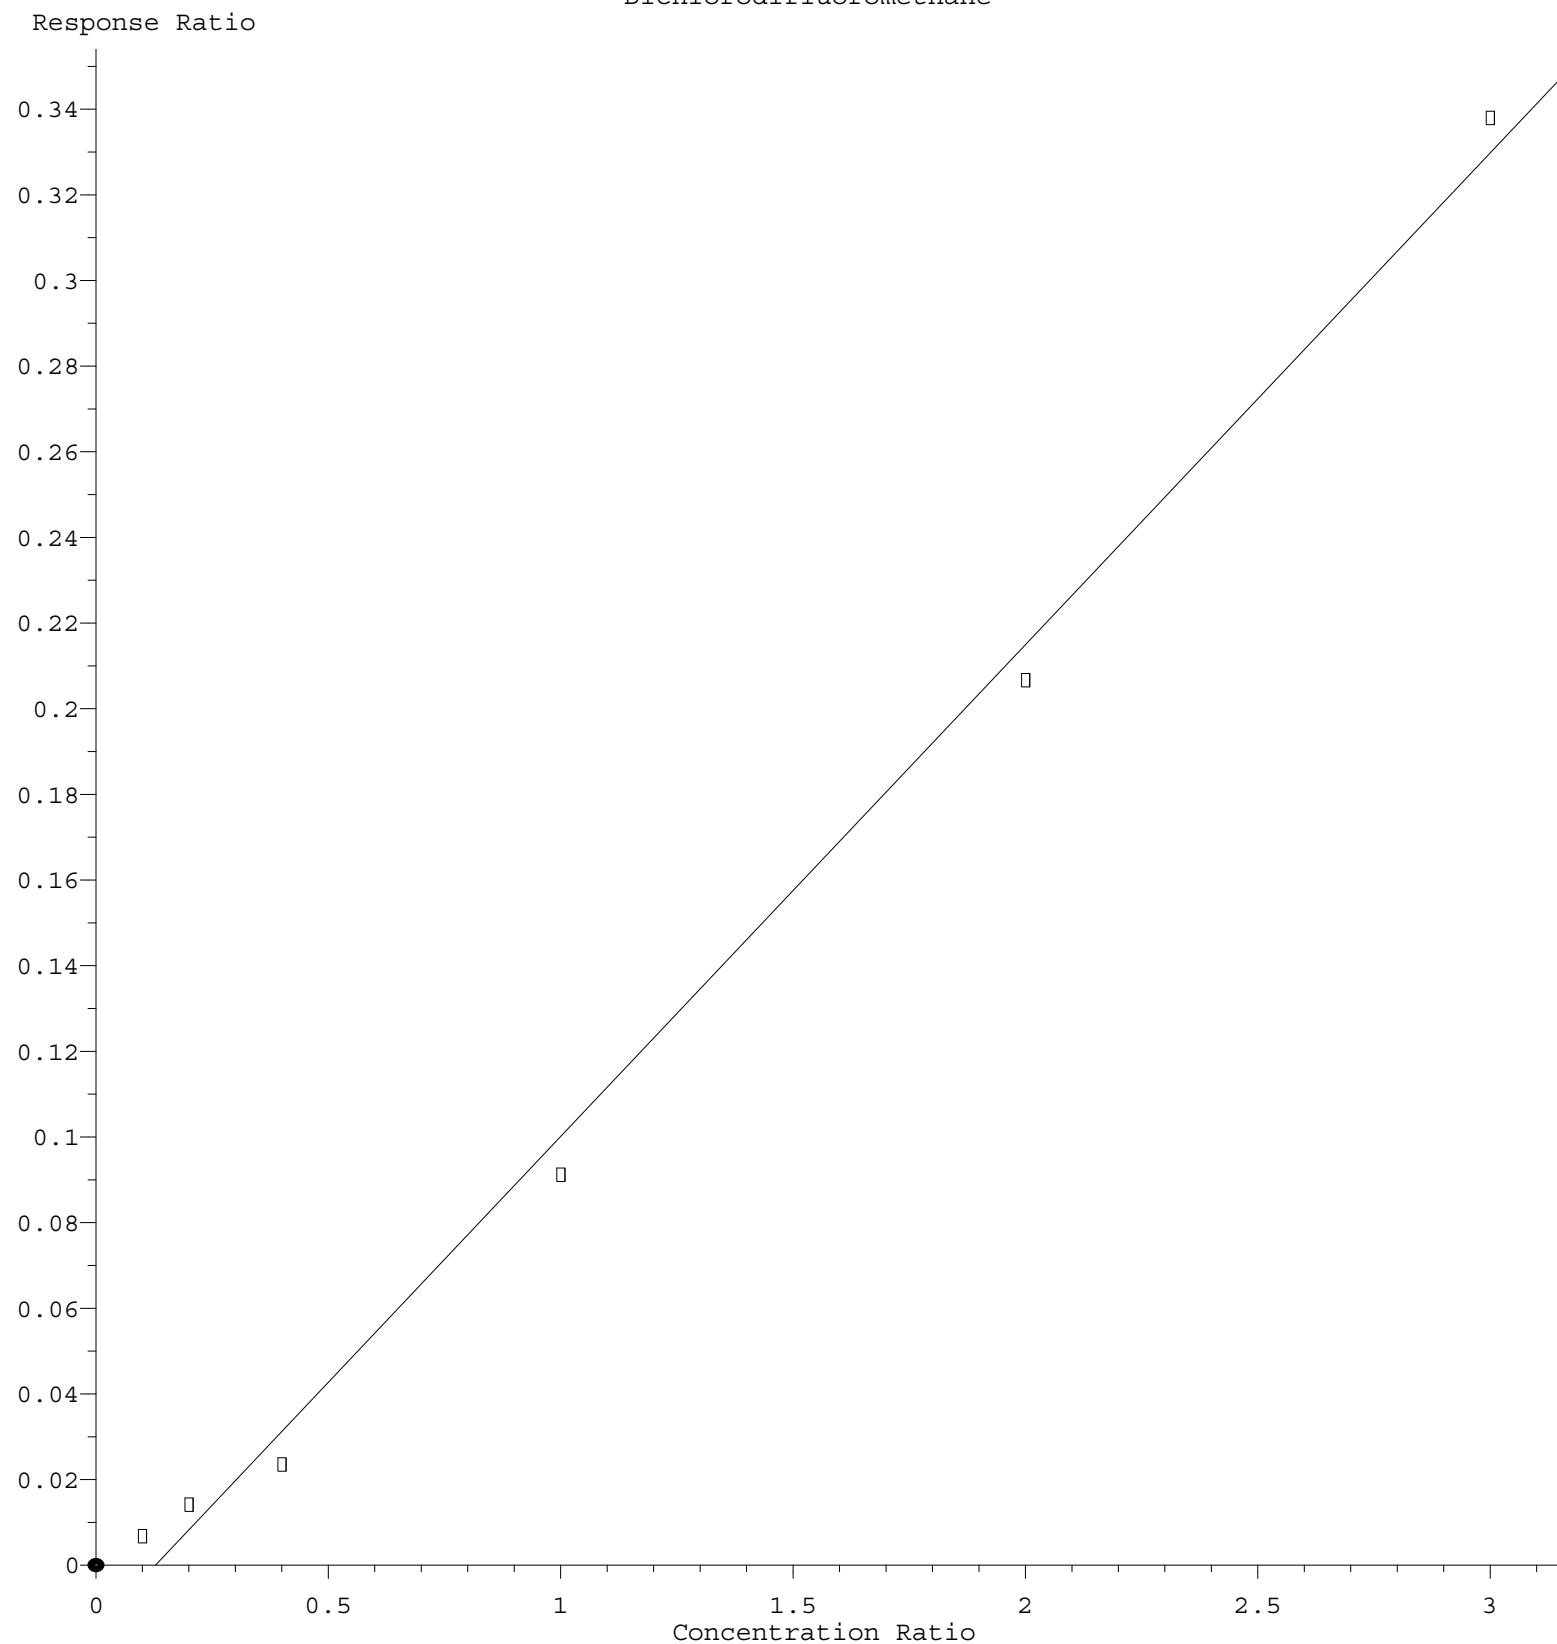

Response = $1.147 \times 10^{-1} \times \text{Amt} - 1.472 \times 10^{-2}$
 Coef of Det (r^2) = 0.995393 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010522S.M
 Calibration Table Last Updated: Wed Jan 05 14:56:42 2022


Tert butyl alcohol

Response Ratio

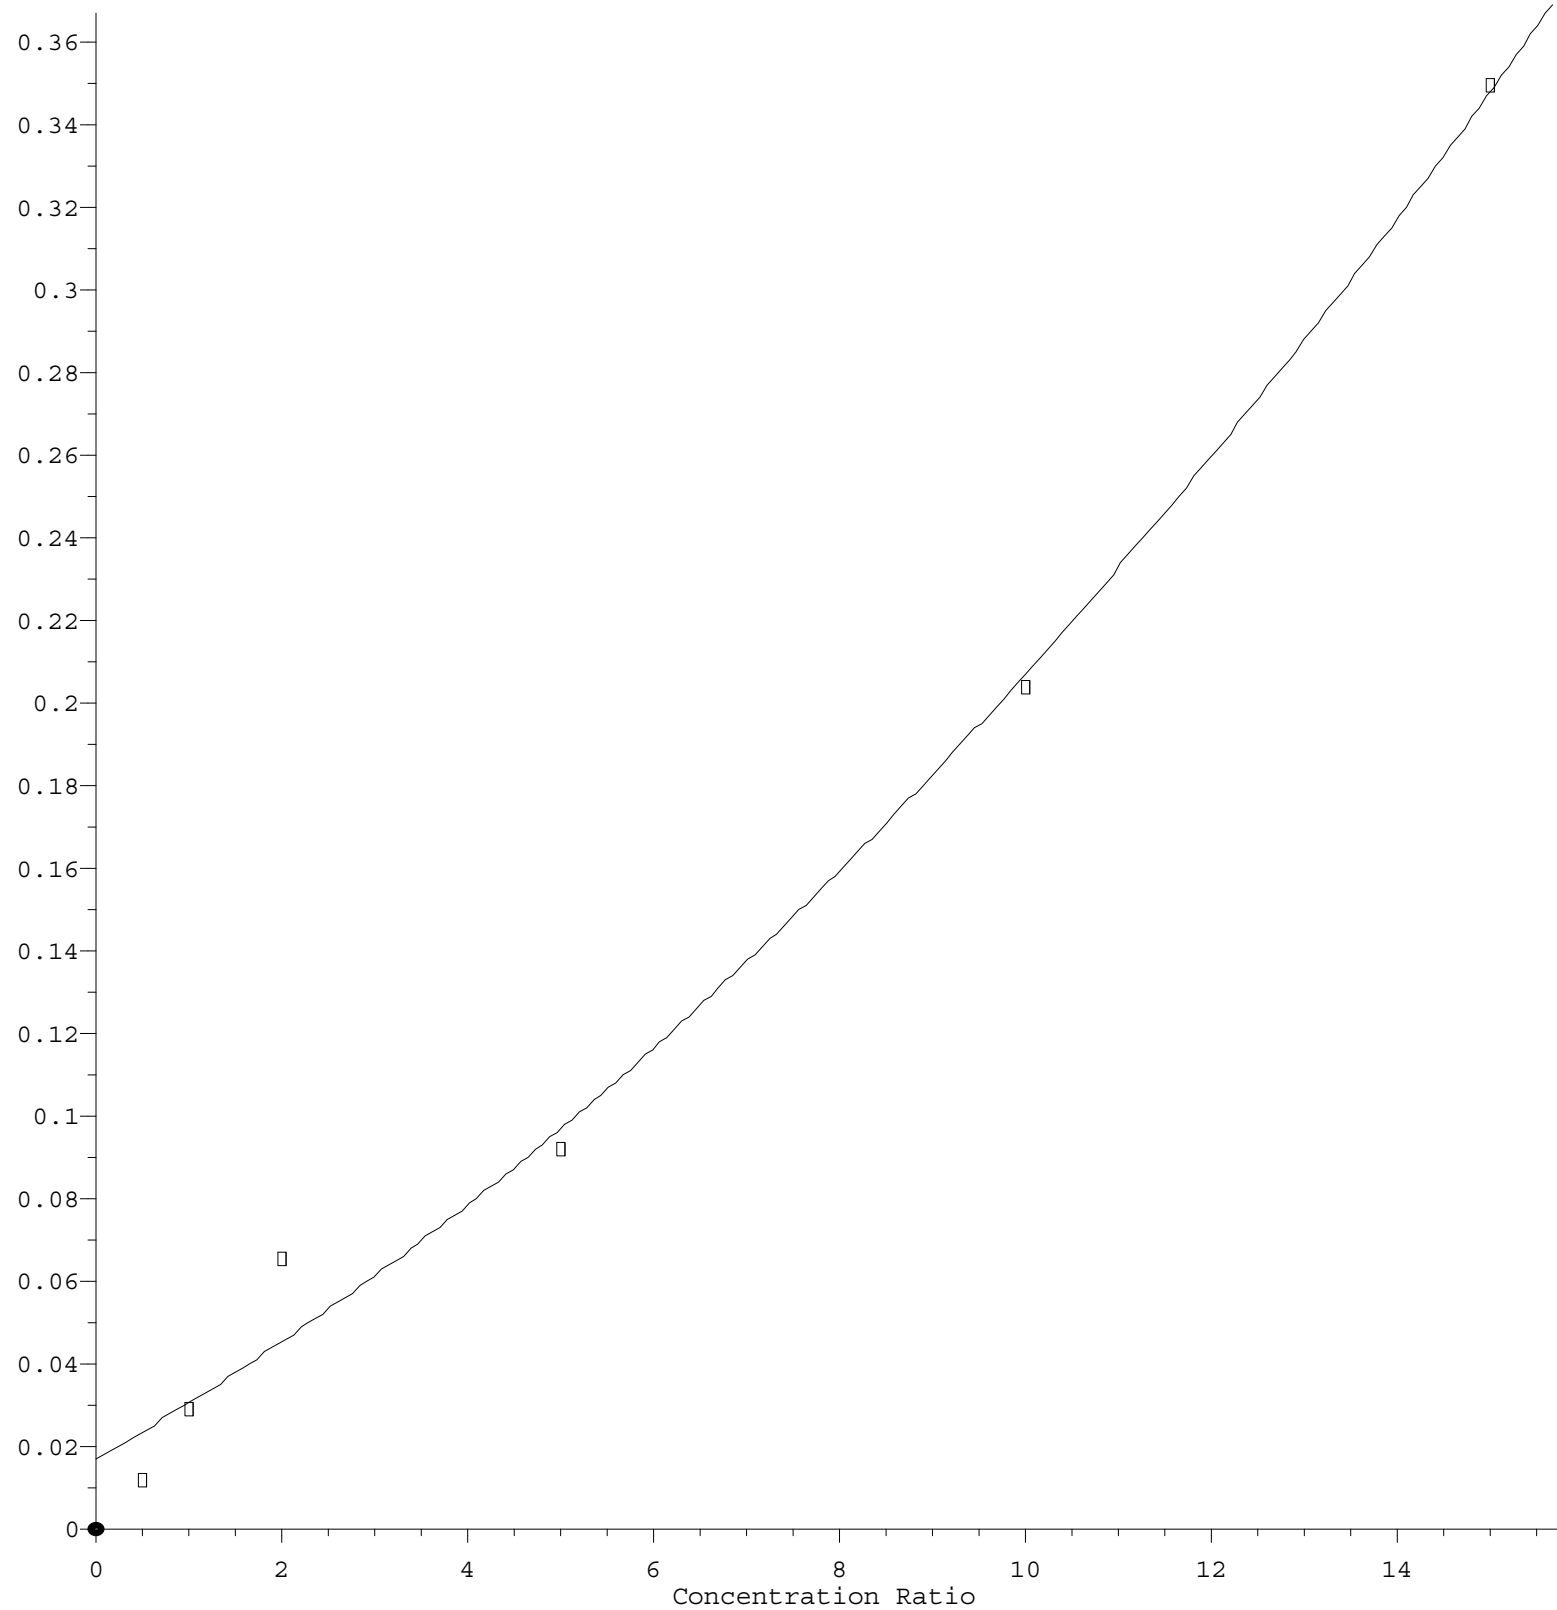

$R = 6.088e-004 A^2 + 1.292e-002 A + 1.711e-002$
 Coef of Det (r^2) = 0.992986 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010522S.M
 Calibration Table Last Updated: Wed Jan 05 14:56:42 2022


Acrolein

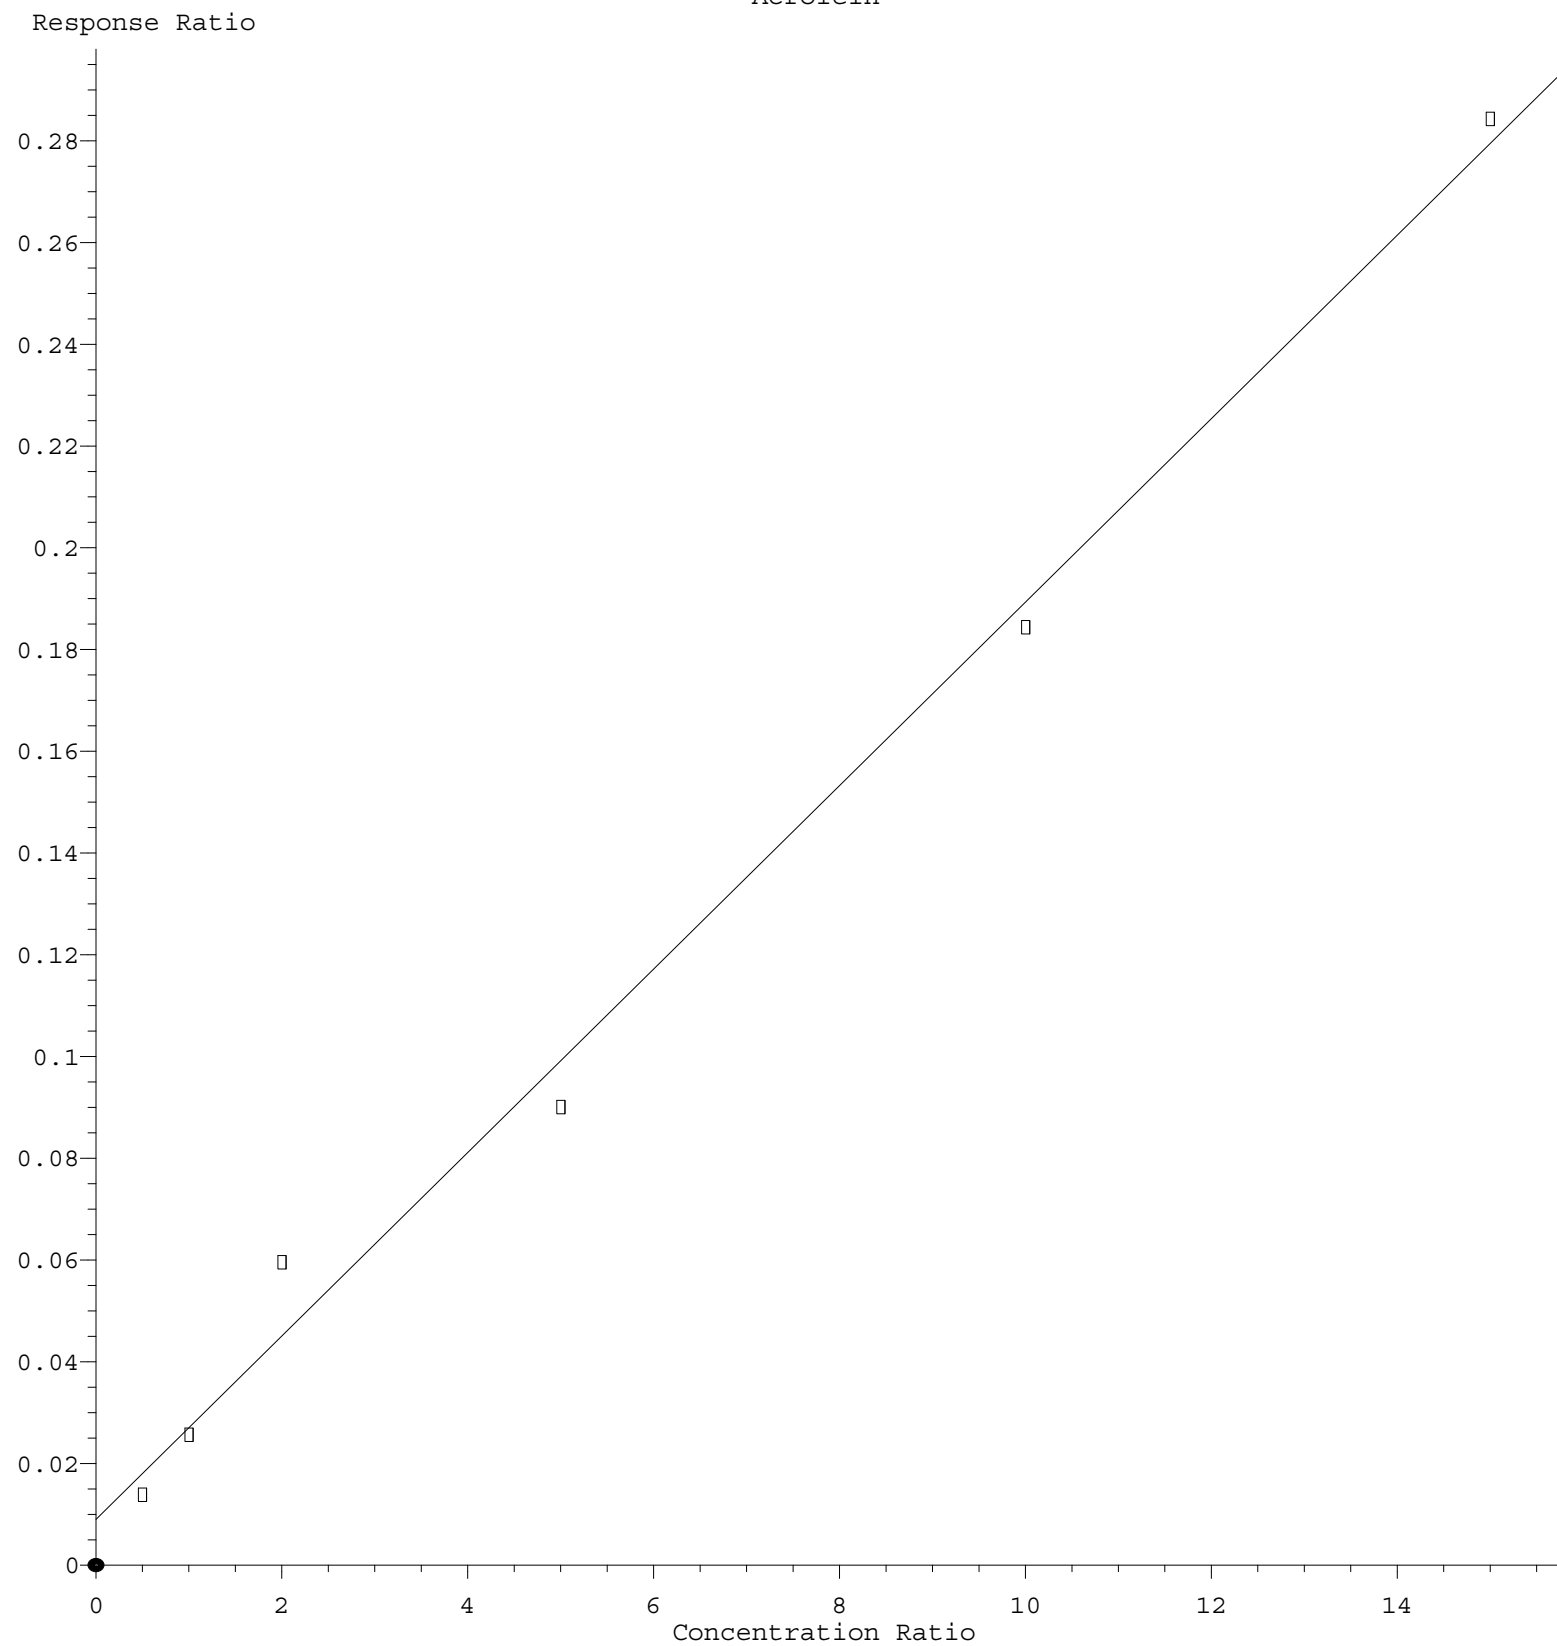

Response = $1.806 \times 10^{-2} \times \text{Amt} + 8.798 \times 10^{-3}$
 Coef of Det (r^2) = 0.993489 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010522S.M
 Calibration Table Last Updated: Wed Jan 05 14:56:42 2022

Methylene Chloride

Response Ratio

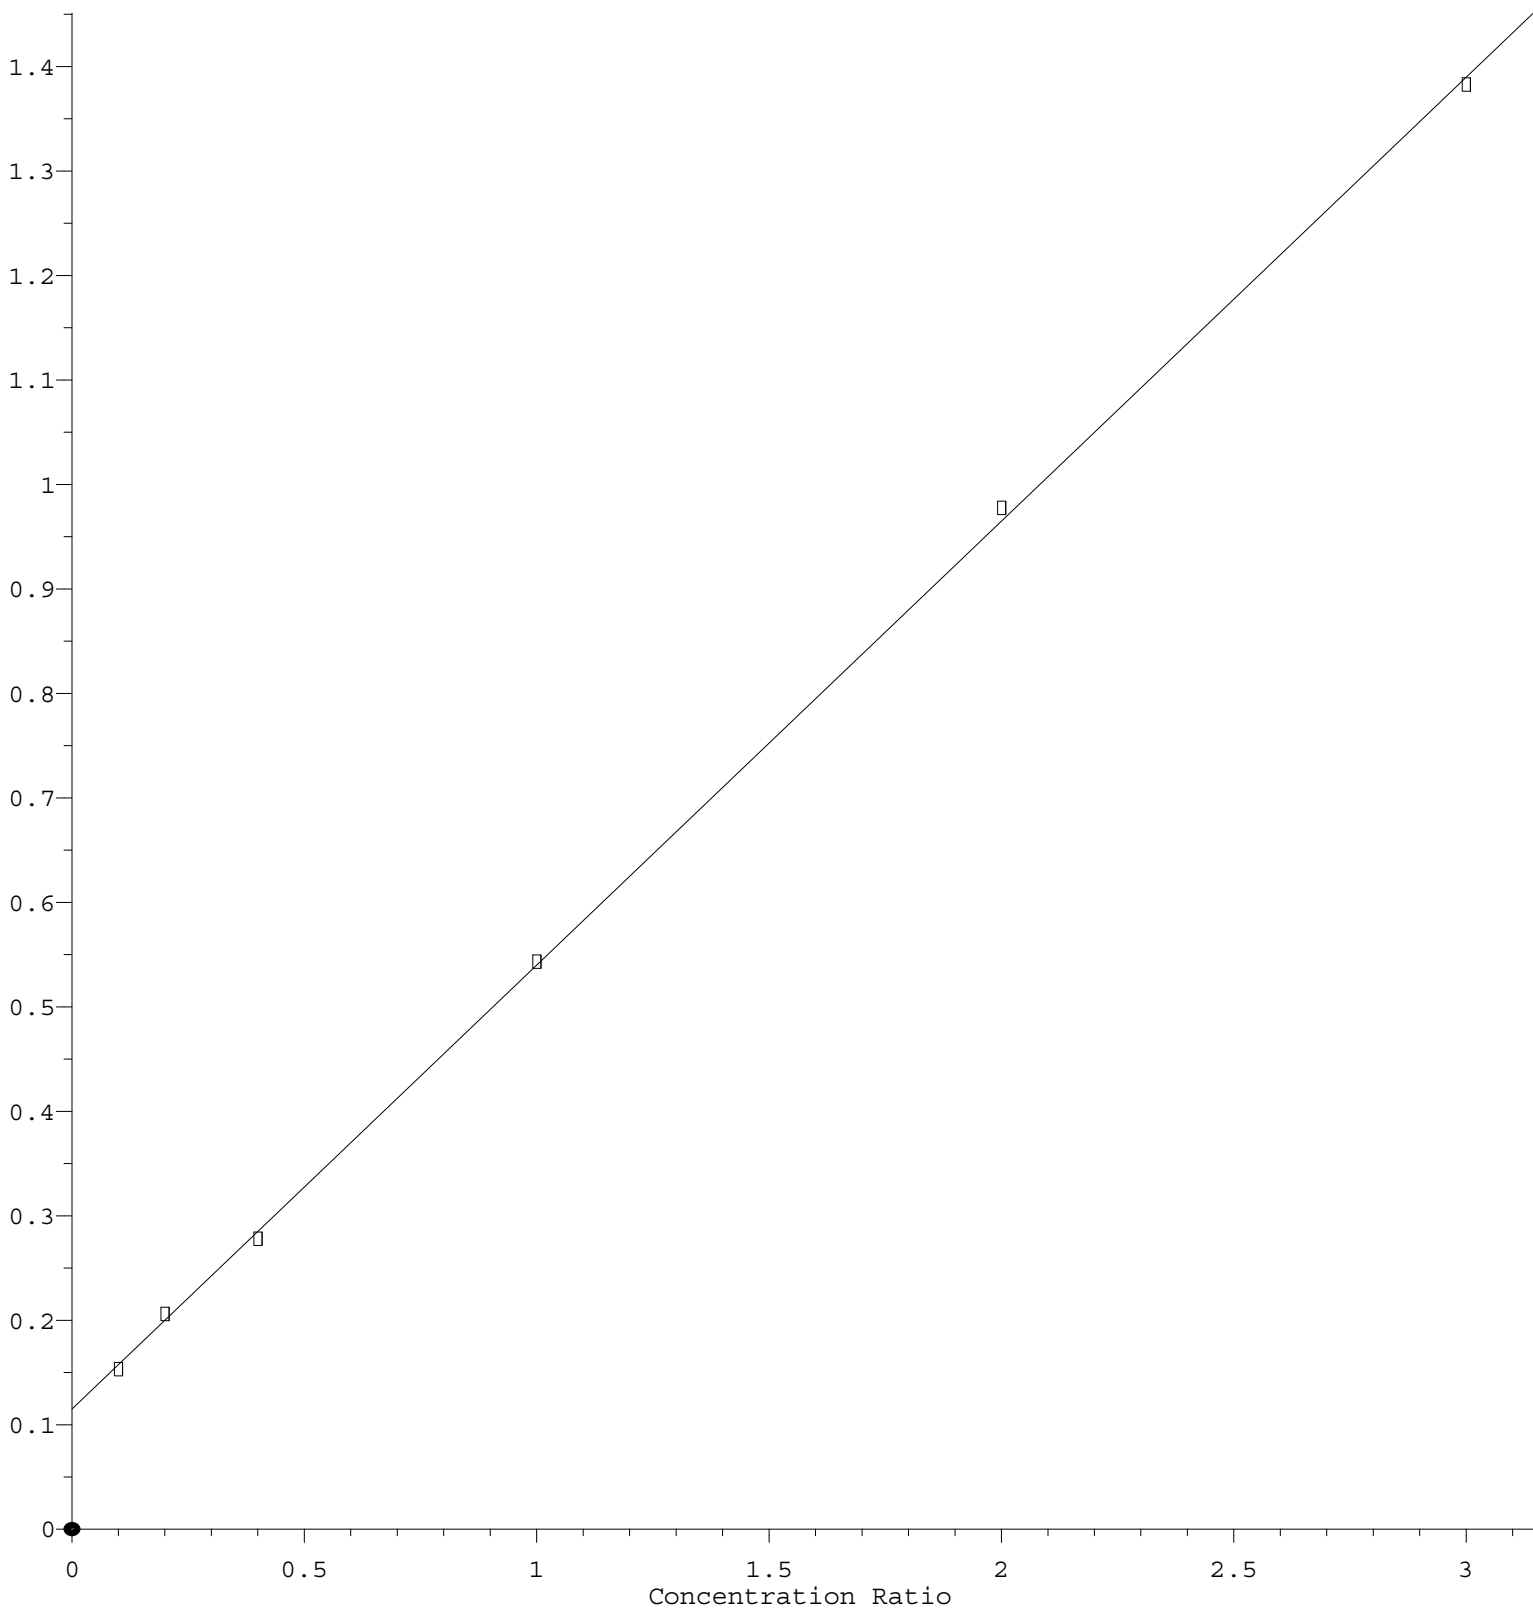


$$\text{Response} = 4.251\text{e-}001 * \text{Amt} + 1.154\text{e-}001$$

Coef of Det (r^2) = 0.999738 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010522S.M

Calibration Table Last Updated: Wed Jan 05 14:56:42 2022

Bromoform

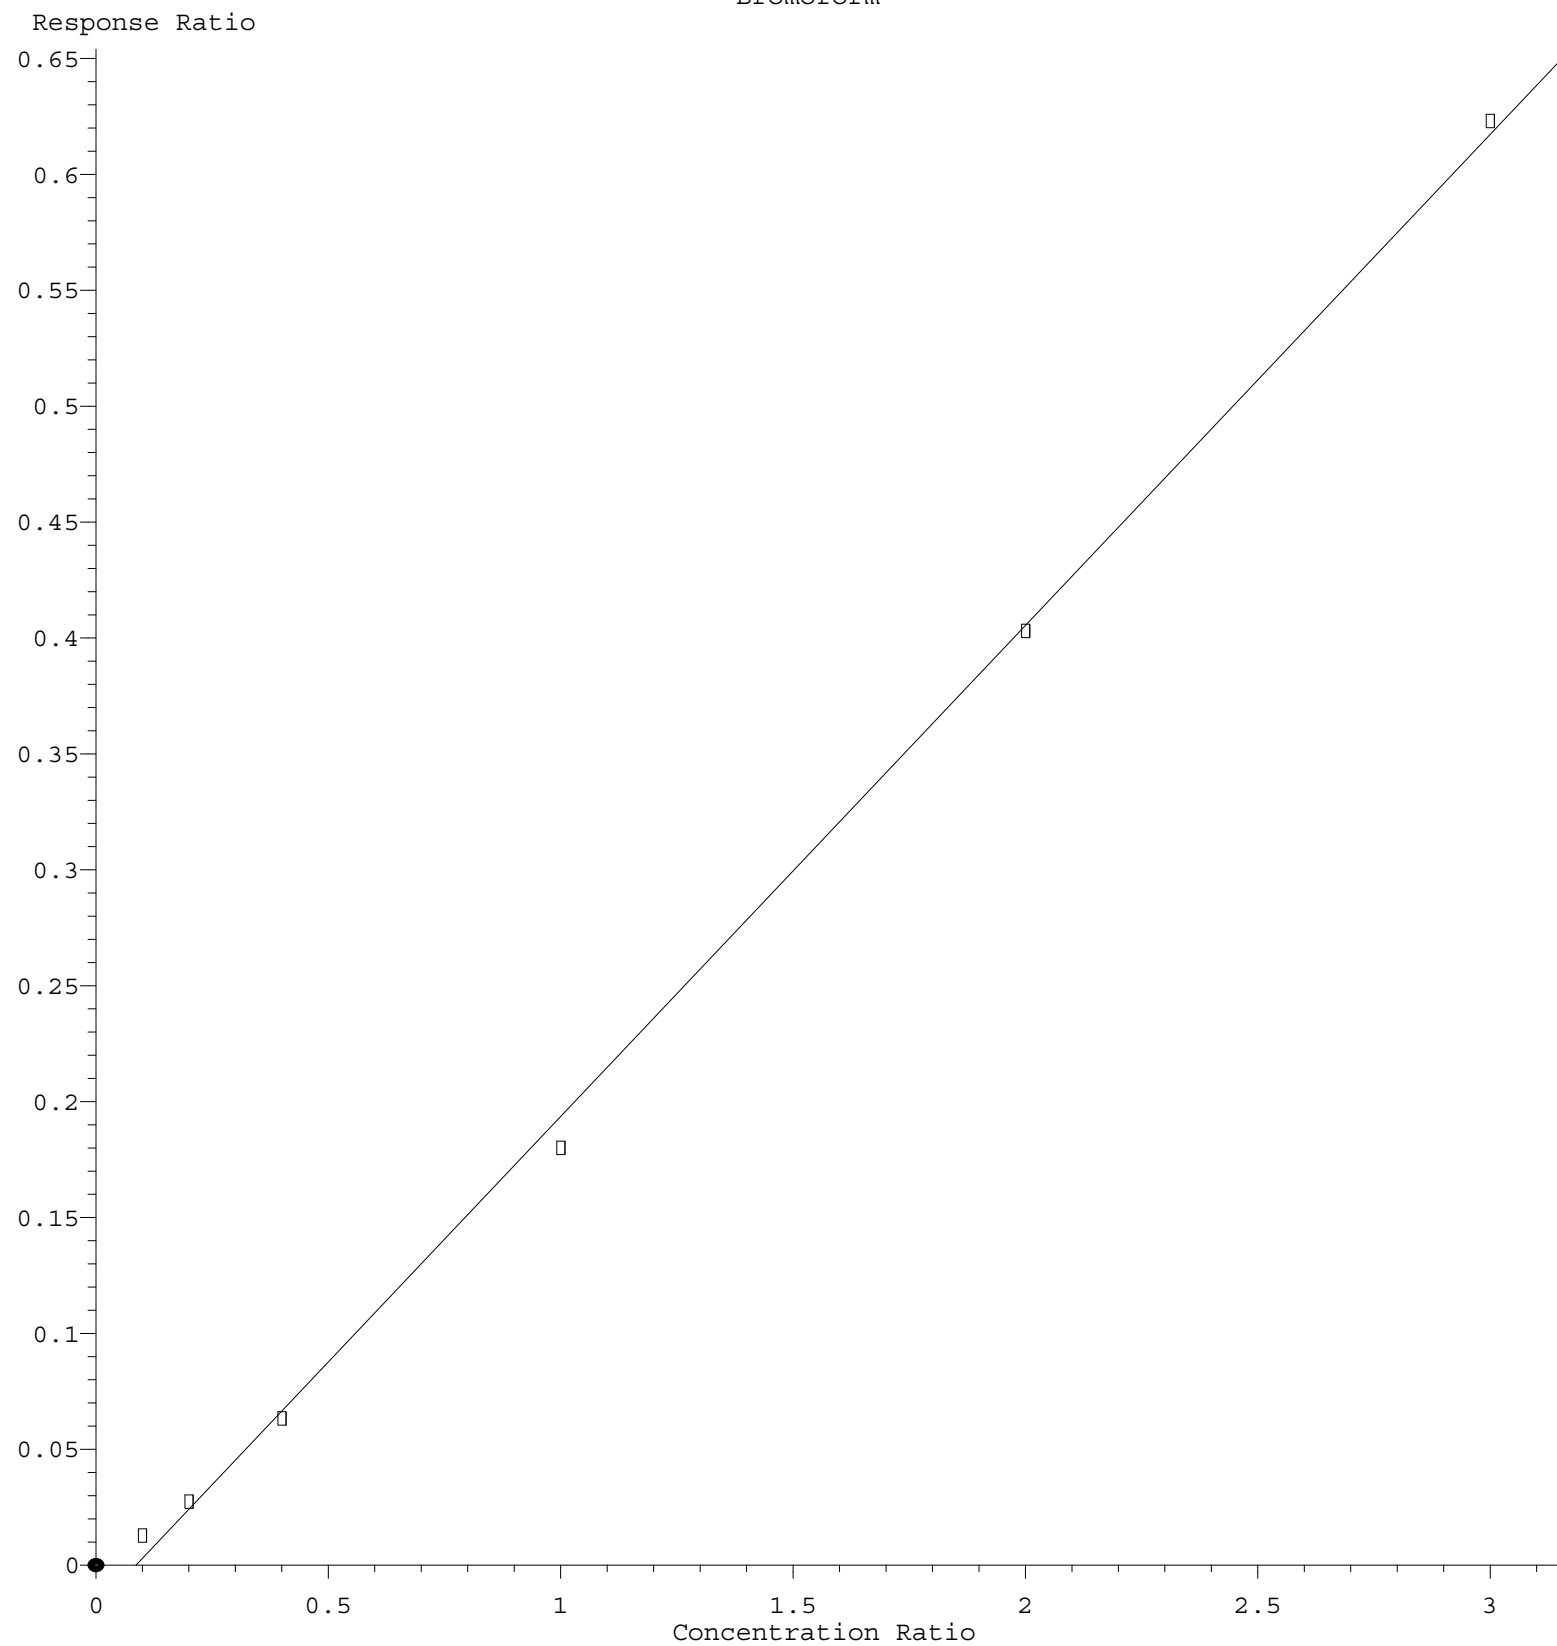

Response = 2.118e-001 * Amt - 1.822e-002
 Coef of Det (r^2) = 0.998867 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010522S.M
 Calibration Table Last Updated: Wed Jan 05 14:56:42 2022