
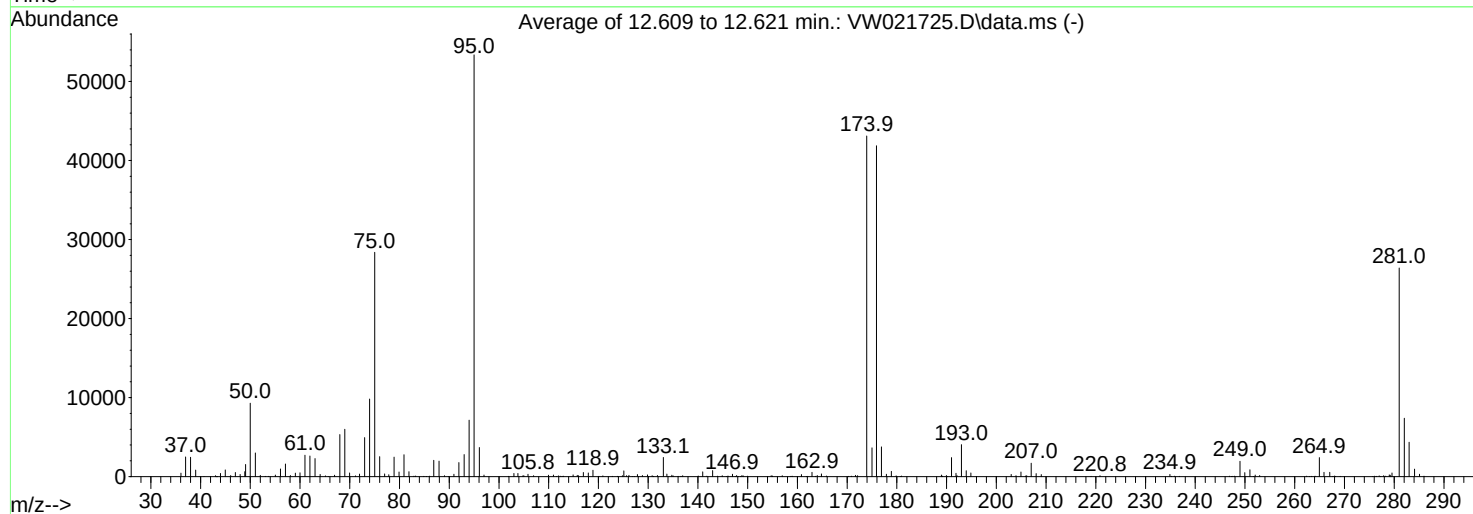


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010522\
Data File : VW021725.D
Acq On : 05 Jan 2022 10:12
Operator : SY/VA
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W010522S.M
Title : SW846 8260
Last Update : Wed Jan 05 14:56:42 2022

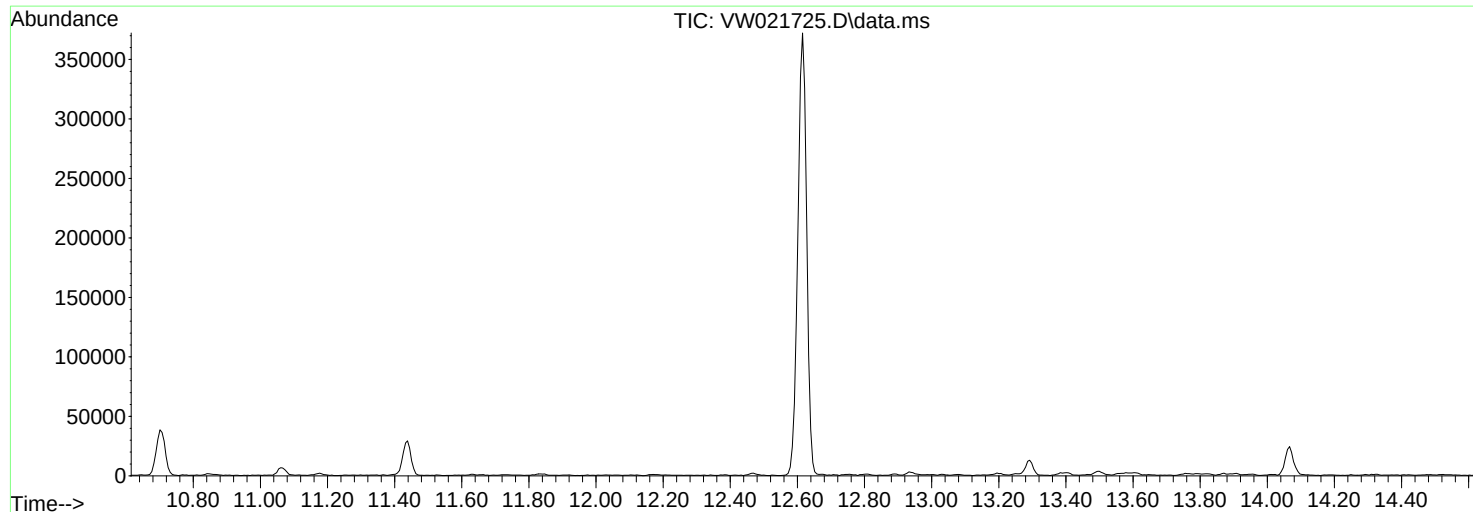

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	9295	PASS
75	95	30	60	53.2	28381	PASS
95	95	100	100	100.0	53373	PASS
96	95	5	9	6.9	3694	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.8	43107	PASS
175	174	5	9	8.5	3653	PASS
176	174	95	101	97.1	41872	PASS
177	176	5	9	9.0	3762	PASS