




Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011421\
 Data File : VW017873.D
 Acq On : 14 Jan 2021 12:32
 Operator : SY/VA
 Sample : M1117-01RE
 Misc : 6.13G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
Client Sampled :
 BFN60

Manual Integrations
APPROVED
 MMDadoda
 1/15/2021 6:29:05 PM

Quant Time: Jan 14 21:45:37 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 14 21:44:45 2021
 Response via : Initial Calibration

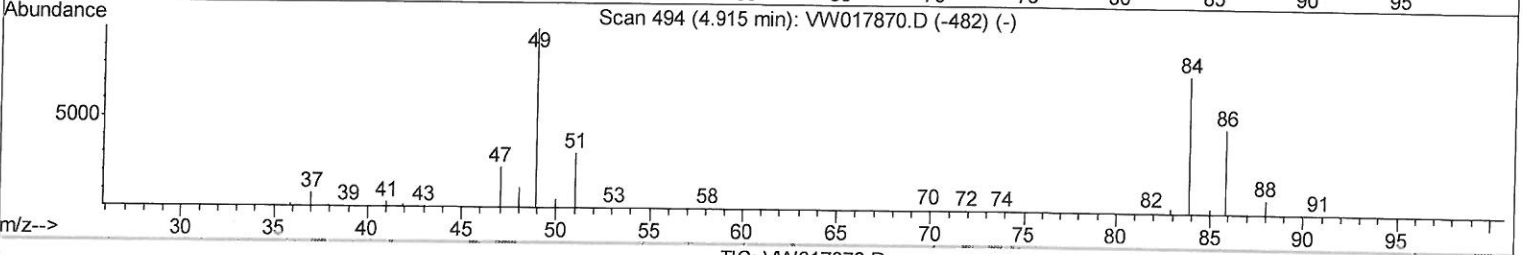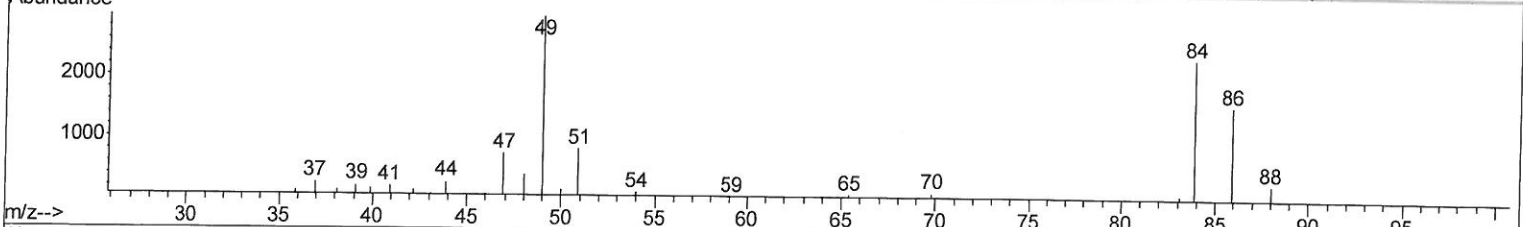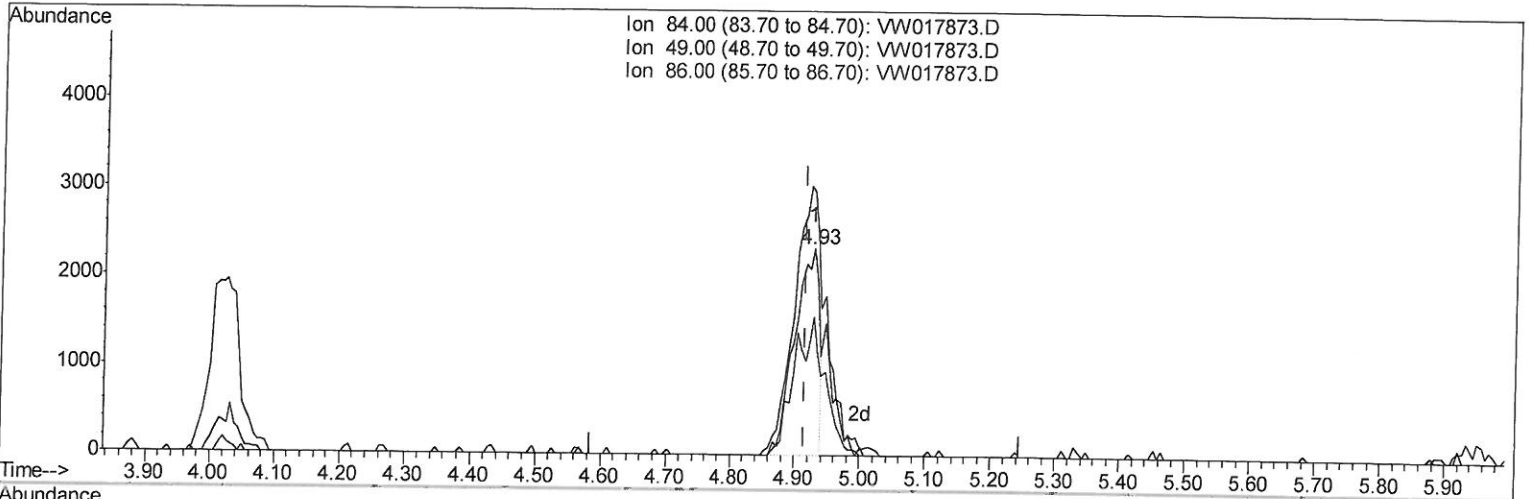

TIC: VW017873.D

(16) Methylene chloride (T)

4.927min (+0.012) 1.25ug/L

response 6101

Ion	Exp%	Act%
84.00	100	100
49.00	129.30	127.51
86.00	64.00	67.14
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011421\
 Data File : VW017873.D
 Acq On : 14 Jan 2021 12:32
 Operator : SY/VA
 Sample : M1117-01RE
 Misc : 6.13G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
Client Sampled :
 BFN60

Manual Integrations
APPROVED
 MMDadoda
 1/15/2021 6:29:05 PM

Quant Time: Jan 14 21:45:37 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 14 21:44:45 2021
 Response via : Initial Calibration

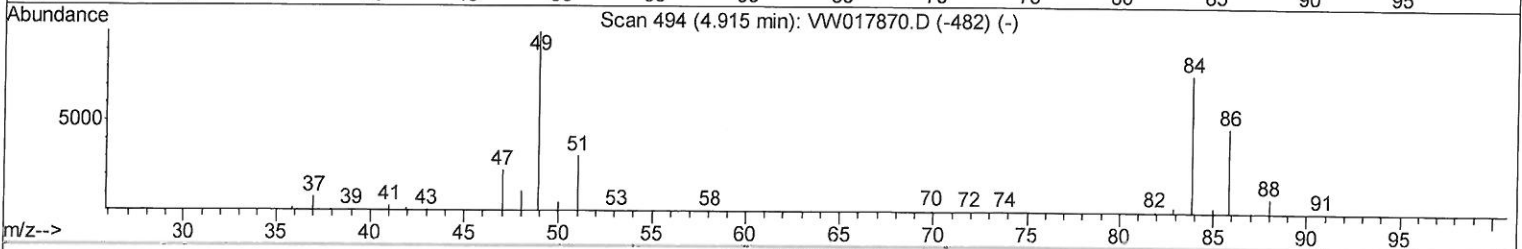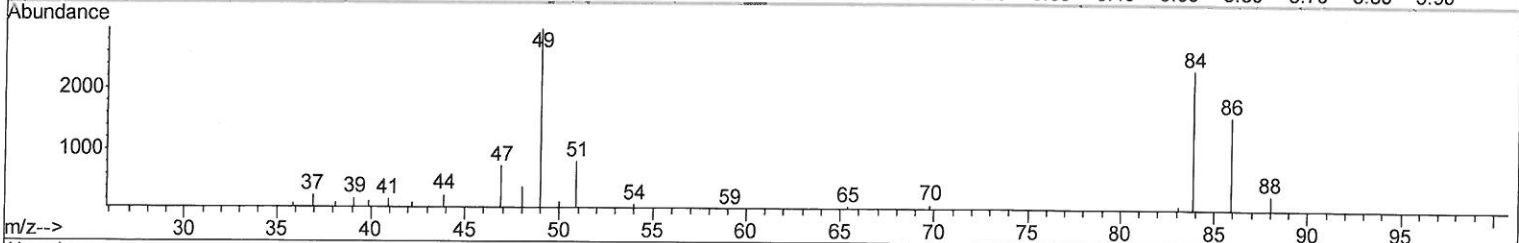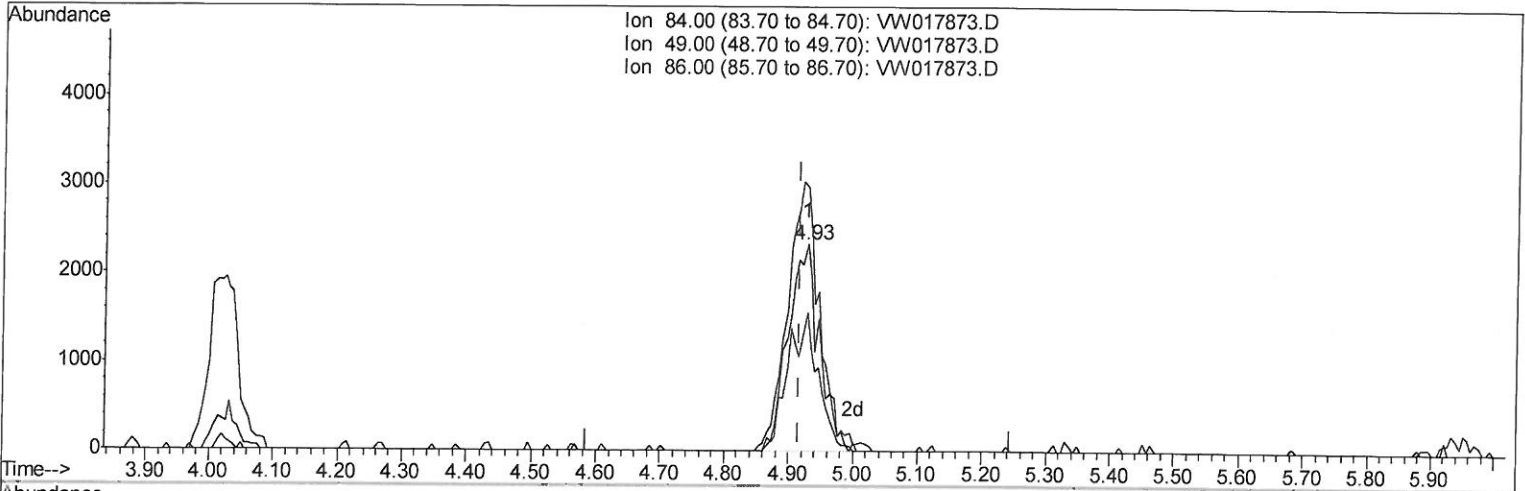

TIC: VW017873.D

(16) Methylene chloride (T)

4.927min (+0.012) 1.60ug/L m

Handwritten: > 01/18/21 SY

response 7825

Ion	Exp%	Act%
84.00	100	100
49.00	129.30	127.51
86.00	64.00	67.14
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011421\
 Data File : VW017873.D
 Acq On : 14 Jan 2021 12:32
 Operator : SY/VA
 Sample : M1117-01RE
 Misc : 6.13G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
Client Sampled :
 BFN60

Manual Integrations
APPROVED
 MMDadoda
 1/15/2021 6:29:05 PM

Quant Time: Jan 14 23:09:30 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 14 21:44:45 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	341139	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	270442	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	81295	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	124579	23.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.40%
7) Chloroethane-d5	2.89	69	104407	23.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.88%
10) 1,1-Dichloroethene-d2	4.03	63	159635	17.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.44%
20) 2-Butanone-d5	7.08	46	46871	54.79	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.58%
24) Chloroform-d	7.65	84	213774	23.98	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.92%
26) 1,2-Dichloroethane-d4	8.30	65	122551	26.56	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.24%
29) Benzene-d6	8.27	84	412254	27.06	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.24%
33) 1,2-Dichloropropane-d6	9.27	67	121127	28.84	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.36%
37) Toluene-d8	10.32	98	356867	24.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.56%
38) trans-1,3-Dichloropropene-	10.58	79	43309	23.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.56%
39) 2-Hexanone-d5	10.93	63	31108	58.99	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.98%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	81626	26.18	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.72%
61) 1,2-Dichlorobenzene-d4	13.85	152	66827	23.61	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.44%

Target Compounds

	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.14	43	1404	1.901	ug/L	69
16) Methylene chloride	4.93	84	7825m	1.604	ug/L	74
47) Tetrachloroethene	10.86	164	1099	0.328	ug/L #	

01/18/21 SY

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011421\
 Data File : VW017873.D
 Acq On : 14 Jan 2021 12:32
 Operator : SY/VA
 Sample : M1117-01RE
 Misc : 6.13G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BFN60

Manual Integrations
APPROVED
 MMDadoda
 1/15/2021 6:29:05 PM

Quant Time: Jan 14 23:09:30 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 14 21:44:45 2021
 Response via : Initial Calibration

