
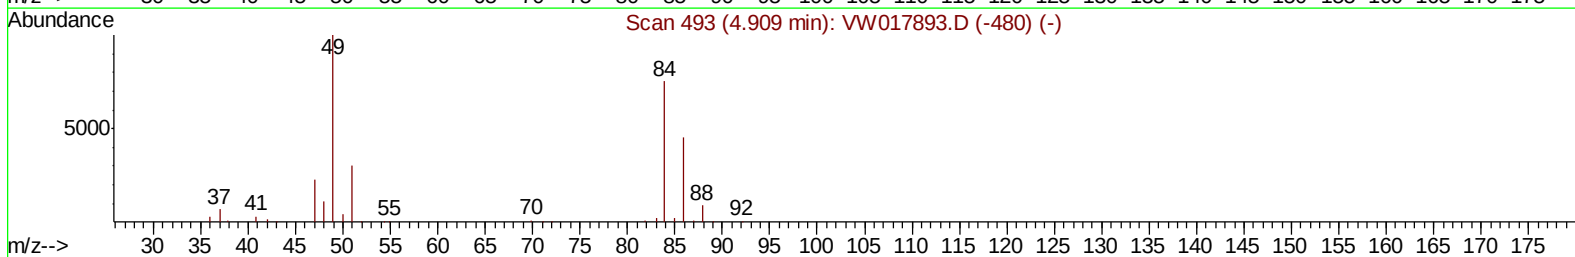
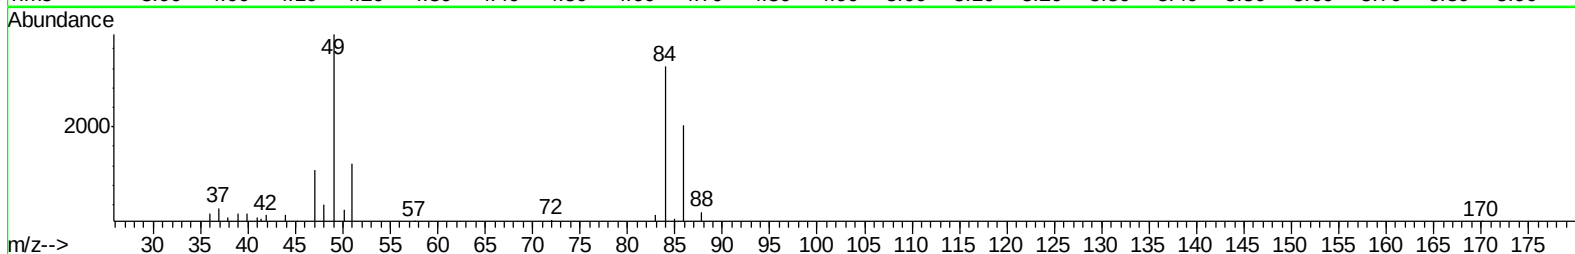


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
Data File : VW017894.D
Acq On : 15 Jan 2021 13:36
Operator : SY/VA
Sample : VW0115SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 02:08:35 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 18 02:07:49 2021
Response via : Initial Calibration

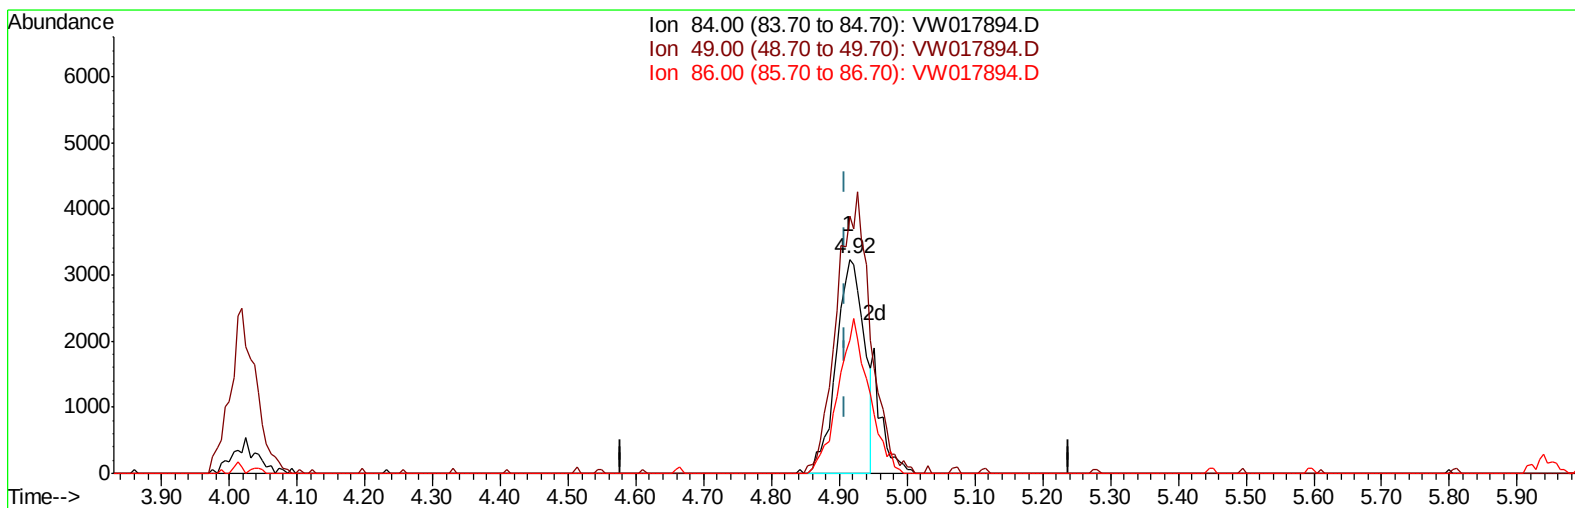

TIC: VW017894.D

(16) Methylene chloride (T)

4.915min (+0.006) 2.04ug/L

response 9332

Ion	Exp%	Act%
84.00	100	100
49.00	116.00	120.59
86.00	63.60	62.53
0.00	0.00	0.00