

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\  
 Data File : VW017901.D  
 Acq On : 15 Jan 2021 16:35  
 Operator : SY/VA  
 Sample : M1099-13  
 Misc : 6.50G/10ML/MSVOA W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :

Quant Time: Jan 18 02:09:25 2021  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\SOM2WLM122420S.M  
 Quant Title : VOC Analysis  
 QLast Update : Mon Jan 18 02:07:49 2021  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Difluorobenzene     | 8.84  | 114  | 289571   | 25.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 11.63 | 117  | 251948   | 25.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 13.55 | 152  | 99743    | 25.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |        |       |          |          |      |          |
|--------------------------------|--------|-------|----------|----------|------|----------|
| 4) Vinyl Chloride-d3           | 2.36   | 65    | 115270   | 25.73    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 30 - 150 | Recovery | =    | 102.92%  |
| 7) Chloroethane-d5             | 2.89   | 69    | 97882    | 26.47    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 30 - 150 | Recovery | =    | 105.88%  |
| 10) 1,1-Dichloroethene-d2      | 4.02   | 63    | 147717   | 18.92    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 45 - 110 | Recovery | =    | 75.68%   |
| 20) 2-Butanone-d5              | 7.08   | 46    | 50906    | 70.10    | ug/L | 0.00     |
| Spiked Amount                  | 50.000 | Range | 20 - 135 | Recovery | =    | 140.20%# |
| 24) Chloroform-d               | 7.65   | 84    | 203551   | 26.90    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 40 - 150 | Recovery | =    | 107.60%  |
| 26) 1,2-Dichloroethane-d4      | 8.31   | 65    | 119681   | 30.56    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 70 - 130 | Recovery | =    | 122.24%  |
| 29) Benzene-d6                 | 8.27   | 84    | 390584   | 27.52    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 20 - 135 | Recovery | =    | 110.08%  |
| 33) 1,2-Dichloropropane-d6     | 9.27   | 67    | 116937   | 29.89    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 70 - 120 | Recovery | =    | 119.56%  |
| 37) Toluene-d8                 | 10.32  | 98    | 348994   | 25.60    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 30 - 130 | Recovery | =    | 102.40%  |
| 38) trans-1,3-Dichloropropene- | 10.58  | 79    | 44814    | 25.70    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 30 - 135 | Recovery | =    | 102.80%  |
| 39) 2-Hexanone-d5              | 10.93  | 63    | 35316    | 71.89    | ug/L | 0.00     |
| Spiked Amount                  | 50.000 | Range | 20 - 135 | Recovery | =    | 143.78%# |
| 48) 1,1,2,2-Tetrachloroethane- | 12.69  | 84    | 89906    | 30.96    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 45 - 120 | Recovery | =    | 123.84%# |
| 61) 1,2-Dichlorobenzene-d4     | 13.85  | 152   | 91837    | 26.44    | ug/L | 0.00     |
| Spiked Amount                  | 25.000 | Range | 75 - 120 | Recovery | =    | 105.76%  |

## Target Compounds


| Target Compounds              | R.T.  | QIon | Response | Conc   | Units  | Ovalue |
|-------------------------------|-------|------|----------|--------|--------|--------|
| 13) Acetone                   | 4.12  | 43   | 30514    | 48.662 | ug/L   | 64     |
| 14) Carbon disulfide          | 4.39  | 76   | 16185    | 1.519  | ug/L   | 100    |
| 16) Methylene chloride        | 4.92  | 84   | 13704    | 3.309  | ug/L   | 97     |
| 21) 2-Butanone                | 7.18  | 43   | 8336     | 9.883  | ug/L # | 64     |
| 42) cis-1,3-Dichloropropene   | 10.04 | 75   | 4483     | 0.826  | ug/L   | 94     |
| 45) trans-1,3-Dichloropropene | 10.58 | 75   | 2605     | 0.564  | ug/L   | 97     |
| 49) 2-Hexanone                | 10.97 | 43   | 695      | 0.593  | ug/L # | 64     |
| 52) Chlorobenzene             | 11.66 | 112  | 15818    | 1.543  | ug/L # | 85     |
| 55) o-xylene                  | 12.16 | 106  | 1774     | 0.259  | ug/L   | 73     |
| 57) Isopropylbenzene          | 12.46 | 105  | 11260    | 0.593  | ug/L # | 96     |
| 59) 1,2,3-Trichloropropane    | 13.55 | 75   | 16905    | 8.151  | ug/L   | 93     |
| 63) 1,3-Dichlorobenzene       | 13.50 | 146  | 10260    | 1.667  | ug/L   | 96     |
| 64) 1,4-Dichlorobenzene       | 13.58 | 146  | 5638     | 0.911  | ug/L   | 93     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW011521\  
Data File : VW017901.D  
Acq On : 15 Jan 2021 16:35  
Operator : SY/VA  
Sample : M1099-13  
Misc : 6.50G/10ML/MSVOA W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :

Quant Time: Jan 18 02:09:25 2021  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_W\METHOD\SOM2WLM122420S.M  
Quant Title : VOC Analysis  
QLast Update : Mon Jan 18 02:07:49 2021  
Response via : Initial Calibration

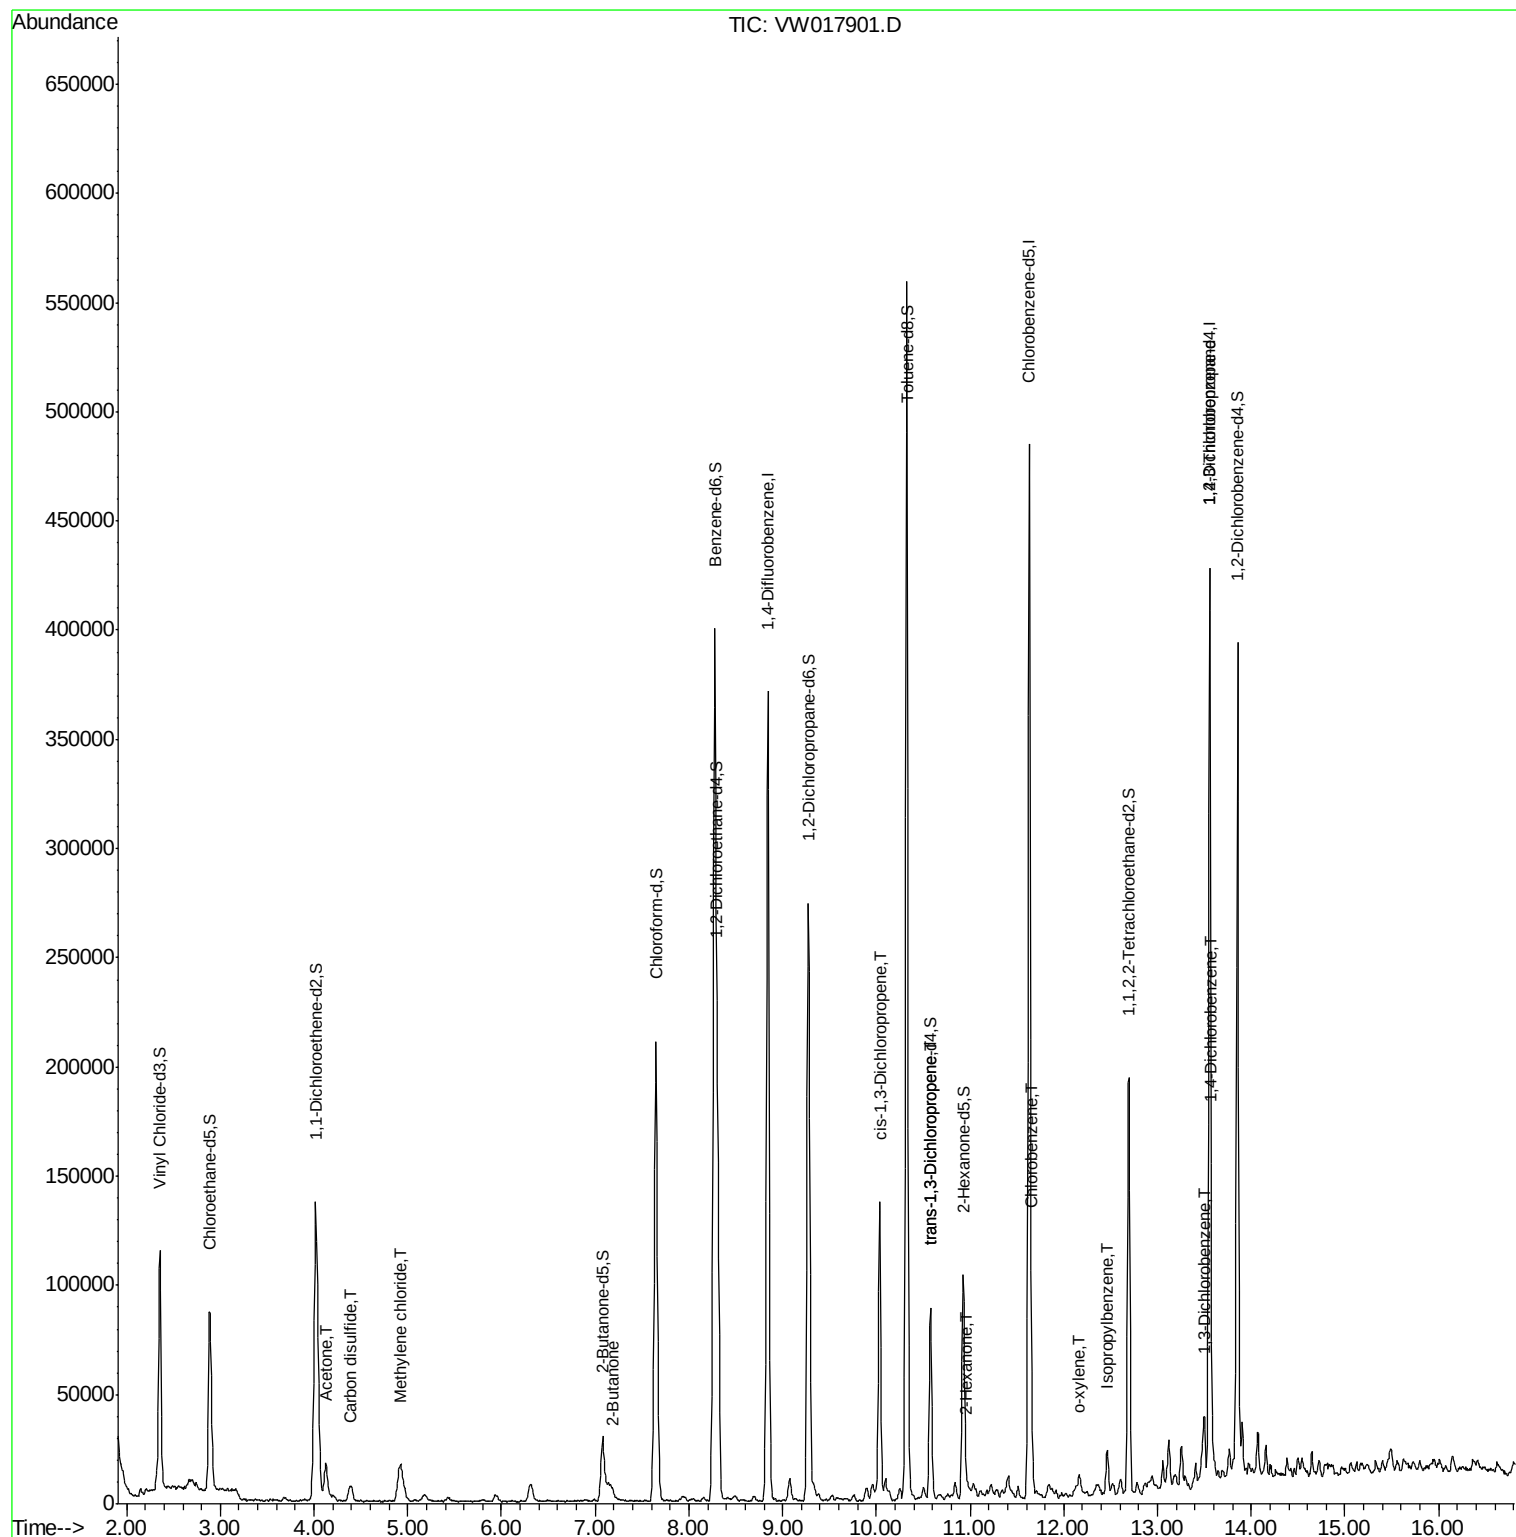

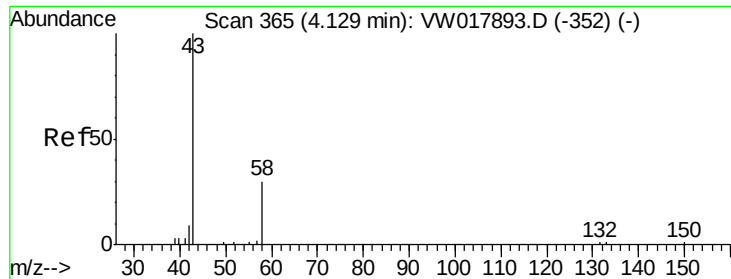

#13

Acetone

Concen: 48.662 ug/L

RT: 4.12 min Scan# 364

Delta R.T. -0.01 min

Lab File: VW017901.D

Acq: 15 Jan 2021 16:35

Instrument :

MSVOA\_W





ClientSampleId :

Tot Ion: 43 Resp: 30514

Ion Ratio Lower Upper

43 100

58 13.4 0.0 68.4

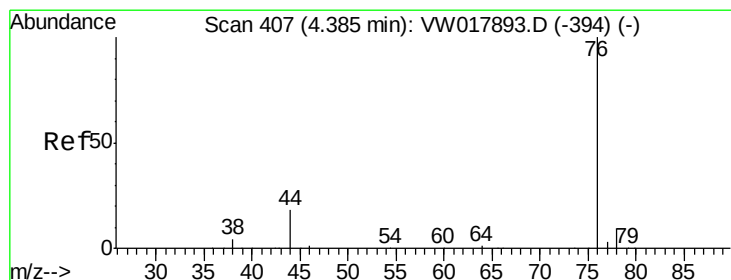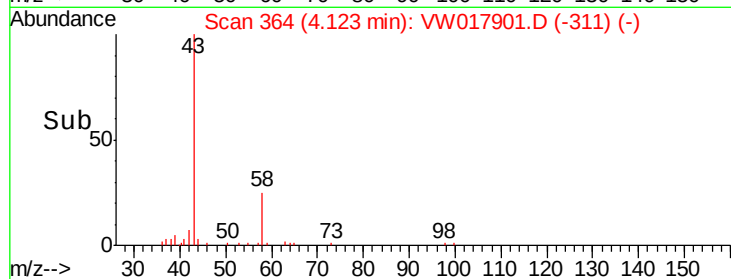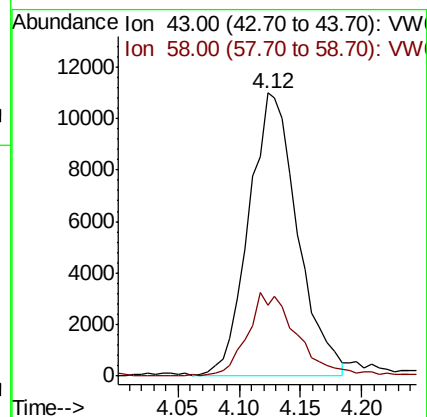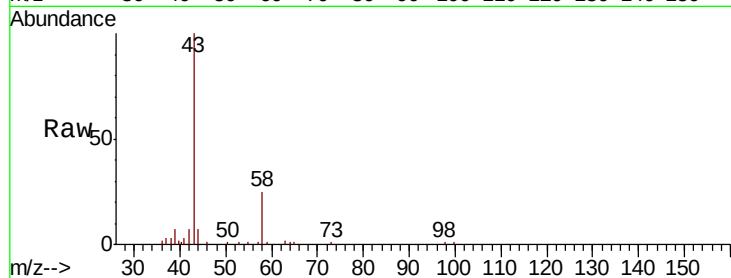

#14

Carbon disulfide

Concen: 1.519 ug/L

RT: 4.39 min Scan# 408

Delta R.T. 0.01 min

Lab File: VW017901.D




Acq: 15 Jan 2021 16:35


Tgt Ion: 76 Resp: 16185

Ion Ratio Lower Upper

76 100

78 8.6 7.0 10.4


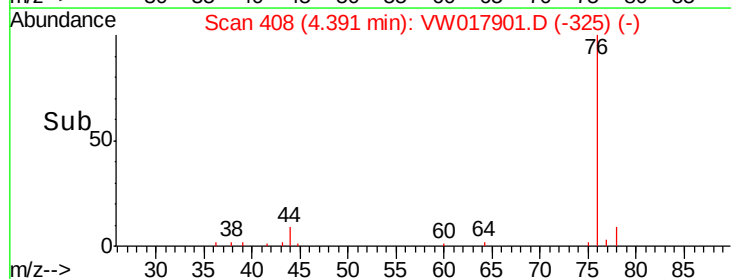
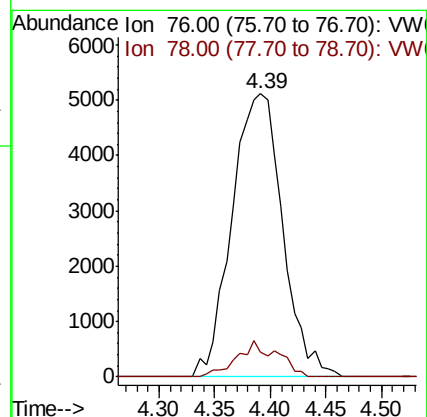
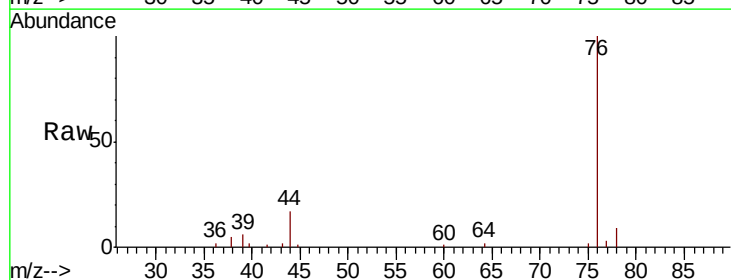


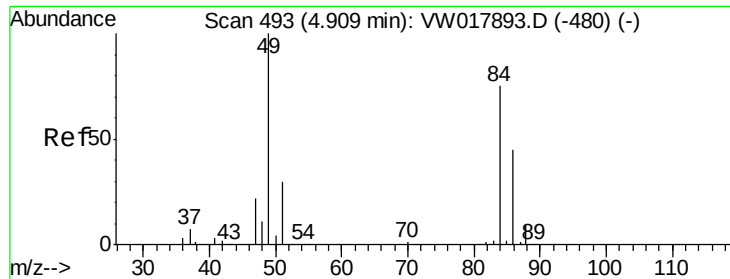

#16  
Methylene chloride  
Concen: 3.309 ug/L  
RT: 4.92 min Scan# 495  
Delta R.T. 0.01 min  
Lab File: VW017901.D  
Acq: 15 Jan 2021 16:35




Instrument :  
MSVOA\_W  
ClientSampleId :


Tot Ion: 84 Resp: 13704  
Ion Ratio Lower Upper  
84 100  
49 116.3 81.2 150.8  
86 58.0 44.5 82.7

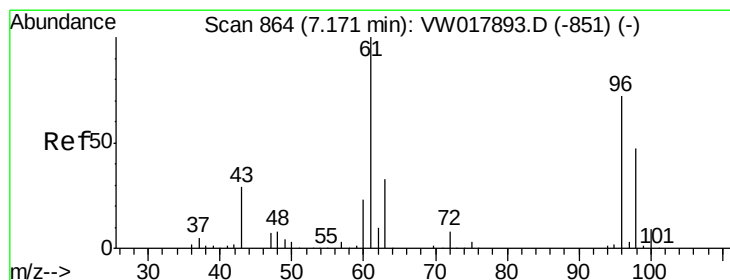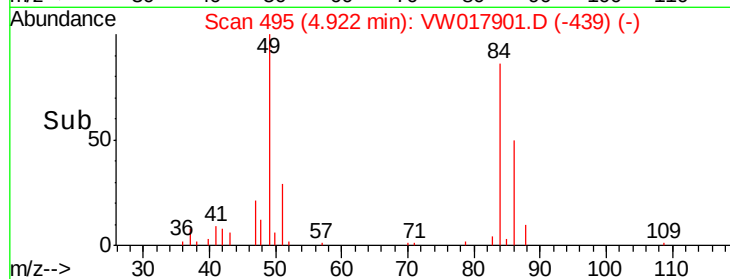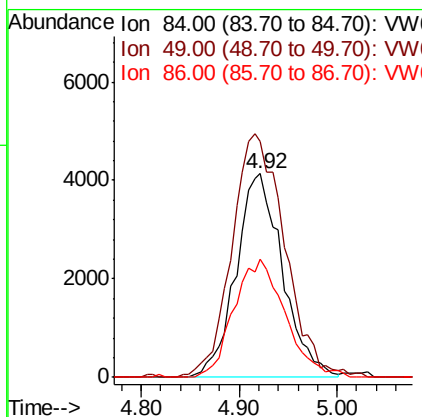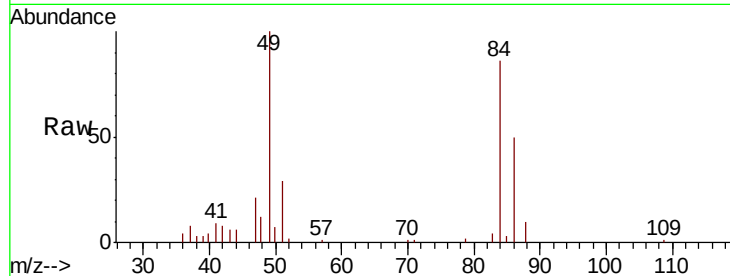

#21  
2-Butanone  
Concen: 9.883 ug/L  
RT: 7.18 min Scan# 866  
Delta R.T. 0.01 min  
Lab File: VW017901.D  
Acq: 15 Jan 2021 16:35

Tgt Ion: 43 Resp: 8336  
Ion Ratio Lower Upper  
43 100  
72 9.6 14.4 43.2#


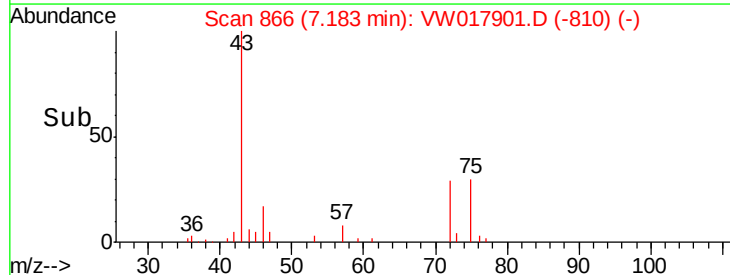
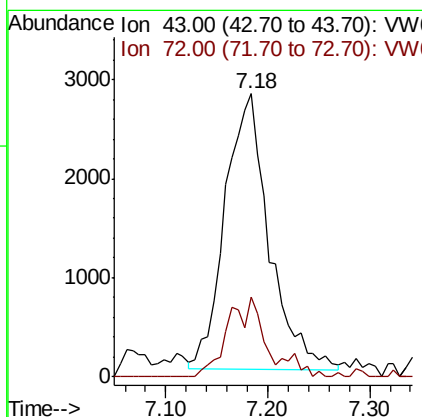
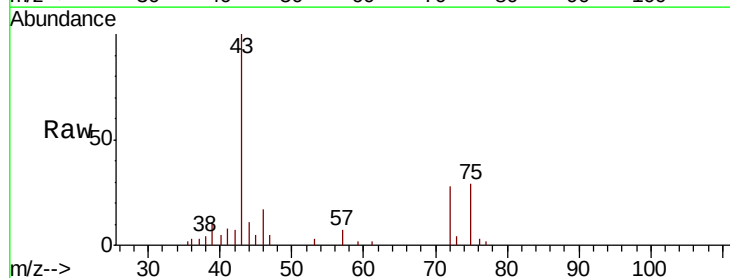


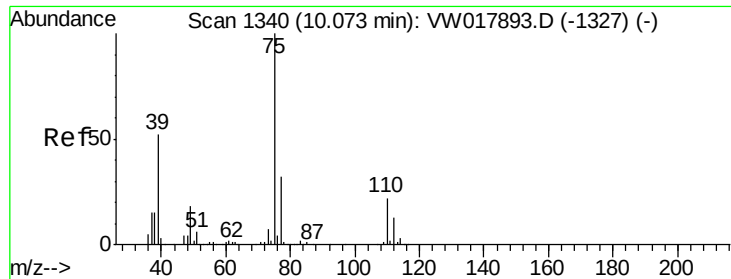

#42  
 cis-1,3-Dichloropropene  
 Concen: 0.826 ug/L  
 RT: 10.04 min Scan# 1334  
 Delta R.T. -0.04 min  
 Lab File: VW017901.D  
 Acq: 15 Jan 2021 16:35




Instrument :  
 MSVOA\_W  
 ClientSampleId :


Tot Ion: 75 Resp: 4483  
 Ion Ratio Lower Upper  
 75 100  
 77 35.6 22.7 42.3

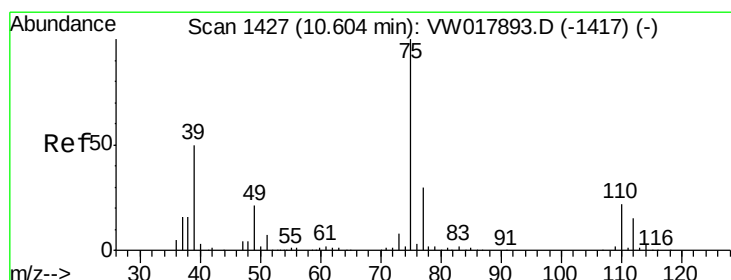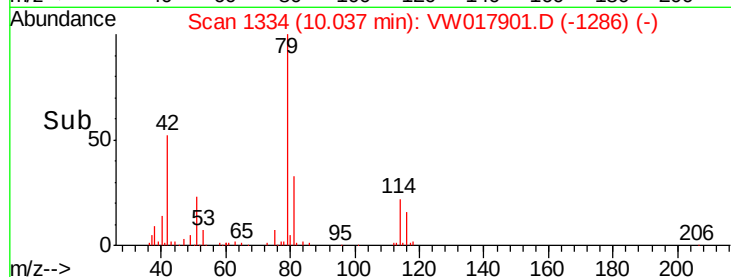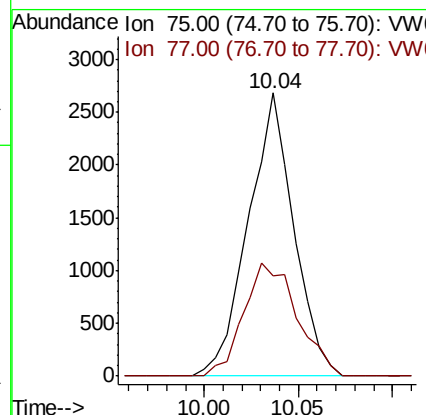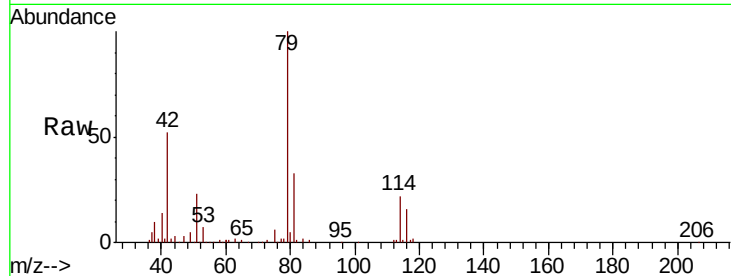

#45  
 trans-1,3-Dichloropropene  
 Concen: 0.564 ug/L  
 RT: 10.58 min Scan# 1423  
 Delta R.T. -0.02 min  
 Lab File: VW017901.D  
 Acq: 15 Jan 2021 16:35

Tgt Ion: 75 Resp: 2605  
 Ion Ratio Lower Upper  
 75 100  
 77 30.5 22.6 42.0


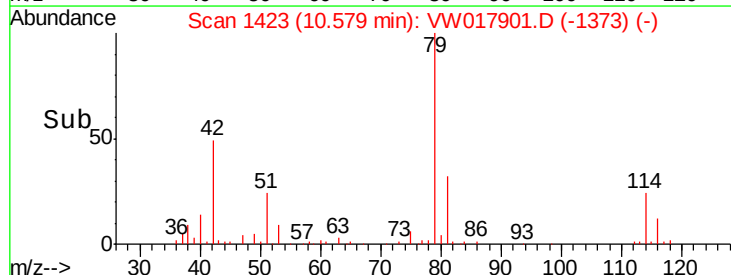
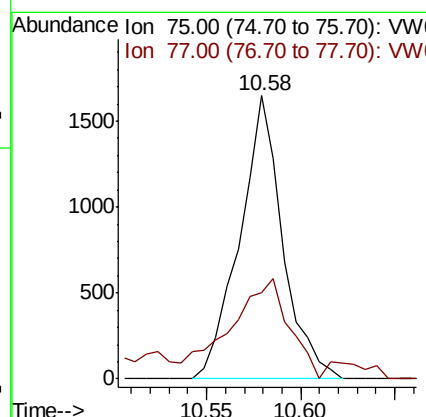
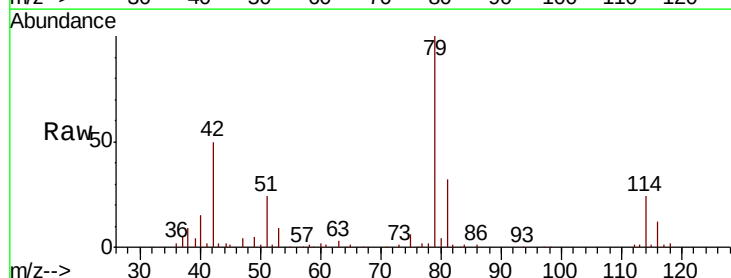


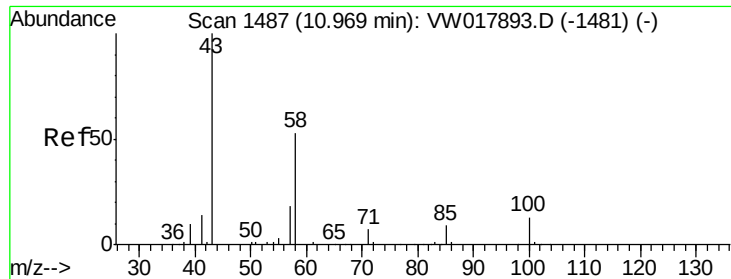

#49  
2-Hexanone  
Concen: 0.593 ug/L  
RT: 10.97 min Scan# 1487  
Delta R.T. 0.00 min  
Lab File: VW017901.D  
Acq: 15 Jan 2021 16:35




Instrument :  
MSVOA\_W  
ClientSampled :


Tot Ion: 43 Resp: 695  
Ion Ratio Lower Upper  
43 100  
58 43.6 51.3 76.9#  
57 58.1 15.0 22.6#  
100 10.6 12.2 18.2#

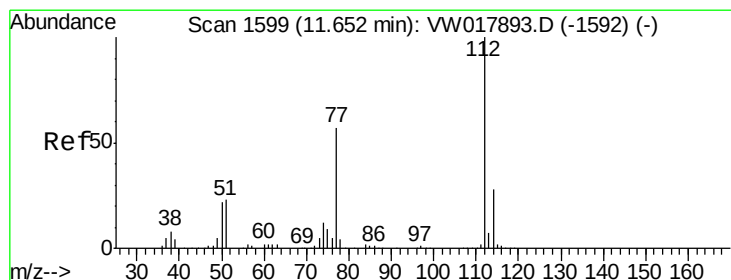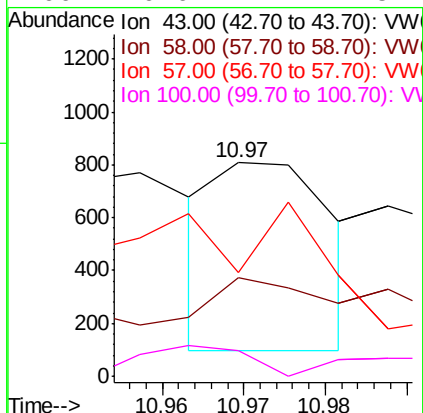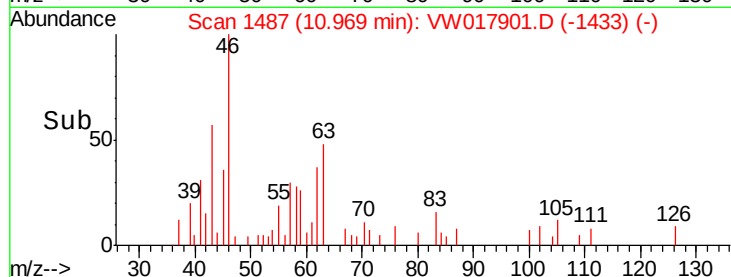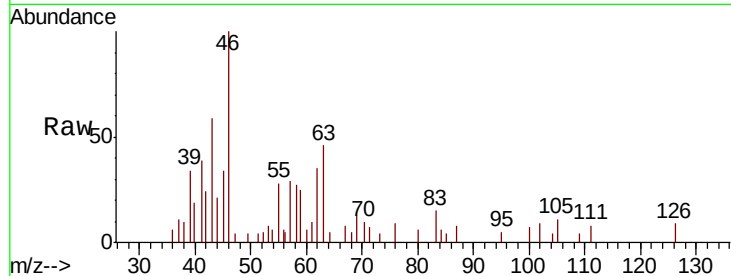

#52  
Chlorobenzene  
Concen: 1.543 ug/L  
RT: 11.66 min Scan# 1600  
Delta R.T. 0.01 min  
Lab File: VW017901.D  
Acq: 15 Jan 2021 16:35

Tgt Ion: 112 Resp: 15818  
Ion Ratio Lower Upper  
112 100  
77 67.8 42.6 64.0#  
114 33.4 21.6 40.2

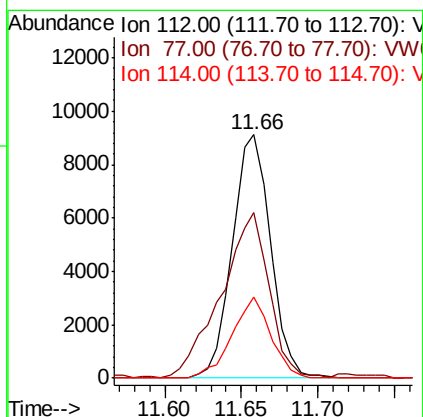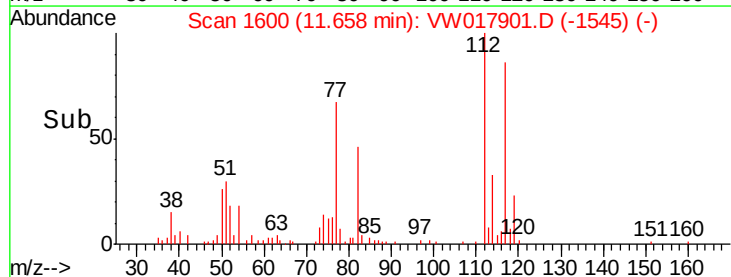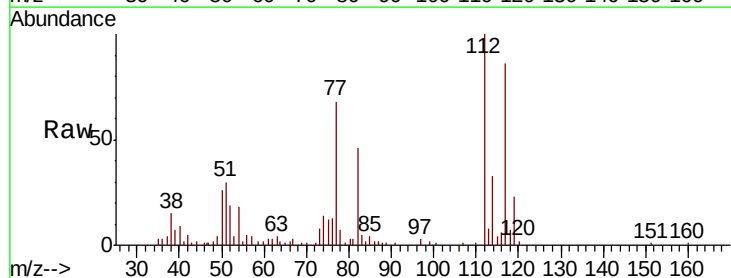

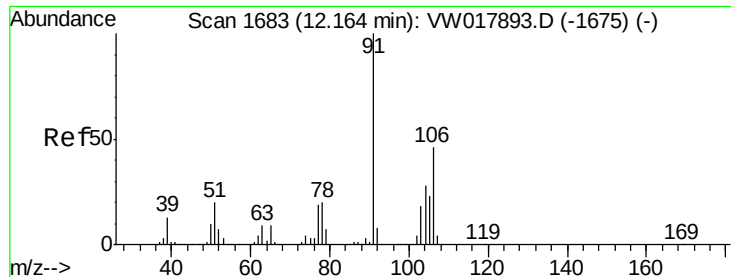

#55

o-xylene

Concen: 0.259 ug/L

RT: 12.16 min Scan# 1683

Delta R.T. 0.00 min

Lab File: VW017901.D

Acq: 15 Jan 2021 16:35

Instrument :

MSVOA\_W


ClientSampled :

Tot Ion:106 Resp: 1774

Ion Ratio Lower Upper




106 100

91 168.3 147.6 274.2

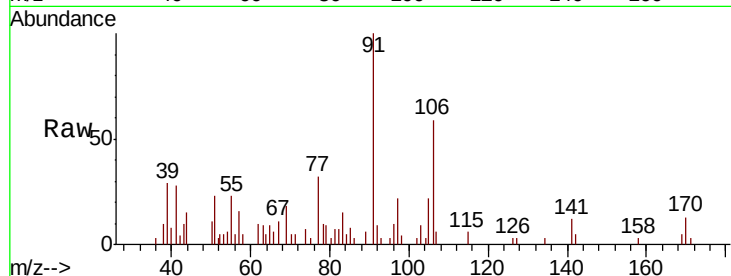

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VW

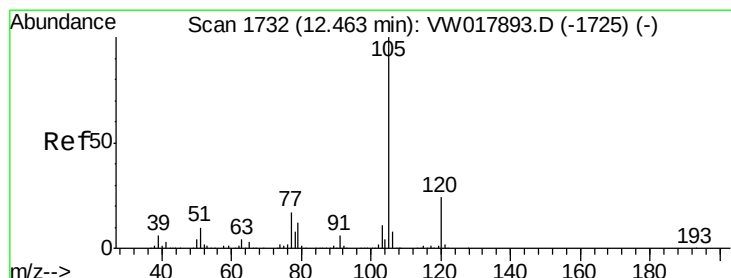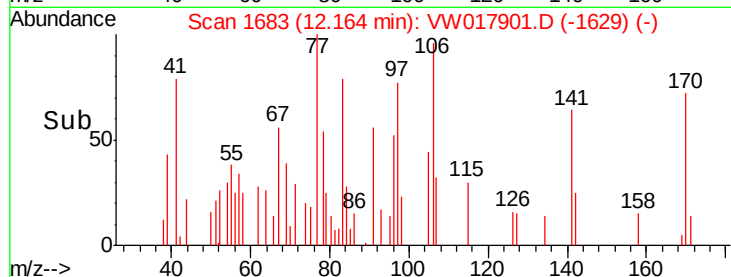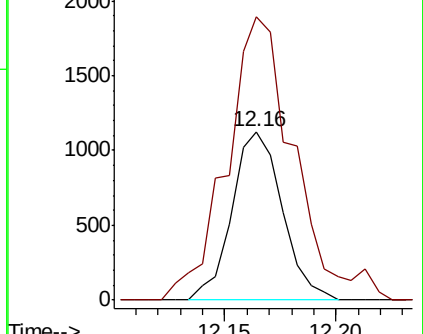

#57

Isopropylbenzene

Concen: 0.593 ug/L

RT: 12.46 min Scan# 1732

Delta R.T. 0.00 min

Lab File: VW017901.D

Acq: 15 Jan 2021 16:35


Tgt Ion:105 Resp: 11260

Ion Ratio Lower Upper

105 100

120 27.0 21.4 32.2



77 18.9 12.1 18.1#

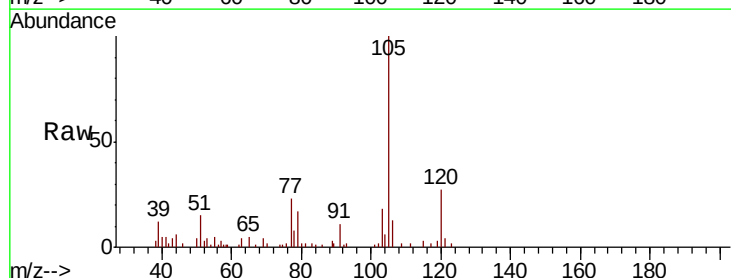


Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

Ion 77.00 (76.70 to 77.70): VW



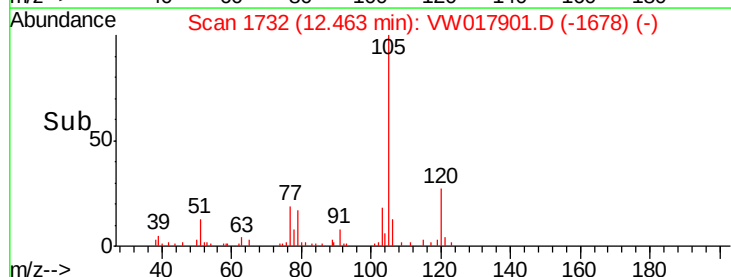
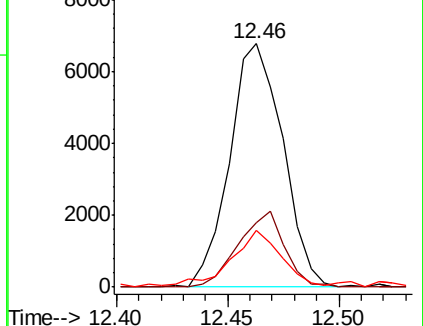


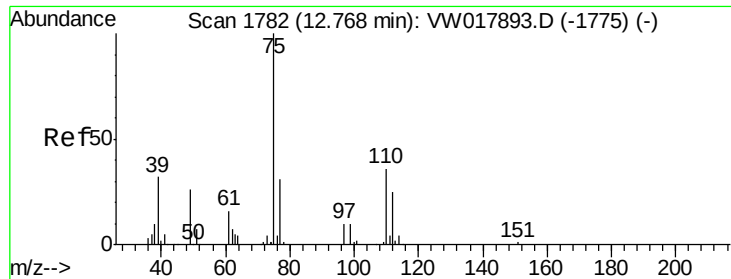

#59  
 1,2,3-Trichloropropane  
 Concen: 8.151 ug/L  
 RT: 13.55 min Scan# 1911  
 Delta R.T. 0.79 min  
 Lab File: VW017901.D  
 Acq: 15 Jan 2021 16:35




Instrument :  
 MSVOA\_W  
 ClientSampleId :

Tot Ion: 75 Resp: 16905  
 Ion Ratio Lower Upper  
 75 100  
 77 29.1 26.6 39.8

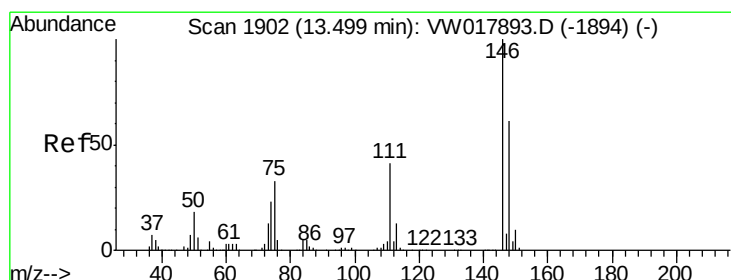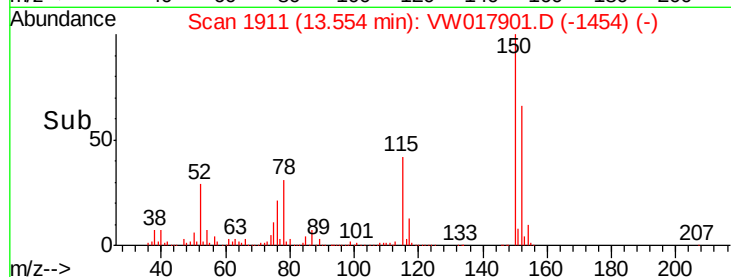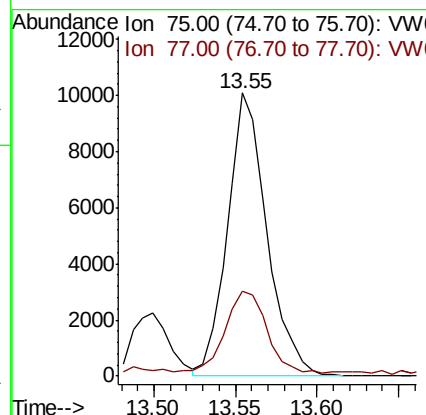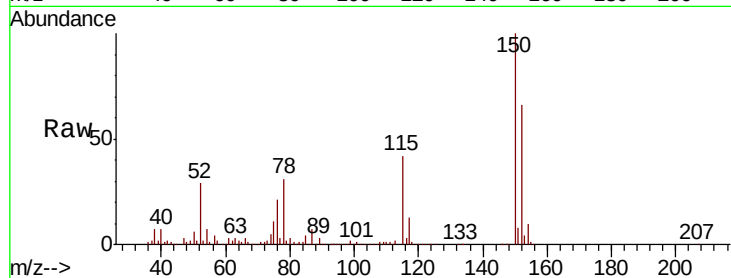


#63  
 1,3-Dichlorobenzene  
 Concen: 1.667 ug/L  
 RT: 13.50 min Scan# 1902  
 Delta R.T. 0.00 min  
 Lab File: VW017901.D  
 Acq: 15 Jan 2021 16:35

Tgt Ion: 146 Resp: 10260  
 Ion Ratio Lower Upper  
 146 100  
 111 46.1 28.5 52.9  
 148 67.4 47.8 88.8

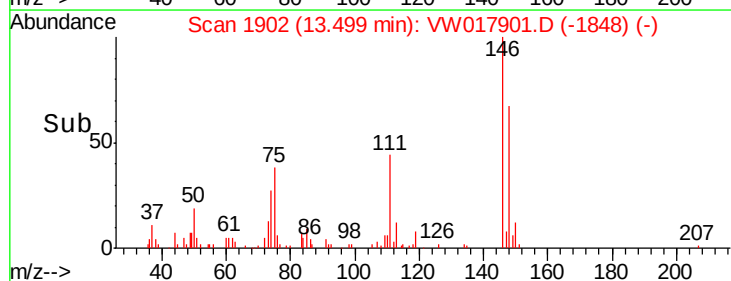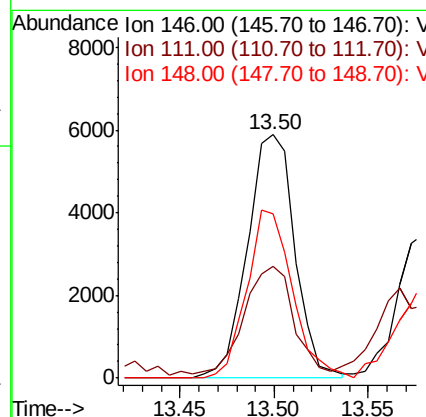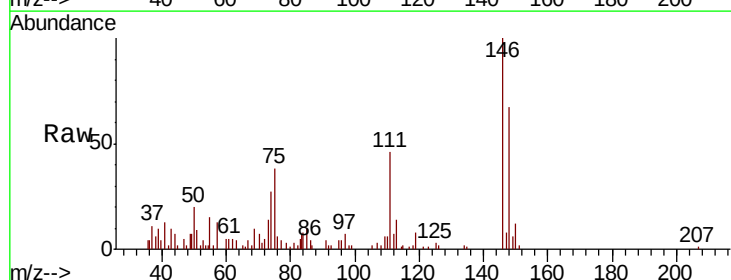




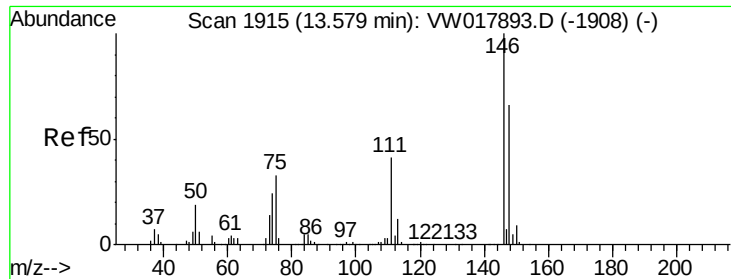

#64  
 1,4-Dichlorobenzene  
 Concen: 0.911 ug/L  
 RT: 13.58 min Scan# 1915  
 Delta R.T. 0.00 min  
 Lab File: VW017901.D  
 Acq: 15 Jan 2021 16:35

Instrument :  
 MSVOA\_W  
 ClientSampleId :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 146     | 100   |       |       |
| 111     | 50.6  | 27.7  | 51.5  |
| 148     | 67.6  | 47.0  | 87.2  |

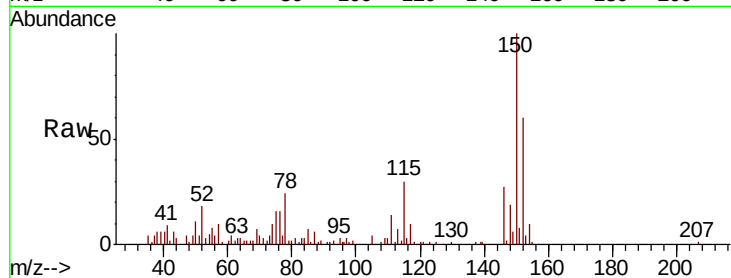

Abundance

Ion 146.00 (145.70 to 146.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

