

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
Data File : VW017896.D
Acq On : 15 Jan 2021 14:38
Operator : SY/VA
Sample : M1117-06
Misc : 5.05G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

apatel
1/18/2021 8:50:53 AM

Quant Time: Jan 18 02:08:49 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 18 02:07:49 2021
Response via : Initial Calibration

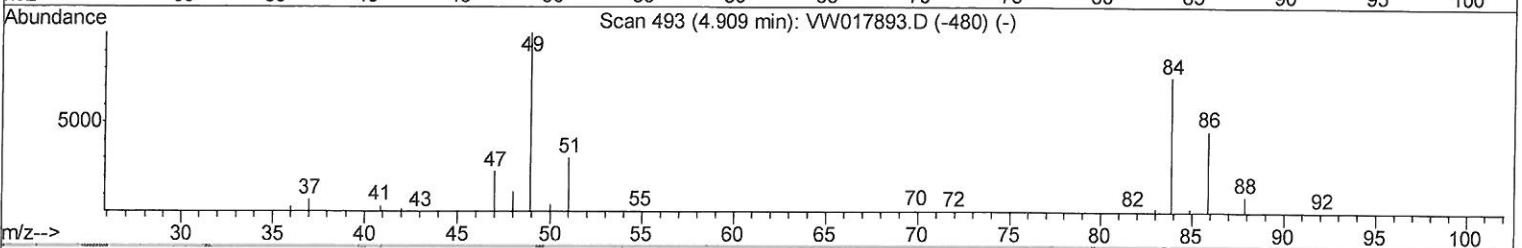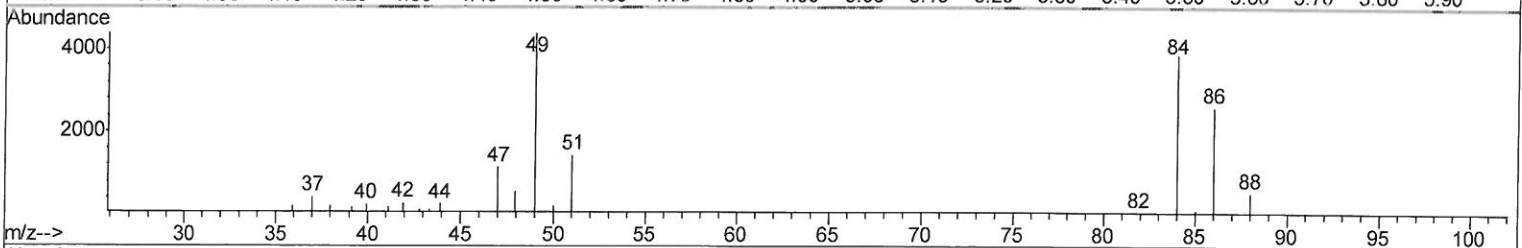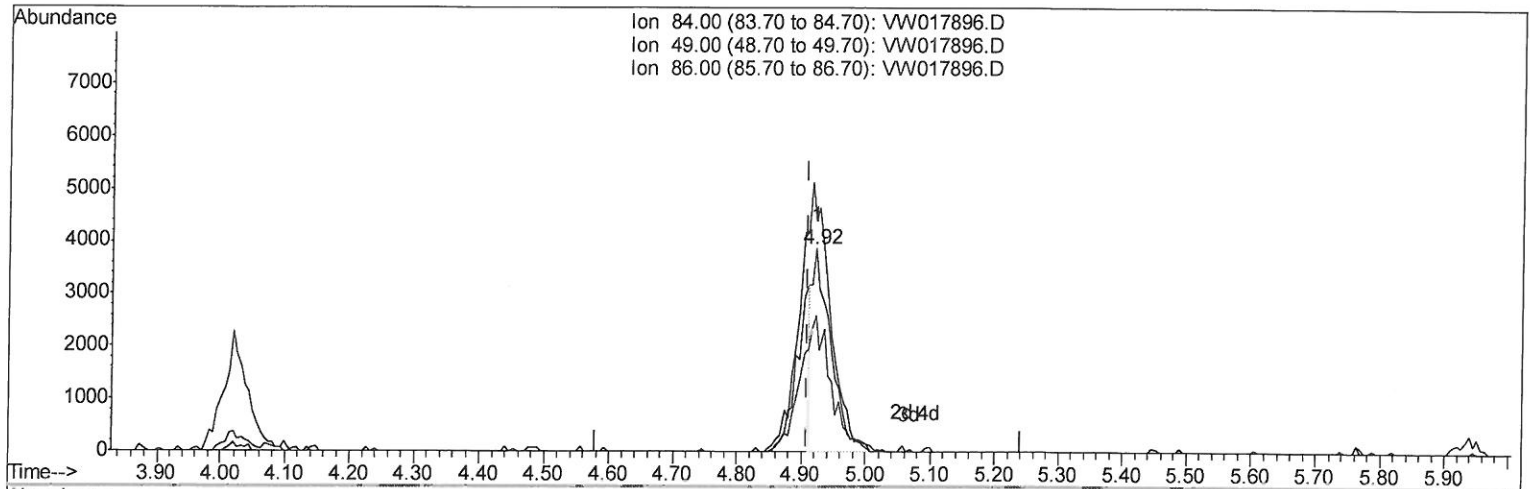

TIC: VW017896.D

(16) Methylene chloride (T)

4.921min (+0.012) 1.76ug/L

response 8072

Ion	Exp%	Act%
84.00	100	100
49.00	116.00	113.13
86.00	63.60	67.22
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
 Data File : VW017896.D
 Acq On : 15 Jan 2021 14:38
 Operator : SY/VA
 Sample : M1117-06
 Misc : 5.05G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

apatel
 1/18/2021 8:50:53 AM

Quant Time: Jan 18 02:08:49 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 18 02:07:49 2021
 Response via : Initial Calibration

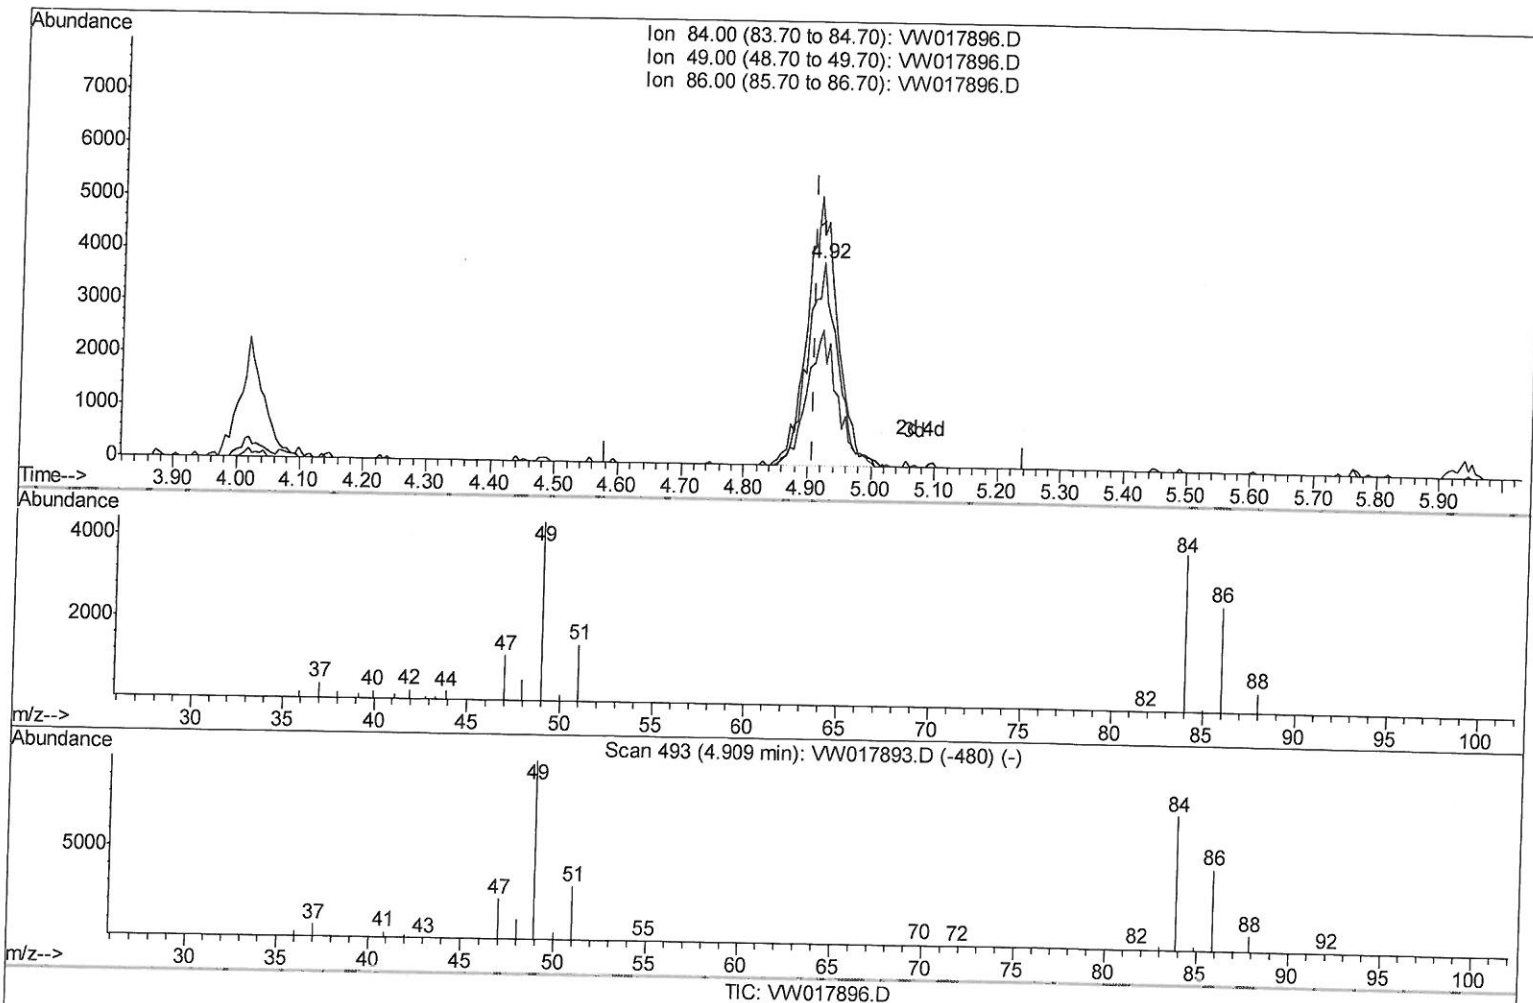

(16) Methylene chloride (T)

4.921min (+0.012) 2.72ug/L m

response 12509

Ion	Exp%	Act%
84.00	100	100
49.00	116.00	113.13
86.00	63.60	67.22
0.00	0.00	0.00

201/22/2021

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
 Data File : VW017896.D
 Acq On : 15 Jan 2021 14:38
 Operator : SY/VA
 Sample : M1117-06
 Misc : 5.05G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleID :
 VHBLK01

Manual Integrations
 APPROVED

apatel
 1/18/2021 8:50:53 AM

Quant Time: Jan 18 02:08:49 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 18 02:07:49 2021
 Response via : Initial Calibration

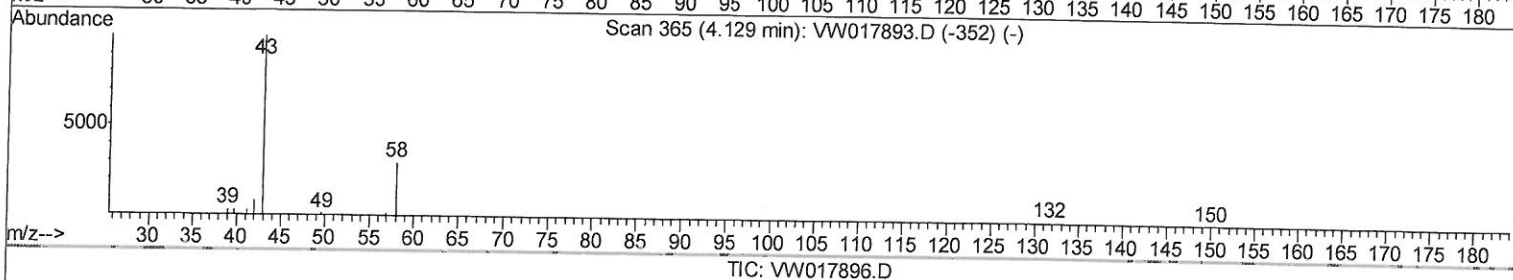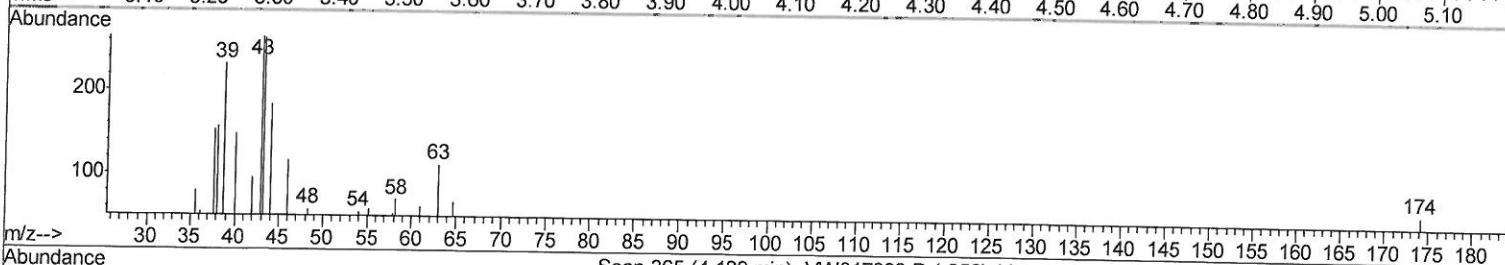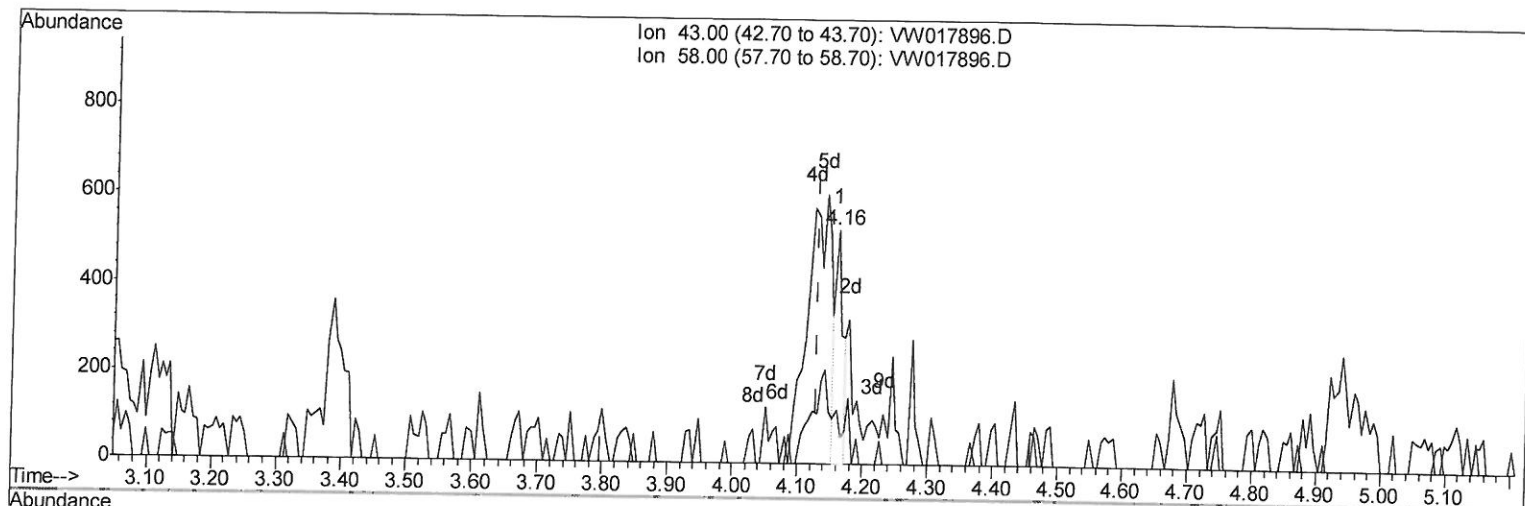

(13) Acetone (T)

4.159min (+0.030) 0.58ug/L

response 405

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	16.54
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
 Data File : VW017896.D
 Acq On : 15 Jan 2021 14:38
 Operator : SY/VA
 Sample : M1117-06
 Misc : 5.05G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

apatel
 1/18/2021 8:50:53 AM

Quant Time: Jan 18 02:08:49 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 18 02:07:49 2021
 Response via : Initial Calibration

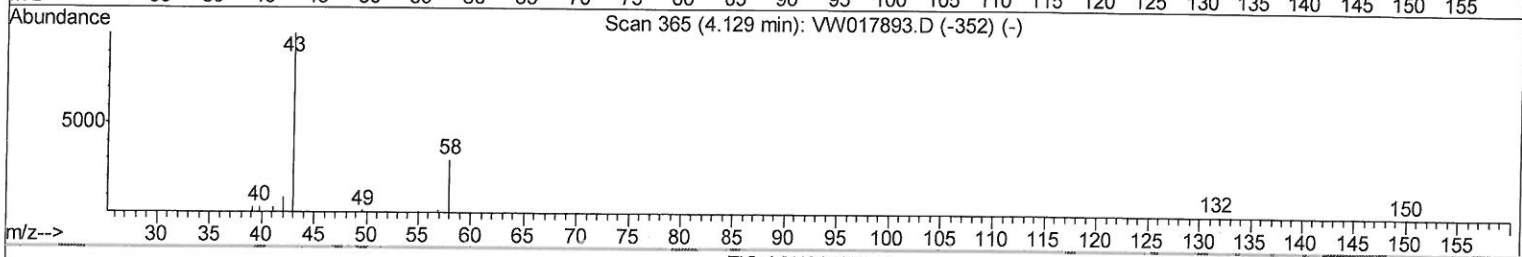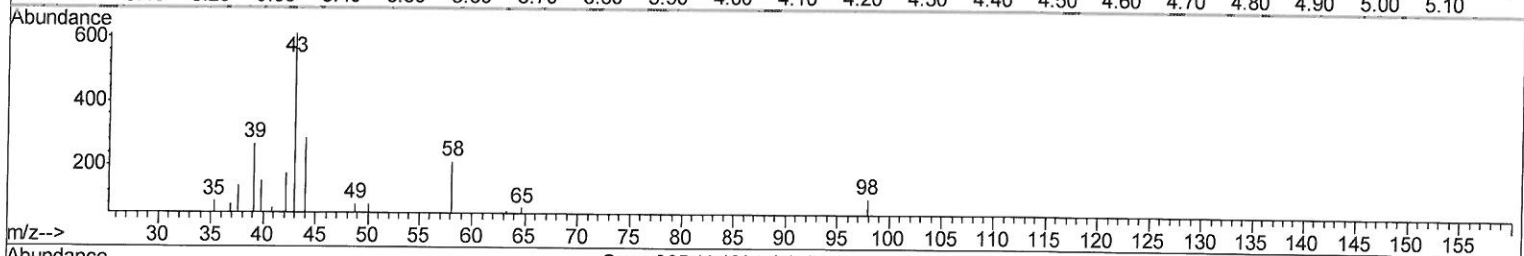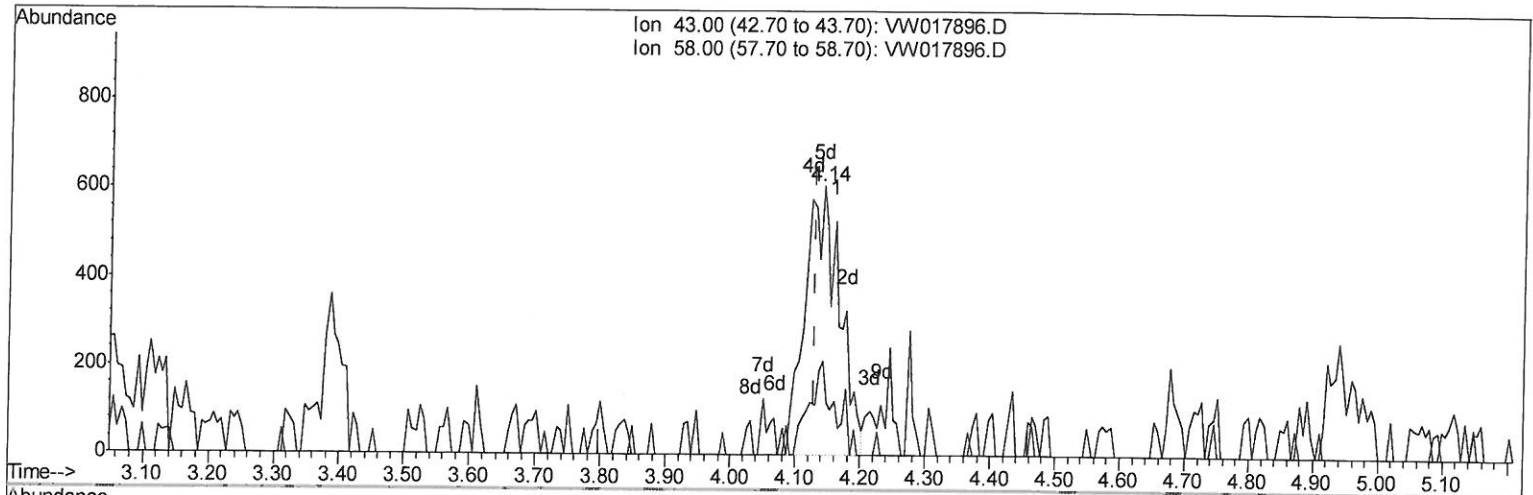

TIC: VW017896.D

(13) Acetone (T)

4.141min (+0.012) 3.20ug/L m

response 2224

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	3.01
0.00	0.00	0.00
0.00	0.00	0.00

Soil/22/21 Sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
 Data File : VW017896.D
 Acq On : 15 Jan 2021 14:38
 Operator : SY/VA
 Sample : M1117-06
 Misc : 5.05G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

apatel
 1/18/2021 8:50:53 AM

Quant Time: Jan 18 02:45:24 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 18 02:07:49 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	321187	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	289107	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	136972	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	100580	20.24	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.96%		
7) Chloroethane-d5	2.89	69	90709	22.12	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.48%		
10) 1,1-Dichloroethene-d2	4.02	63	139289	16.09	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.36%		
20) 2-Butanone-d5	7.08	46	46988	58.34	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	116.68%		
24) Chloroform-d	7.65	84	197309	23.51	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.04%		
26) 1,2-Dichloroethane-d4	8.30	65	112871	25.98	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	103.92%		
29) Benzene-d6	8.27	84	383518	23.55	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.20%		
33) 1,2-Dichloropropane-d6	9.27	67	110282	24.57	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.28%		
37) Toluene-d8	10.32	98	348824	22.30	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	89.20%		
38) trans-1,3-Dichloropropene-	10.58	79	42916	21.45	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.80%		
39) 2-Hexanone-d5	10.93	63	30192	53.56	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	107.12%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	87417	26.23	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	104.92%		
61) 1,2-Dichlorobenzene-d4	13.85	152	110607	23.19	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.76%		

Target Compounds

	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.14	43	2224m	3.198	ug/L	
16) Methylene chloride	4.92	84	12509m	2.723	ug/L	

01/22/21 SCY

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
Data File : VW017896.D
Acq On : 15 Jan 2021 14:38
Operator : SY/VA
Sample : M1117-06
Misc : 5.05G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

apatel
1/18/2021 8:50:53 AM

Quant Time: Jan 18 02:45:24 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 18 02:07:49 2021
Response via : Initial Calibration

