

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
 Data File : VW017912.D
 Acq On : 15 Jan 2021 20:54
 Operator : SY/VA
 Sample : VIBLK26
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VIBLK26

Manual Integrations
APPROVED

apatel
 1/18/2021 8:51:01 AM

Quant Time: Jan 18 02:11:16 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 18 02:07:49 2021
 Response via : Initial Calibration

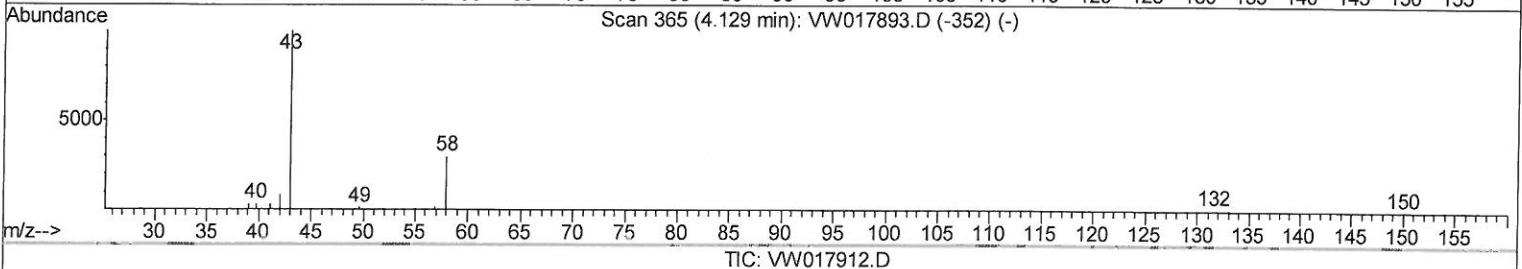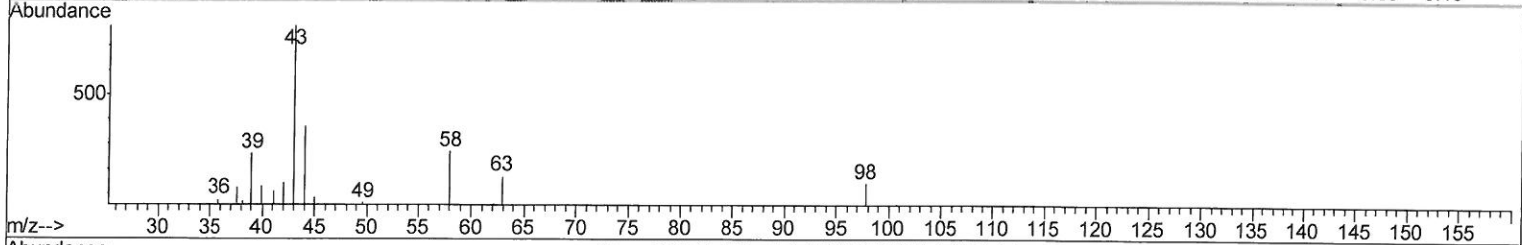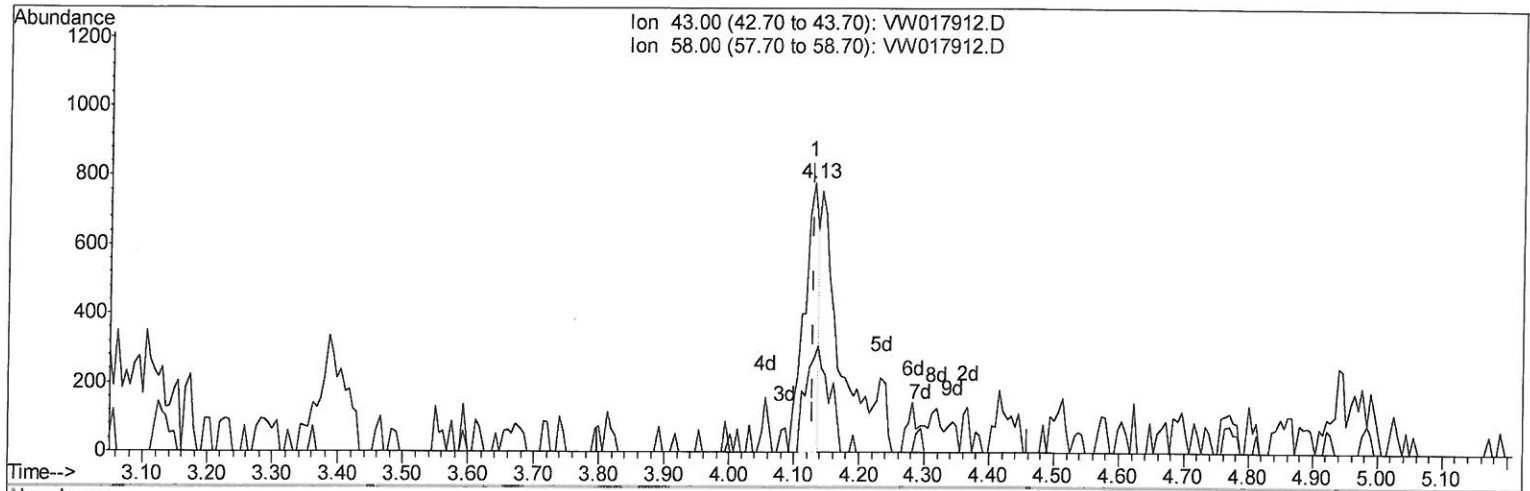

(13) Acetone (T)

4.129min (+0.000) 1.44ug/L

response 1195

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	63.60
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
 Data File : VW017912.D
 Acq On : 15 Jan 2021 20:54
 Operator : SY/VA
 Sample : VIBLK26
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VIBLK26

Manual Integrations
APPROVED

apatel
 1/18/2021 8:51:01 AM

Quant Time: Jan 18 02:11:16 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 18 02:07:49 2021
 Response via : Initial Calibration

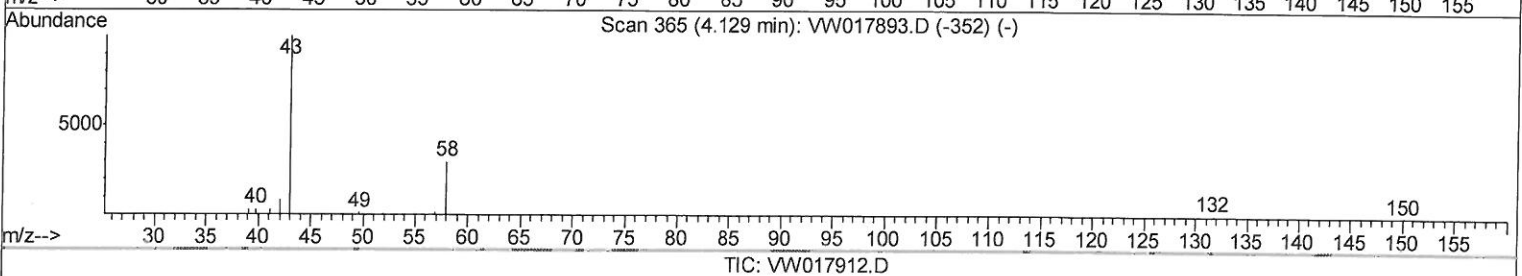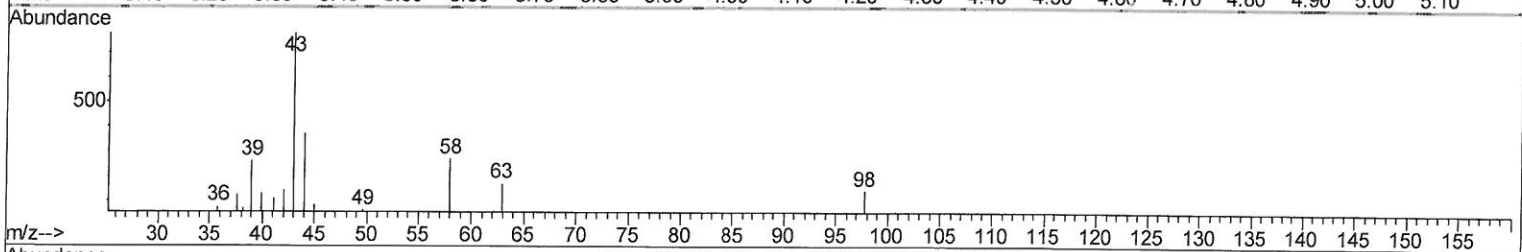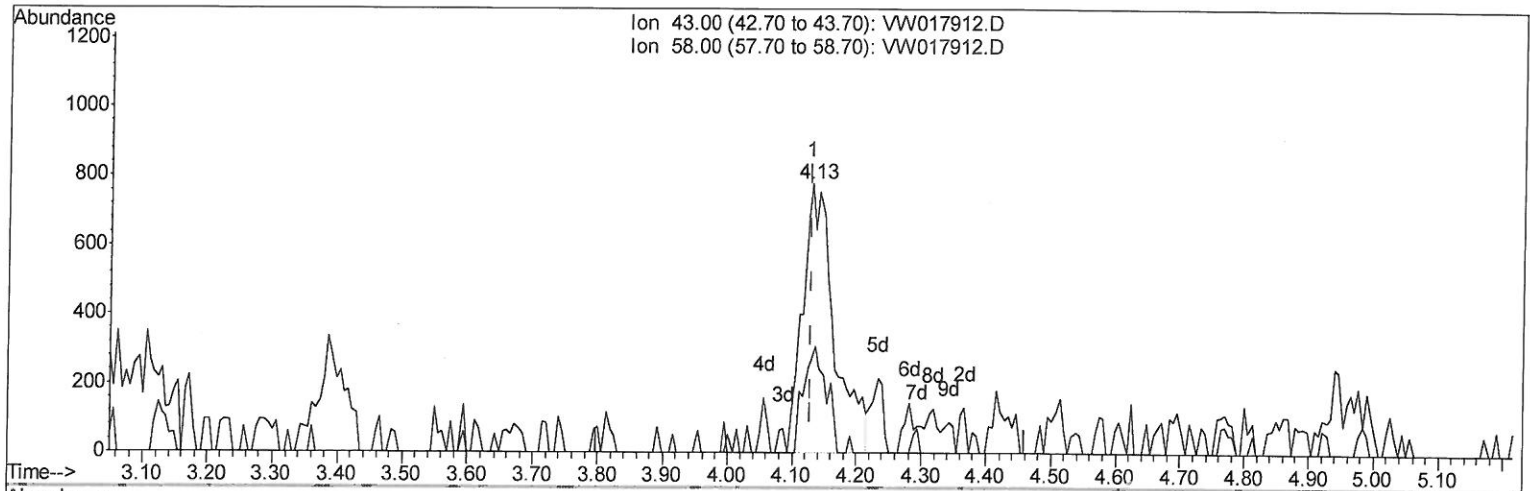

(13) Acetone (T)

4.129min (+0.000) 3.20ug/L m

response 2651

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	28.67
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
 Data File : VW017912.D
 Acq On : 15 Jan 2021 20:54
 Operator : SY/VA
 Sample : VIBLK26
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VIBLK26

Manual Integrations
 APPROVED

apatel
 1/18/2021 8:51:01 AM

Quant Time: Jan 18 04:32:08 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 18 02:07:49 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	382810	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	354437	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	171923	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	113069	19.09	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	76.36%		
7) Chloroethane-d5	2.89	69	97532	19.95	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.80%		
10) 1,1-Dichloroethene-d2	4.02	63	161184	15.62	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.48%		
20) 2-Butanone-d5	7.08	46	60445	62.96	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	125.92%		
24) Chloroform-d	7.65	84	231732	23.16	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.64%		
26) 1,2-Dichloroethane-d4	8.31	65	130485	25.20	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.80%		
29) Benzene-d6	8.27	84	450866	22.58	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	90.32%		
33) 1,2-Dichloropropane-d6	9.27	67	133589	24.27	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.08%		
37) Toluene-d8	10.32	98	424882	22.16	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	88.64%		
38) trans-1,3-Dichloropropene-	10.58	79	50042	20.40	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.60%		
39) 2-Hexanone-d5	10.93	63	44018	63.69	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	127.38%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	107714	26.36	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	105.44%		
61) 1,2-Dichlorobenzene-d4	13.85	152	148051	24.73	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.92%		

Target Compounds

13) Acetone	4.13	43	2651m	3.198	ug/L	Ovalue
16) Methylene chloride	4.92	84	12778	2.334	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
Data File : VW017912.D
Acq On : 15 Jan 2021 20:54
Operator : SY/VA
Sample : VIBLK26
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK26

Manual Integrations
APPROVED

apatel
1/18/2021 8:51:01 AM

Quant Time: Jan 18 04:32:08 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 18 02:07:49 2021
Response via : Initial Calibration

