

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011521\
 Data File : VW017903.D
 Acq On : 15 Jan 2021 17:22
 Operator : SY/VA
 Sample : M1099-14
 Misc : 6.70G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F1C10

Manual Integrations
 APPROVED

apatel
 1/18/2021 8:50:58 AM

Quant Time: Jan 18 03:14:07 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jan 18 02:07:49 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	296728	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	251313	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	96691	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	114267	24.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.56%
7) Chloroethane-d5	2.89	69	102835	27.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.56%
10) 1,1-Dichloroethene-d2	4.02	63	150655	18.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.32%
20) 2-Butanone-d5	7.09	46	49098	65.98	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	131.96%
24) Chloroform-d	7.65	84	209551	27.02	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	108.08%
26) 1,2-Dichloroethane-d4	8.31	65	126596	31.54	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	126.16%
29) Benzene-d6	8.27	84	412698	29.15	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	116.60%
33) 1,2-Dichloropropane-d6	9.27	67	121145	31.05	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	124.20%#
37) Toluene-d8	10.32	98	356876	26.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.00%
38) trans-1,3-Dichloropropene-	10.58	79	44900	25.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	103.24%
39) 2-Hexanone-d5	10.93	63	34657	70.72	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	141.44%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	88258	30.47	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.88%#
61) 1,2-Dichlorobenzene-d4	13.85	152	89545	26.59	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.36%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.14	43	24544	38.197	ug/L	65
14) Carbon disulfide	4.39	76	11858	1.086	ug/L	100
16) Methylene chloride	4.92	84	10123m	2.386	ug/L	
21) 2-Butanone	7.19	43	7075m	8.186	ug/L	
52) Chlorobenzene	11.66	112	21628	2.114	ug/L #	86
54) m,p-Xylene	11.84	106	1833	0.252	ug/L	90
55) o-xylene	12.16	106	1703	0.249	ug/L	78
57) Isopropylbenzene	12.46	105	12760	0.674	ug/L #	95
63) 1,3-Dichlorobenzene	13.50	146	10766	1.804	ug/L	92
64) 1,4-Dichlorobenzene	13.58	146	6414	1.069	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW011521\
Data File : VW017903.D
Acq On : 15 Jan 2021 17:22
Operator : SY/VA
Sample : M1099-14
Misc : 6.70G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
F1C10

Manual Integrations
APPROVED

apatel
1/18/2021 8:50:58 AM

Quant Time: Jan 18 03:14:07 2021
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Mon Jan 18 02:07:49 2021
Response via : Initial Calibration

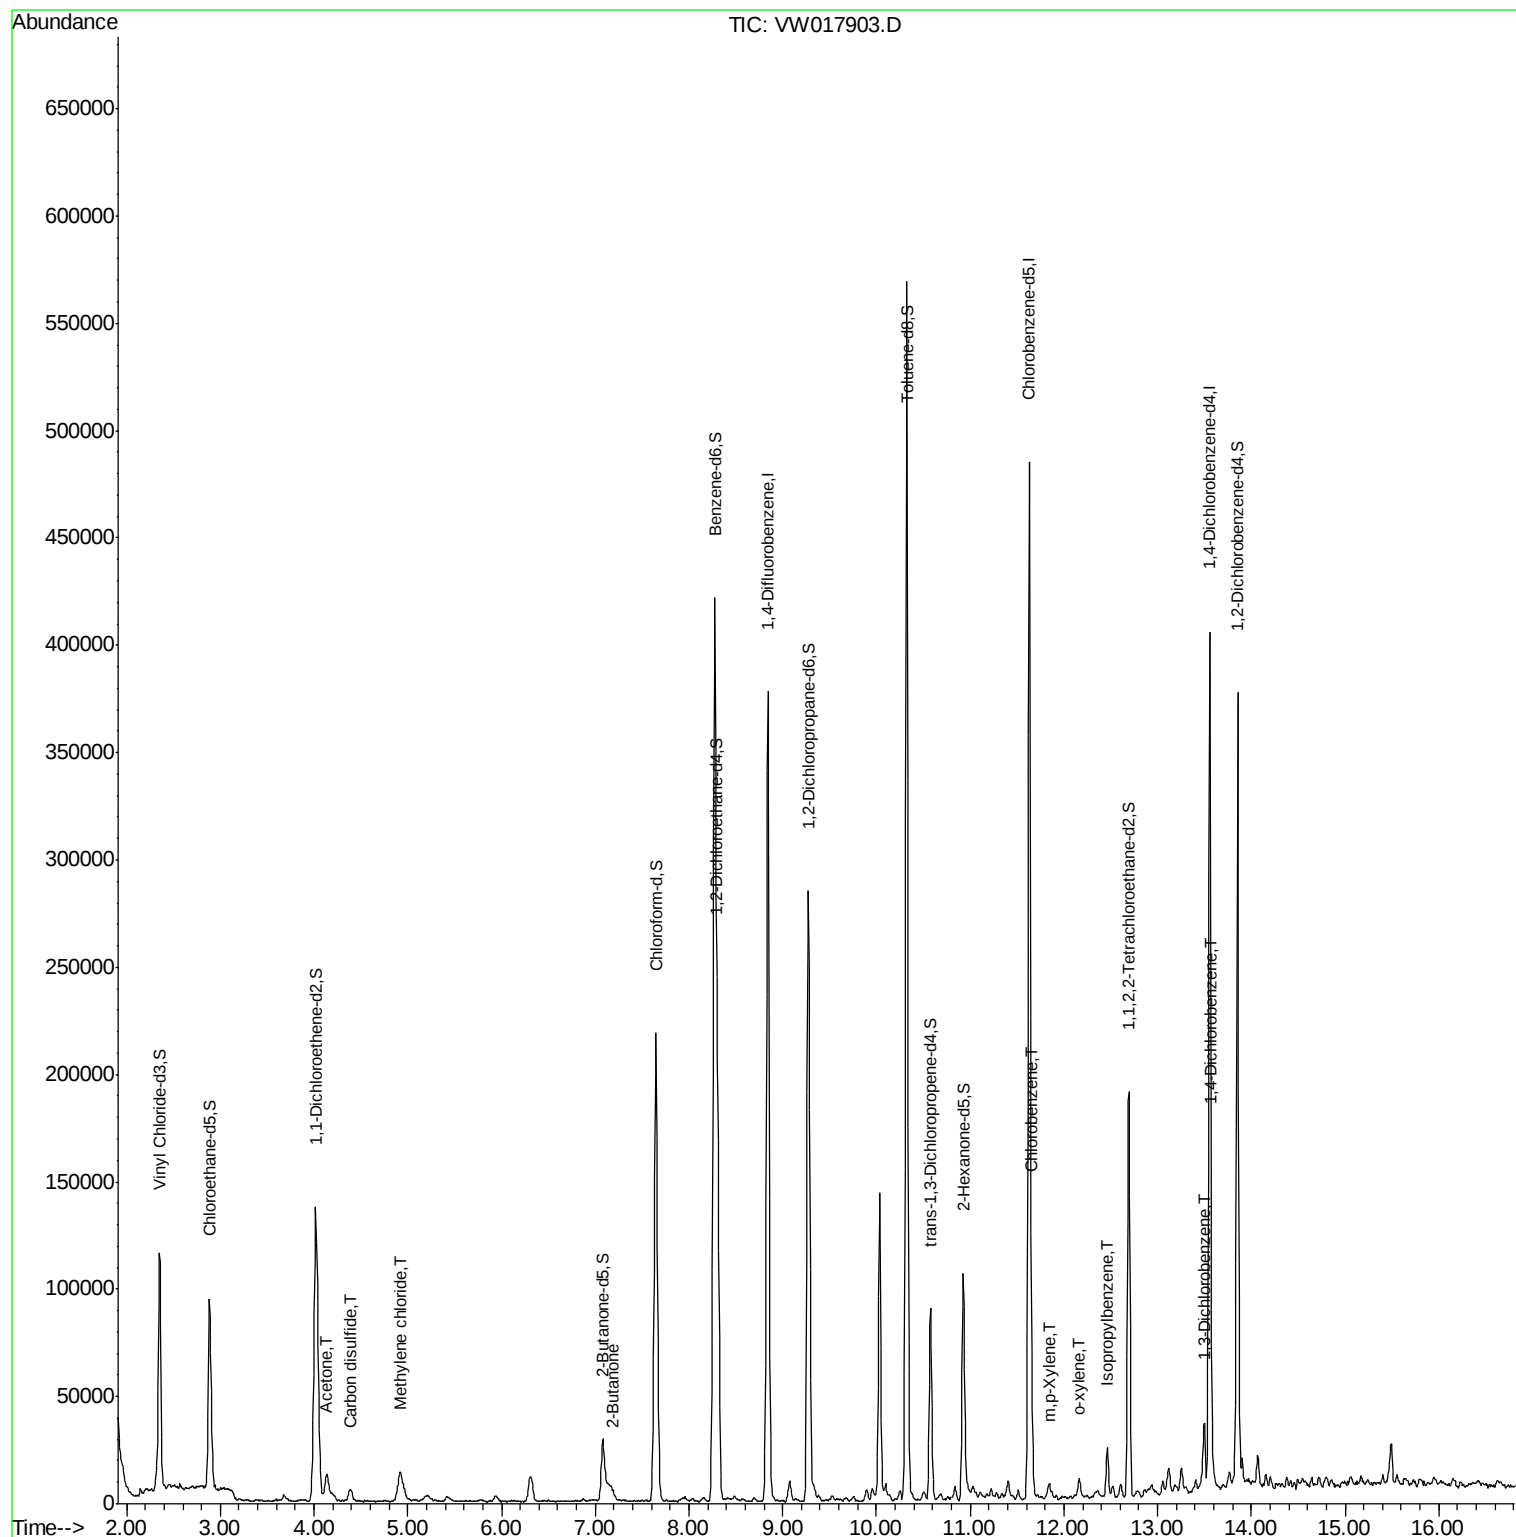

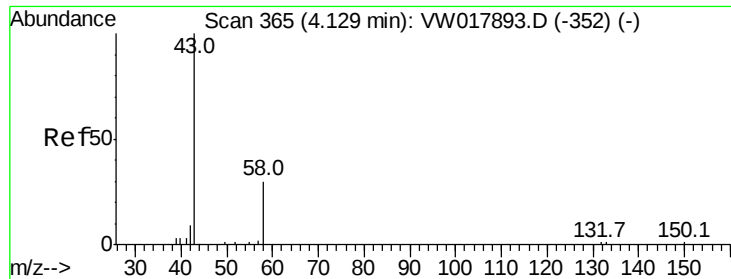

#13

Acetone

Concen: 38.197 ug/L

RT: 4.14 min Scan# 366

Delta R.T. 0.01 min

Lab File: VW017903.D

Acq: 15 Jan 2021 17:22

Instrument :

MSVOA_W

ClientSampleId :

F1C10

Tot Ion: 43 Resp: 24544

Ion Ratio Lower Upper

43 100





58 13.8 0.0 68.4

Manual Integrations

APPROVED

apatel

1/18/2021 8:50:58 AM

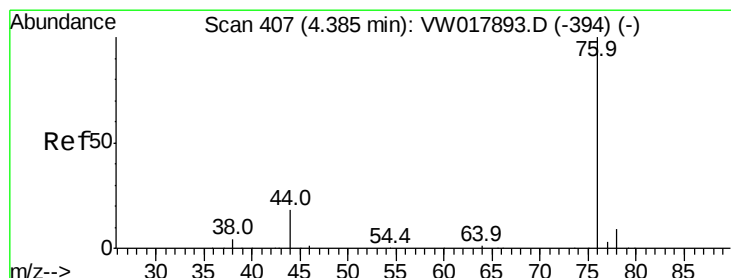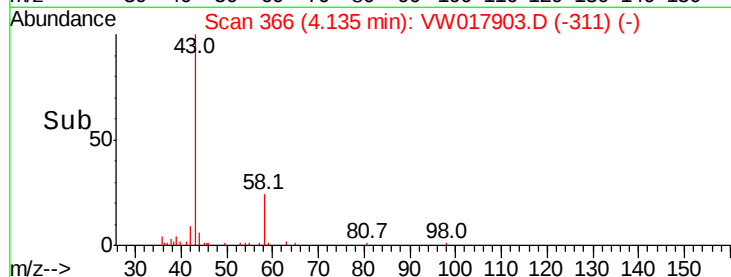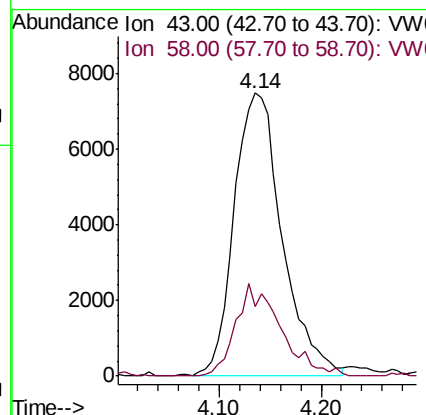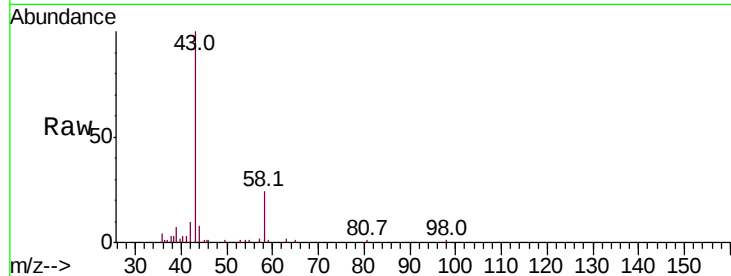

#14

Carbon disulfide

Concen: 1.086 ug/L

RT: 4.39 min Scan# 408

Delta R.T. 0.01 min

Lab File: VW017903.D




Acq: 15 Jan 2021 17:22


Tgt Ion: 76 Resp: 11858

Ion Ratio Lower Upper

76 100

78 8.8 7.0 10.4

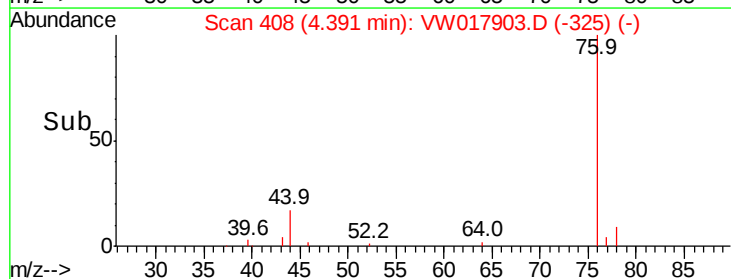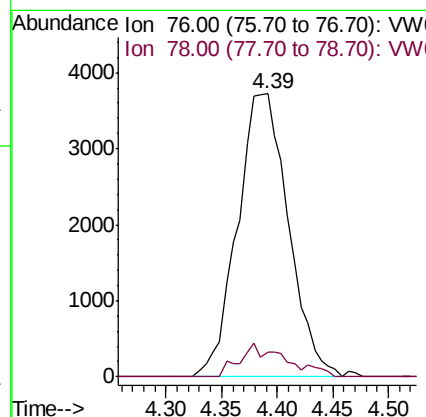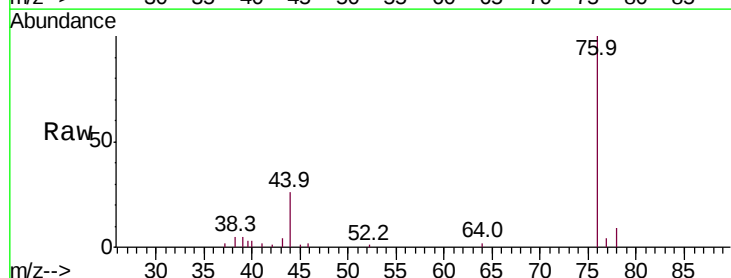

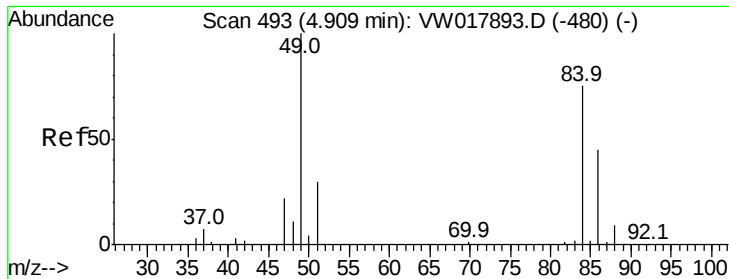





#16
Methvlene chloride
Concen: 2.386 ug/L m
RT: 4.92 min Scan# 495
Delta R.T. 0.01 min
Lab File: VW017903.D
Acq: 15 Jan 2021 17:22

Instrument :
MSVOA_W
ClientSampled :
F1C10

Tot Ion	Ratio	Lower	Upper
84	100		
49	139.7	81.2	150.8
86	67.9	44.5	82.7




Manual Integrations
APPROVED


apatel
1/18/2021 8:50:58 AM

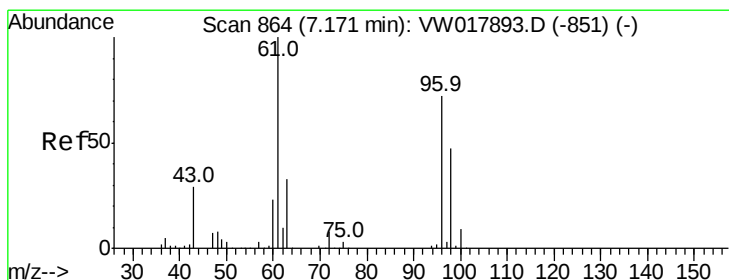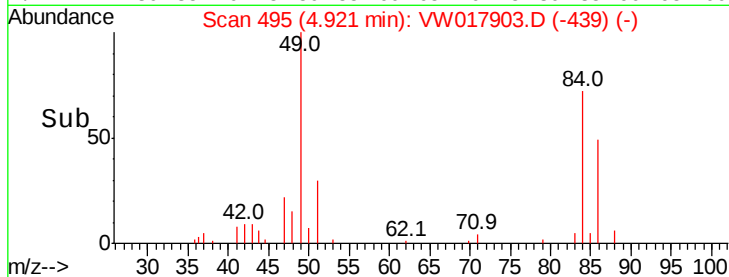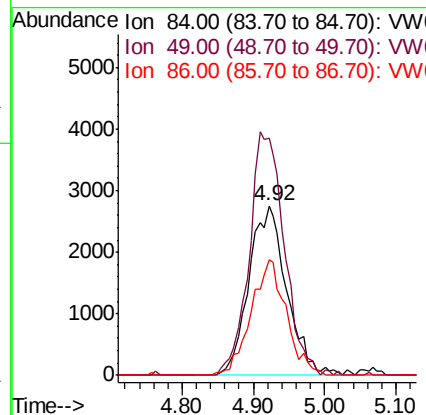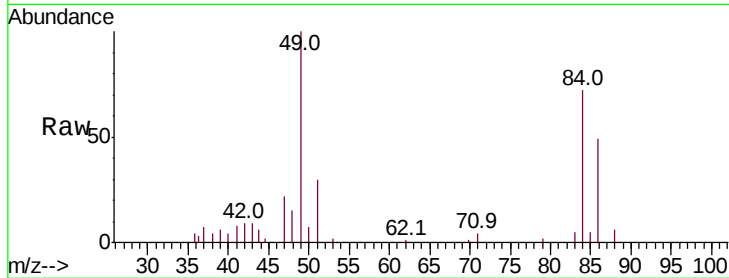

#21
2-Butanone
Concen: 8.186 ug/L m
RT: 7.19 min Scan# 867
Delta R.T. 0.02 min
Lab File: VW017903.D
Acq: 15 Jan 2021 17:22

Tgt Ion	Ratio	Lower	Upper
43	100		
72	8.8	14.4	43.2#

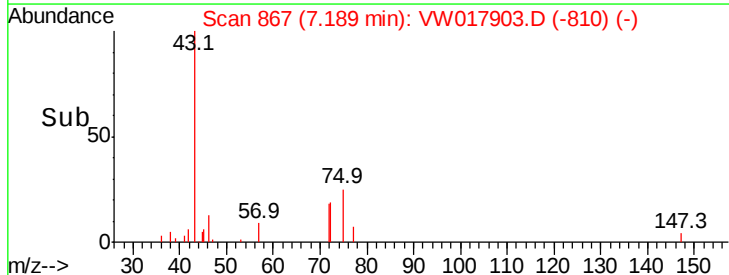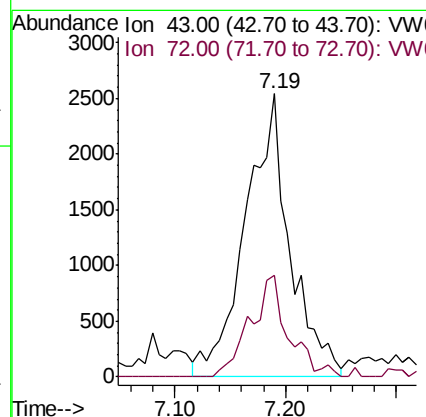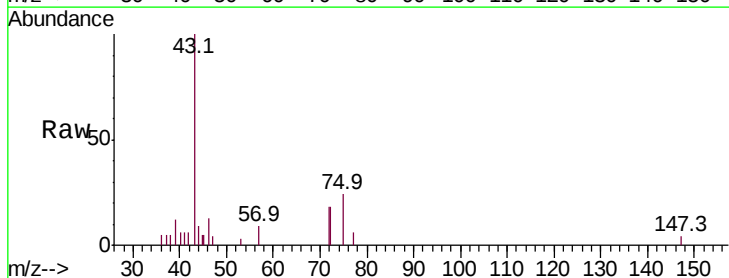

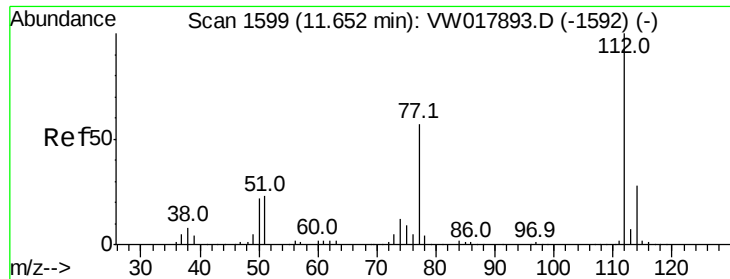





#52
Chlorobenzene
Concen: 2.114 ug/L
RT: 11.66 min Scan# 1600
Delta R.T. 0.01 min
Lab File: VW017903.D
Acq: 15 Jan 2021 17:22

Instrument :
MSVOA_W
ClientSampleId :
F1C10

Tot Ion:112 Resp: 21628
Ion Ratio Lower Upper
112 100
77 68.8 42.6 64.0#
114 30.4 21.6 40.2




Manual Integrations
APPROVED


apatel
1/18/2021 8:50:58 AM

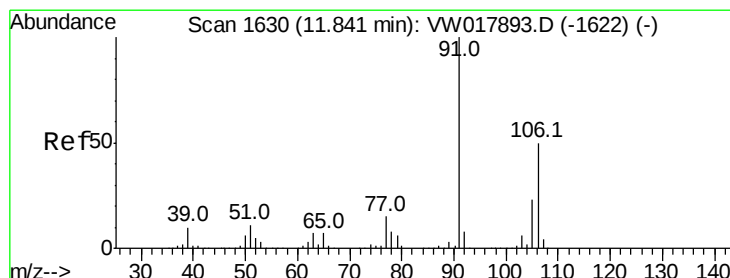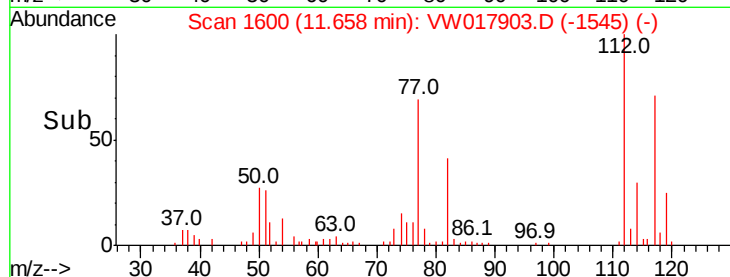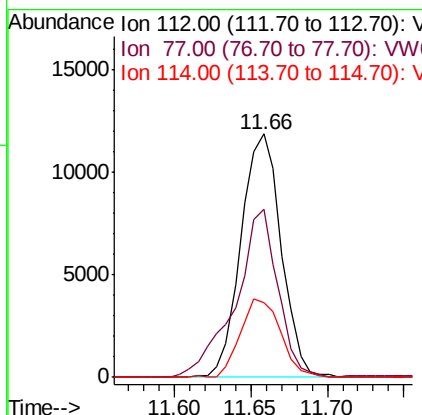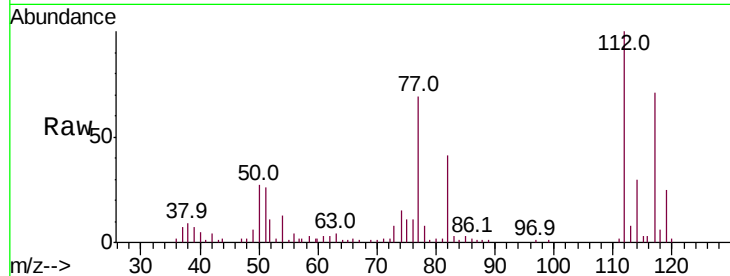

#54
m,p-Xylene
Concen: 0.252 ug/L
RT: 11.84 min Scan# 1630
Delta R.T. -0.00 min
Lab File: VW017903.D
Acq: 15 Jan 2021 17:22

Tgt Ion:106 Resp: 1833
Ion Ratio Lower Upper
106 100
91 179.8 136.4 253.4

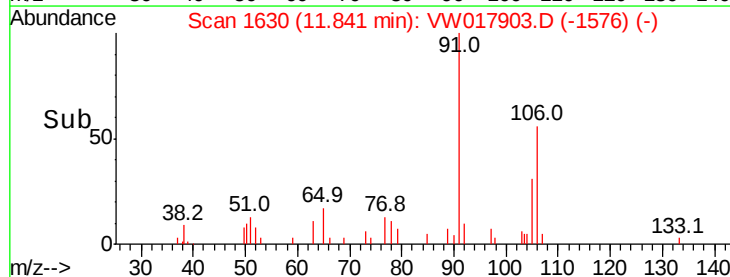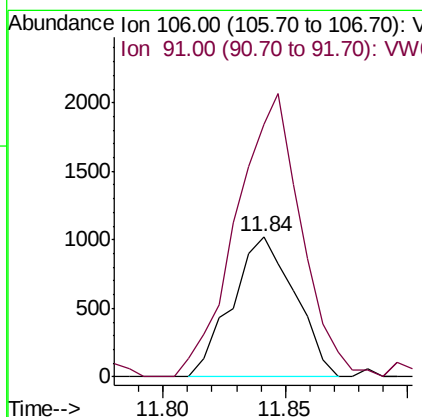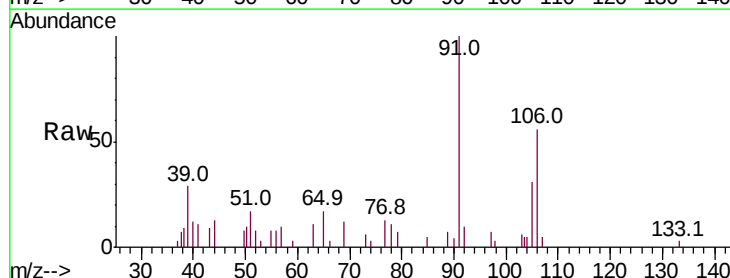

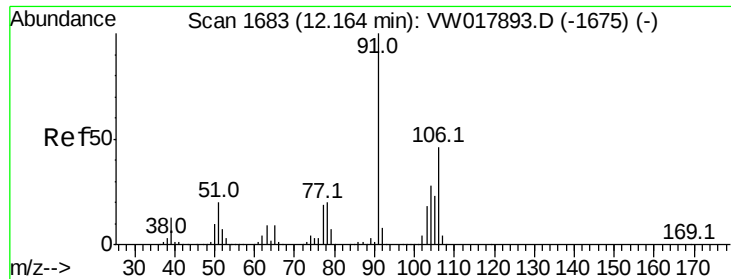





#55
o-xylene
Concen: 0.249 ug/L
RT: 12.16 min Scan# 1683
Delta R.T. -0.00 min
Lab File: VW017903.D
Acq: 15 Jan 2021 17:22

Instrument :
MSVOA_W
ClientSampled :
F1C10

Tot Ion:106 Resp: 1703
Ion Ratio Lower Upper
106 100
91 244.9 147.6 274.2




Manual Integrations
APPROVED


apatel
1/18/2021 8:50:58 AM

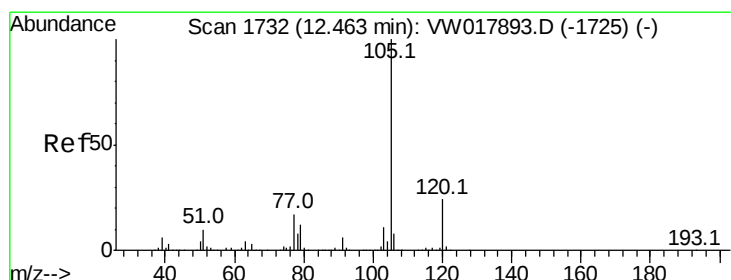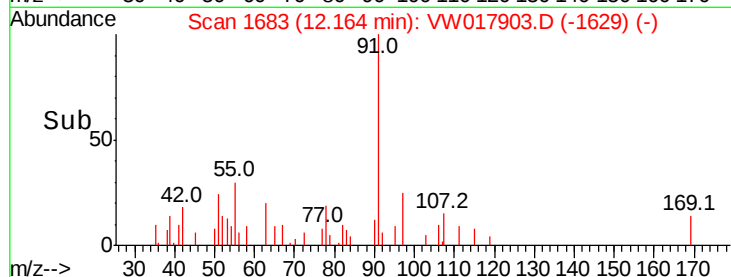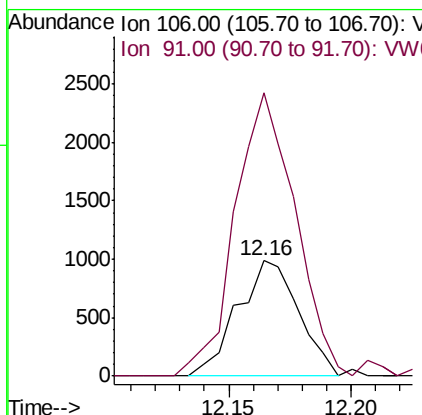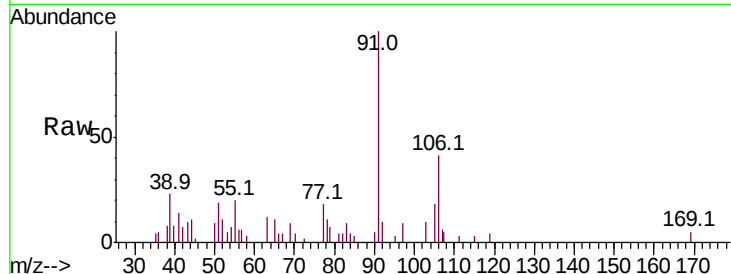

#57
Isopropylbenzene
Concen: 0.674 ug/L
RT: 12.46 min Scan# 1732
Delta R.T. -0.00 min
Lab File: VW017903.D
Acq: 15 Jan 2021 17:22

Tgt Ion:105 Resp: 12760
Ion Ratio Lower Upper
105 100
120 27.4 21.4 32.2
77 20.0 12.1 18.1#

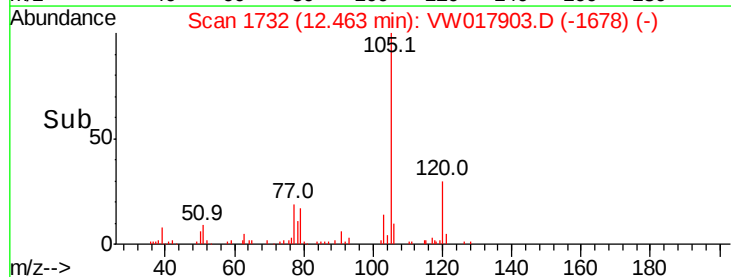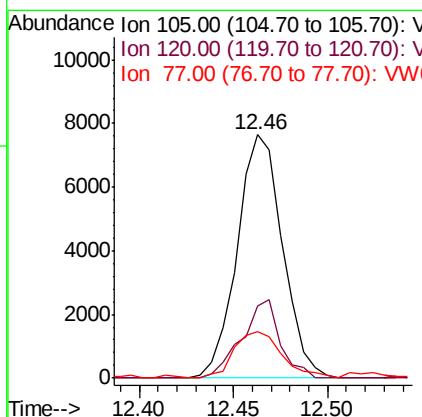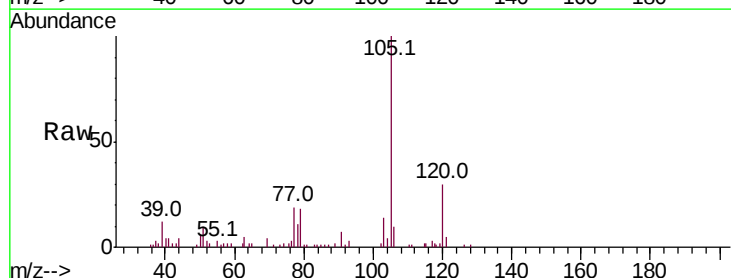

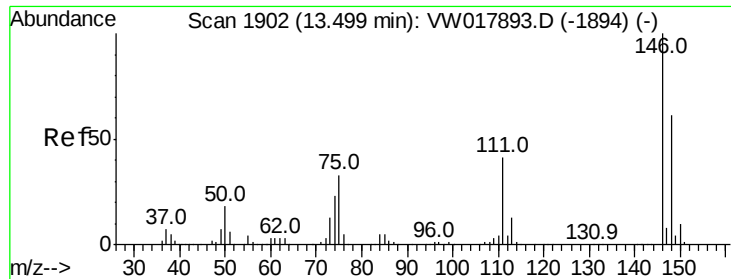





#63
 1,3-Dichlorobenzene
 Concen: 1.804 ug/L
 RT: 13.50 min Scan# 1902
 Delta R.T. -0.00 min
 Lab File: VW017903.D
 Acq: 15 Jan 2021 17:22

Instrument :
 MSVOA_W
 ClientSampled :
 F1C10

Tot Ion	Ratio	Lower	Upper
146	100		
111	40.9	28.5	52.9
148	58.2	47.8	88.8

Manual Integrations
 APPROVED

apatel
 1/18/2021 8:50:58 AM

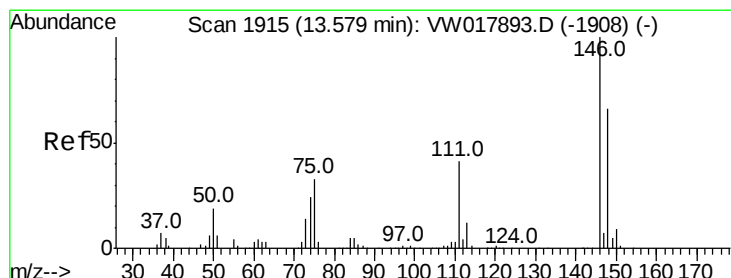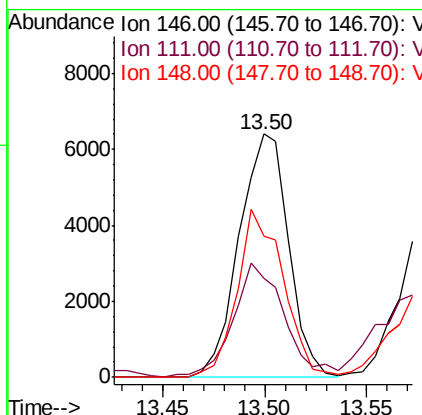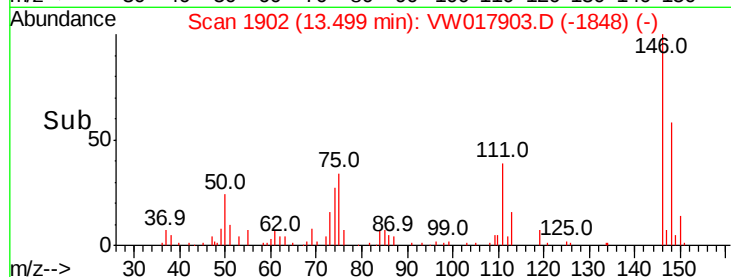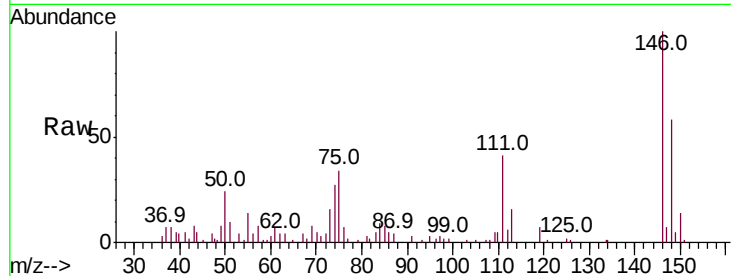

#64
 1,4-Dichlorobenzene
 Concen: 1.069 ug/L
 RT: 13.58 min Scan# 1915
 Delta R.T. -0.00 min
 Lab File: VW017903.D
 Acq: 15 Jan 2021 17:22

Tgt Ion	Ratio	Lower	Upper
146	100		
111	45.0	27.7	51.5
148	68.1	47.0	87.2

