

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011821\
 Data File : VW017925.D
 Acq On : 18 Jan 2021 13:43
 Operator : SY/VA
 Sample : VW0118SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK25

Manual Integrations
 APPROVED

MMDadoda
 1/20/2021 4:57:47 PM

Quant Time: Jan 19 06:55:50 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM011821S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 19 06:55:11 2021
 Response via : Initial Calibration

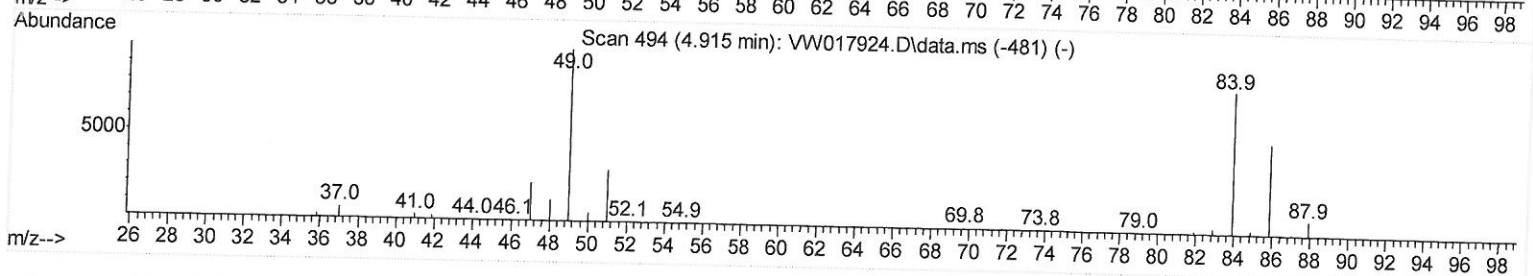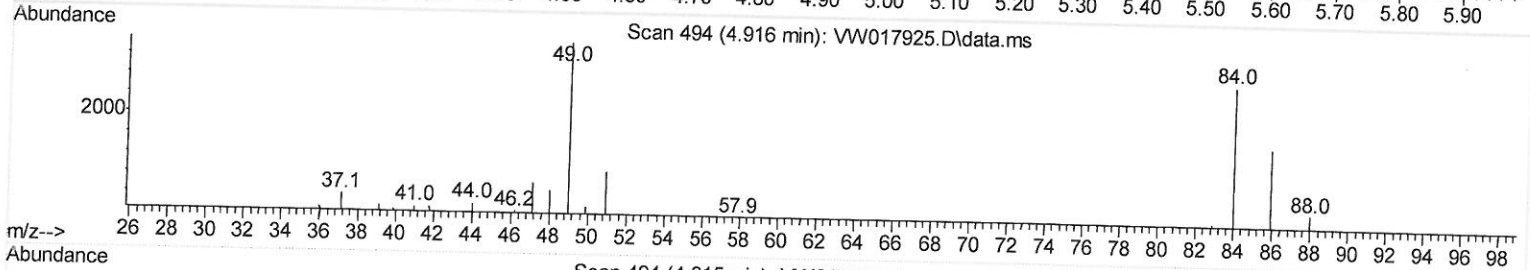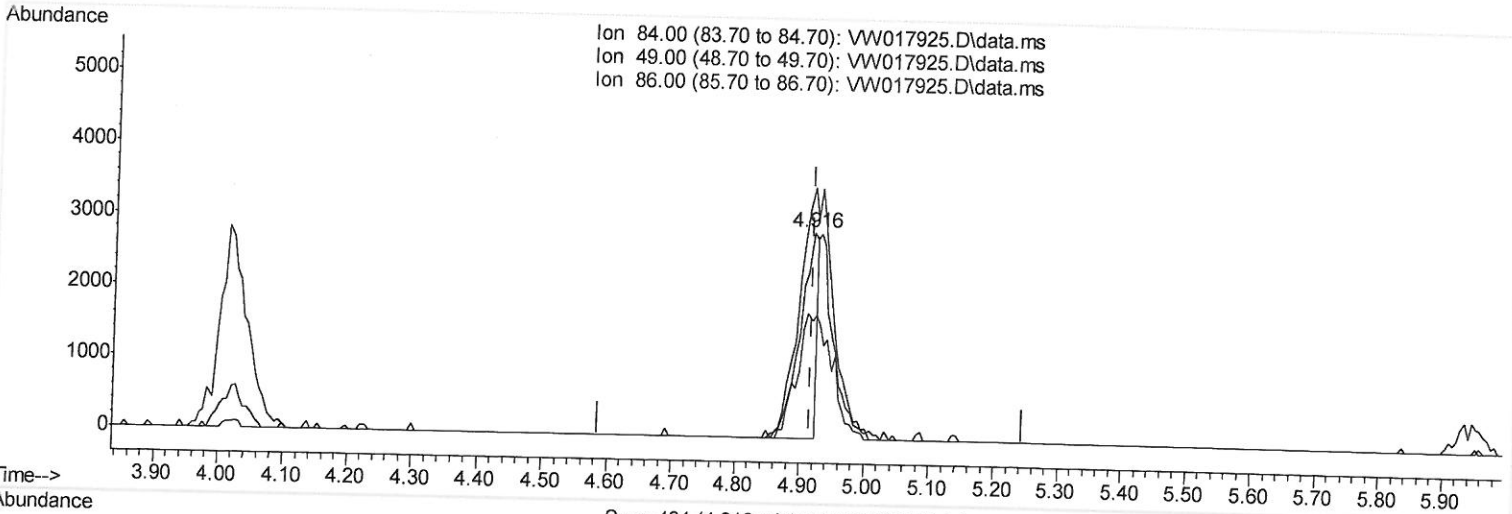

TIC: VW017925.D\data.ms

(16) Methylene chloride (T)

4.916min (+ 0.000) 0.87 ug/L

response 5307

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	116.00	122.10
86.00	63.60	59.28
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011821\
 Data File : VW017925.D
 Acq On : 18 Jan 2021 13:43
 Operator : SY/VA
 Sample : VW0118SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VBLK25

Manual Integrations
 APPROVED

MMDadoda
 1/20/2021 4:57:47 PM

Quant Time: Jan 19 06:55:50 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM011821S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 19 06:55:11 2021
 Response via : Initial Calibration

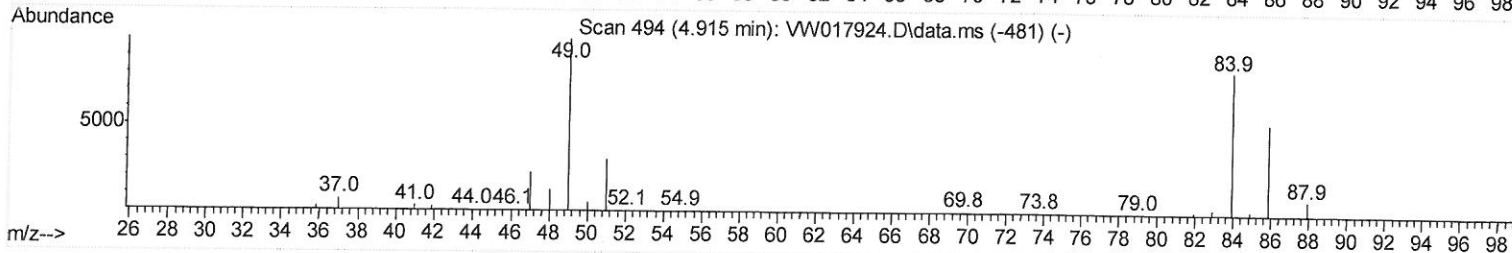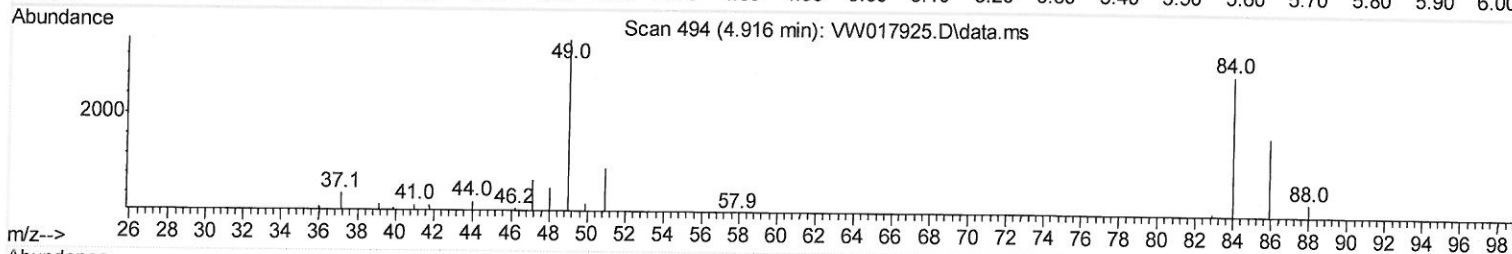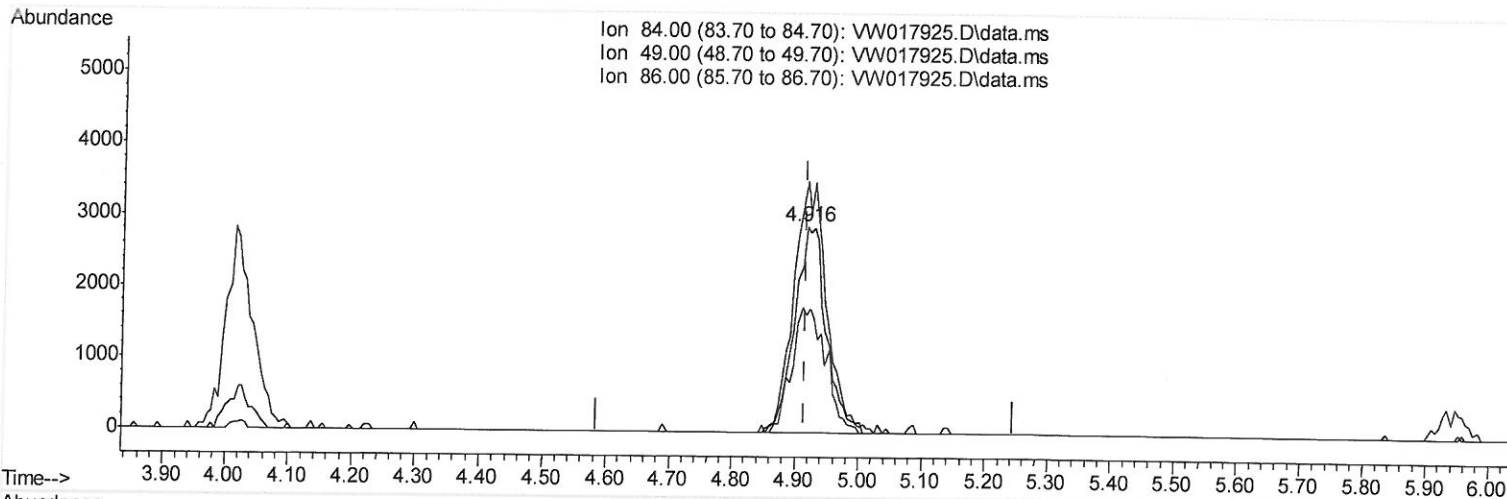

TIC: VW017925.D\data.ms

(16) Methylene chloride (T)

4.916min (+ 0.000) 1.64 ug/L m

response 9966

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	116.00	122.10
86.00	63.60	57.05
0.00	0.00	0.00

01/21/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011821\
 Data File : VW017925.D
 Acq On : 18 Jan 2021 13:43
 Operator : SY/VA
 Sample : VW0118SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK25

Manual Integrations
 APPROVED

MMDadoda
 1/20/2021 4:57:47 PM

Quant Time: Jan 19 06:55:50 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM011821S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 19 06:55:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	419548	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	392248	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	188578	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	168495	25.59	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	102.36%		
7) Chloroethane-d5	2.892	69	140418	25.83	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	103.32%		
10) 1,1-Dichloroethene-d2	4.019	63	231120	19.43	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	77.72%		
20) 2-Butanone-d5	7.074	46	84887	53.31	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.62%		
24) Chloroform-d	7.647	84	290639	25.39	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	101.56%		
26) 1,2-Dichloroethane-d4	8.305	65	177041	27.34	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	109.36%		
29) Benzene-d6	8.275	84	582259	25.94	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	103.76%		
33) 1,2-Dichloropropane-d6	9.275	67	169901	26.59	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	106.36%		
37) Toluene-d8	10.323	98	553446	26.26	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	105.04%		
38) trans-1,3-Dichloroprop...	10.579	79	74630	25.58	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	102.32%		
39) 2-Hexanone-d5	10.927	63	61210	53.44	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.88%		
48) 1,1,2,2-Tetrachloroeth...	0.000	84	0d	0.00	ug/L	
Spiked Amount 25.000	Range 45 - 120		Recovery =	0.00%#		
61) 1,2-Dichlorobenzene-d4	13.853	152	187102	28.52	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	114.08%		

Target Compounds

16) Methylene chloride	4.916	84	9966m	> 1.64 ug/L	Qvalue
------------------------	-------	----	-------	-------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

01/21/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011821\
Data File : VW017925.D
Acq On : 18 Jan 2021 13:43
Operator : SY/VA
Sample : VW0118SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VBLK25

Manual Integrations
APPROVED

MMDadoda
1/20/2021 4:57:47 PM

Quant Time: Jan 19 06:55:50 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM011821S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 19 06:55:11 2021
Response via : Initial Calibration

