

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011821\
Data File : VW017939.D
Acq On : 18 Jan 2021 19:27
Operator : SY/VA
Sample : M1167-05
Misc : 5.32G/10ML/MSVOA_W/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFT75

Manual Integrations
APPROVED

MMDadoda
1/20/2021 4:58:12 PM

Quant Time: Jan 19 07:00:15 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM011821S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 19 06:55:11 2021
Response via : Initial Calibration

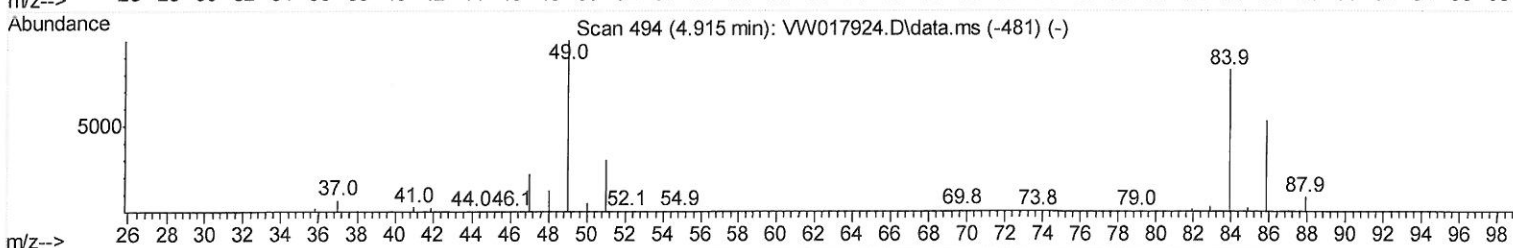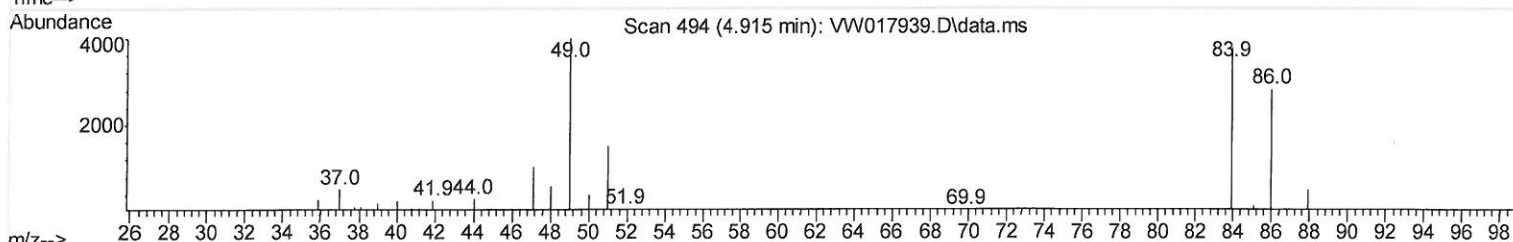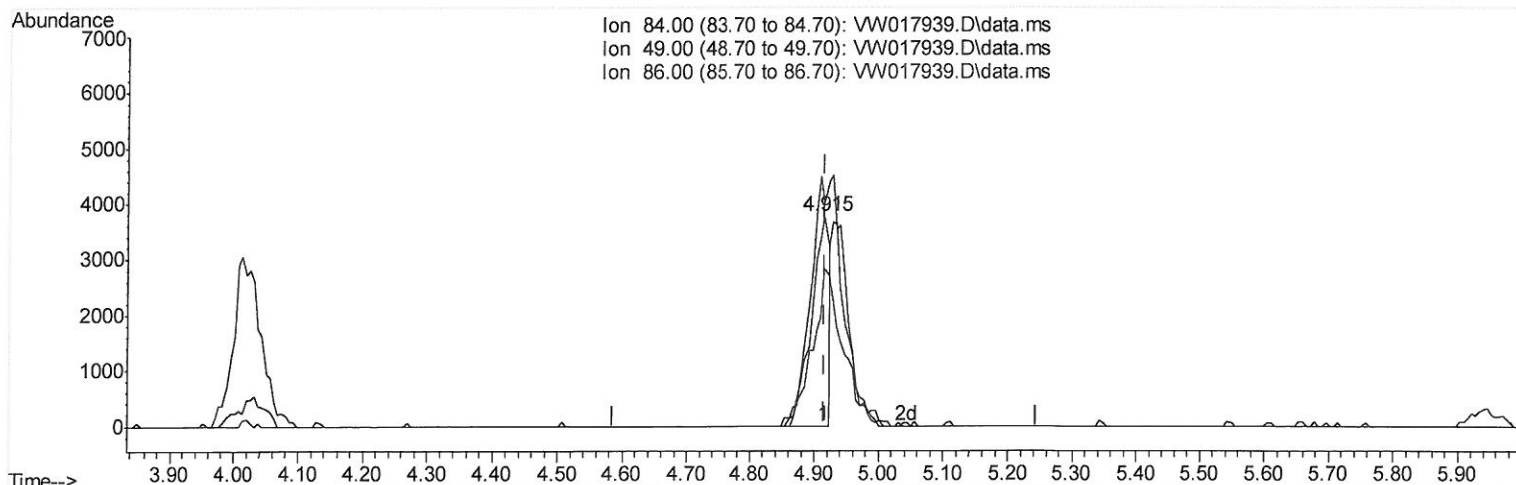

TIC: VW017939.D\data.ms

(16) Methylene chloride (T)

4.915min (-0.000) 1.06 ug/L

response 7272

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	116.00	106.24
86.00	63.60	74.99
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011821\
Data File : VW017939.D
Acq On : 18 Jan 2021 19:27
Operator : SY/VA
Sample : M1167-05
Misc : 5.32G/10ML/MSVOA_W/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFT75

Manual Integrations
APPROVED

MMDadoda
1/20/2021 4:58:12 PM

Quant Time: Jan 19 07:00:15 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM011821S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 19 06:55:11 2021
Response via : Initial Calibration

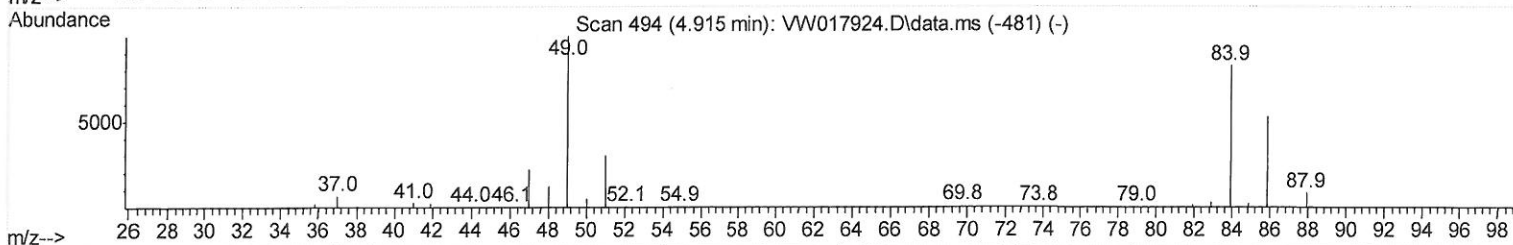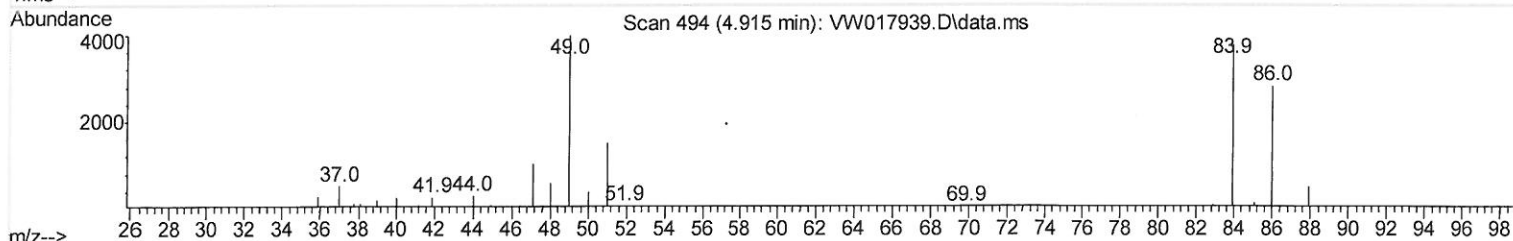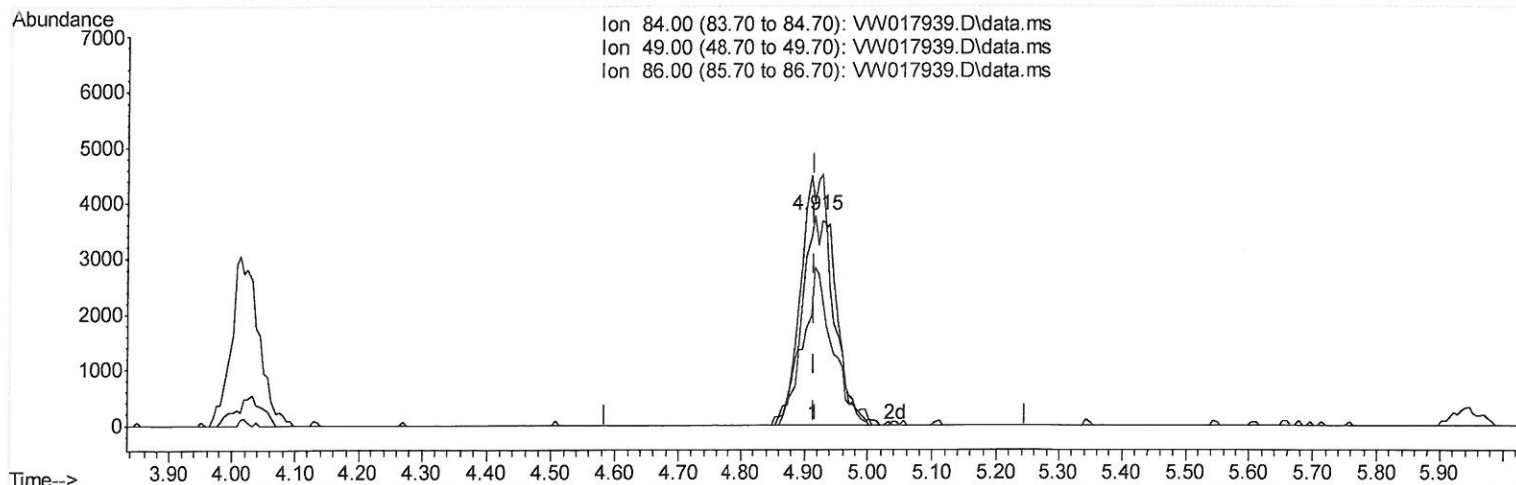

TIC: VW017939.D\data.ms

(16) Methylene chloride (T)

4.915min (-0.000) 1.95 ug/L m

response 13339

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	116.00	106.24
86.00	63.60	74.99
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011821\
 Data File : VW017939.D
 Acq On : 18 Jan 2021 19:27
 Operator : SY/VA
 Sample : M1167-05
 Misc : 5.32G/10ML/MSVOA_W/SOIL
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFT75

Manual Integrations
 APPROVED

MMDadoda
 1/20/2021 4:58:12 PM

Quant Time: Jan 19 07:00:15 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM011821S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 19 06:55:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	472813	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	443262	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	211289	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	178455	24.05	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	96.20%		
7) Chloroethane-d5	2.891	69	157726	25.74	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	102.96%		
10) 1,1-Dichloroethene-d2	4.019	63	238813	17.81	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	71.24%		
20) 2-Butanone-d5	7.086	46	69215	38.57	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	77.14%		
24) Chloroform-d	7.647	84	312706	24.24	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	96.96%		
26) 1,2-Dichloroethane-d4	8.305	65	176672	24.21	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	96.84%		
29) Benzene-d6	8.275	84	620596	24.46	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	97.84%		
33) 1,2-Dichloropropane-d6	9.274	67	176031	24.38	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	97.52%		
37) Toluene-d8	10.323	98	582159	24.44	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	97.76%		
38) trans-1,3-Dichloroprop...	10.579	79	74548	22.61	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	90.44%		
39) 2-Hexanone-d5	10.927	63	53166	41.08	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	82.16%		
48) 1,1,2,2-Tetrachloroeth...	12.695	84	134575	20.96	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	83.84%		
61) 1,2-Dichlorobenzene-d4	13.853	152	192915	26.24	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	104.96%		
Target Compounds						
13) Acetone	4.135	43	3411	2.70	ug/L	50
16) Methylene chloride	4.915	84	13339m	1.95	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

01/21/21 fy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011821\
Data File : VW017939.D
Acq On : 18 Jan 2021 19:27
Operator : SY/VA
Sample : M1167-05
Misc : 5.32G/10ML/MSVOA_W/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BFT75

Manual Integrations
APPROVED

MMDadoda
1/20/2021 4:58:12 PM

Quant Time: Jan 19 07:00:15 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM011821S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 19 06:55:11 2021
Response via : Initial Calibration

