

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020521\
 Data File : VW018040.D
 Acq On : 05 Feb 2021 17:59
 Operator : SY/VA
 Sample : M1330-10
 Misc : 5.55G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG540

Quant Time: Feb 06 01:09:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Feb 06 01:06:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	514746	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	439412	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	211363	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	86619	13.54	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	54.16%		
7) Chloroethane-d5	2.891	69	71090	14.00	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	56.00%		
10) 1,1-Dichloroethene-d2	4.019	63	133102	10.41	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	41.64%#		
20) 2-Butanone-d5	7.074	46	42269	24.76	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	49.52%		
24) Chloroform-d	7.647	84	203921	15.10	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	60.40%		
26) 1,2-Dichloroethane-d4	8.305	65	104427	14.51	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	58.04%#		
29) Benzene-d6	8.275	84	409839	16.99	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	67.96%		
33) 1,2-Dichloropropane-d6	9.274	67	113741	16.86	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	67.44%#		
37) Toluene-d8	10.323	98	372876	16.24	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	64.96%		
38) trans-1,3-Dichloroprop...	10.579	79	45955	15.02	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	60.08%		
39) 2-Hexanone-d5	10.927	63	35002	27.13	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	54.26%		
48) 1,1,2,2-Tetrachloroeth...	12.695	84	86005	14.51	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	58.04%		
61) 1,2-Dichlorobenzene-d4	13.853	152	125041	16.58	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	66.32%#		
Target Compounds						
13) Acetone	4.123	43	18784	14.87	ug/L	97
14) Carbon disulfide	4.391	76	6004	0.30	ug/L	97
16) Methylene chloride	4.922	84	20619	2.50	ug/L	89
21) 2-Butanone	7.177	43	6953	3.62	ug/L	95
22) cis-1,2-Dichloroethene	7.171	96	33486	4.39	ug/L	94
35) Trichloroethene	8.842	95	14656	2.03	ug/L #	3
40) 1,2-Dichloropropane	9.274	63	12790	2.17	ug/L #	84
42) cis-1,3-Dichloropropene	10.037	75	3153	0.33	ug/L #	66
59) 1,2,3-Trichloropropane	13.554	75	21167	4.70	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW020521\
Data File : VW018040.D
Acq On : 05 Feb 2021 17:59
Operator : SY/VA
Sample : M1330-10
Misc : 5.55G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG540

Quant Time: Feb 06 01:09:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 06 01:06:17 2021
Response via : Initial Calibration




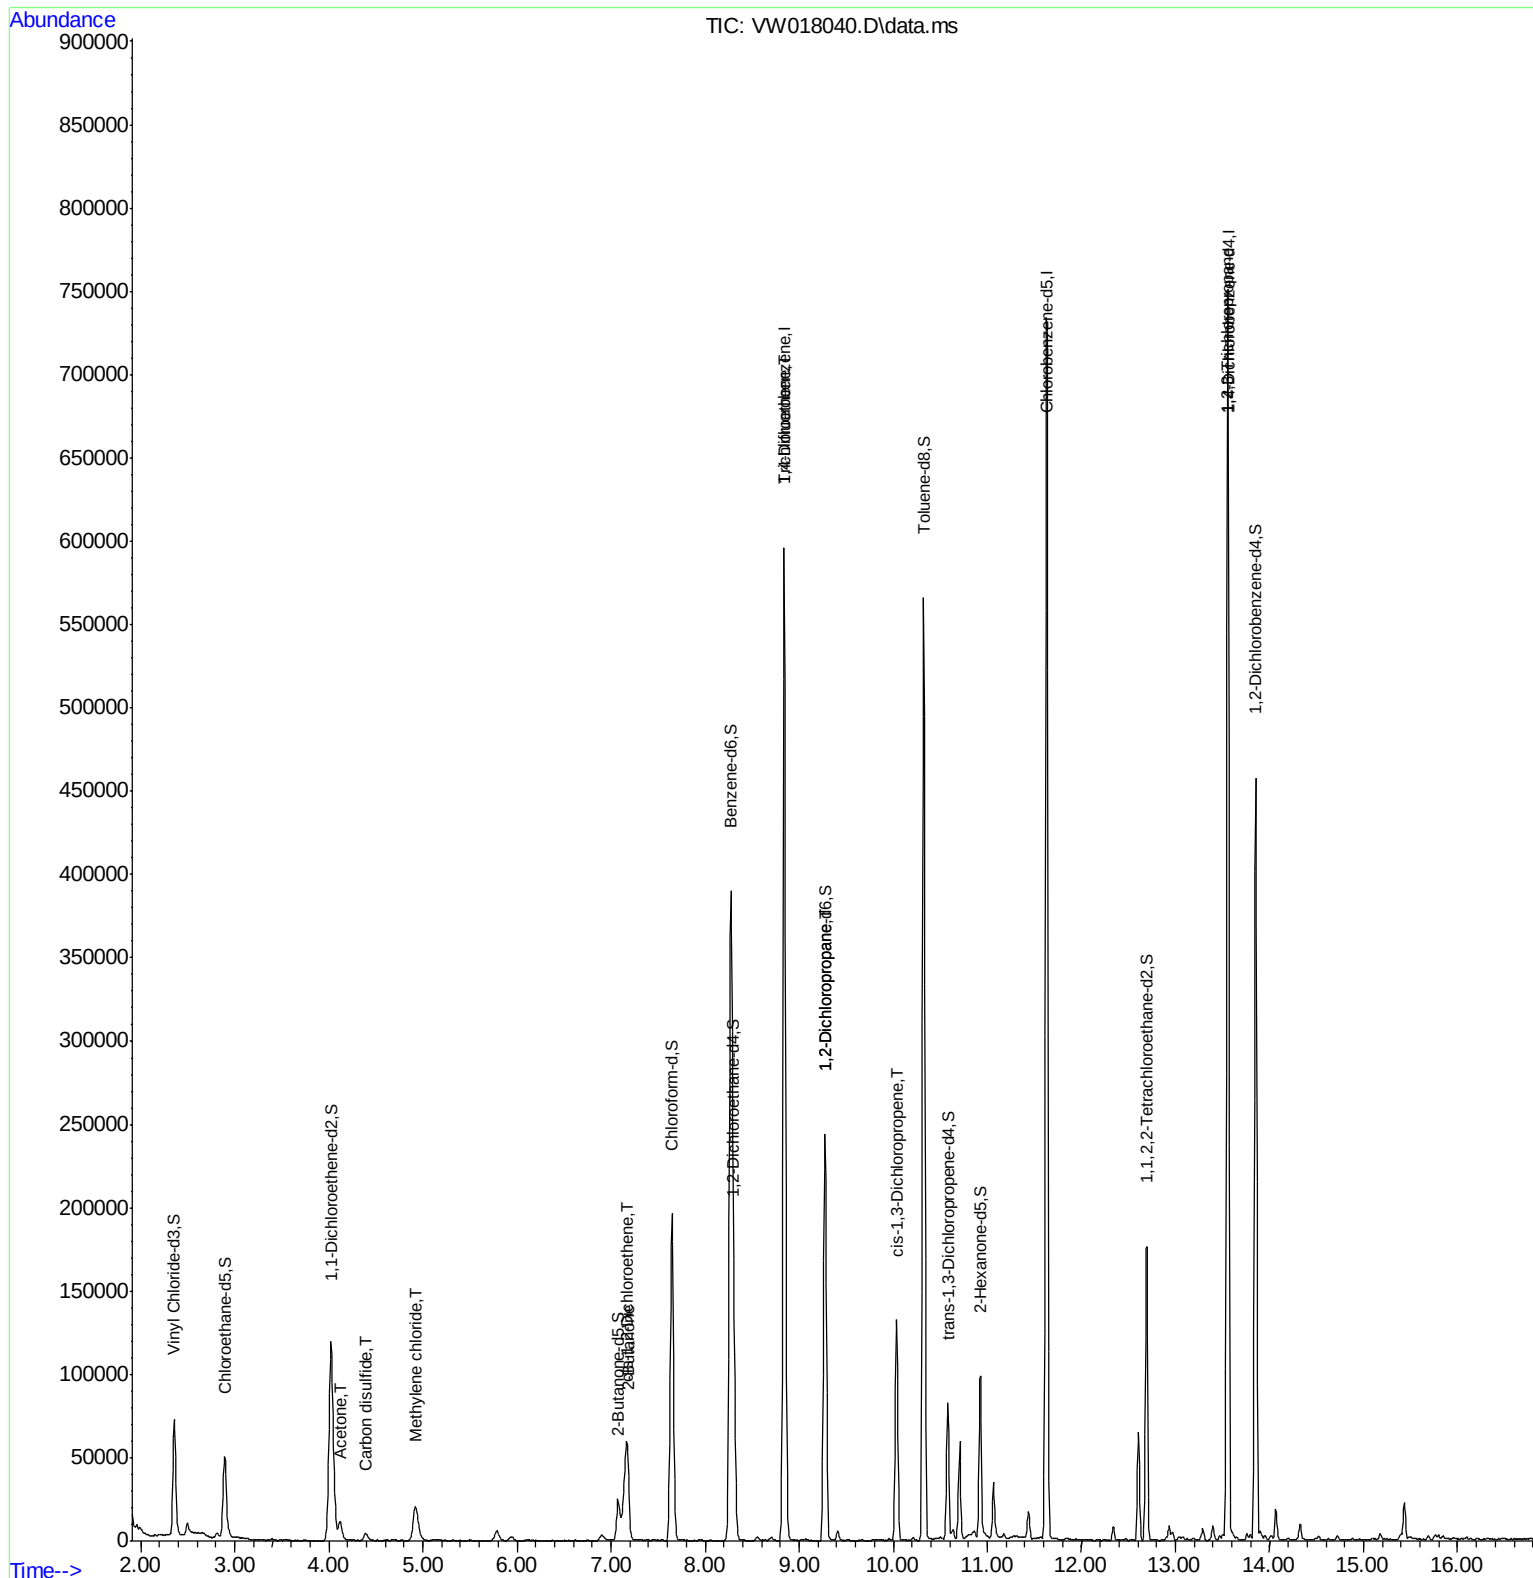


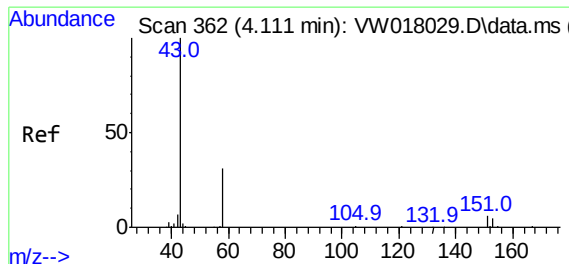

#13
Acetone
Concen: 14.87 ug/L
RT: 4.123 min Scan# 364
Delta R.T. 0.012 min
Lab File: VW018040.D
Acq: 05 Feb 2021 17:59




Instrument :
MSVOA_W
ClientSampled :
BG540


Tgt Ion: 43 Resp: 18784
Ion Ratio Lower Upper
43 100
58 32.2 0.0 68.4

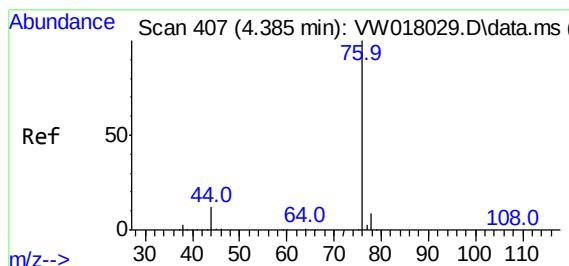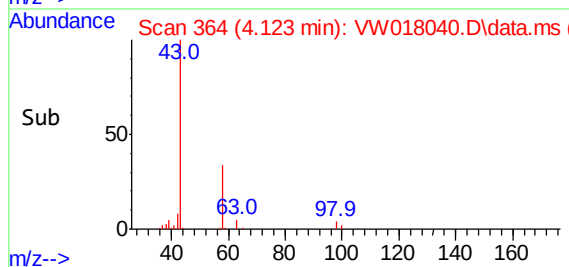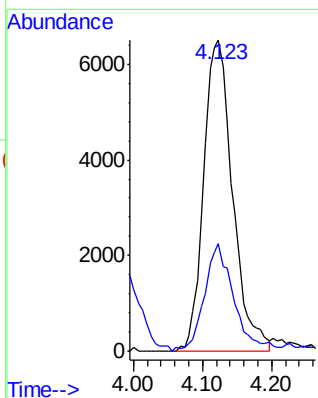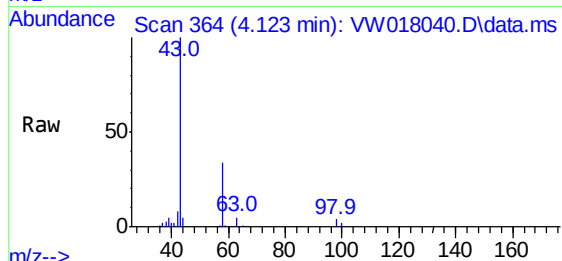

#14
Carbon disulfide
Concen: 0.30 ug/L
RT: 4.391 min Scan# 408
Delta R.T. 0.006 min
Lab File: VW018040.D
Acq: 05 Feb 2021 17:59

Tgt Ion: 76 Resp: 6004
Ion Ratio Lower Upper
76 100
78 9.9 7.0 10.4

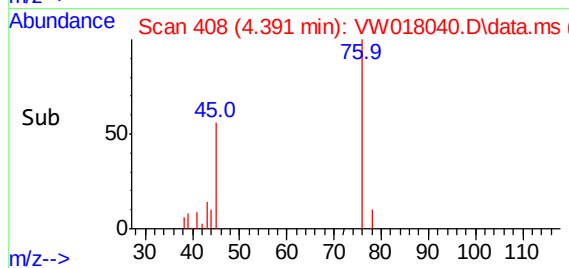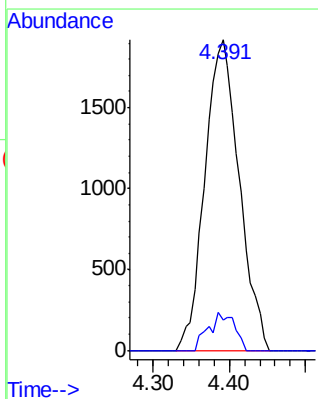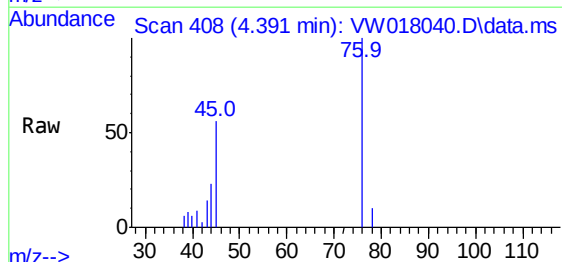




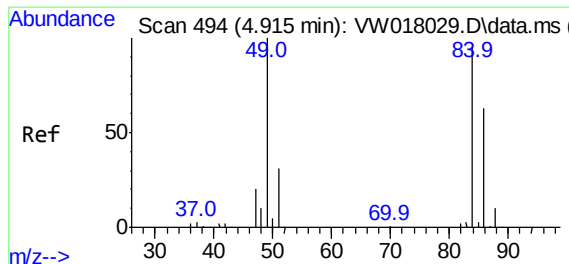


#16
Methylene chloride
Concen: 2.50 ug/L
RT: 4.922 min Scan# 495
Delta R.T. 0.006 min
Lab File: VW018040.D
Acq: 05 Feb 2021 17:59

Instrument :
MSVOA_W
ClientSampled :
BG540

Tgt Ion: 84 Resp: 20619




Ion	Ratio	Lower	Upper
84	100		
49	97.3	81.2	150.8
86	63.9	44.5	82.7

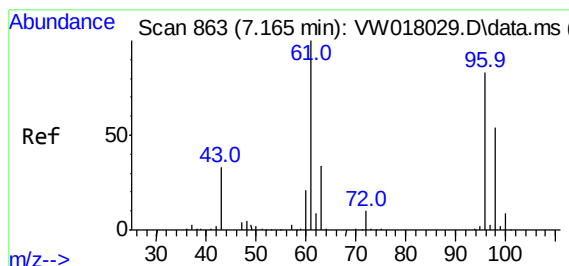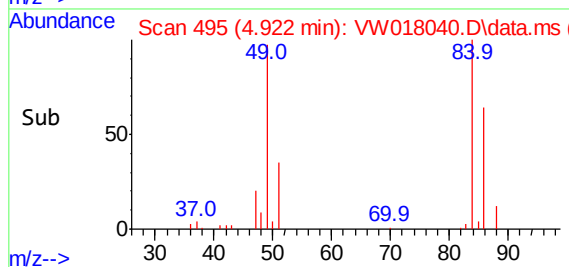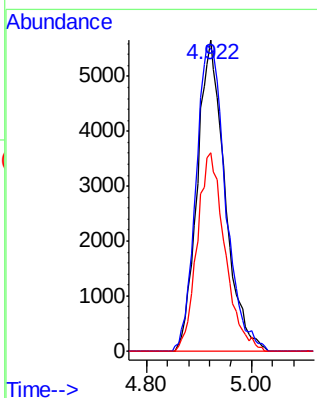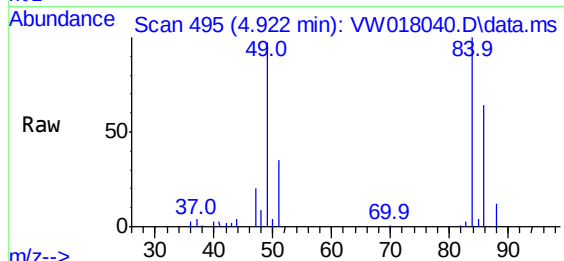


#21
2-Butanone
Concen: 3.62 ug/L
RT: 7.177 min Scan# 865
Delta R.T. 0.012 min
Lab File: VW018040.D
Acq: 05 Feb 2021 17:59

Tgt Ion: 43 Resp: 6953

Ion	Ratio	Lower	Upper
43	100		
72	31.6	14.4	43.2

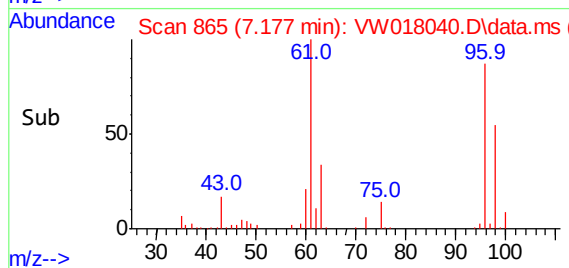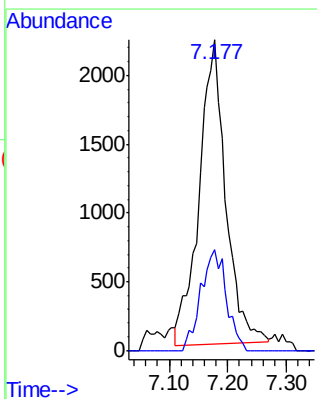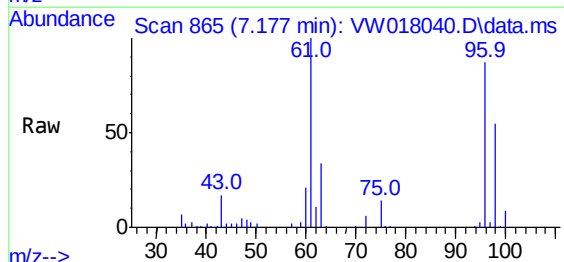




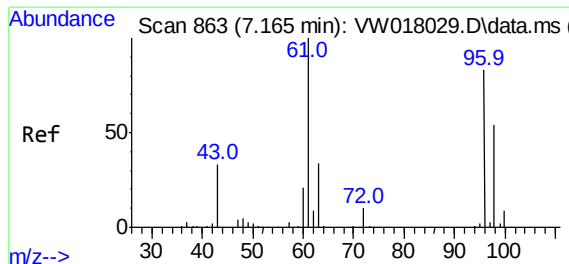


#22
cis-1,2-Dichloroethene
Concen: 4.39 ug/L
RT: 7.171 min Scan# 864
Delta R.T. 0.006 min
Lab File: VW018040.D
Acq: 05 Feb 2021 17:59

Instrument :
MSVOA_W
ClientSampleId :
BG540

Tgt Ion: 96 Resp: 33486




Ion	Ratio	Lower	Upper
96	100		
61	111.3	84.6	157.2
98	65.3	44.7	82.9

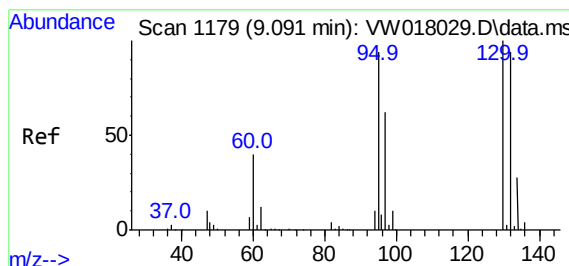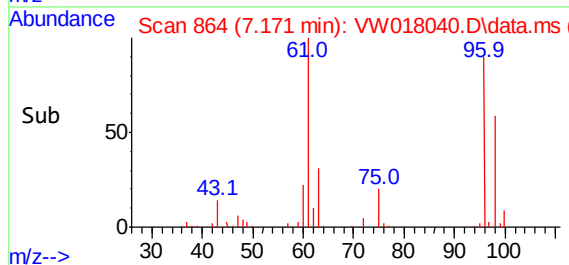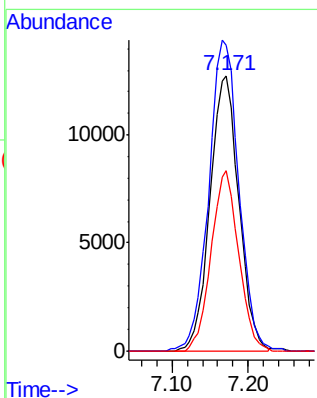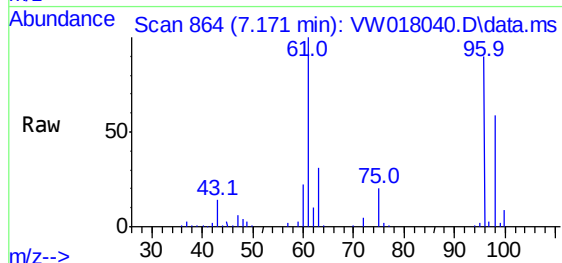


#35
Trichloroethene
Concen: 2.03 ug/L
RT: 8.842 min Scan# 1138
Delta R.T. -0.250 min
Lab File: VW018040.D
Acq: 05 Feb 2021 17:59

Tgt Ion: 95 Resp: 14656

Ion	Ratio	Lower	Upper
95	100		
97	0.0	45.0	83.6#
132	0.0	71.0	131.8#
130	0.0	75.6	140.4#


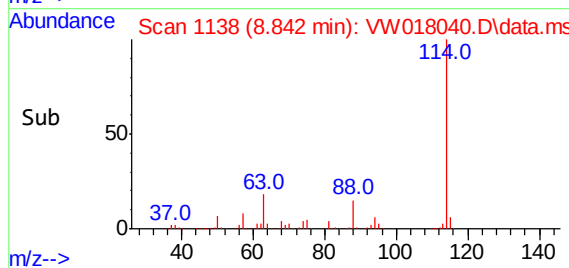
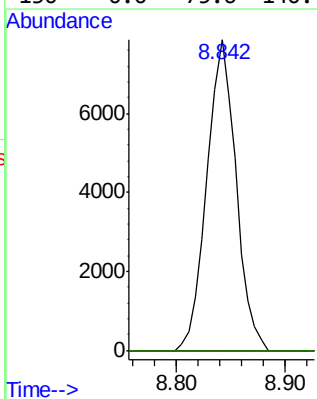
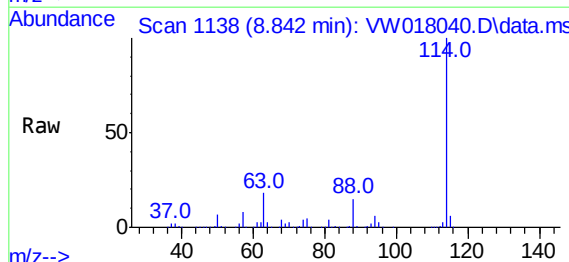


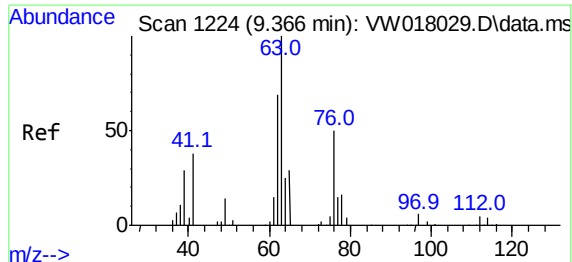

#40
1,2-Dichloropropane
Concen: 2.17 ug/L
RT: 9.274 min Scan# 1209
Delta R.T. -0.091 min
Lab File: VW018040.D
Acq: 05 Feb 2021 17:59




Instrument :
MSVOA_W
ClientSampled :
BG540


Tgt Ion: 63 Resp: 12790
Ion Ratio Lower Upper
63 100
112 0.0 4.2 6.4#

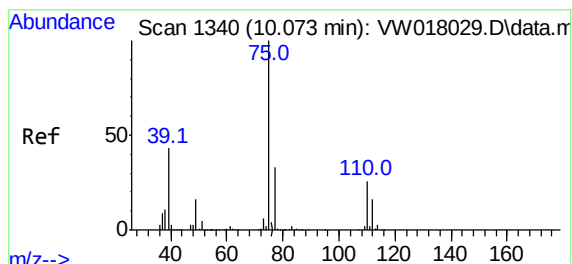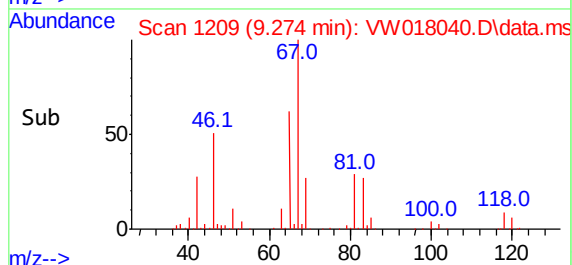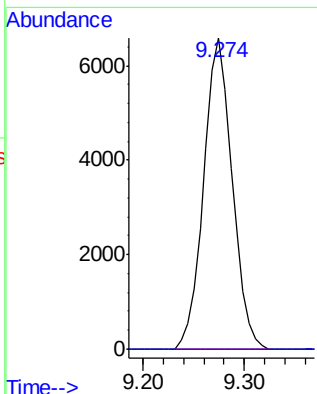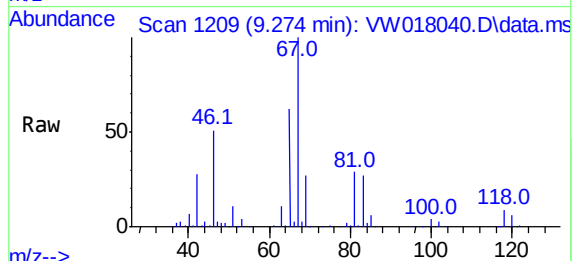

#42
cis-1,3-Dichloropropene
Concen: 0.33 ug/L
RT: 10.037 min Scan# 1334
Delta R.T. -0.036 min
Lab File: VW018040.D
Acq: 05 Feb 2021 17:59


Tgt Ion: 75 Resp: 3153
Ion Ratio Lower Upper
75 100
77 51.3 22.7 42.3#

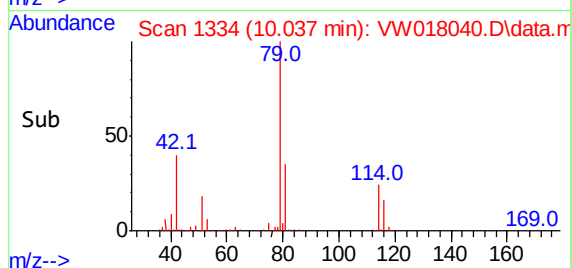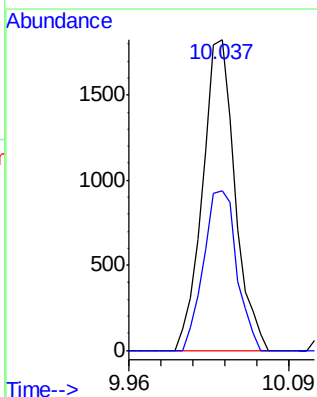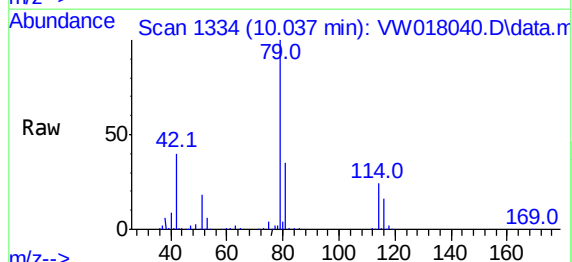

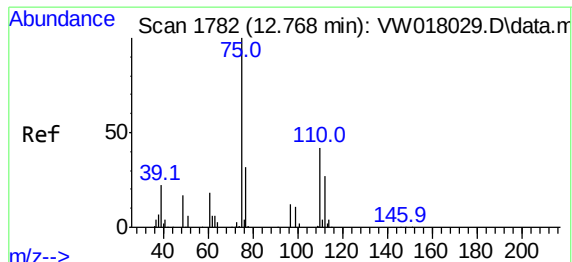

#59
 1,2,3-Trichloropropane
 Concen: 4.70 ug/L
 RT: 13.554 min Scan# 1911
 Delta R.T. 0.787 min
 Lab File: VW018040.D
 Acq: 05 Feb 2021 17:59

Instrument :
 MSVOA_W
 ClientSampleId :
 BG540

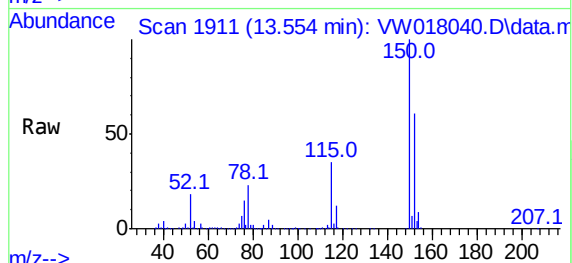

Tgt Ion: 75 Resp: 21167
 Ion Ratio Lower Upper
 75 100
 77 34.3 26.6 39.8

