

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021921\
 Data File : VW018211.D
 Acq On : 19 Feb 2021 14:32
 Operator : SY/VA
 Sample : M1371-21
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Quant Time: Feb 19 17:44:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 19 17:37:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	390720	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	358786	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	191731	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	86480	17.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.24%
7) Chloroethane-d5	2.891	69	76750	19.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.64%
10) 1,1-Dichloroethene-d2	4.019	63	148921	15.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.36%
20) 2-Butanone-d5	7.074	46	56544	43.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.26%
24) Chloroform-d	7.647	84	243510	23.75	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.00%
26) 1,2-Dichloroethane-d4	8.305	65	125768	23.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.12%
29) Benzene-d6	8.275	84	474860	24.10	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.40%
33) 1,2-Dichloropropane-d6	9.274	67	136250	24.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.92%
37) Toluene-d8	10.323	98	452666	24.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.60%
38) trans-1,3-Dichloroprop...	10.579	79	58212	23.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.24%
39) 2-Hexanone-d5	10.920	63	48285	45.84	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.68%
48) 1,1,2,2-Tetrachloroeth...	12.688	84	118837	24.55	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.20%
61) 1,2-Dichlorobenzene-d4	13.853	152	182983	26.75	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.00%
Target Compounds						
					Qvalue	
13) Acetone	4.129	43	1225	1.28	ug/L	49
16) Methylene chloride	4.915	84	34855	5.57	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW021921\
Data File : VW018211.D
Acq On : 19 Feb 2021 14:32
Operator : SY/VA
Sample : M1371-21
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Feb 19 17:44:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM012921S.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 19 17:37:31 2021
Response via : Initial Calibration




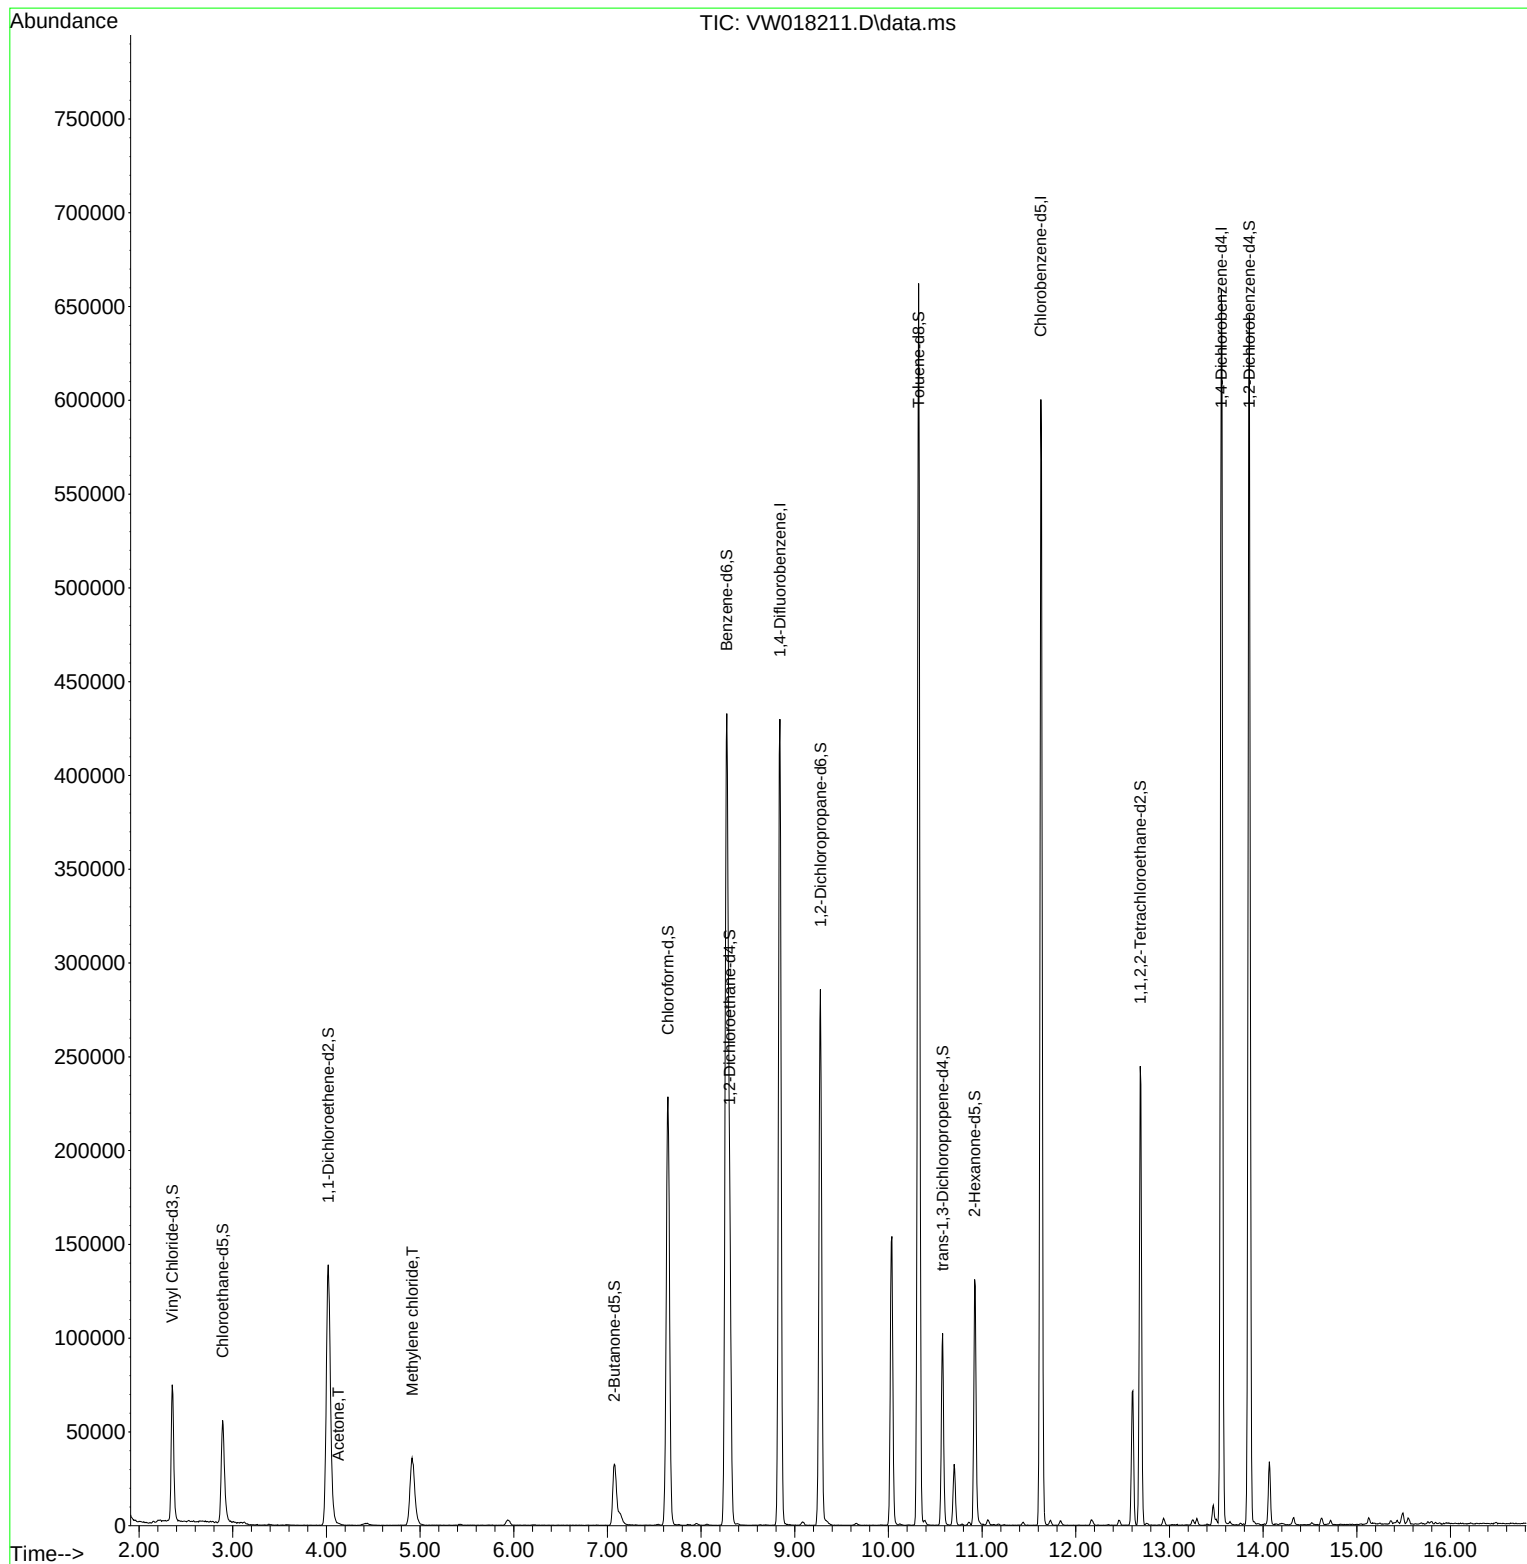


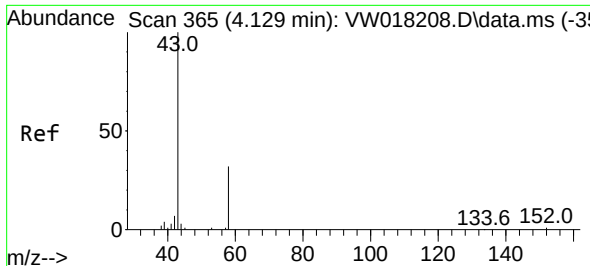

#13
Acetone
Concen: 1.28 ug/L
RT: 4.129 min Scan# 365
Delta R.T. 0.012 min
Lab File: VW018211.D
Acq: 19 Feb 2021 14:32

Instrument :
MSVOA_W
ClientSampled :
VHBLK01

Tgt Ion: 43 Resp: 1225
Ion Ratio Lower Upper
43 100
58 4.8 0.0 68.4

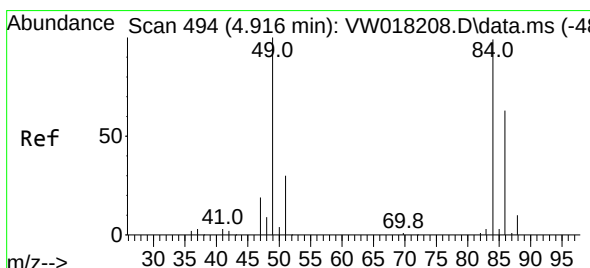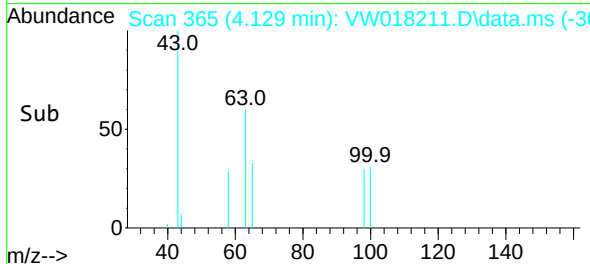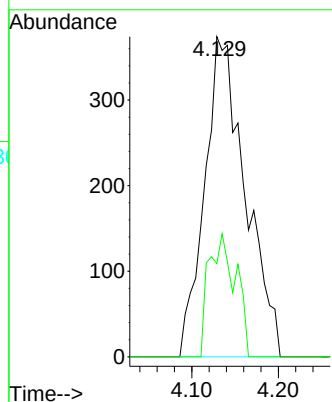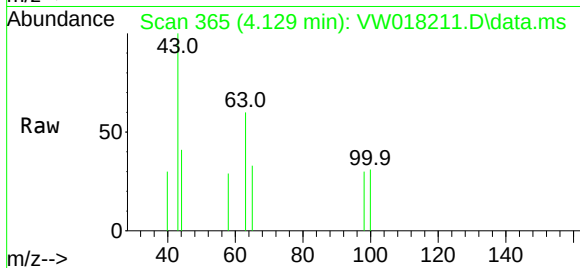

#16
Methylene chloride
Concen: 5.57 ug/L
RT: 4.915 min Scan# 494
Delta R.T. 0.006 min
Lab File: VW018211.D
Acq: 19 Feb 2021 14:32

Tgt Ion: 84 Resp: 34855
Ion Ratio Lower Upper
84 100
49 105.5 81.2 150.8
86 62.9 44.5 82.7

