

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032119\
 Data File : VW009326.D
 Acq On : 21 Mar 2019 14:58
 Operator : SY/VA
 Sample : K2017-02
 Misc : 7.02G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0D5

Manual Integrations
 APPROVED

MMDadoda
 3/23/2019 3:00:41 AM

Quant Time: Mar 22 09:43:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 22 09:38:27 2019
 Response via : Initial Calibration

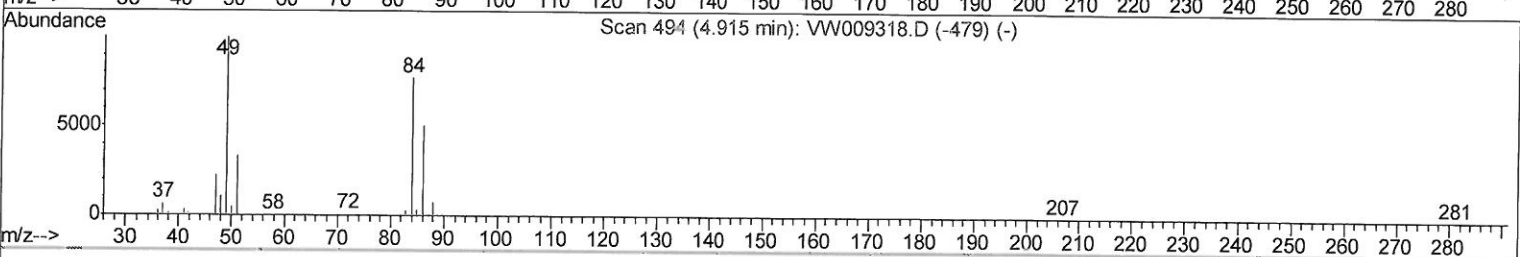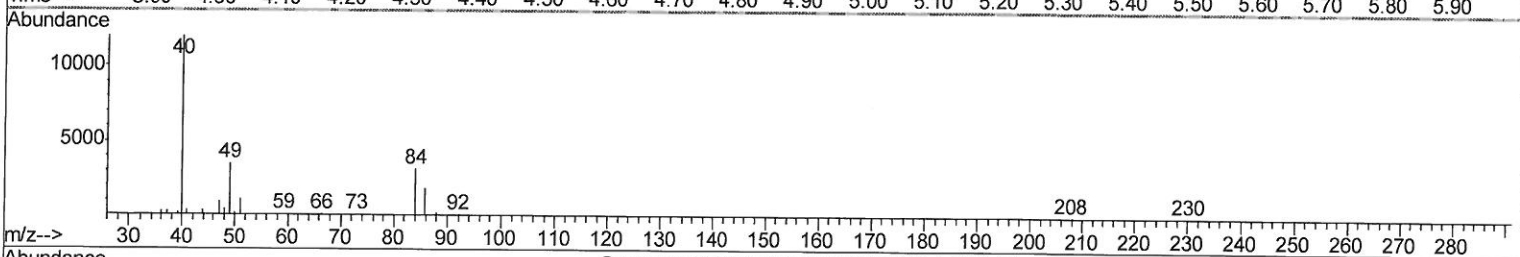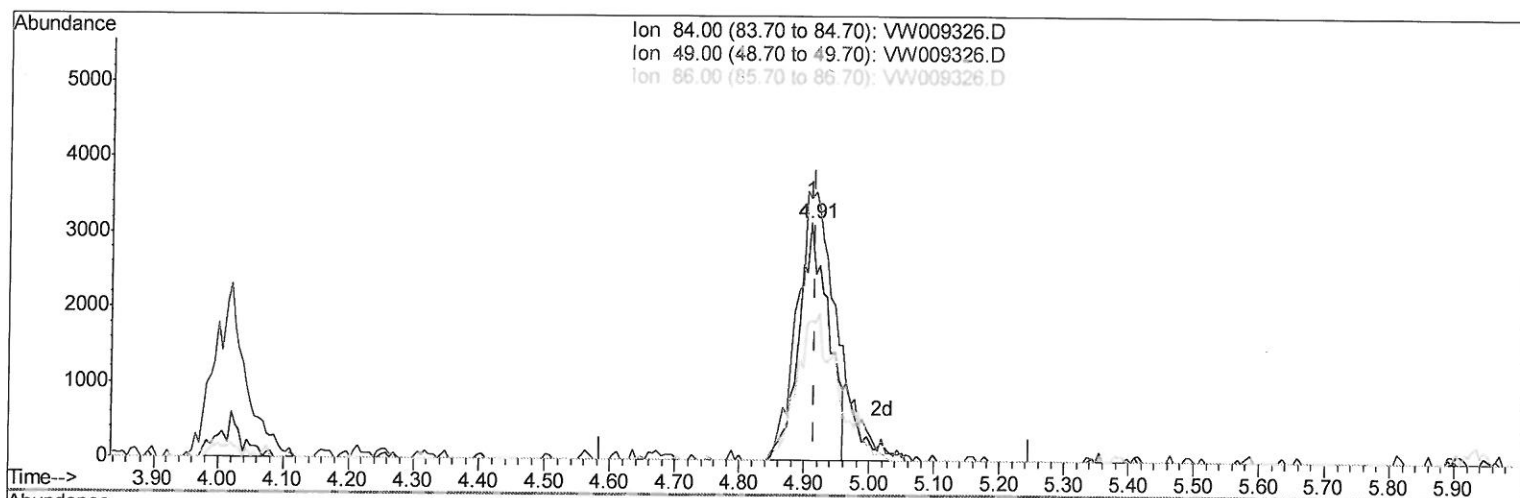

TIC: VW009326.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.66ug/L

response 10077

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	110.32
86.00	63.50	58.89
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032119\
 Data File : VW009326.D
 Acq On : 21 Mar 2019 14:58
 Operator : SY/VA
 Sample : K2017-02
 Misc : 7.02G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0D5

Manual Integrations
 APPROVED

MMDadoda
 3/23/2019 3:00:41 AM

Quant Time: Mar 22 09:43:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 22 09:38:27 2019
 Response via : Initial Calibration

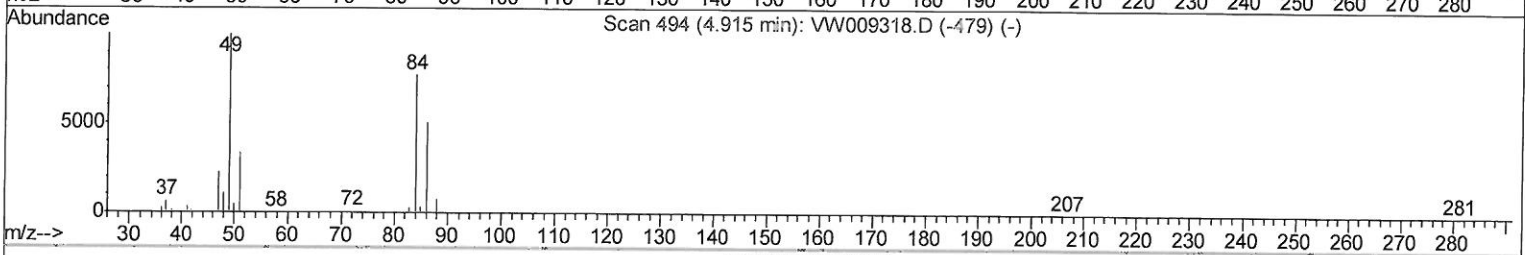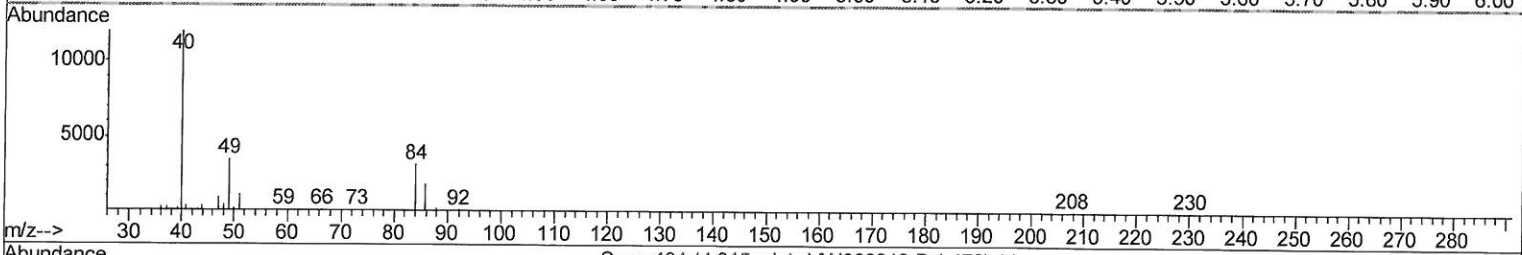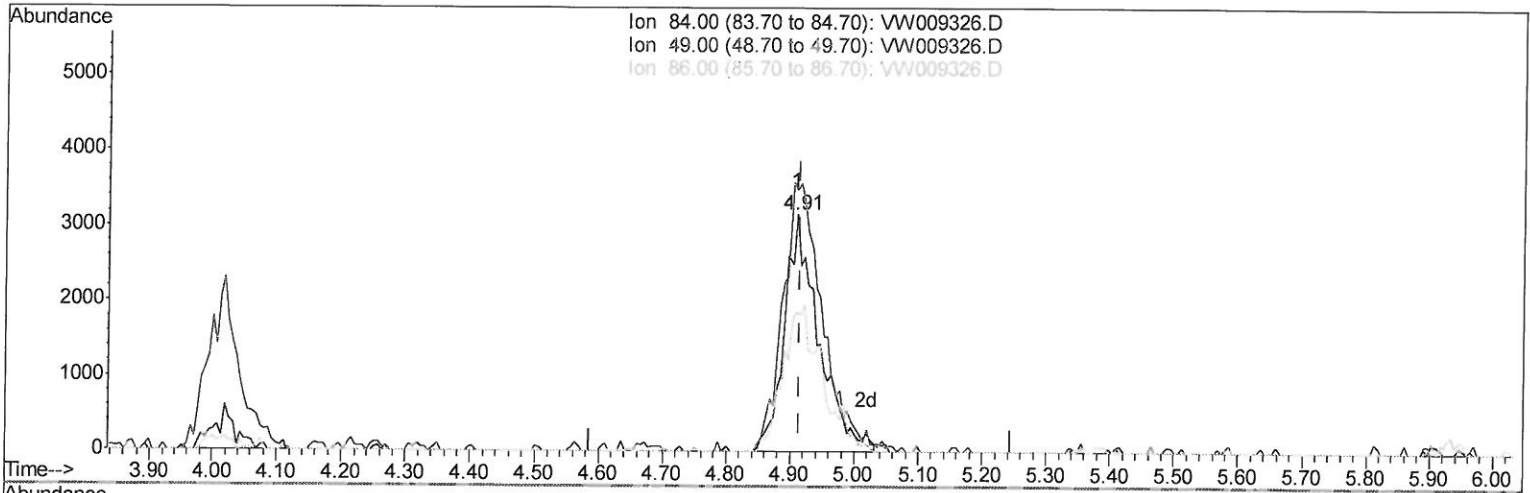

TIC: VW009326.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.93ug/L m

>03/24/1954

response 11689

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	110.32
86.00	63.50	58.89
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032119\
 Data File : VW009326.D
 Acq On : 21 Mar 2019 14:58
 Operator : SY/VA
 Sample : K2017-02
 Misc : 7.02G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF0D5

Manual Integrations
 APPROVED

MMDadoda
 3/23/2019 3:00:41 AM

Quant Time: Mar 22 10:12:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 22 09:38:27 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	415593	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	395156	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	185873	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	128066	25.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.16%
7) Chloroethane-d5	2.89	69	119754	20.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.44%
10) 1,1-Dichloroethene-d2	4.01	63	194427	18.11	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.44%
20) 2-Butanone-d5	7.07	46	79075	38.50	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.00%
24) Chloroform-d	7.64	84	273524	24.12	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.48%
26) 1,2-Dichloroethane-d4	8.31	65	159712	23.38	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.52%
29) Benzene-d6	8.27	84	513627	23.57	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.28%
33) 1,2-Dichloropropane-d6	9.27	67	159144	24.31	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.24%
37) Toluene-d8	10.32	98	460747	22.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.48%
38) trans-1,3-Dichloropropene-	10.58	79	68696	20.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.60%
39) 2-Hexanone-d5	10.93	63	57751	36.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.86%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	135602	21.04	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.16%
61) 1,2-Dichlorobenzene-d4	13.86	152	178508	25.05	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.20%

Target Compounds

16) Methylene chloride	4.91	84	11689m	1.929	ug/L	92
22) cis-1,2-Dichloroethene	7.16	96	22446	3.851	ug/L	99
35) Trichloroethene	9.09	95	1646592	285.708	ug/L	98
47) Tetrachloroethene	10.86	164	45507	9.345	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032119\
Data File : VW009326.D
Acq On : 21 Mar 2019 14:58
Operator : SY/VA
Sample : K2017-02
Misc : 7.02G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF0D5

Manual Integrations
APPROVED

MMDadoda
3/23/2019 3:00:41 AM

Quant Time: Mar 22 10:12:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 22 09:38:27 2019
Response via : Initial Calibration

