

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032621\
 Data File : VW018469.D
 Acq On : 26 Mar 2021 14:29
 Operator : SY/VA
 Sample : M1816-07
 Misc : 5.91G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG3M5

Manual Integrations
 APPROVED

MMDadoda
 3/29/2021 4:47:46 PM

Quant Time: Mar 27 01:33:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 27 01:30:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	554972	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	501031	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	245507	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	128465	16.63	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.52%		
7) Chloroethane-d5	2.892	69	120581	17.84	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.36%		
10) 1,1-Dichloroethene-d2	4.019	63	175646m	13.17	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	52.68%		
20) 2-Butanone-d5	7.086	46	60352	35.10	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	70.20%		
24) Chloroform-d	7.647	84	265842	18.81	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	75.24%		
26) 1,2-Dichloroethane-d4	8.305	65	157020	19.03	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	76.12%		
29) Benzene-d6	8.275	84	497821	18.69	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	74.76%		
33) 1,2-Dichloropropane-d6	9.275	67	147278	19.17	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	76.68%		
37) Toluene-d8	10.323	98	481614	18.78	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	75.12%		
38) trans-1,3-Dichloroprop...	10.579	79	67058	16.92	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	67.68%		
39) 2-Hexanone-d5	10.927	63	51601	34.32	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	68.64%		
48) 1,1,2,2-Tetrachloroeth...	12.689	84	132878	19.33	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	77.32%		
61) 1,2-Dichlorobenzene-d4	13.853	152	167092	19.14	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	76.56%		
Target Compounds					Qvalue	
13) Acetone	4.147	43	5355m	4.34	ug/L	
14) Carbon disulfide	4.391	76	4885	0.23	ug/L	99
16) Methylene chloride	4.910	84	15813m	1.74	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032621\
Data File : VW018469.D
Acq On : 26 Mar 2021 14:29
Operator : SY/VA
Sample : M1816-07
Misc : 5.91G/10ML/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BG3M5

Manual Integrations
APPROVED

MMDadoda
3/29/2021 4:47:46 PM

Quant Time: Mar 27 01:33:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 27 01:30:53 2021
Response via : Initial Calibration

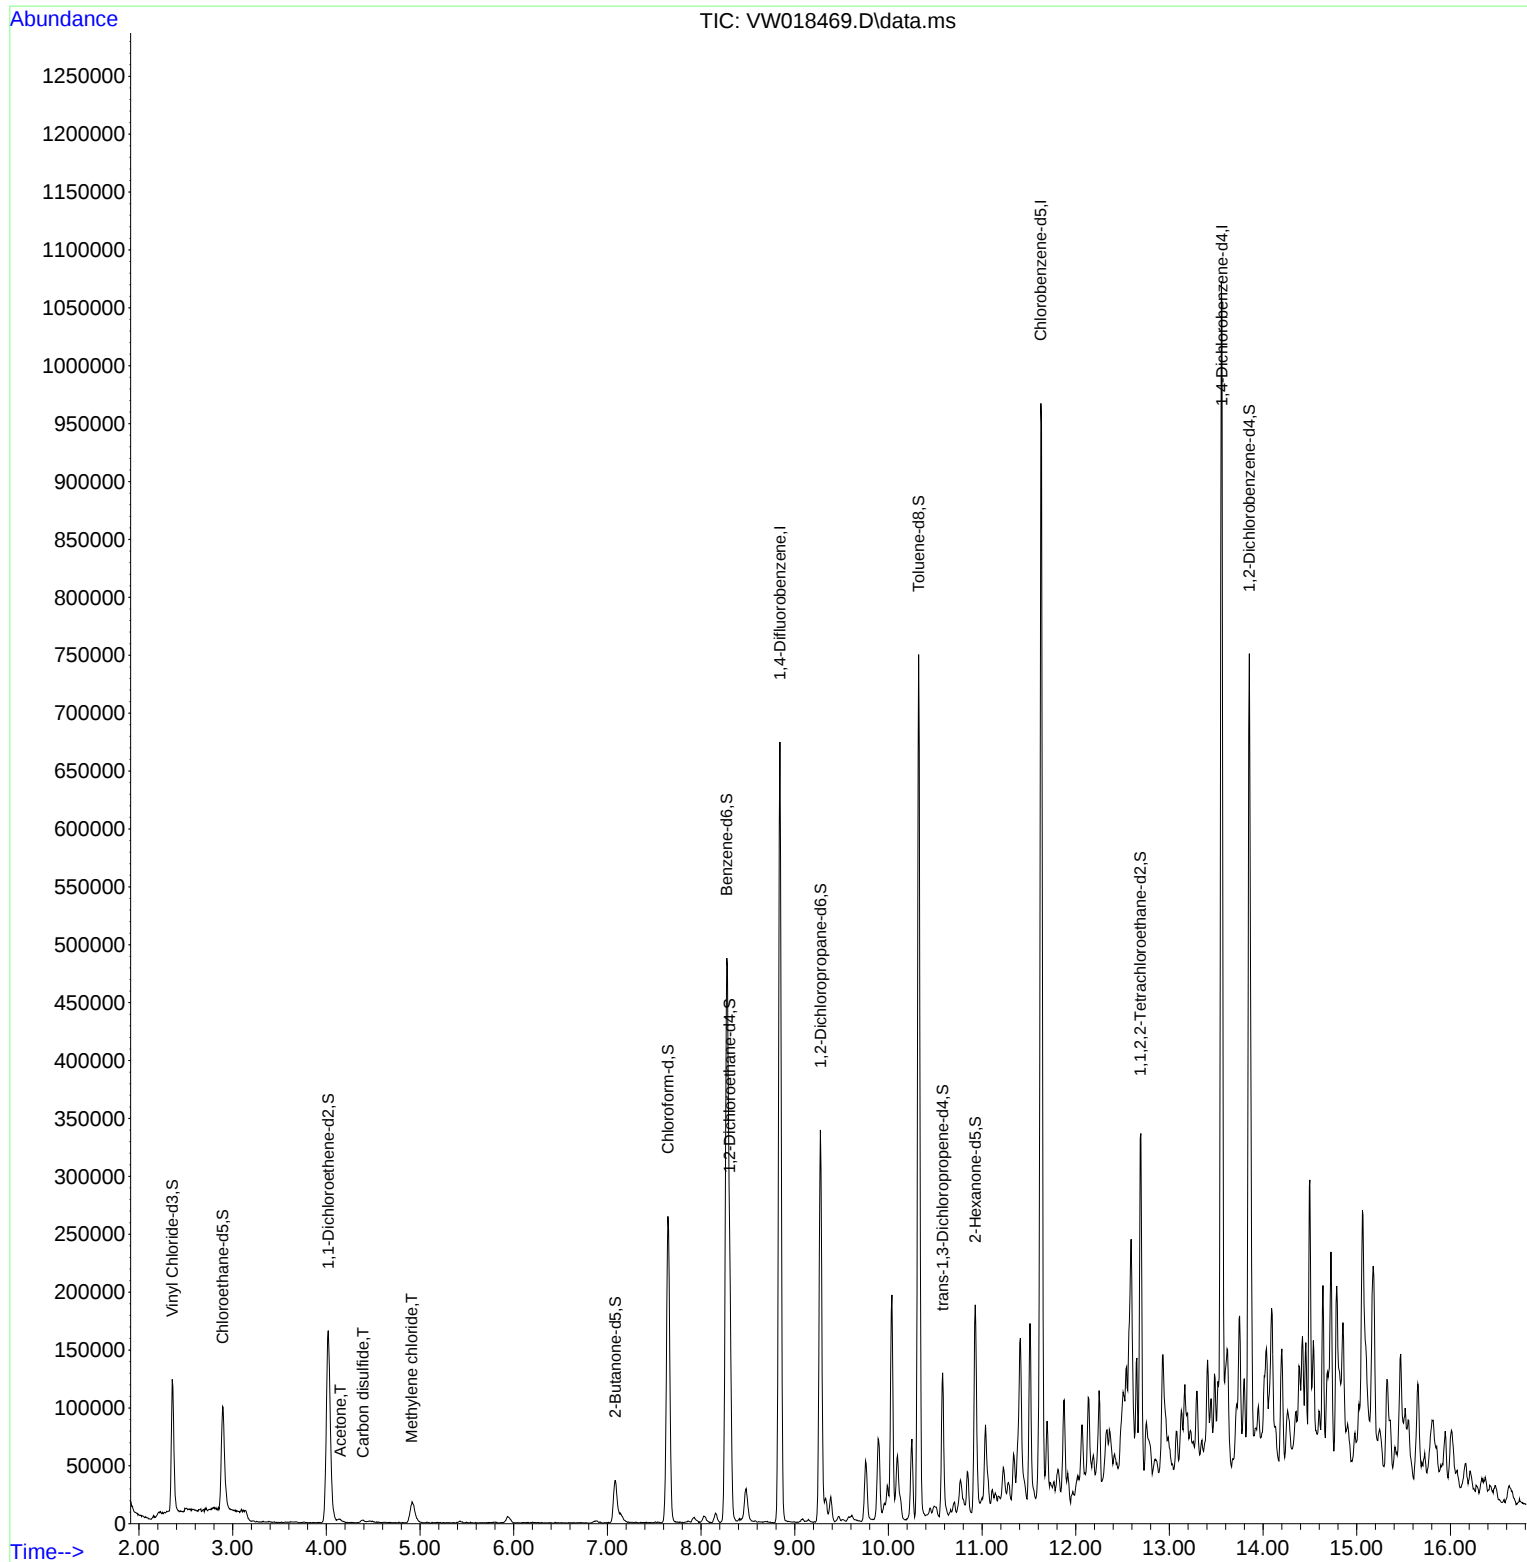

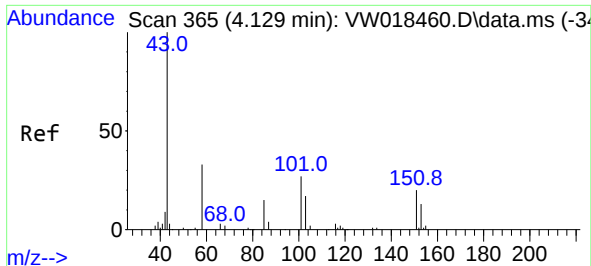





#13
Acetone
Concen: 4.34 ug/L m
RT: 4.147 min Scan# 368
Delta R.T. 0.018 min
Lab File: VW018469.D
Acq: 26 Mar 2021 14:29

Tgt Ion: 43 Resp: 5355
Ion Ratio Lower Upper
43 100
58 17.5 0.0 62.2

Instrument :
MSVOA_W
ClientSampled :
BG3M5




Manual Integrations
APPROVED


MMDadoda
3/29/2021 4:47:46 PM

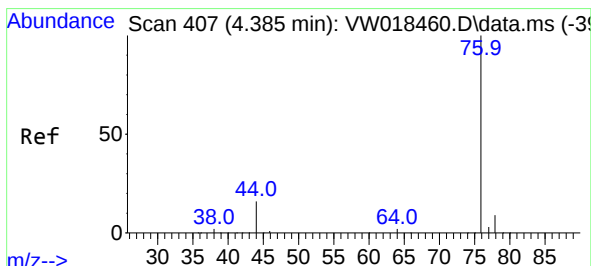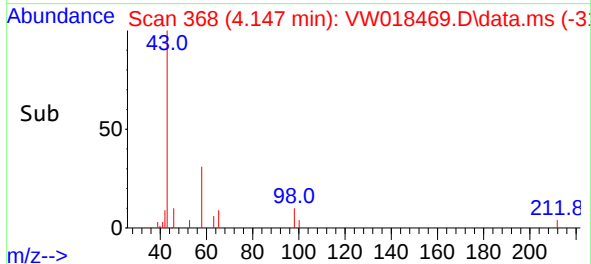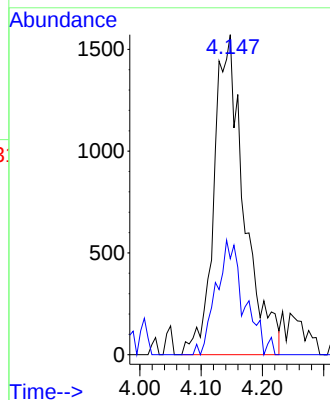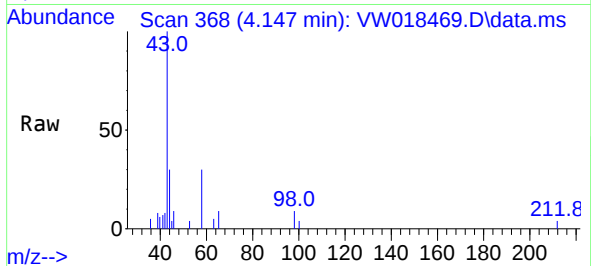

#14
Carbon disulfide
Concen: 0.23 ug/L
RT: 4.391 min Scan# 408
Delta R.T. 0.006 min
Lab File: VW018469.D
Acq: 26 Mar 2021 14:29


Tgt Ion: 76 Resp: 4885
Ion Ratio Lower Upper
76 100
78 9.8 7.4 11.2

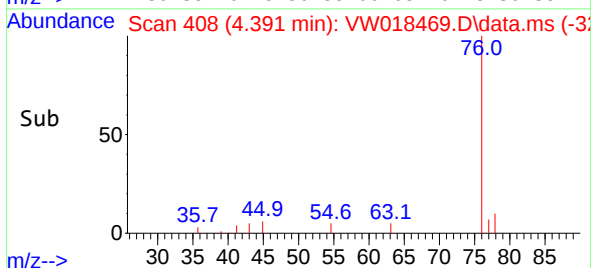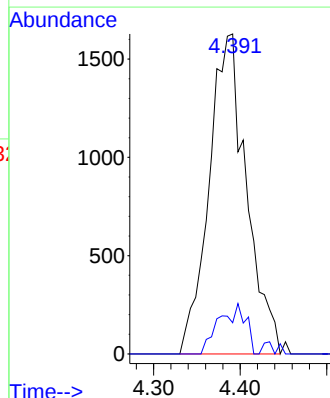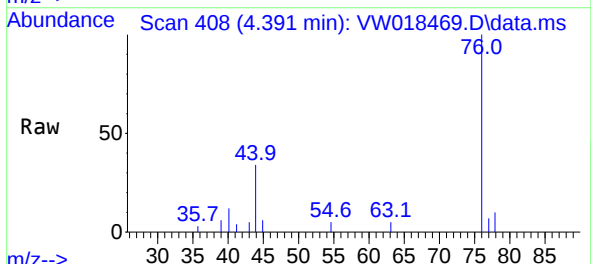

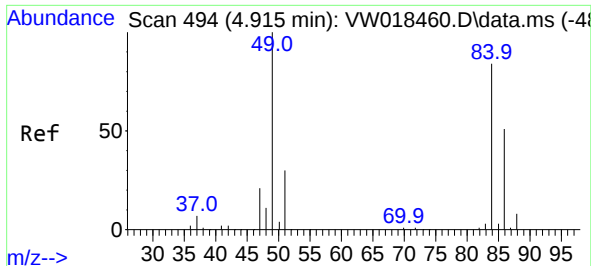

#16
Methylene chloride
Concen: 1.74 ug/L m
RT: 4.910 min Scan# 493
Delta R.T. -0.006 min
Lab File: VW018469.D
Acq: 26 Mar 2021 14:29

Instrument :
MSVOA_W
ClientSampled :
BG3M5

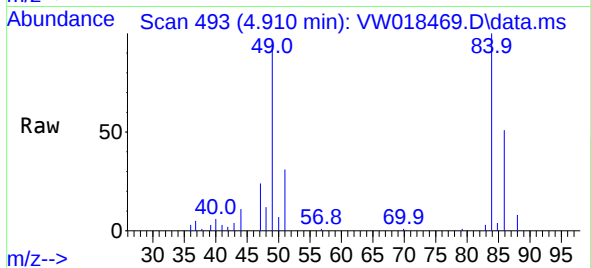

Tgt Ion:	84	Resp:	15813
Ion	Ratio	Lower	Upper
84	100		
49	95.6	74.4	138.2
86	51.4	46.1	85.7

Manual Integrations
APPROVED

MMDadoda
3/29/2021 4:47:46 PM

