

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062320\
 Data File : VW015667.D
 Acq On : 23 Jun 2020 17:39
 Operator : SY/VA
 Sample : L3079-09
 Misc : 2.22G/5ML/MSVOA W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JFK-SB-01-0.0-2.0-D

Quant Time: Jun 24 03:07:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062320S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 23 13:20:19 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.95
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.85
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.63
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.56

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062320\
Data File : VW015667.D
Acq On : 23 Jun 2020 17:39
Operator : SY/VA
Sample : L3079-09
Misc : 2.22G/5ML/MSVOA W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JFK-SB-01-0.0-2.0-D

Quant Time: Jun 24 03:07:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W062320S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 23 13:20:19 2020
Response via : Initial Calibration

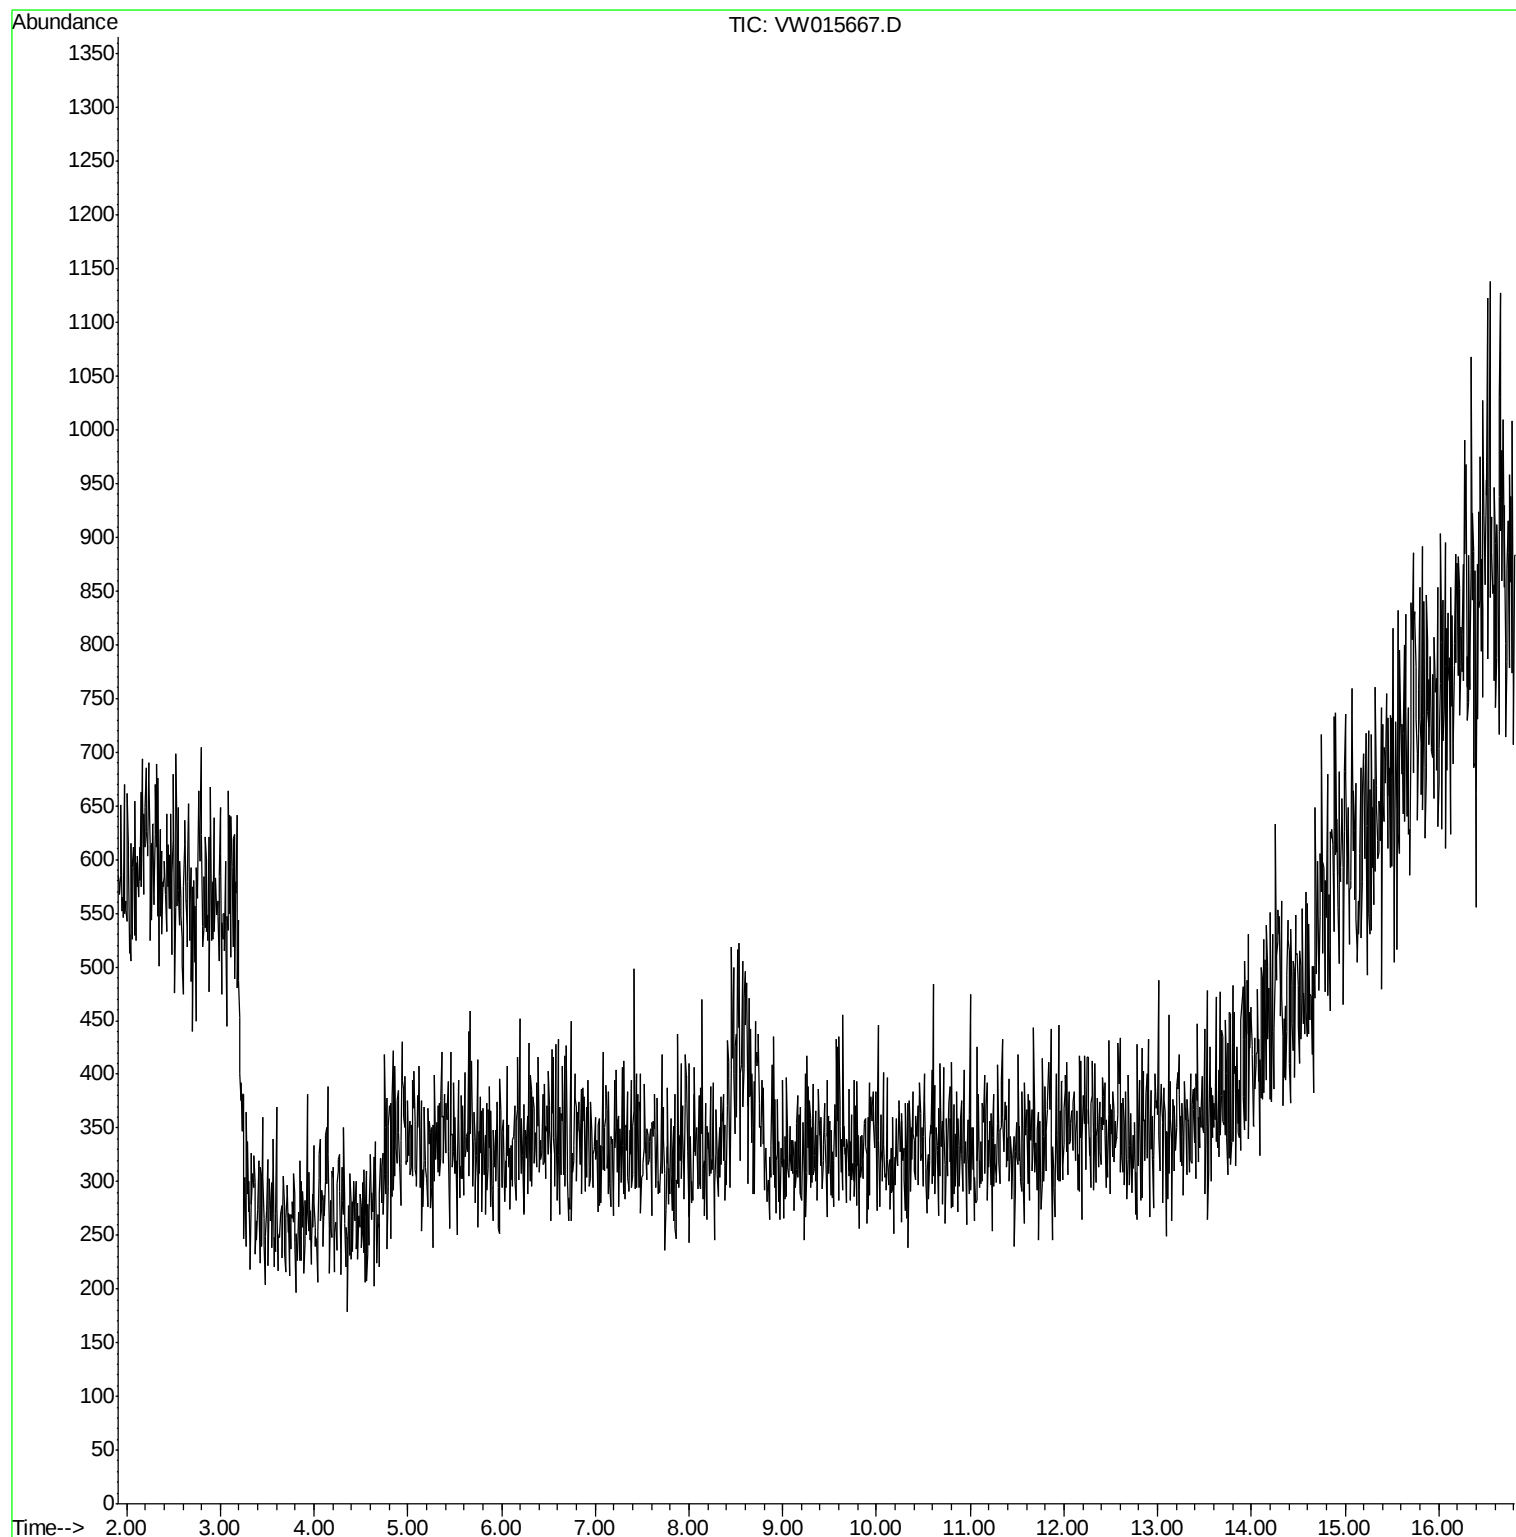

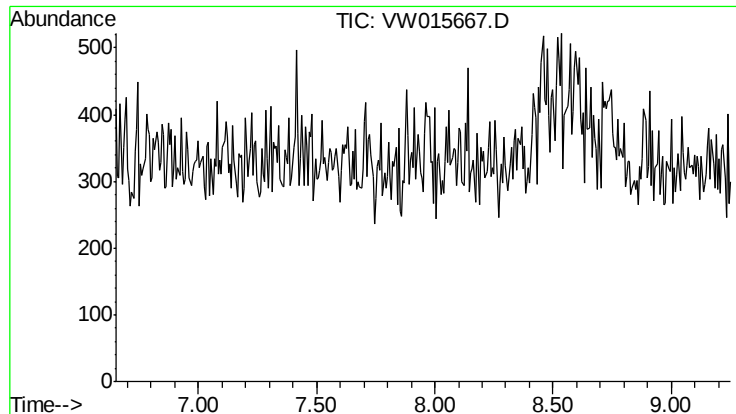

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.95 min

Lab File: VW015667.D

Acq: 23 Jun 2020 17:39

Tot Ion: 168

Sig Exp Ratio

168 100



99 60.8

Instrument :

MSVOA_W

ClientSampleId :

JFK-SB-01-0.0-2.0-D

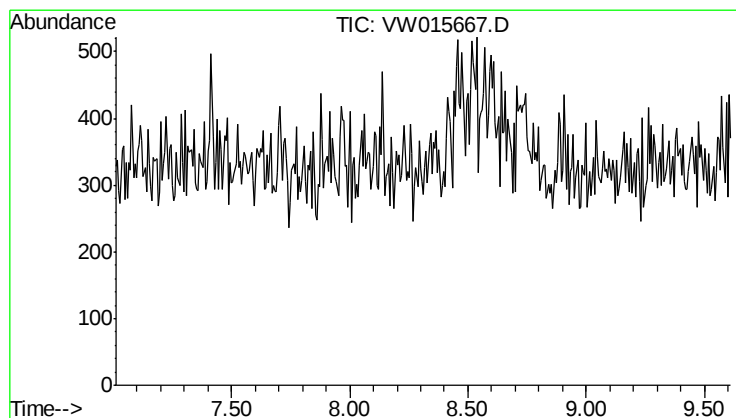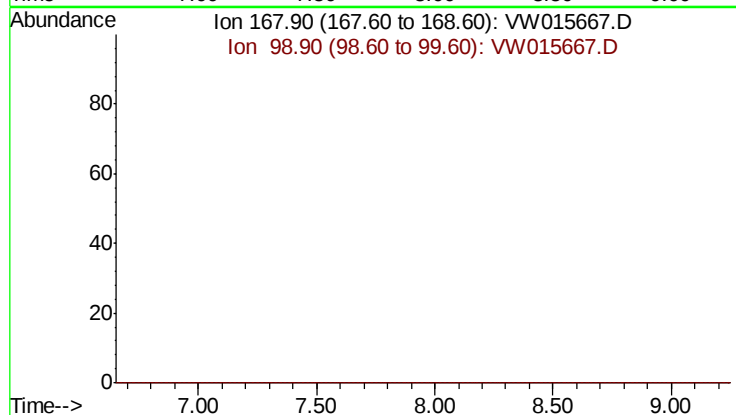

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 8.31 min

Lab File: VW015667.D


Acq: 23 Jun 2020 17:39


Tgt Ion: 65

Sig Exp Ratio

65 100

67 51.1

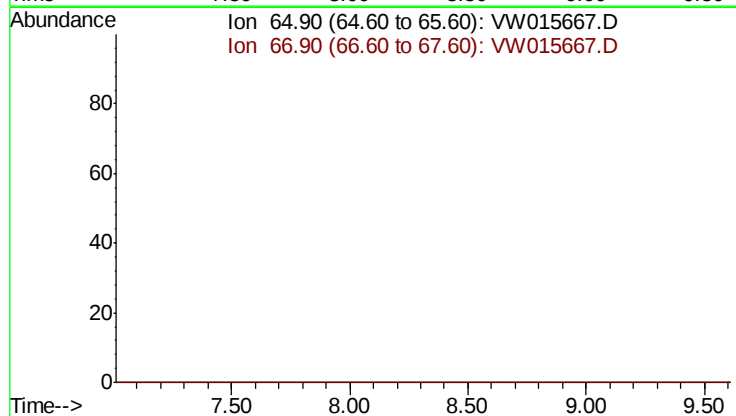


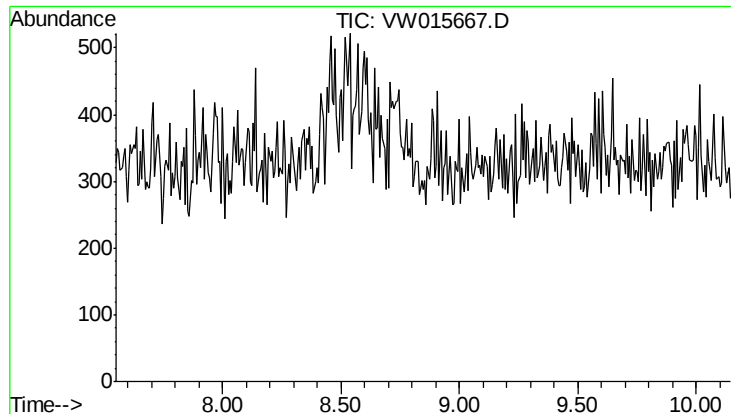


#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.85 min

Lab File: VW015667.D
 Acq: 23 Jun 2020 17:39

Instrument :
 MSVOA_W
 ClientSampleId :
 JFK-SB-01-0.0-2.0-D


Tot Ion	114
Sig	Exp Ratio
114	100
63	21.2
88	16.3

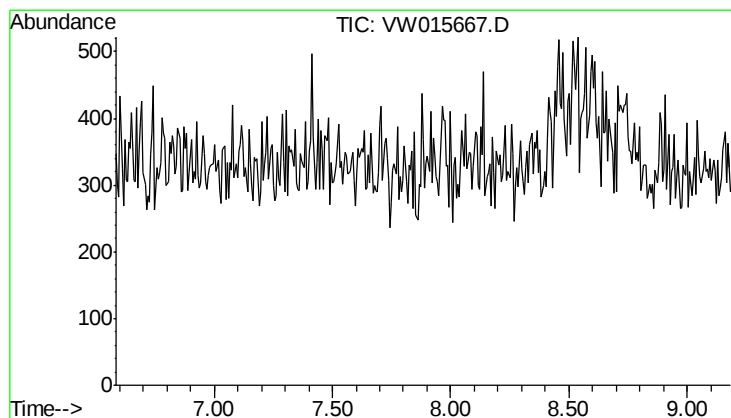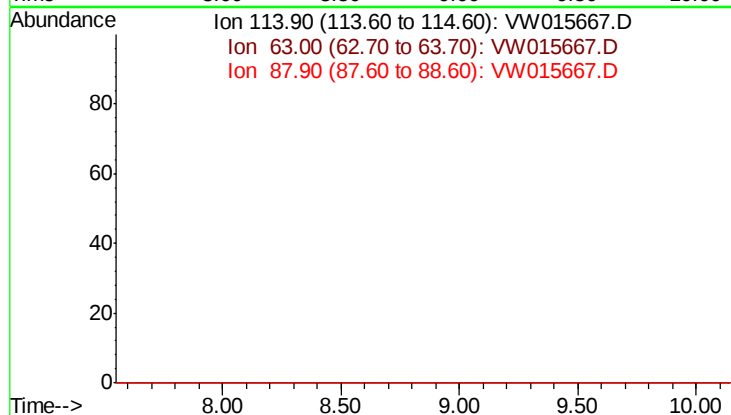


#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.88 min

Lab File: VW015667.D
 Acq: 23 Jun 2020 17:39

Tgt Ion	113
Sig	Exp Ratio
113	100
111	102.9
192	20.5

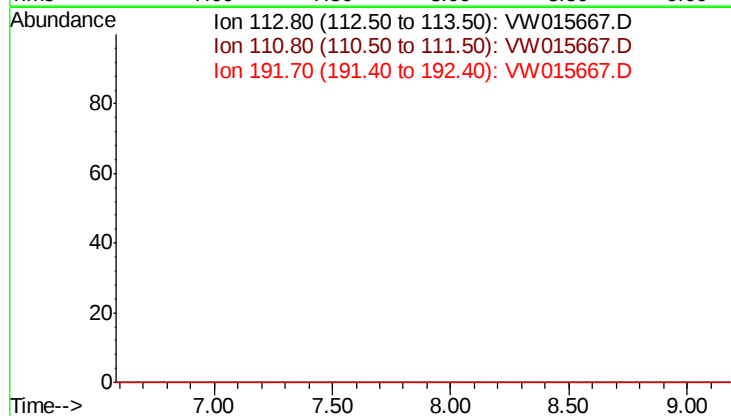


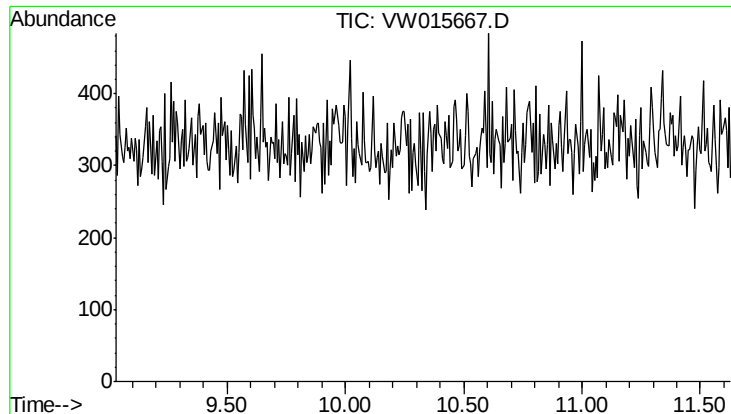


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.33 min

Lab File: VW015667.D
Acq: 23 Jun 2020 17:39

Instrument :
MSVOA_W
ClientSampleId :
JFK-SB-01-0.0-2.0-D


Tot Ion	98
Sig	Exp Ratio
98	100
100	66.0

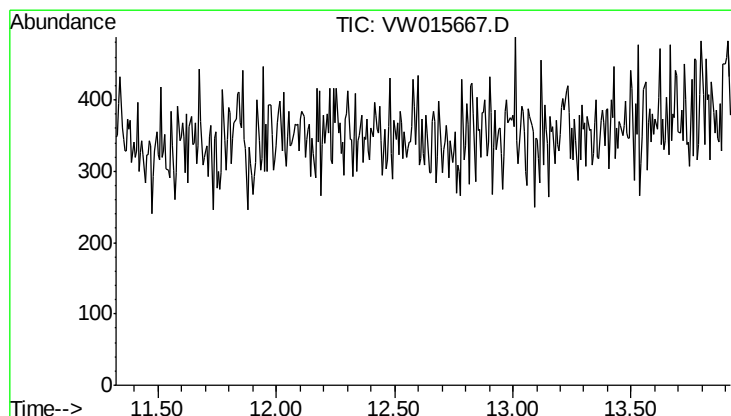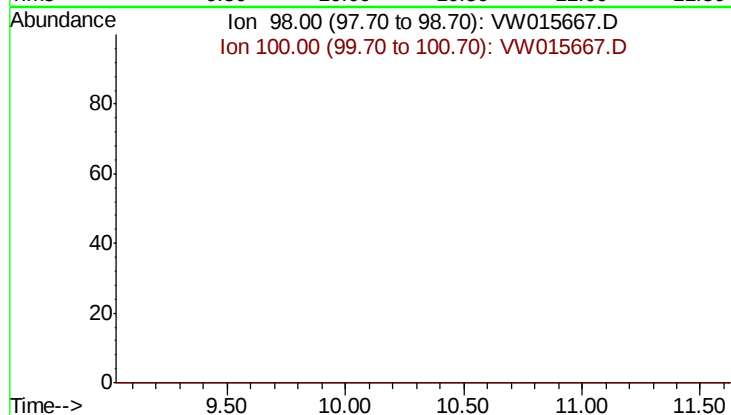


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.62 min

Lab File: VW015667.D
Acq: 23 Jun 2020 17:39

Tgt Ion	95
Sig	Exp Ratio
95	100
174	78.5
176	75.7


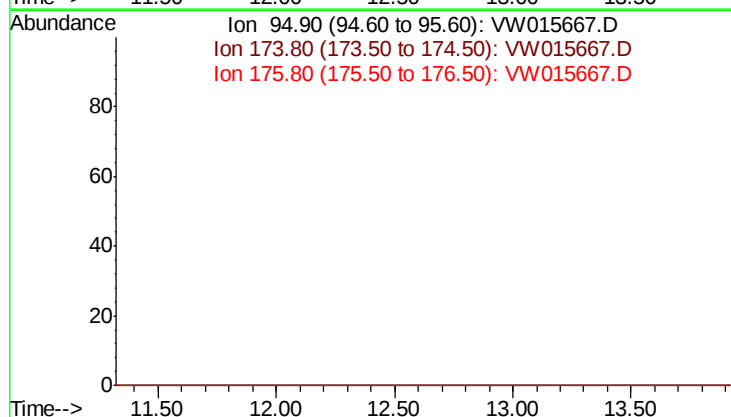


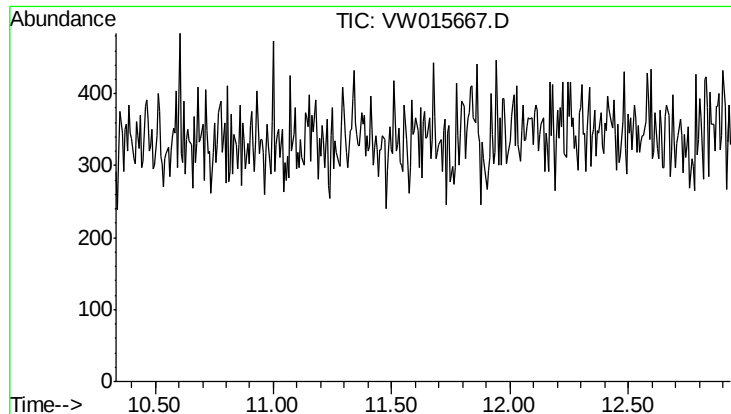

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.63 min
 Lab File: VW015667.D
 Acq: 23 Jun 2020 17:39

Instrument :
 MSVOA_W
 ClientSampleId :
 JFK-SB-01-0.0-2.0-D

Tot Ion: 117
 Sig Exp Ratio
 117 100
 82 56.4
 119 32.3

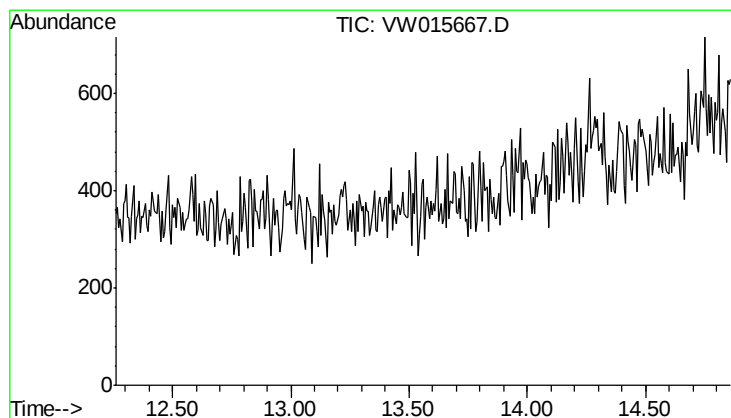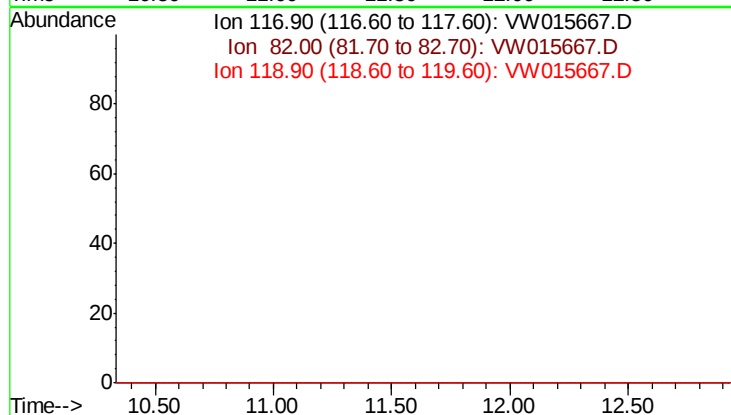

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.56 min
 Lab File: VW015667.D
 Acq: 23 Jun 2020 17:39

Tgt Ion: 152
 Sig Exp Ratio
 152 100
 115 60.3
 150 172.8

