



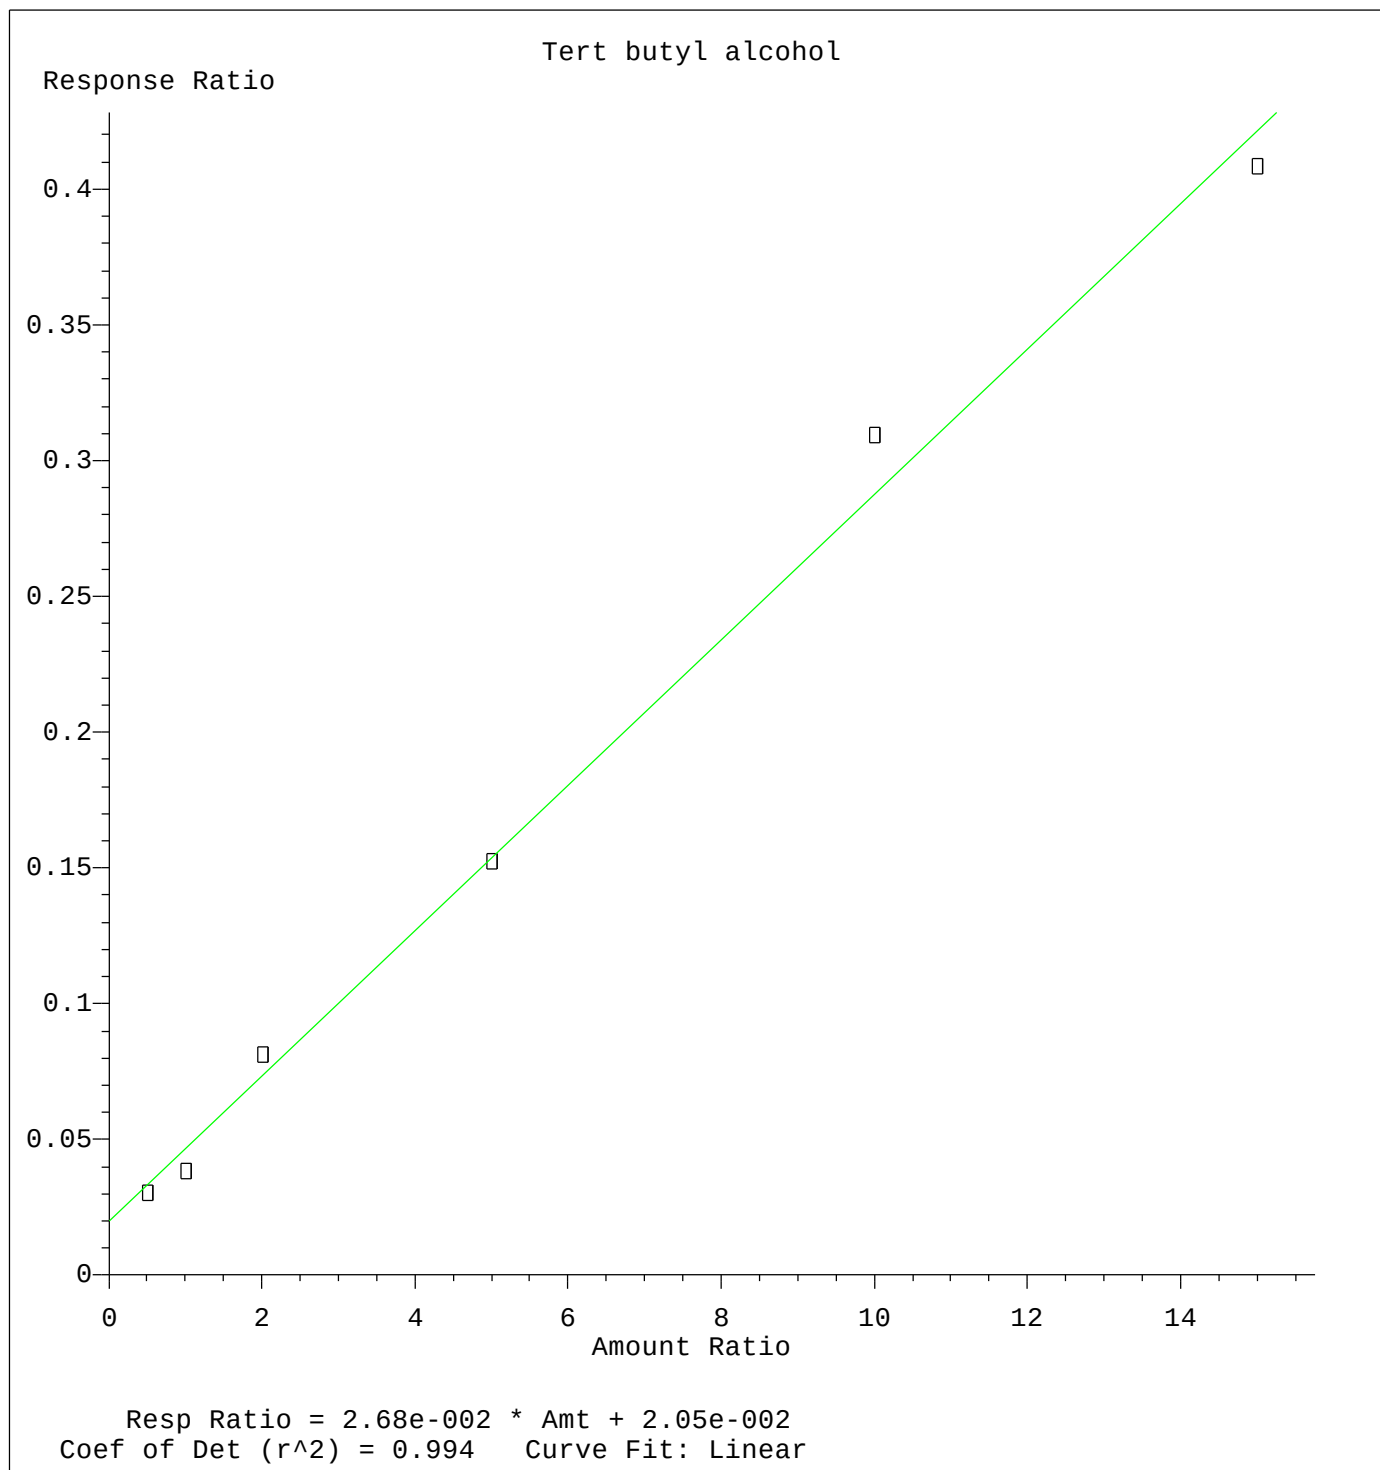


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062320S.M
Calibration Table Last Updated: Tue Jun 23 13:20:19 2020

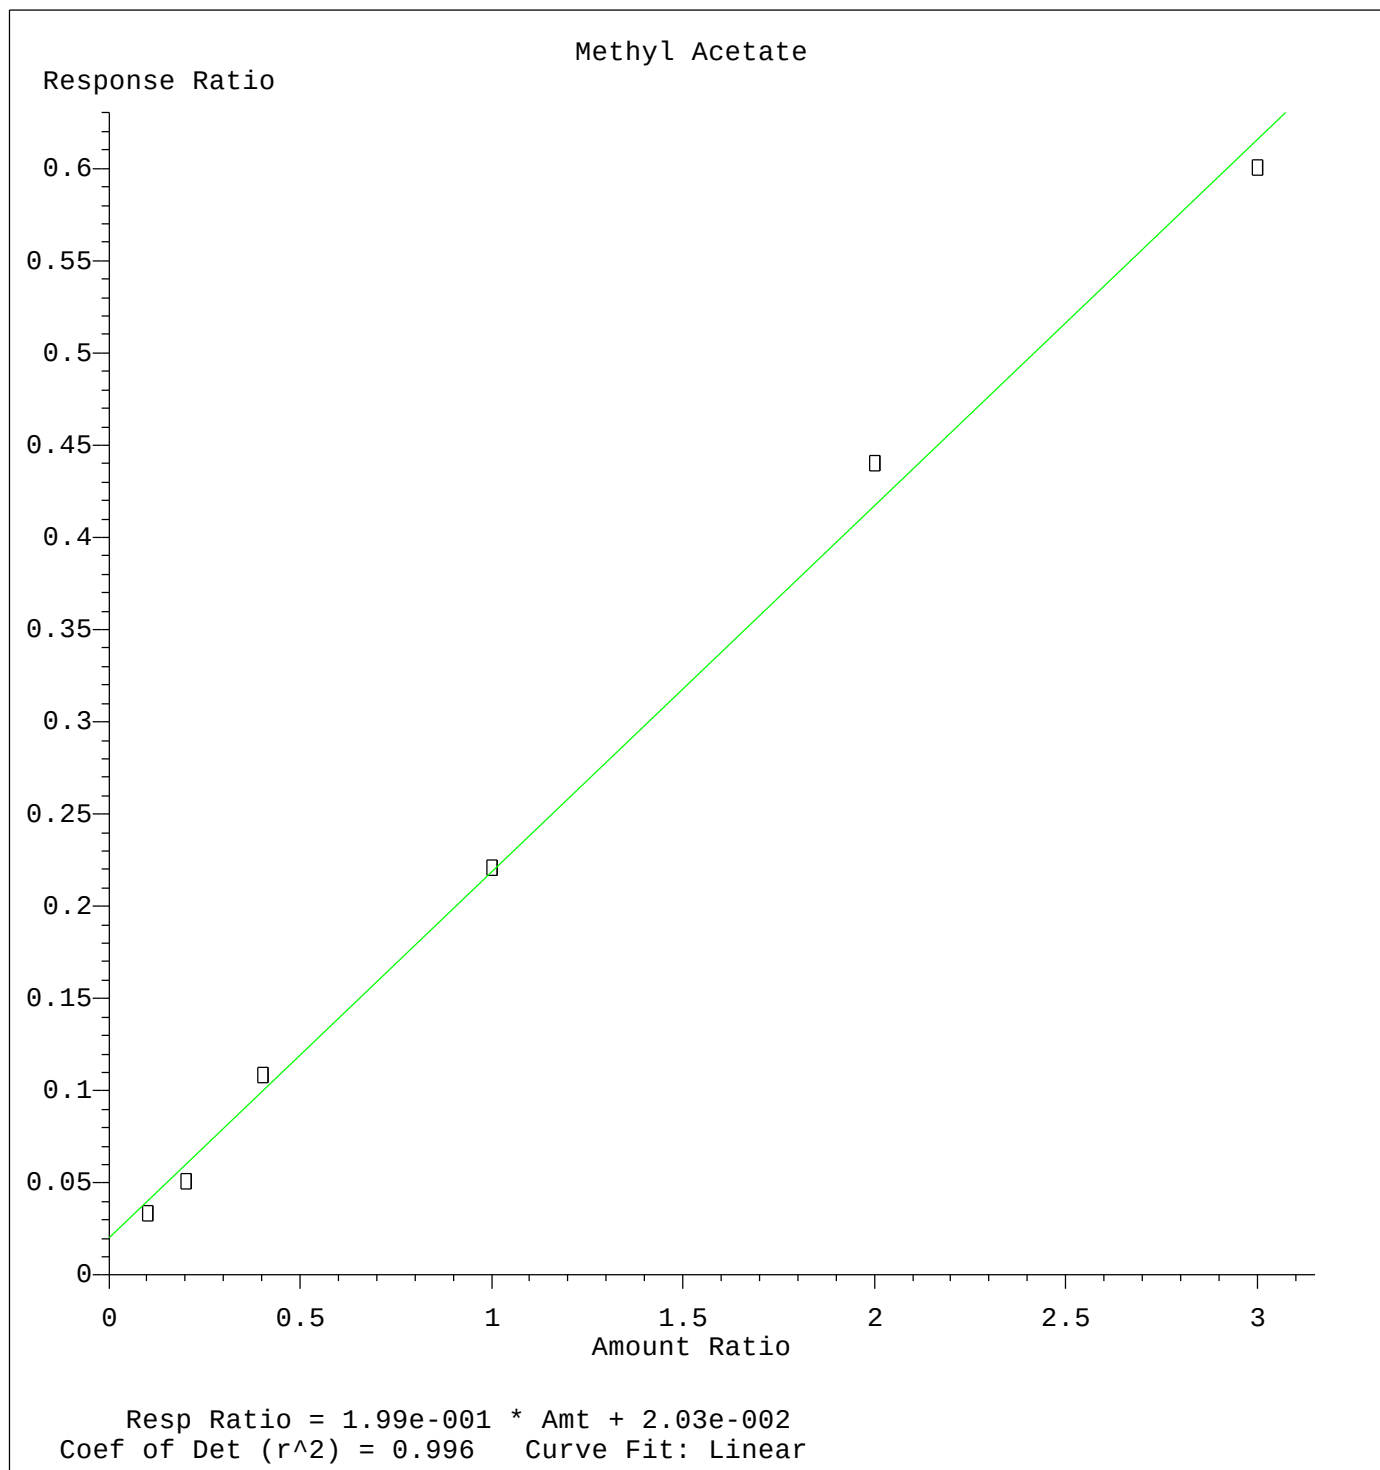

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062320S.M
Calibration Table Last Updated: Tue Jun 23 13:20:19 2020


Methylene Chloride

Response Ratio

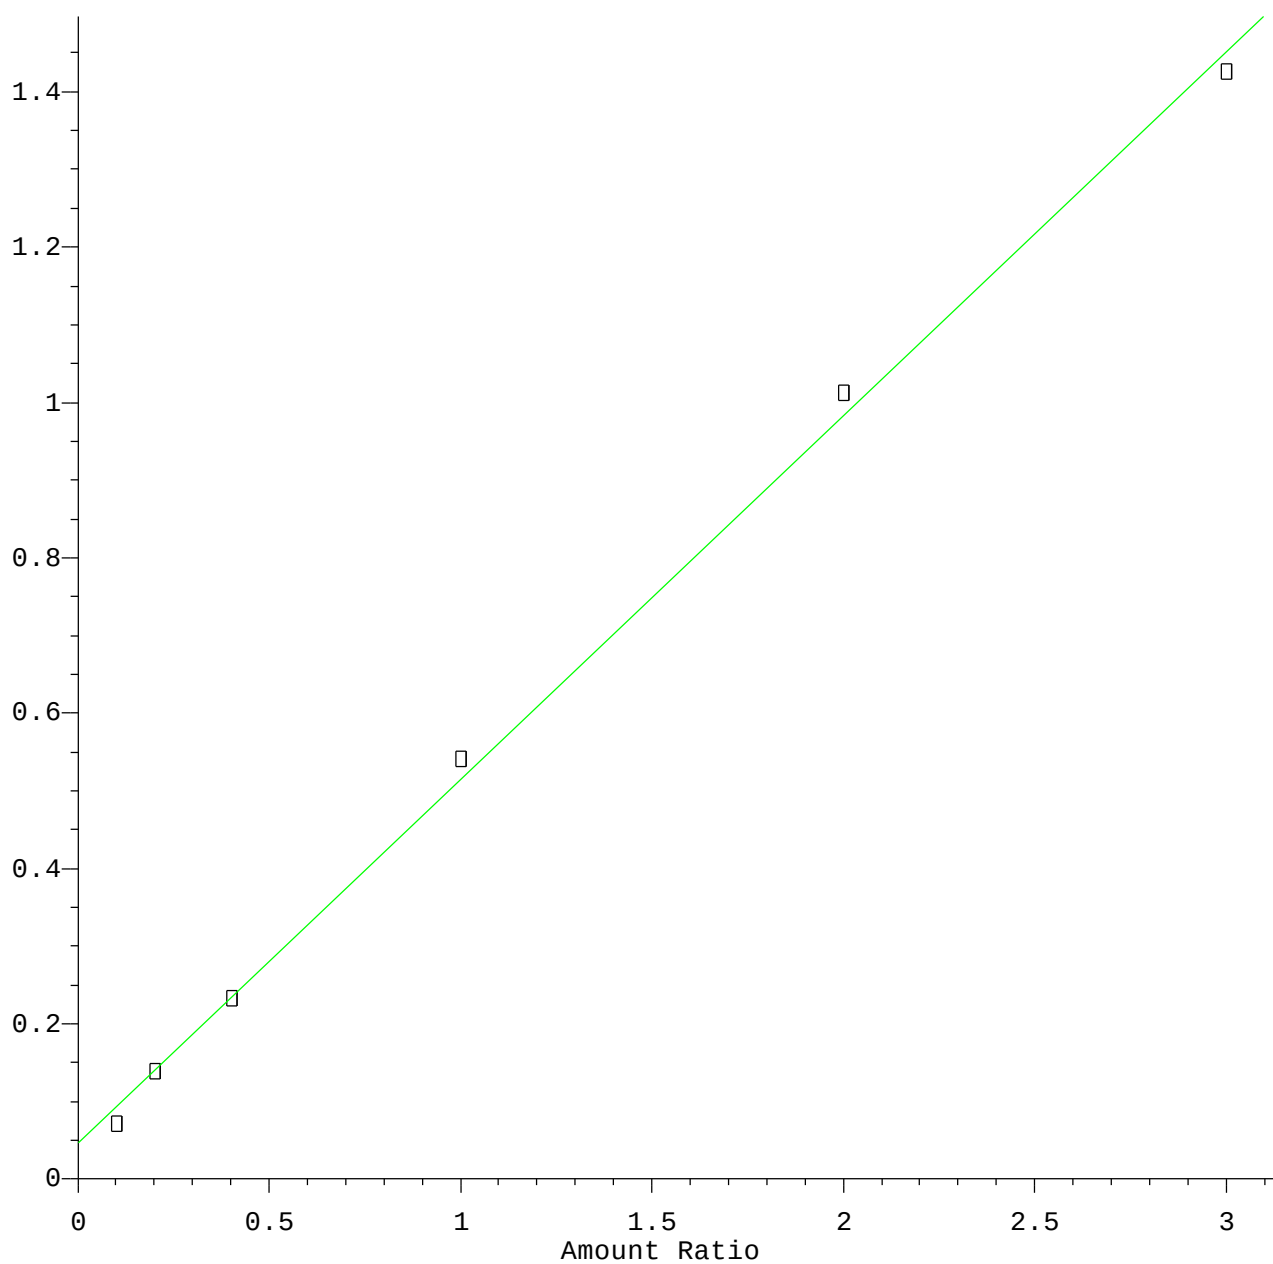


Resp Ratio = $4.68 \times 10^{-1} \times \text{Amt} + 4.69 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062320S.M
Calibration Table Last Updated: Tue Jun 23 13:20:19 2020

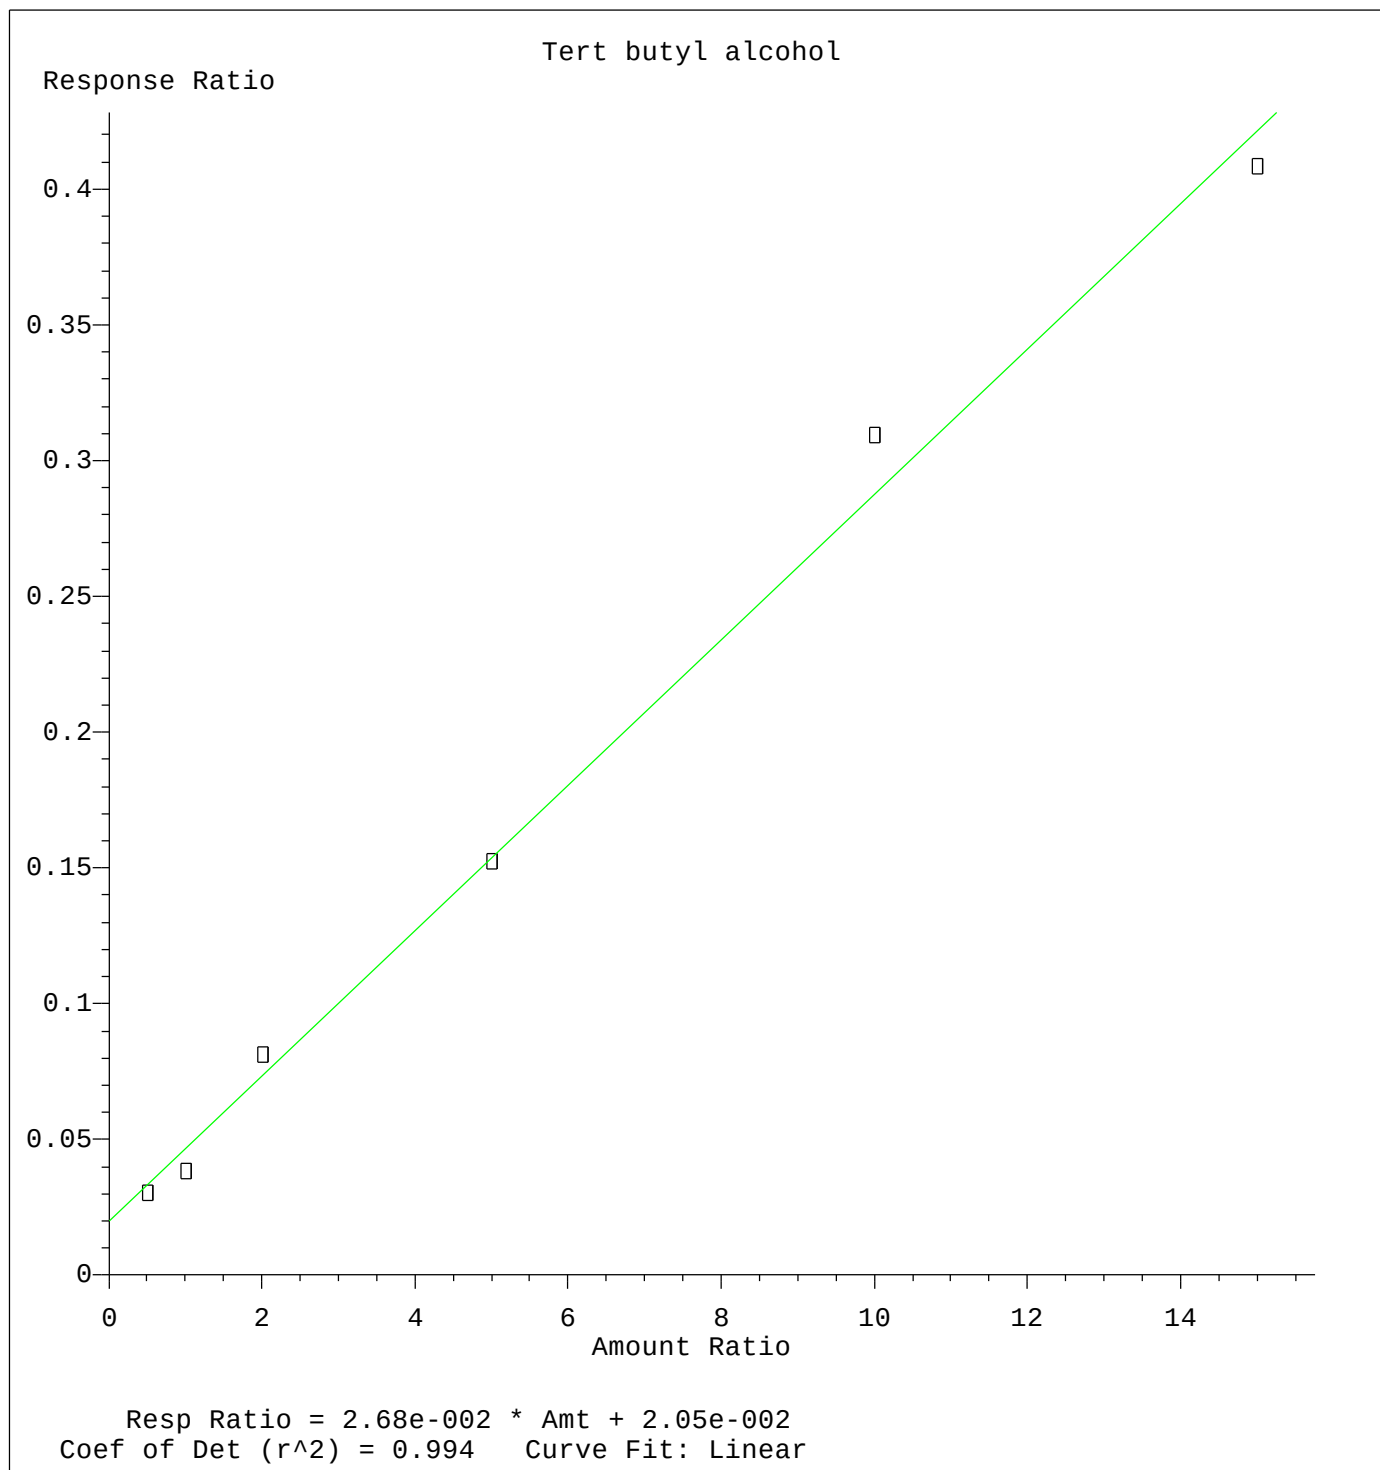


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062320S.M
Calibration Table Last Updated: Tue Jun 23 13:20:19 2020

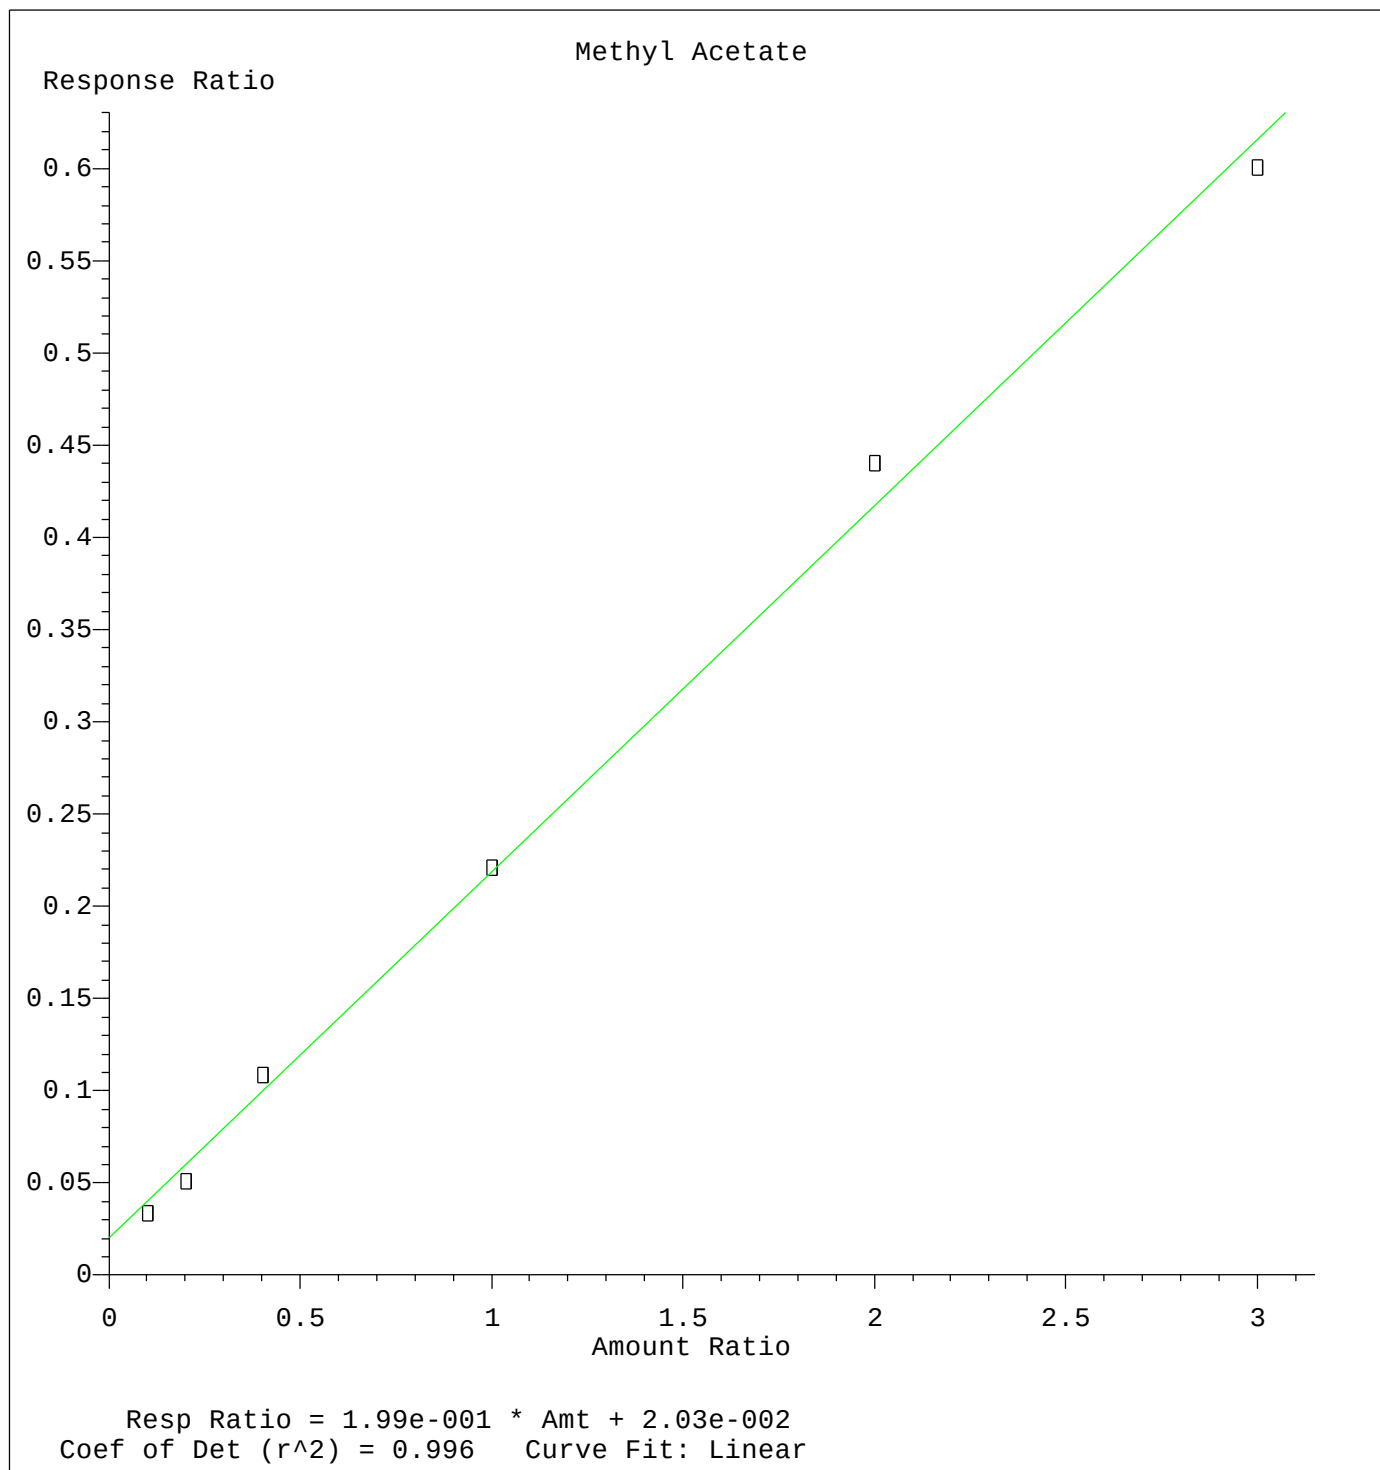

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062320S.M
Calibration Table Last Updated: Tue Jun 23 13:20:19 2020

Methylene Chloride

Response Ratio

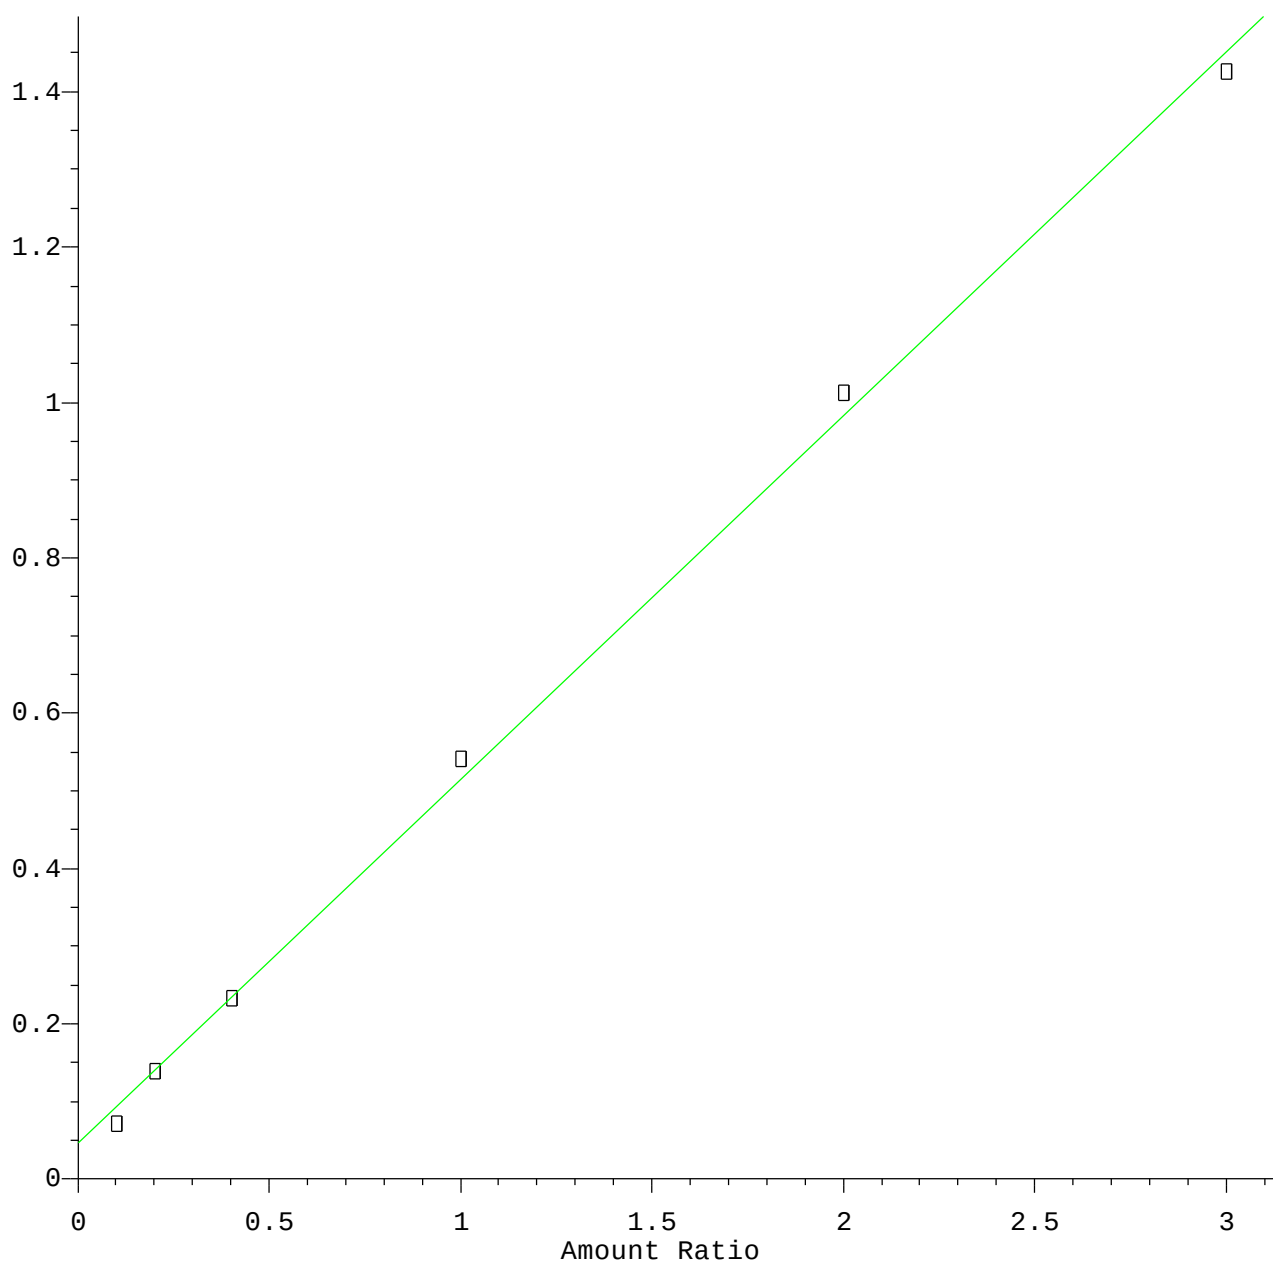

Resp Ratio = $4.68 \times 10^{-1} \times \text{Amt} + 4.69 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062320S.M
Calibration Table Last Updated: Tue Jun 23 13:20:19 2020